

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
 Data File : PD082870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2024 17:09
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:38:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 04:33:00 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.777	7545757	19755372	4.994	5.042
27)	SA Decachlor...	9.121	7.905	21199992	41477607	10.666	10.585
Target Compounds							
2)	A alpha-BHC	4.022	3.276	11740312	29759223	4.620	4.824
3)	MA gamma-BHC...	4.356	3.604	11609694	28097776	4.728	4.866
4)	MA Heptachlor	4.948	3.943	12224736	27311256	4.836	4.908
9)	A Endosulfan I	6.107	5.092	10441214	22284176	5.011	4.943
13)	MA Dieldrin	6.382	5.356	21222254	48456199	9.664	9.647
14)	MA Endrin	6.613	5.631	17336439	43381580	9.669	9.921
16)	A 4,4'-DDD	6.746	5.778	14807392	35961106	9.439	9.526
17)	MA 4,4'-DDT	7.062	6.029	15305350	35243483	9.356	9.159
20)	A Methoxychlor	7.539	6.604	45023860	105.1E6	51.179	52.718


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 17:09
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:38:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 04:33:00 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

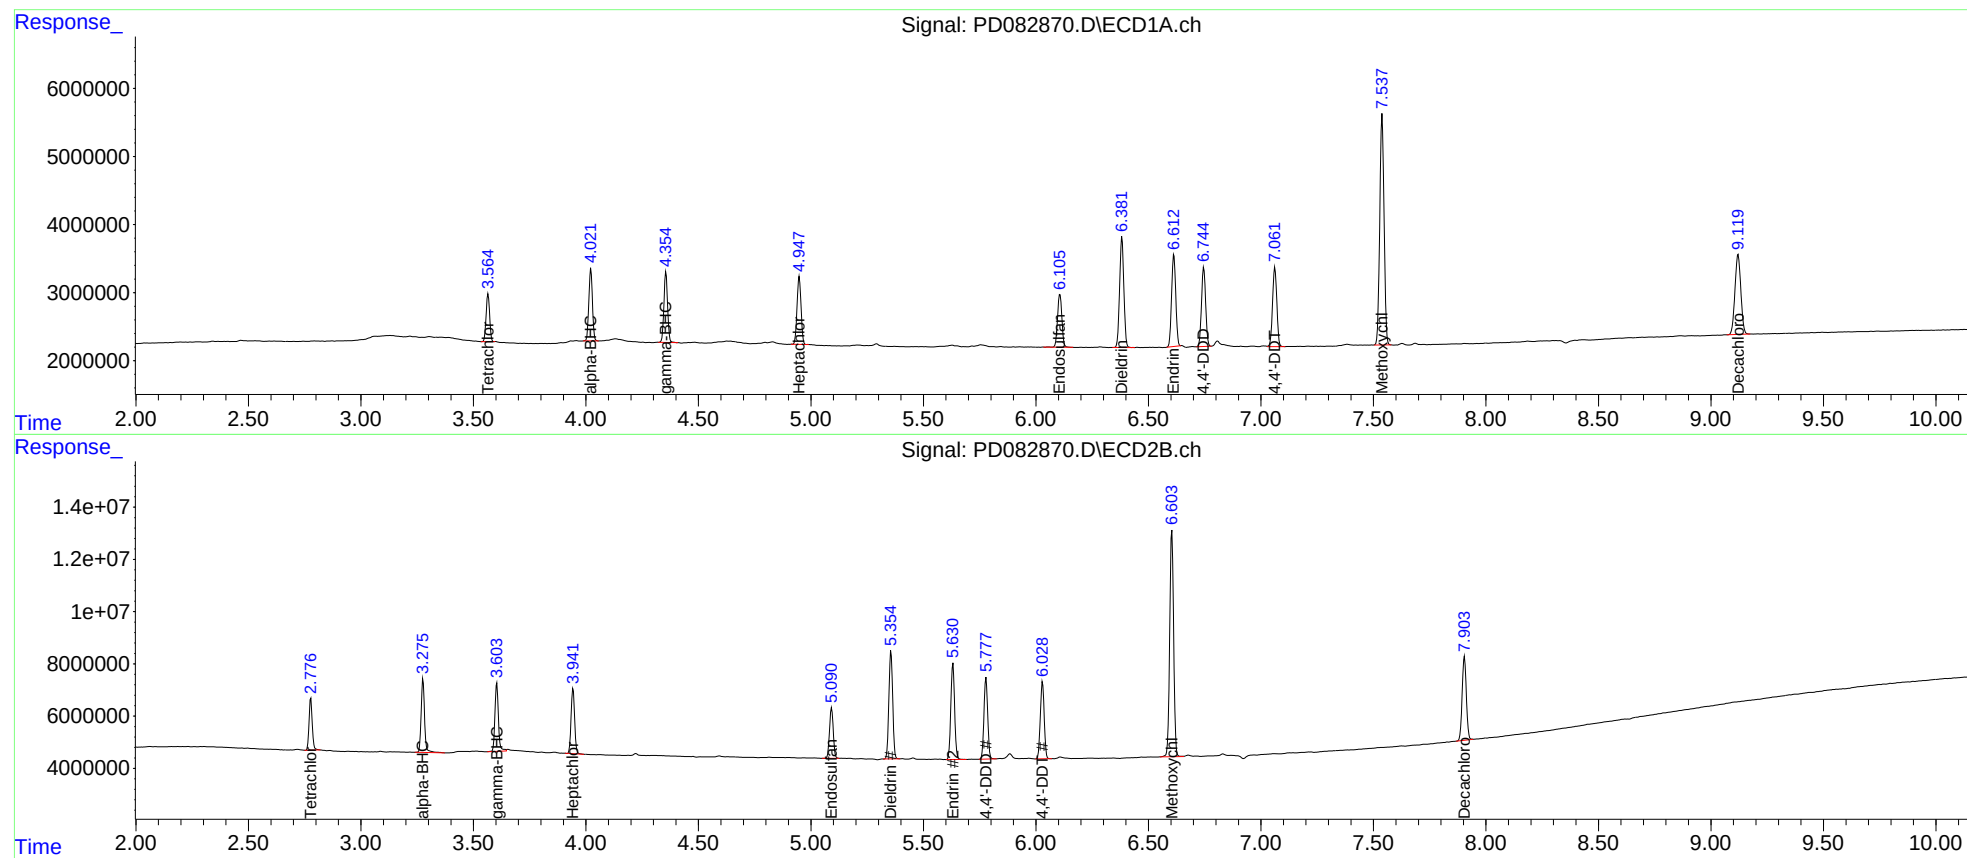

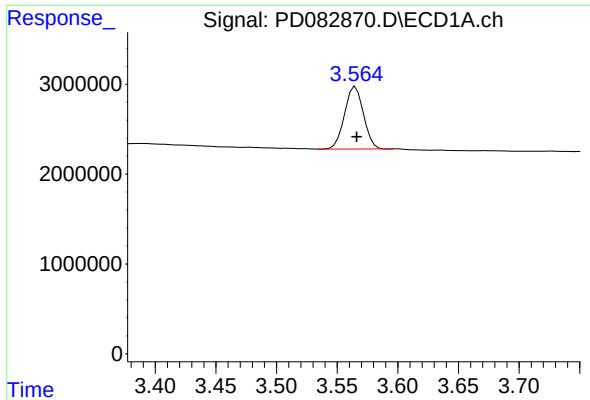


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 7545757
Conc: 4.99 ng/ml

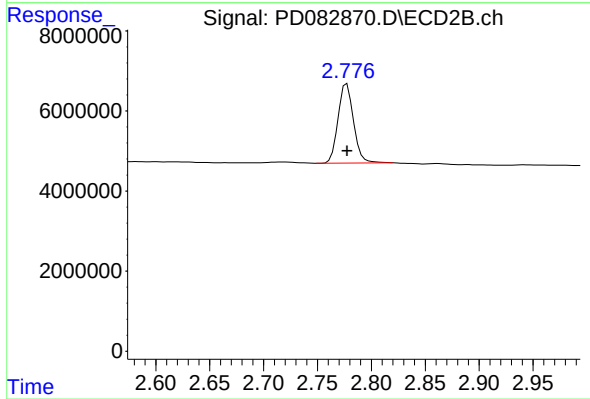


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 19755372
Conc: 5.04 ng/ml

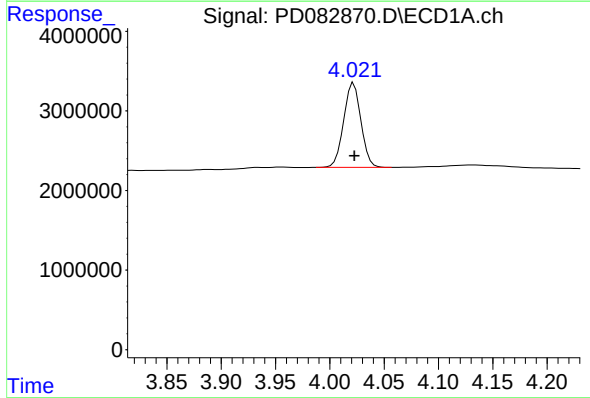


#2 alpha-BHC

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 11740312
Conc: 4.62 ng/ml

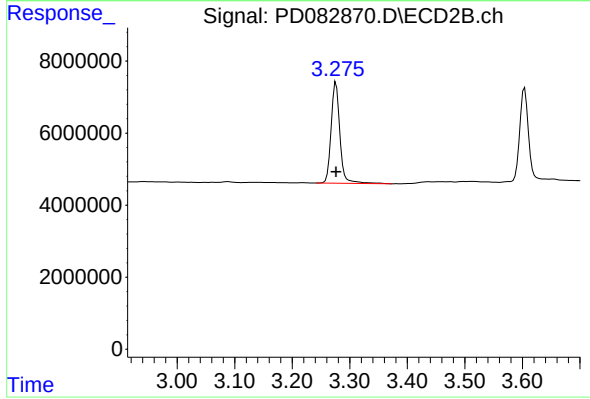


#2 alpha-BHC

R.T.: 3.276 min
Delta R.T.: 0.000 min
Response: 29759223
Conc: 4.82 ng/ml

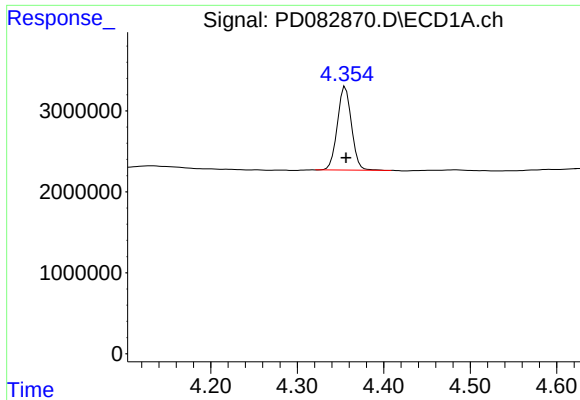


#3 gamma-BHC (Lindane)

R.T.: 4.356 min
Delta R.T.: 0.000 min
Response: 11609694
Conc: 4.73 ng/ml

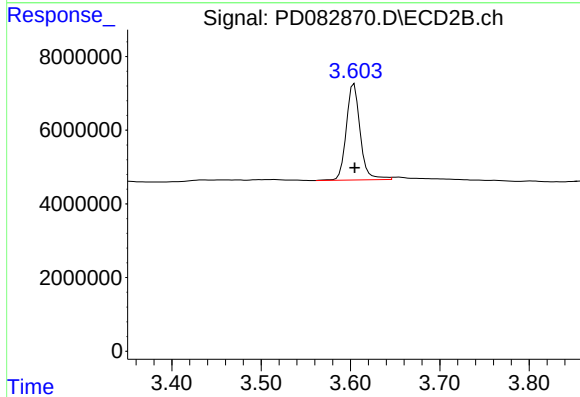


#3 gamma-BHC (Lindane)

R.T.: 3.604 min
Delta R.T.: 0.000 min
Response: 28097776
Conc: 4.87 ng/ml

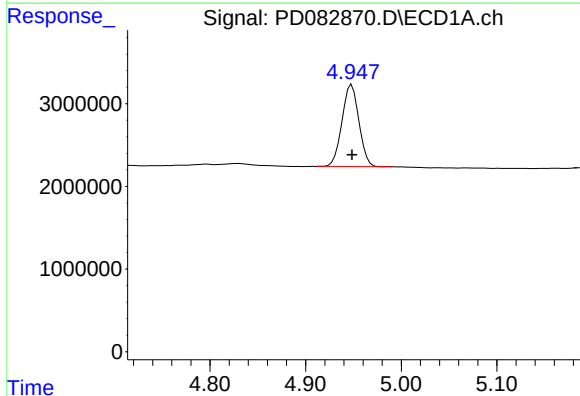


#4 Heptachlor

R.T.: 4.948 min
Delta R.T.: 0.000 min
Response: 12224736
Conc: 4.84 ng/ml

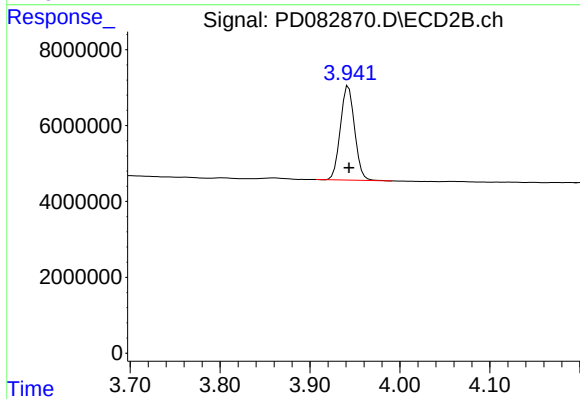


#4 Heptachlor

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 27311256
Conc: 4.91 ng/ml

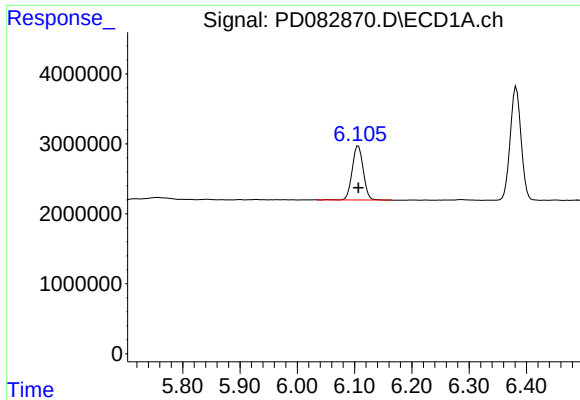


#9 Endosulfan I

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 10441214
Conc: 5.01 ng/ml

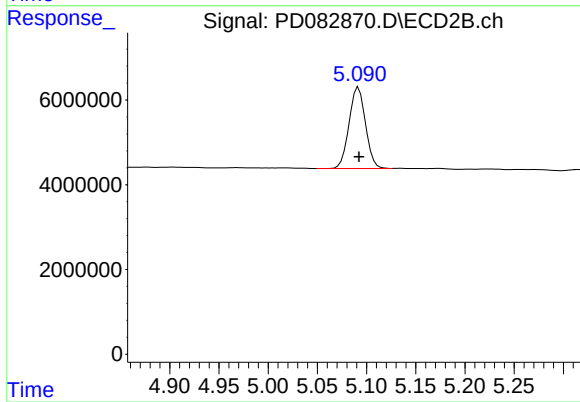


#9 Endosulfan I

R.T.: 5.092 min
Delta R.T.: 0.000 min
Response: 22284176
Conc: 4.94 ng/ml

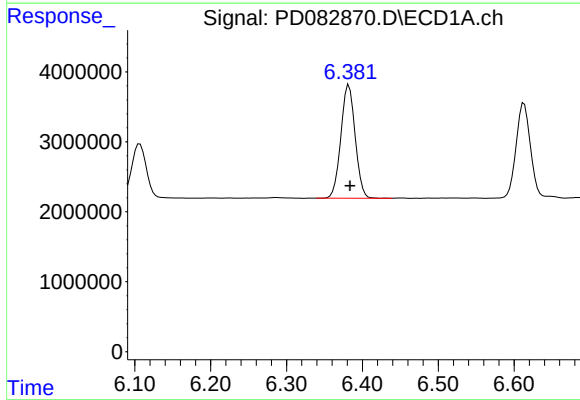


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: -0.001 min
Response: 21222254
Conc: 9.66 ng/ml

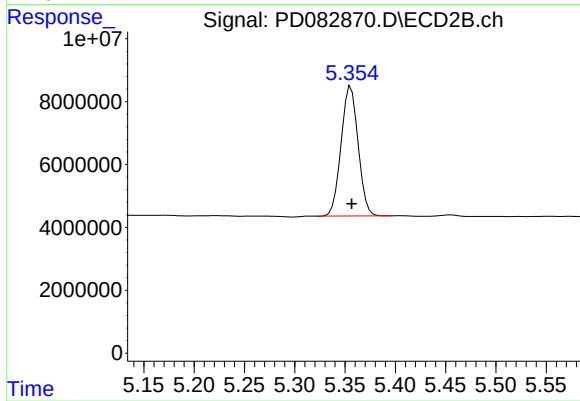


#13 Dieldrin

R.T.: 5.356 min
Delta R.T.: 0.000 min
Response: 48456199
Conc: 9.65 ng/ml

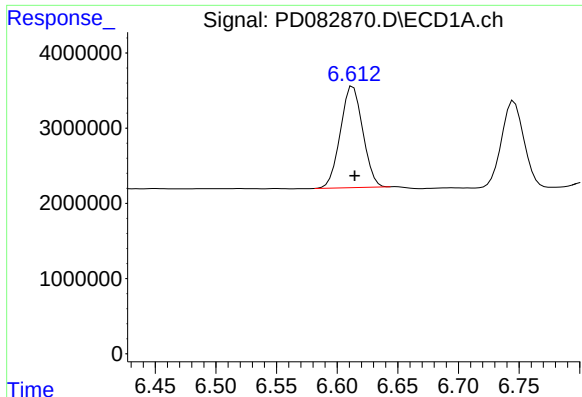


#14 Endrin

R.T.: 6.613 min
Delta R.T.: -0.001 min
Response: 17336439
Conc: 9.67 ng/ml

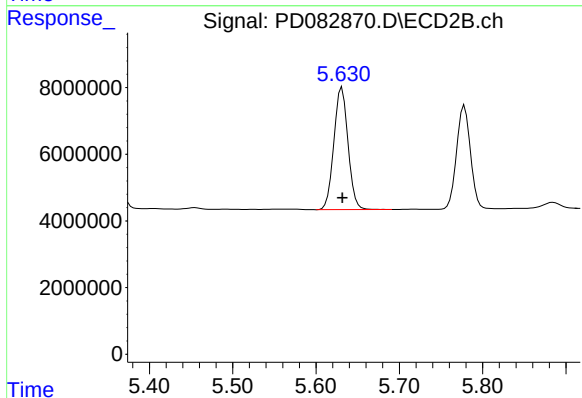


#14 Endrin

R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 43381580
Conc: 9.92 ng/ml

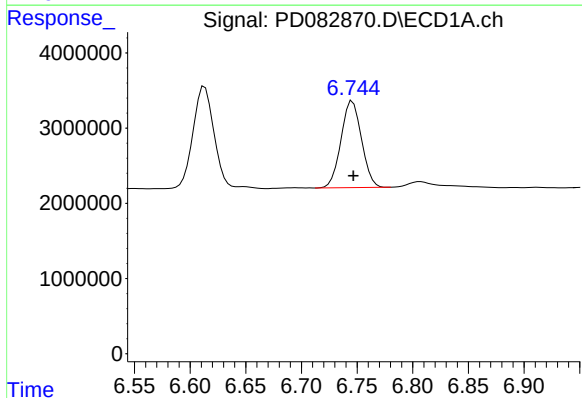


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 14807392
Conc: 9.44 ng/ml

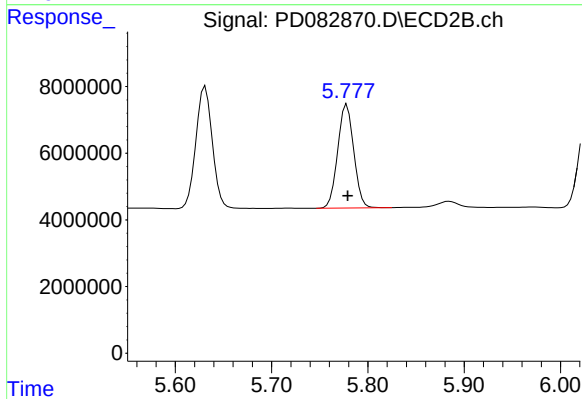


#16 4,4'-DDD

R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 35961106
Conc: 9.53 ng/ml

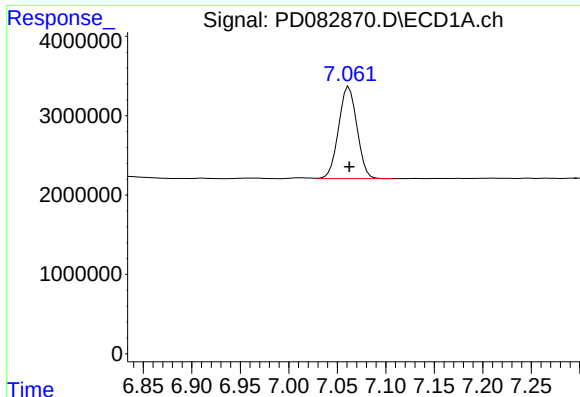


#17 4,4'-DDT

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 15305350
Conc: 9.36 ng/ml

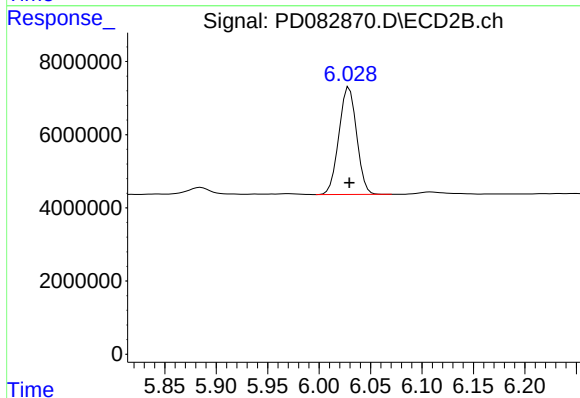


#17 4,4'-DDT

R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 35243483
Conc: 9.16 ng/ml

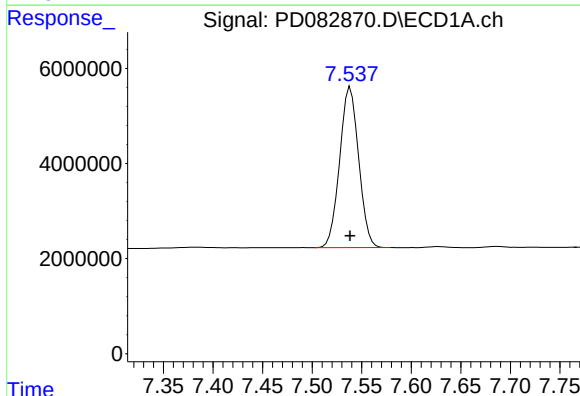


#20 Methoxychlor

R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 45023860
Conc: 51.18 ng/ml

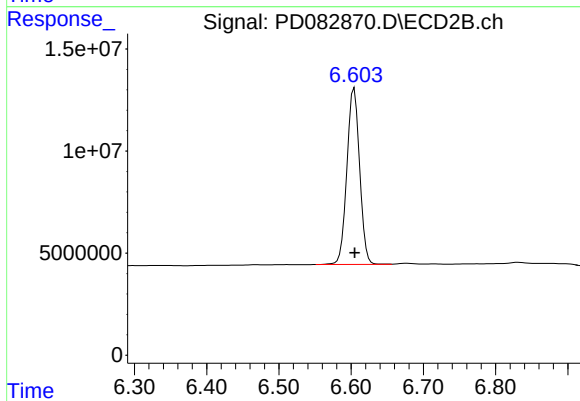


#20 Methoxychlor

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 105125280
Conc: 52.72 ng/ml

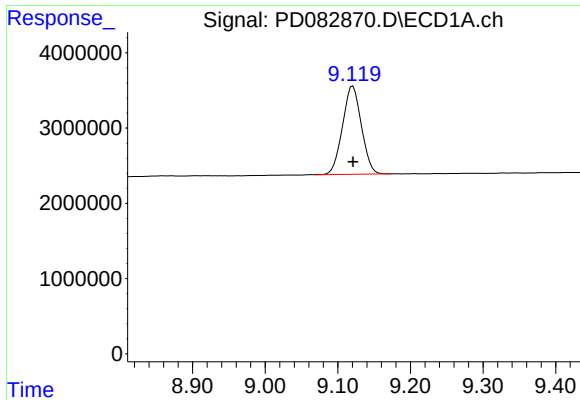

#27 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 21199992
Conc: 10.67 ng/ml

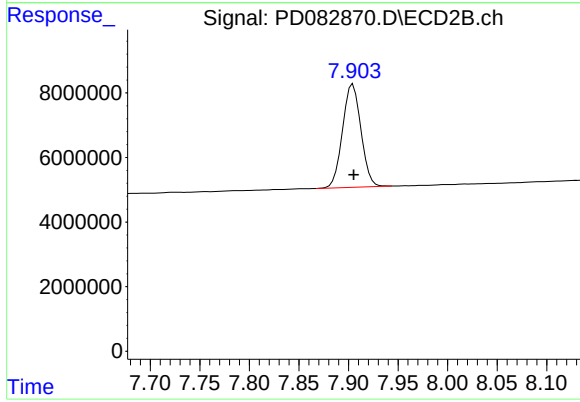

#27 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: 0.000 min
Response: 41477607
Conc: 10.59 ng/ml