

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
 Data File : PD082872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2024 17:36
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:38:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 04:33:00 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.798	14815450	37204005	9.805	9.495
27)	SA Decachlor...	9.121	7.925	41168378	70111564	20.712	17.893
Target Compounds							
2)	A alpha-BHC	4.022	3.296	23396052	59610310	9.208	9.662
3)	MA gamma-BHC...	4.356	3.624	23203893	56464262	9.450	9.779
4)	MA Heptachlor	4.949	3.963	23962922	53775560	9.480	9.665
9)	A Endosulfan I	6.107	5.112	20271373	44469901	9.728	9.863
13)	MA Dieldrin	6.383	5.376	41577269	97804433	18.934	19.472
14)	MA Endrin	6.614	5.652	34035514	86116738	18.982	19.695
16)	A 4,4'-DDD	6.746	5.798	29349326	73199298	18.709	19.390
17)	MA 4,4'-DDT	7.063	6.049	30800556	70038080	18.828	18.201
20)	A Methoxychlor	7.539	6.624	87297890	206.9E6	99.232	103.738


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 17:36
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:38:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 04:33:00 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

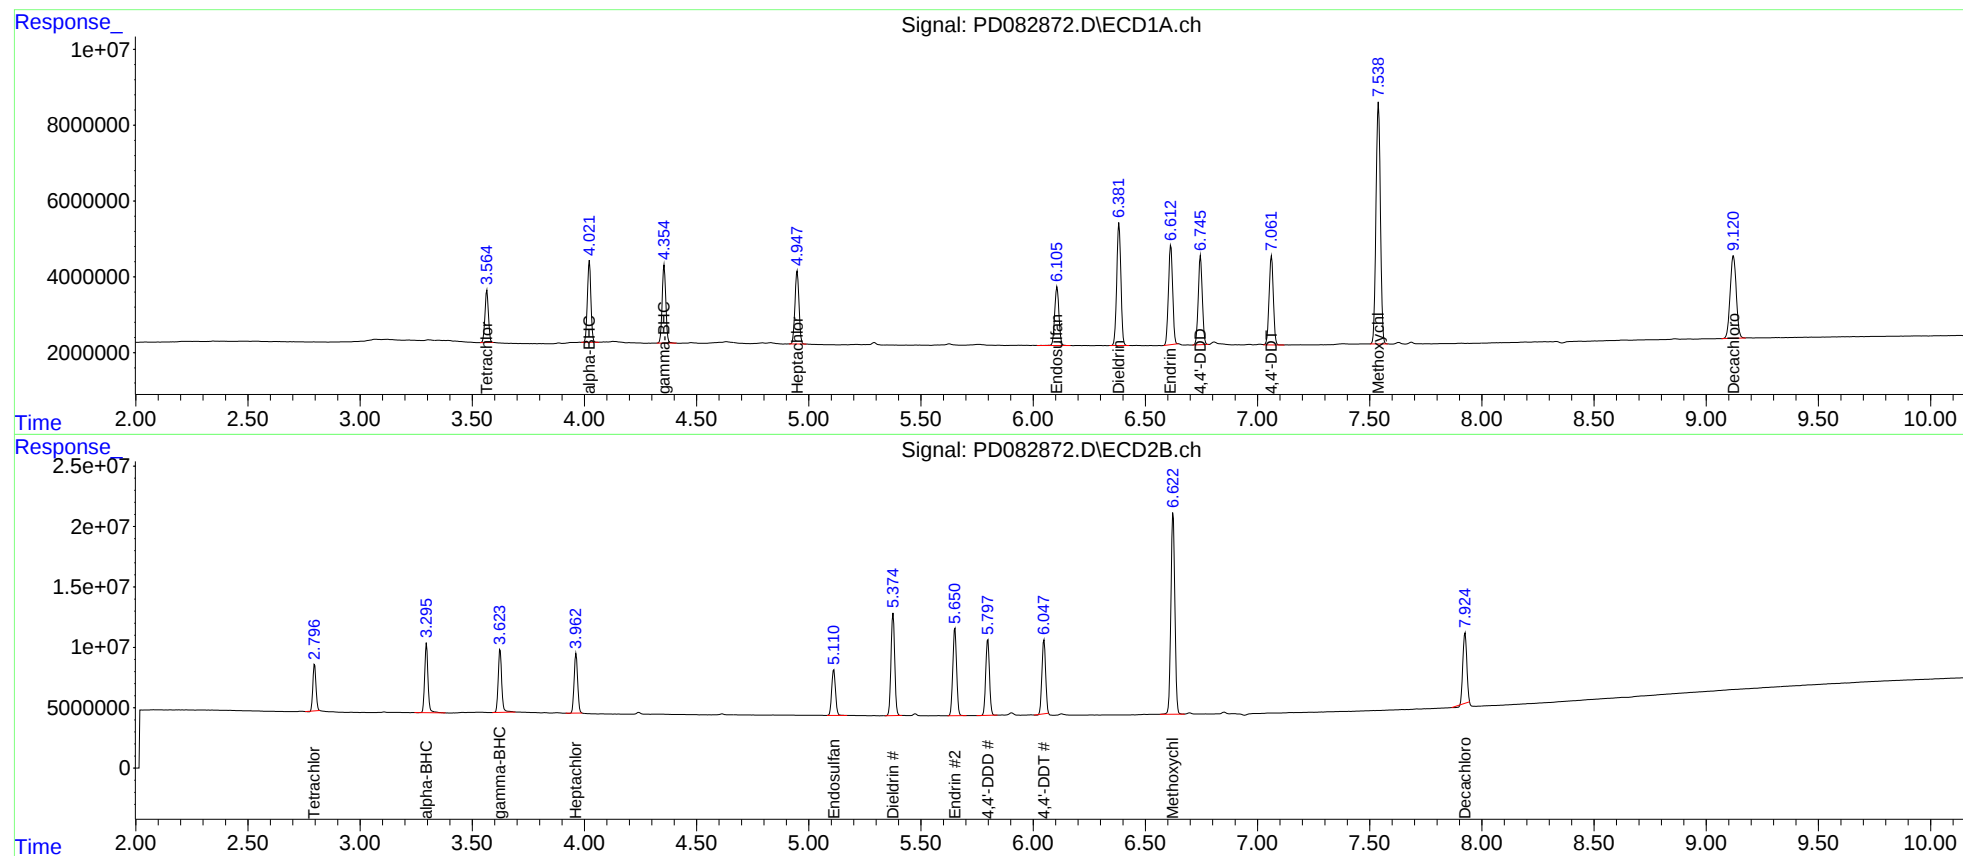

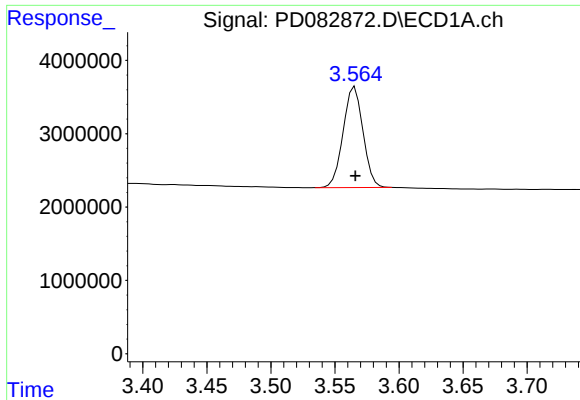


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 14815450
Conc: 9.80 ng/ml

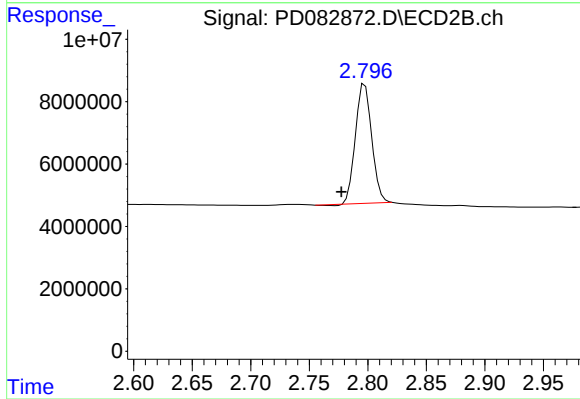


#1 Tetrachloro-m-xylene

R.T.: 2.798 min
Delta R.T.: 0.020 min
Response: 37204005
Conc: 9.49 ng/ml

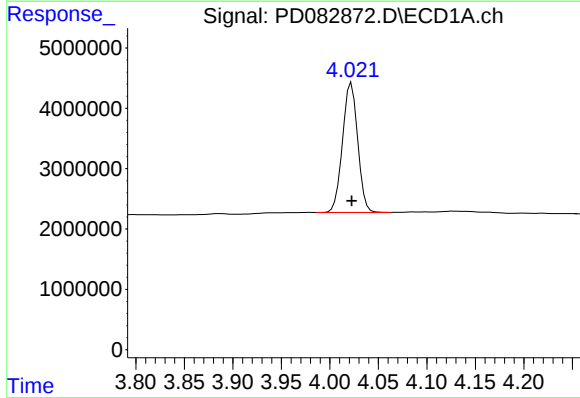


#2 alpha-BHC

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 23396052
Conc: 9.21 ng/ml

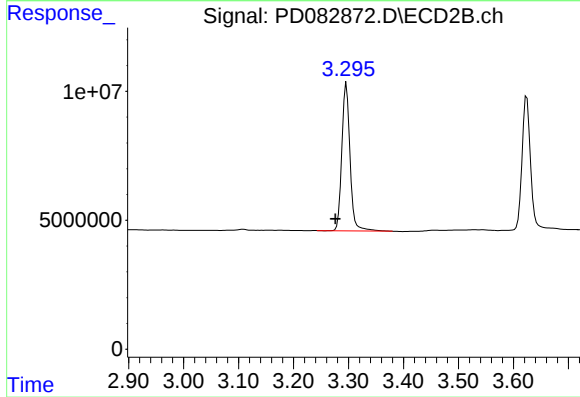


#2 alpha-BHC

R.T.: 3.296 min
Delta R.T.: 0.020 min
Response: 59610310
Conc: 9.66 ng/ml

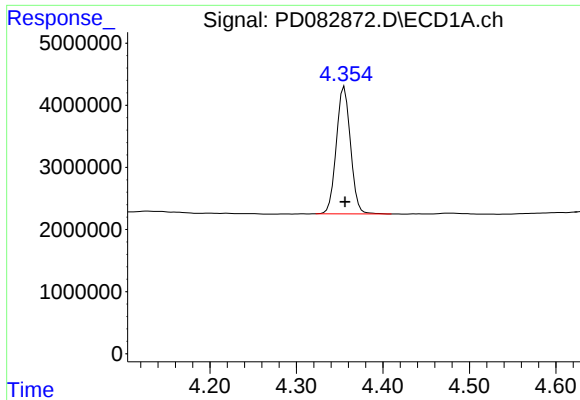


#3 gamma-BHC (Lindane)

R.T.: 4.356 min
Delta R.T.: 0.000 min
Response: 23203893
Conc: 9.45 ng/ml

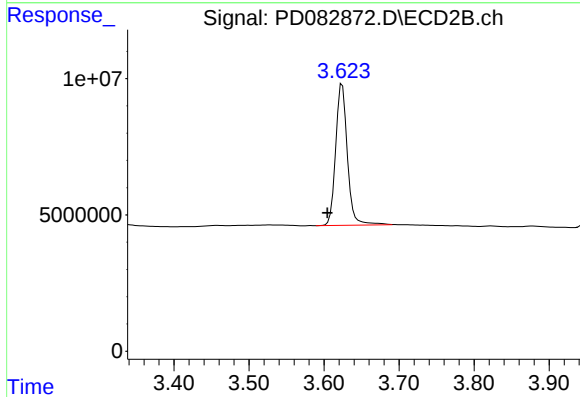


#3 gamma-BHC (Lindane)

R.T.: 3.624 min
Delta R.T.: 0.020 min
Response: 56464262
Conc: 9.78 ng/ml

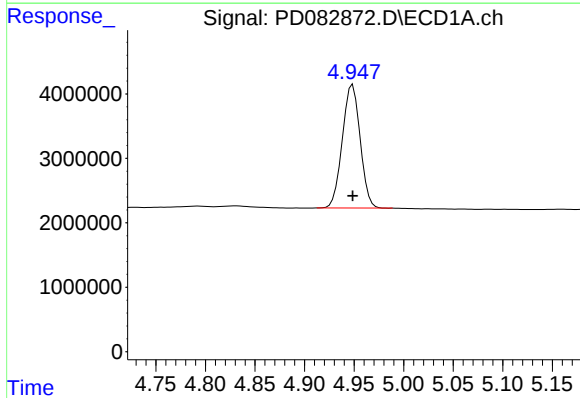


#4 Heptachlor

R.T.: 4.949 min
Delta R.T.: 0.000 min
Response: 23962922
Conc: 9.48 ng/ml

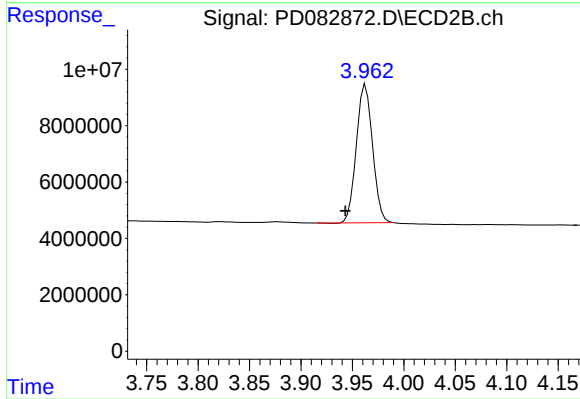


#4 Heptachlor

R.T.: 3.963 min
Delta R.T.: 0.020 min
Response: 53775560
Conc: 9.66 ng/ml

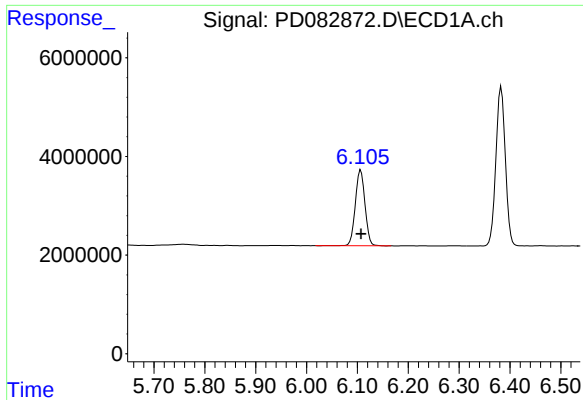


#9 Endosulfan I

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 20271373
Conc: 9.73 ng/ml

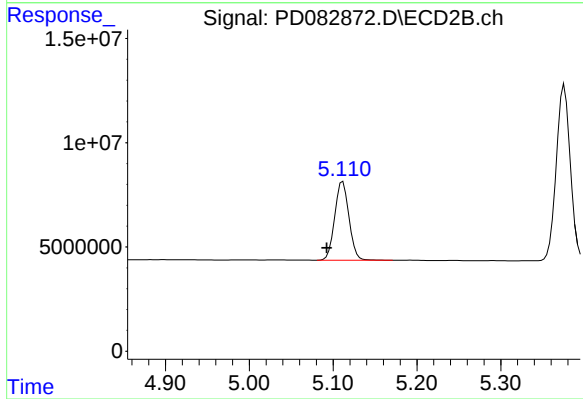


#9 Endosulfan I

R.T.: 5.112 min
Delta R.T.: 0.019 min
Response: 44469901
Conc: 9.86 ng/ml

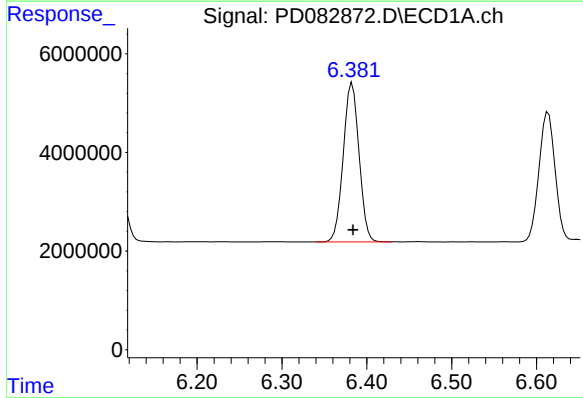


#13 Dieldrin

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 41577269
Conc: 18.93 ng/ml

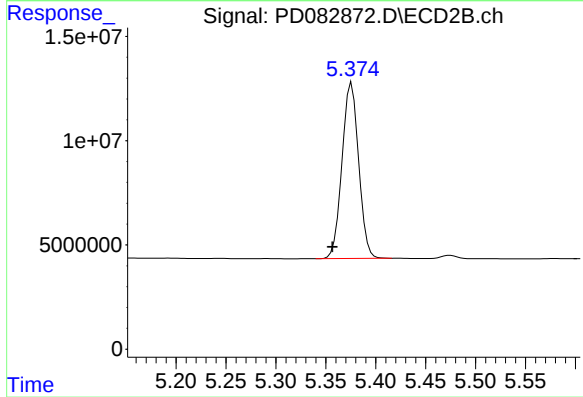


#13 Dieldrin

R.T.: 5.376 min
Delta R.T.: 0.019 min
Response: 97804433
Conc: 19.47 ng/ml

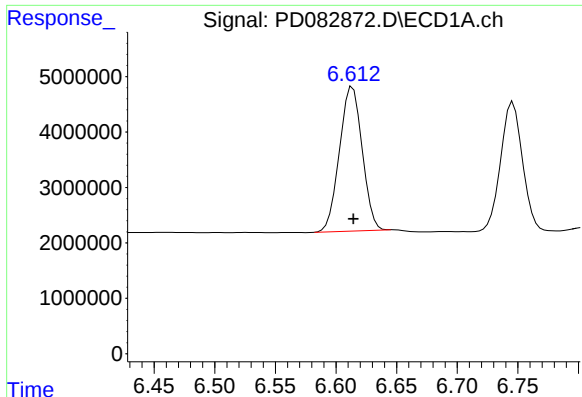


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 34035514
Conc: 18.98 ng/ml

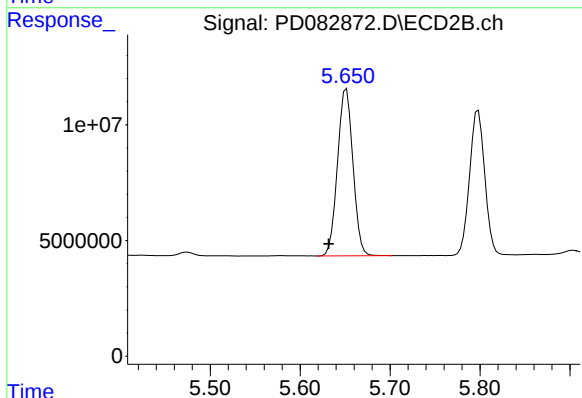


#14 Endrin

R.T.: 5.652 min
Delta R.T.: 0.020 min
Response: 86116738
Conc: 19.69 ng/ml

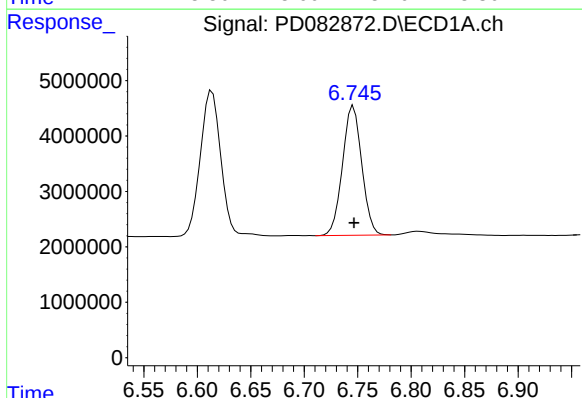


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 29349326
Conc: 18.71 ng/ml

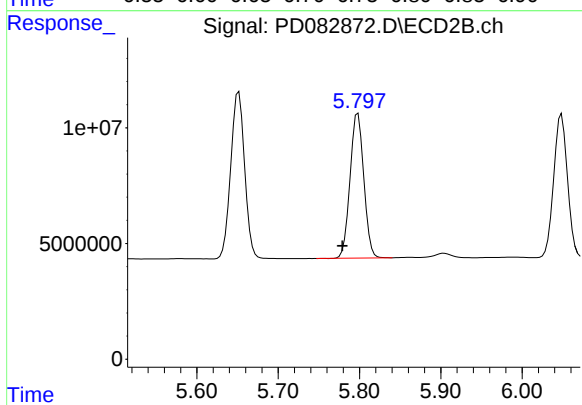


#16 4,4'-DDD

R.T.: 5.798 min
Delta R.T.: 0.019 min
Response: 73199298
Conc: 19.39 ng/ml

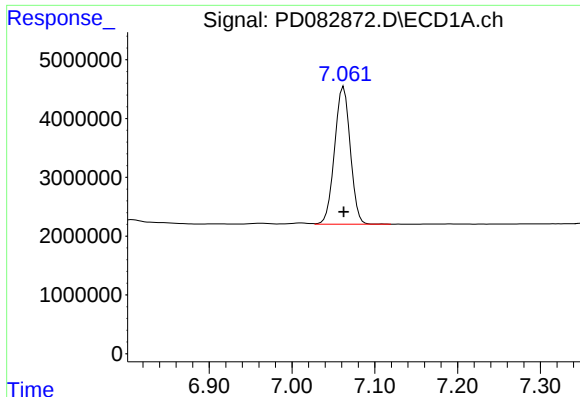


#17 4,4'-DDT

R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 30800556
Conc: 18.83 ng/ml

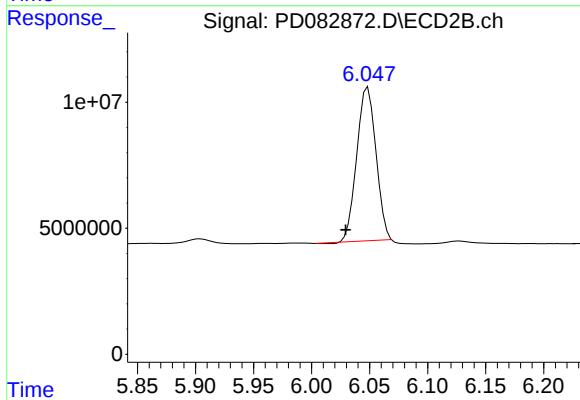


#17 4,4'-DDT

R.T.: 6.049 min
Delta R.T.: 0.019 min
Response: 70038080
Conc: 18.20 ng/ml

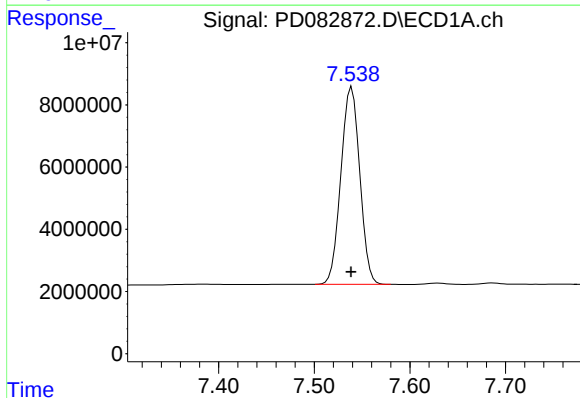


#20 Methoxychlor

R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 87297890
Conc: 99.23 ng/ml

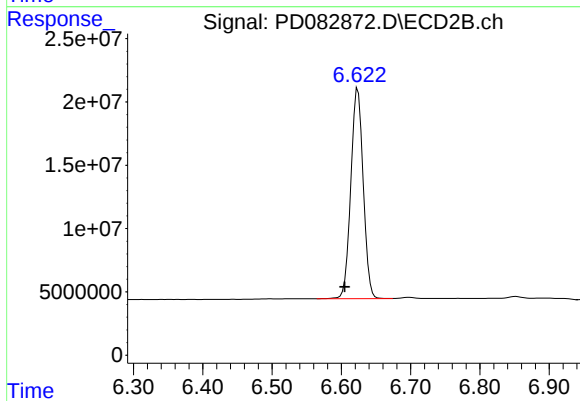


#20 Methoxychlor

R.T.: 6.624 min
Delta R.T.: 0.019 min
Response: 206864357
Conc: 103.74 ng/ml

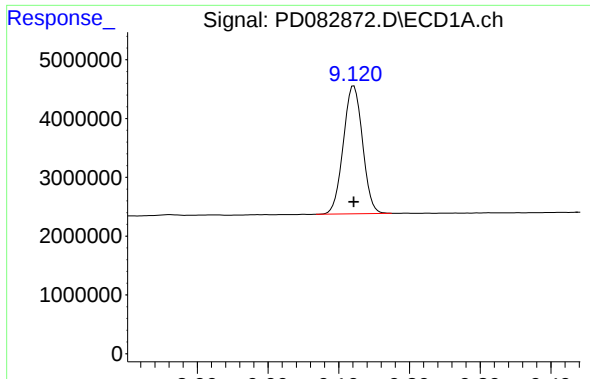

#27 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 41168378
Conc: 20.71 ng/ml

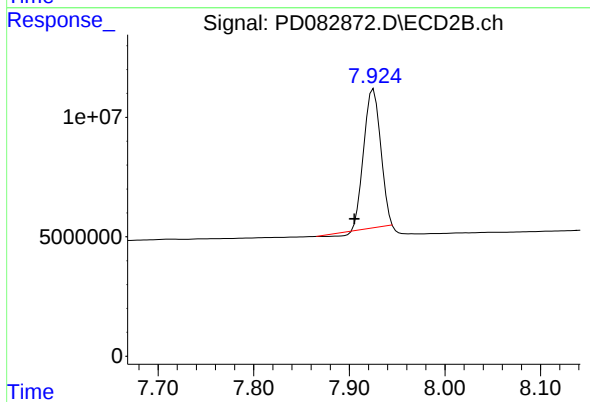

#27 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.020 min
Response: 70111564
Conc: 17.89 ng/ml