

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
 Data File : PD082874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2024 18:03
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:38:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 04:33:00 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.778	30221053	78368853	20.000	20.000
27)	SA Decachlor...	9.121	7.905	79508028	156.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.023	3.276	50819215	123.4E6	20.000	20.000
3)	MA gamma-BHC...	4.356	3.605	49111216	115.5E6	20.000	20.000
4)	MA Heptachlor	4.949	3.943	50552130	111.3E6	20.000	20.000
9)	A Endosulfan I	6.107	5.092	41676749	90170782	20.000	20.000
13)	MA Dieldrin	6.384	5.356	87836446	200.9E6	40.000	40.000
14)	MA Endrin	6.614	5.632	71722855	174.9E6	40.000	40.000
16)	A 4,4'-DDD	6.747	5.779	62749228	151.0E6	40.000	40.000
17)	MA 4,4'-DDT	7.063	6.029	65436415	153.9E6	40.000	40.000
20)	A Methoxychlor	7.538	6.605	175.9E6	398.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 18:03
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:38:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 04:33:00 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

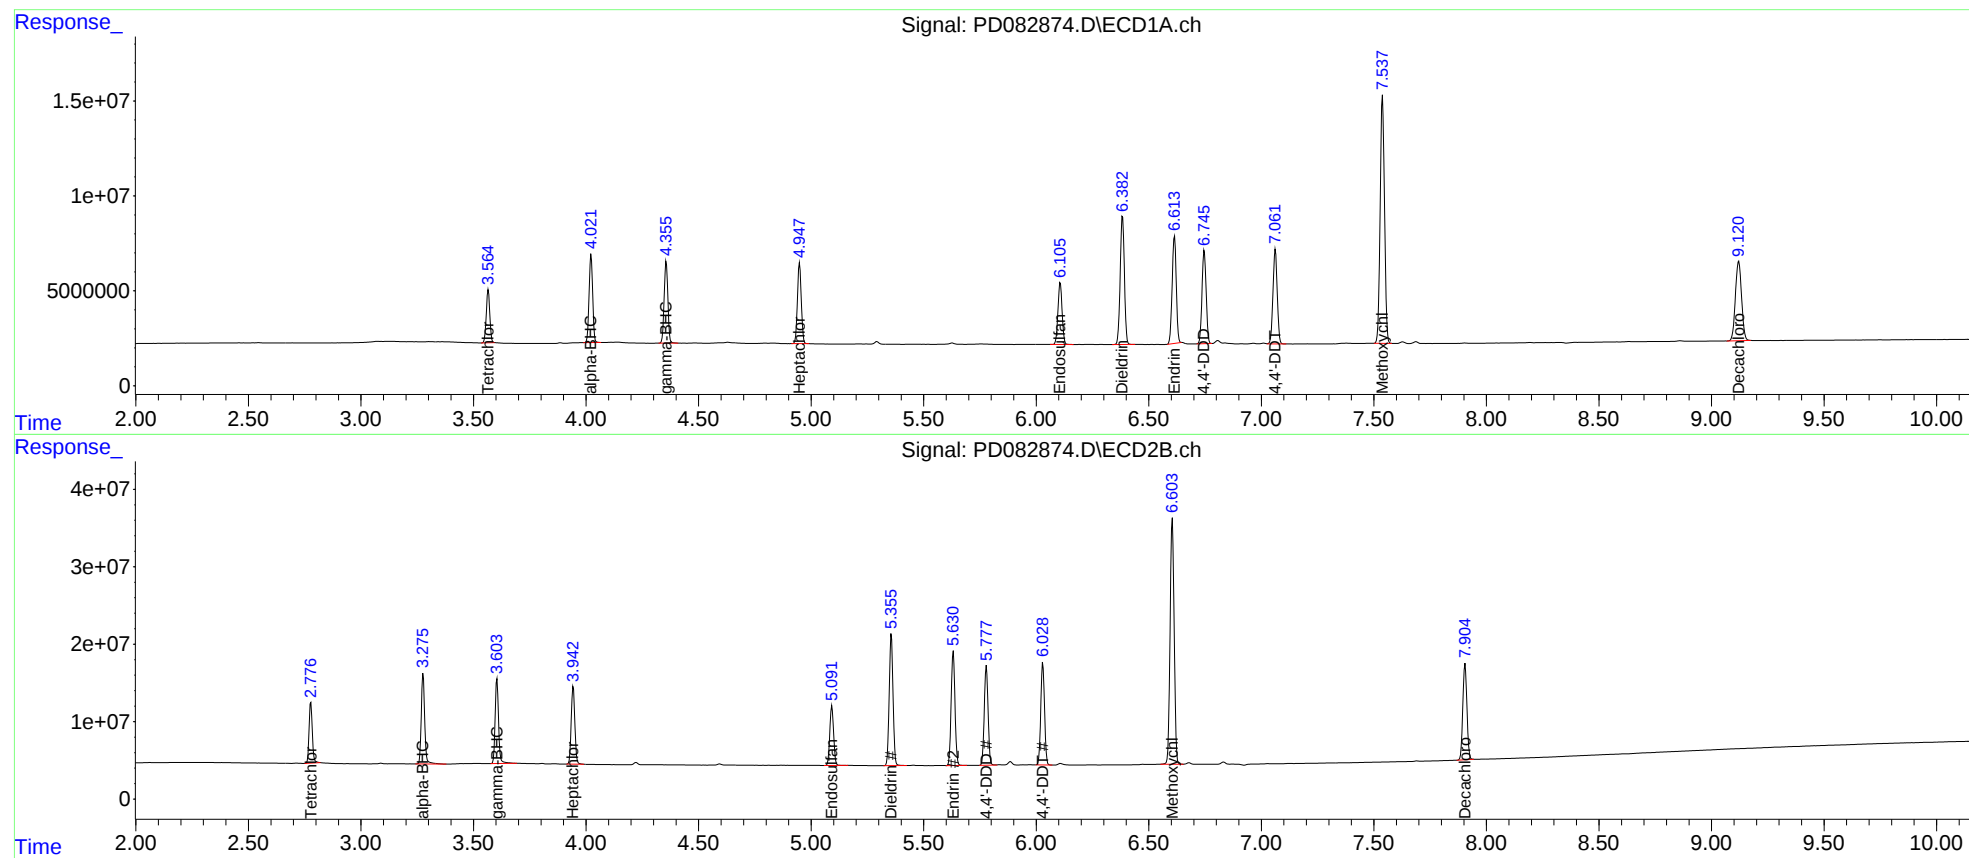

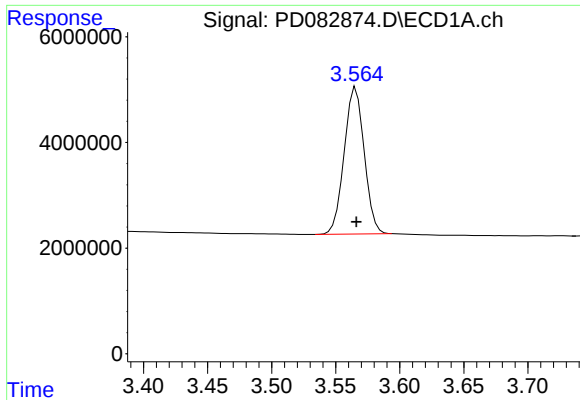


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 30221053
Conc: 20.00 ng/ml

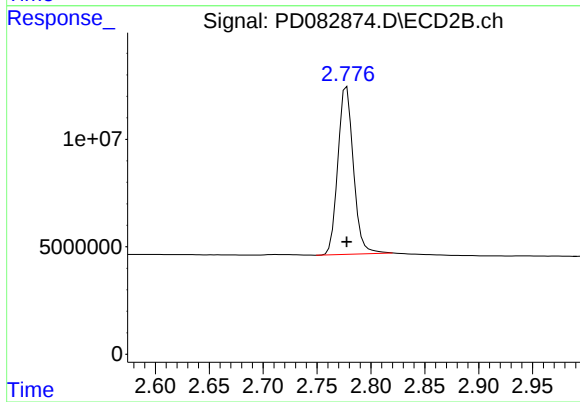


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 78368853
Conc: 20.00 ng/ml

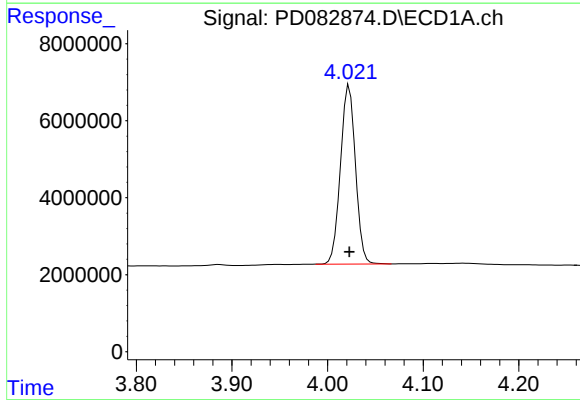


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 50819215
Conc: 20.00 ng/ml

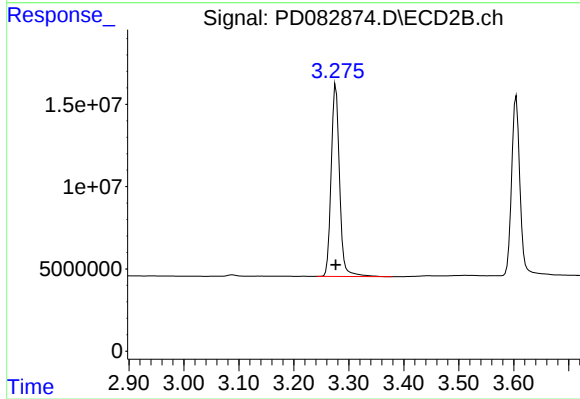


#2 alpha-BHC

R.T.: 3.276 min
Delta R.T.: 0.000 min
Response: 123392496
Conc: 20.00 ng/ml

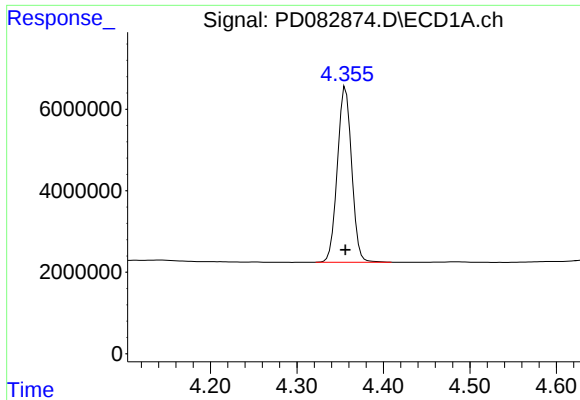


#3 gamma-BHC (Lindane)

R.T.: 4.356 min
Delta R.T.: 0.000 min
Response: 49111216
Conc: 20.00 ng/ml

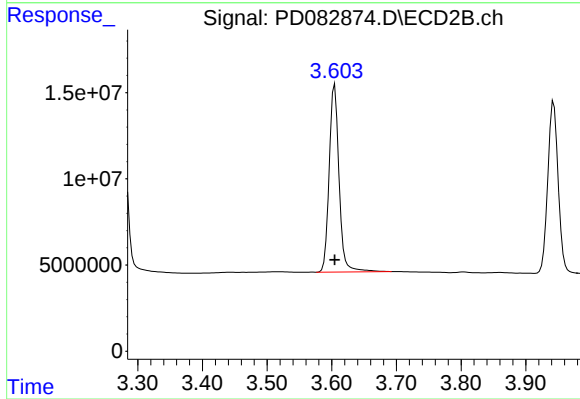


#3 gamma-BHC (Lindane)

R.T.: 3.605 min
Delta R.T.: 0.000 min
Response: 115483478
Conc: 20.00 ng/ml

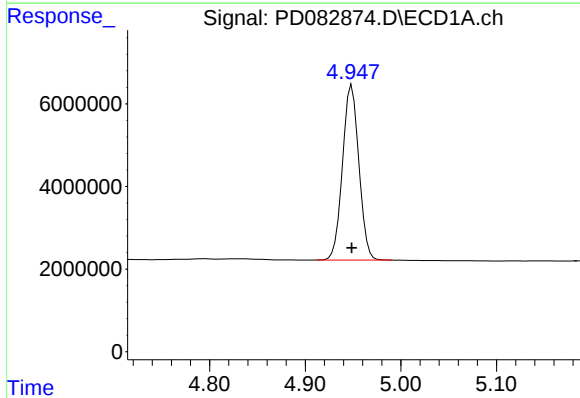


#4 Heptachlor

R.T.: 4.949 min
Delta R.T.: 0.000 min
Response: 50552130
Conc: 20.00 ng/ml

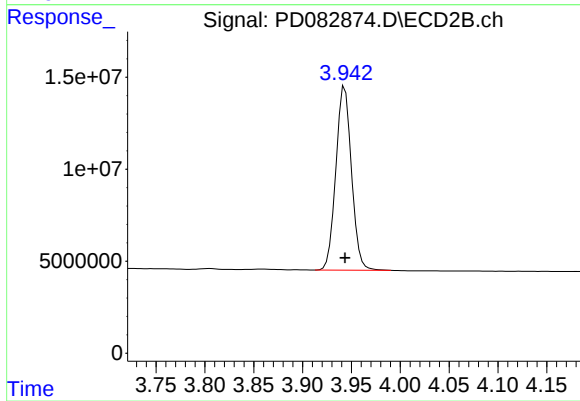


#4 Heptachlor

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 111283432
Conc: 20.00 ng/ml

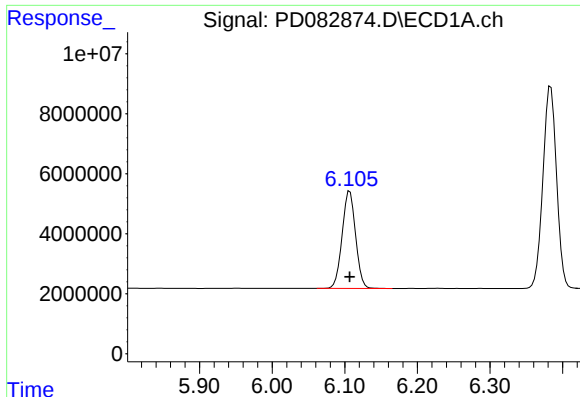


#9 Endosulfan I

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 41676749
Conc: 20.00 ng/ml

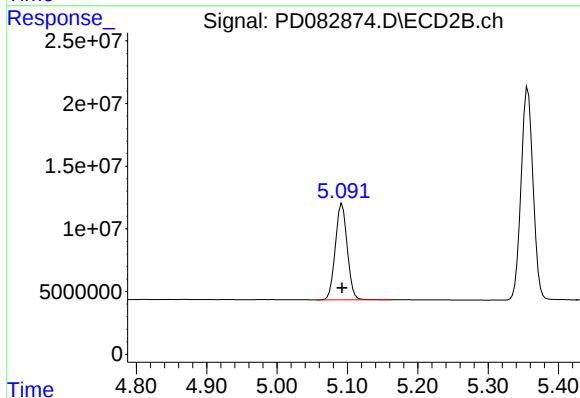


#9 Endosulfan I

R.T.: 5.092 min
Delta R.T.: 0.000 min
Response: 90170782
Conc: 20.00 ng/ml

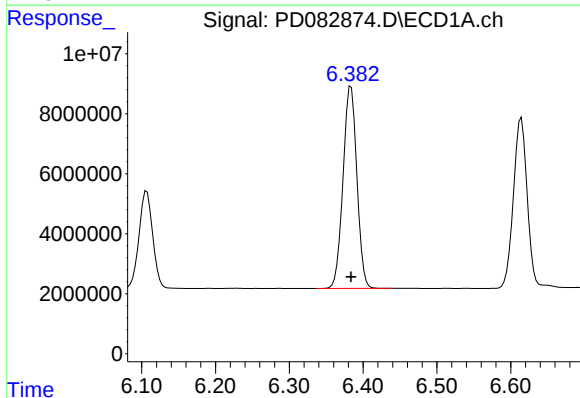


#13 Dieldrin

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 87836446
Conc: 40.00 ng/ml

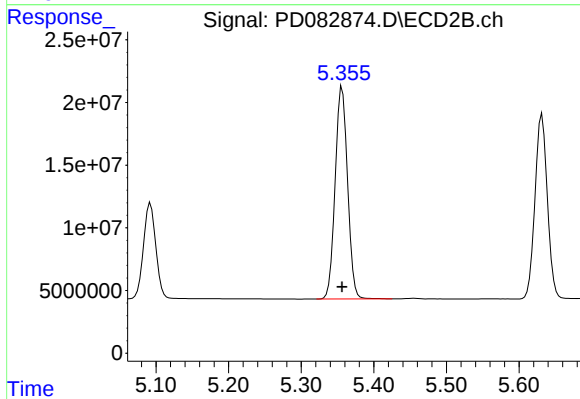


#13 Dieldrin

R.T.: 5.356 min
Delta R.T.: 0.000 min
Response: 200913261
Conc: 40.00 ng/ml

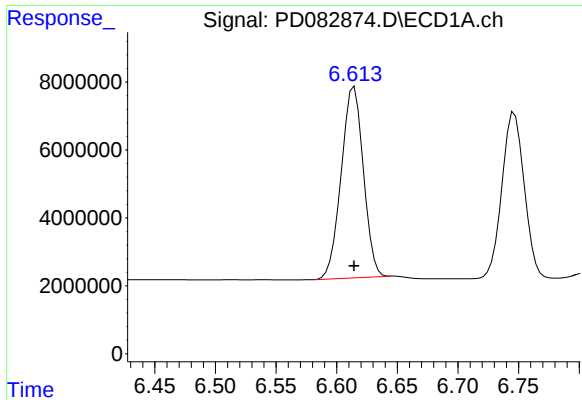


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 71722855
Conc: 40.00 ng/ml

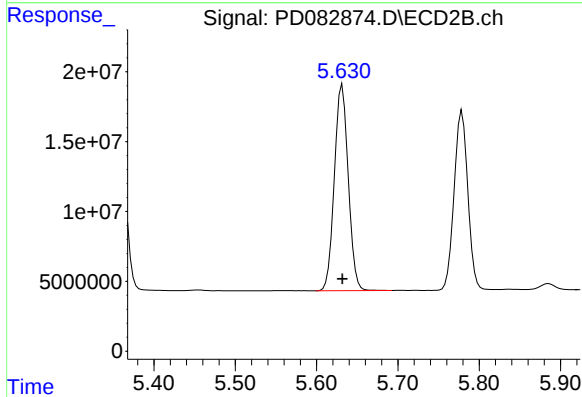


#14 Endrin

R.T.: 5.632 min
Delta R.T.: 0.000 min
Response: 174904058
Conc: 40.00 ng/ml

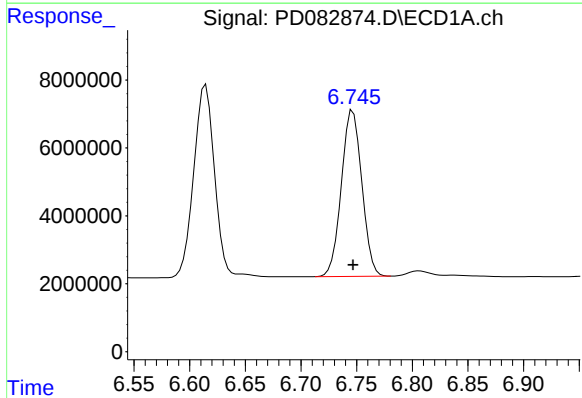


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 62749228
Conc: 40.00 ng/ml

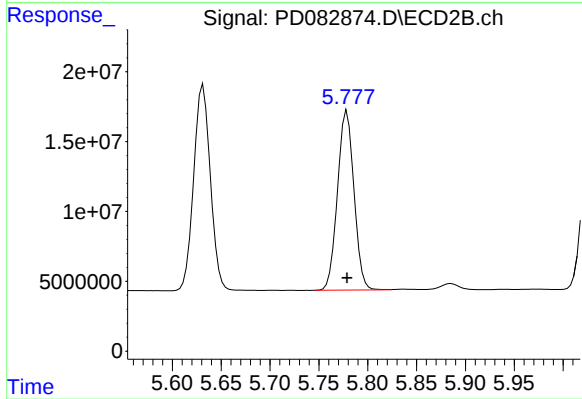


#16 4,4'-DDD

R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 151003149
Conc: 40.00 ng/ml

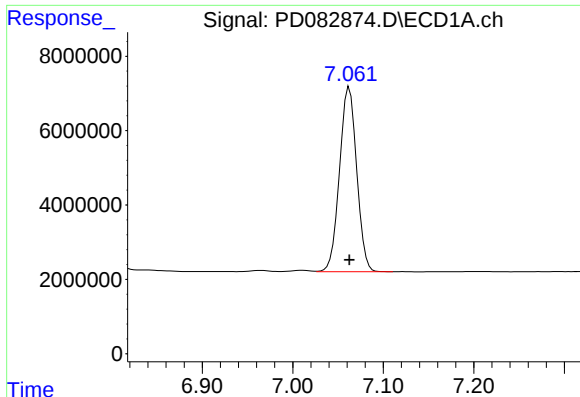


#17 4,4'-DDT

R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 65436415
Conc: 40.00 ng/ml

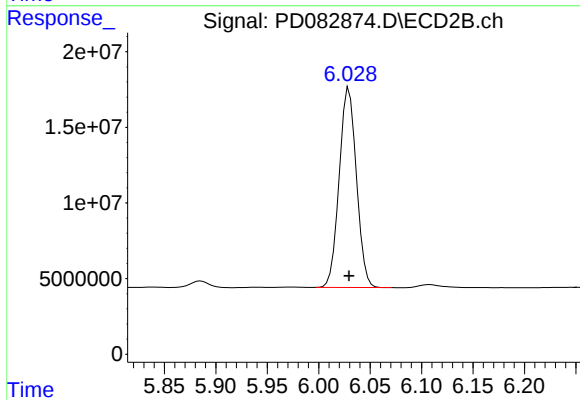


#17 4,4'-DDT

R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 153917981
Conc: 40.00 ng/ml

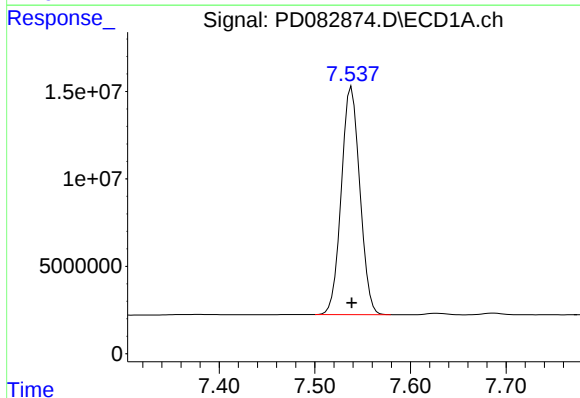


#20 Methoxychlor

R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 175946539
Conc: 200.00 ng/ml

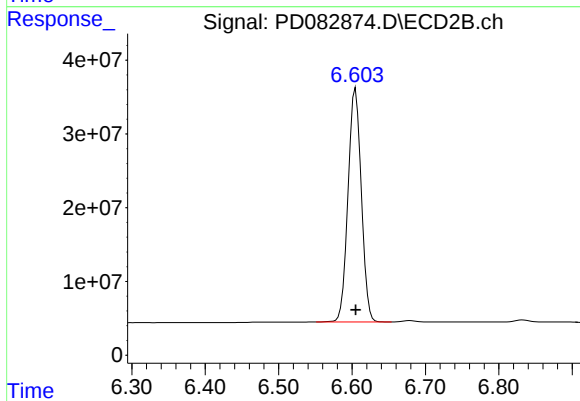


#20 Methoxychlor

R.T.: 6.605 min
Delta R.T.: 0.000 min
Response: 398820070
Conc: 200.00 ng/ml

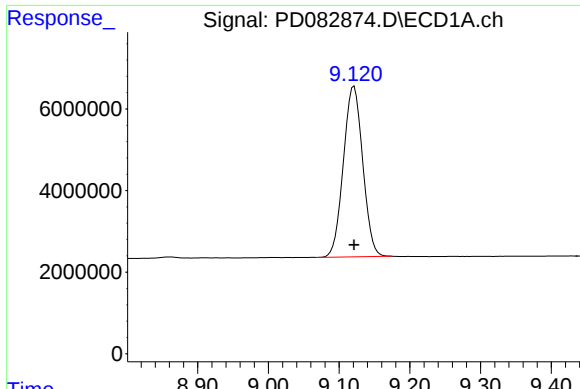

#27 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 79508028
Conc: 40.00 ng/ml

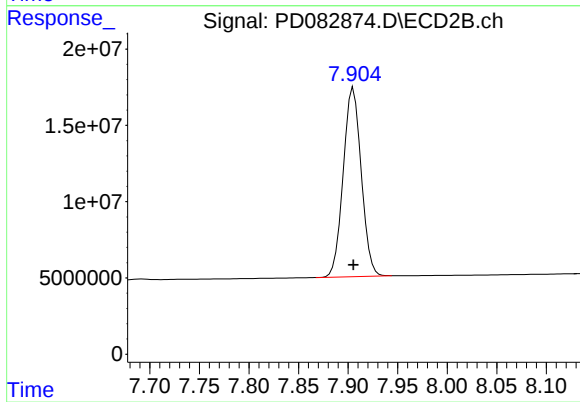

#27 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: 0.000 min
Response: 156738210
Conc: 40.00 ng/ml