

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
 Data File : PD082878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2024 18:56
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:39:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 04:33:00 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.778	121.9E6	320.0E6	80.666	81.677
27)	SA Decachlor...	9.122	7.905	310.1E6	620.0E6	156.025	158.238
Target Compounds							
2)	A alpha-BHC	4.023	3.276	234.3E6	537.2E6	92.199	87.073
3)	MA gamma-BHC...	4.357	3.604	219.6E6	489.0E6	89.435	84.692
4)	MA Heptachlor	4.949	3.943	217.4E6	469.7E6	85.998	84.411
9)	A Endosulfan I	6.107	5.092	171.2E6	371.8E6	82.149	82.461
13)	MA Dieldrin	6.383	5.357	378.3E6	831.1E6	172.289	165.471
14)	MA Endrin	6.614	5.632	302.0E6	717.8E6	168.453	164.149
16)	A 4,4'-DDD	6.747	5.778	266.0E6	637.1E6	169.554	168.758
17)	MA 4,4'-DDT	7.063	6.029	272.8E6	669.8E6	166.778	174.078
20)	A Methoxychlor	7.539	6.604	664.5E6	1419.9E6	755.334	712.035


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 18:56
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:39:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 04:33:00 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

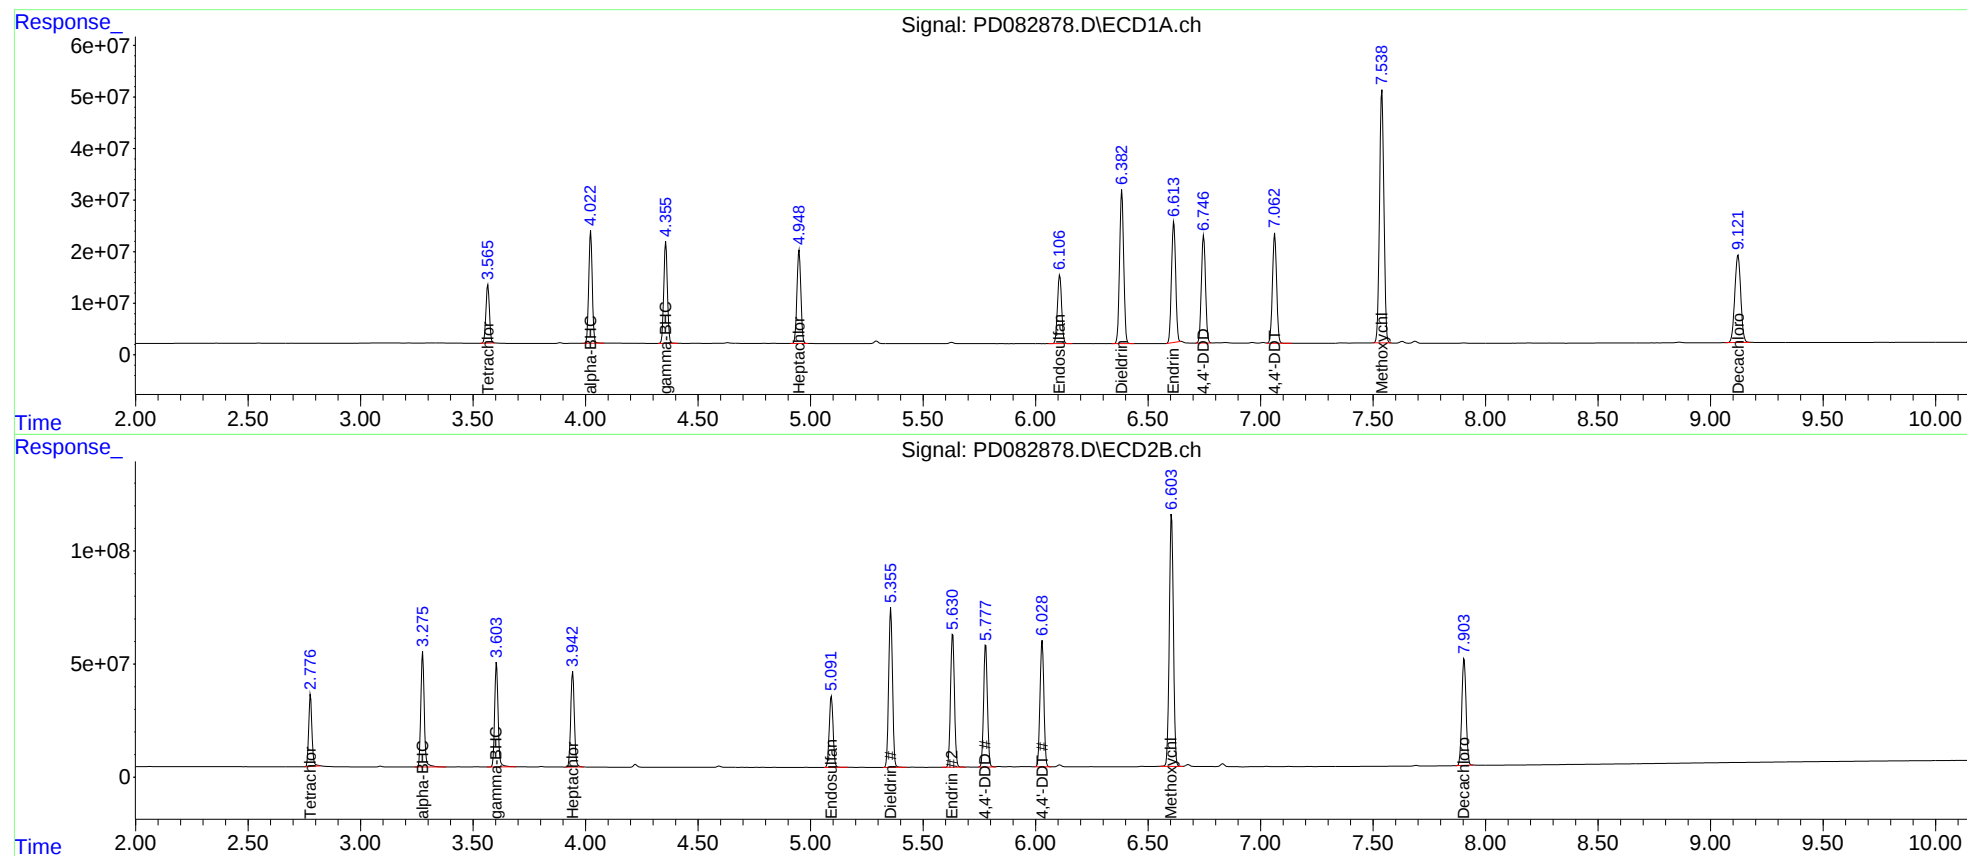

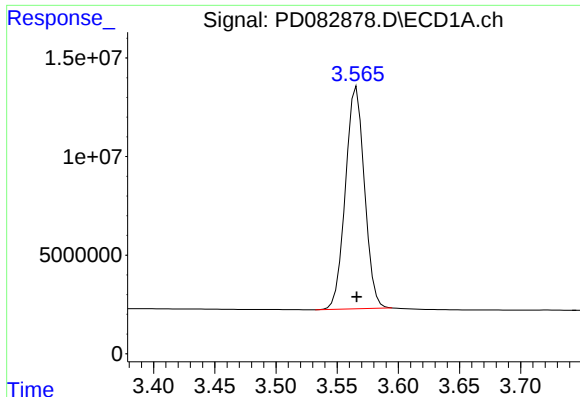


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 121891091
Conc: 80.67 ng/ml

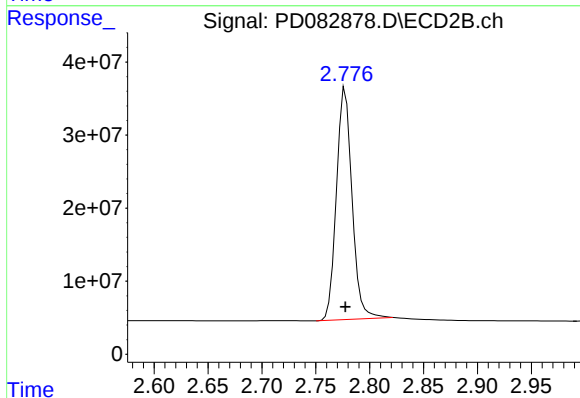


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 320044917
Conc: 81.68 ng/ml

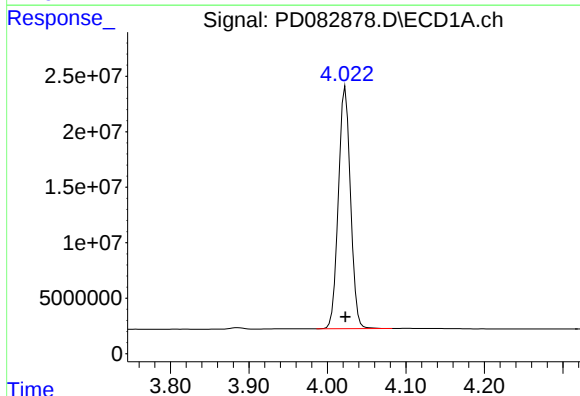


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 234273569
Conc: 92.20 ng/ml

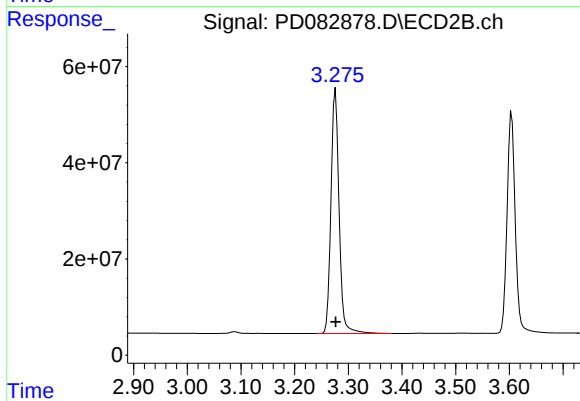


#2 alpha-BHC

R.T.: 3.276 min
Delta R.T.: 0.000 min
Response: 537209789
Conc: 87.07 ng/ml

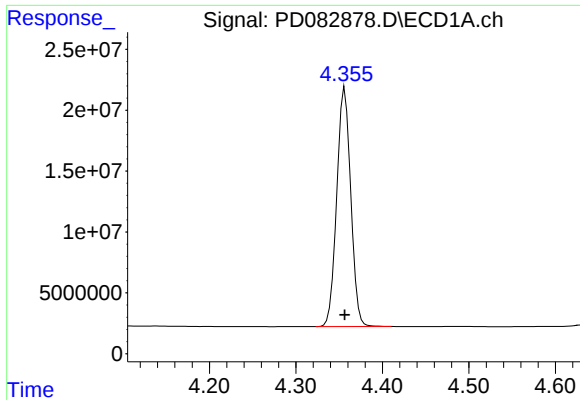


#3 gamma-BHC (Lindane)

R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 219613859
Conc: 89.44 ng/ml

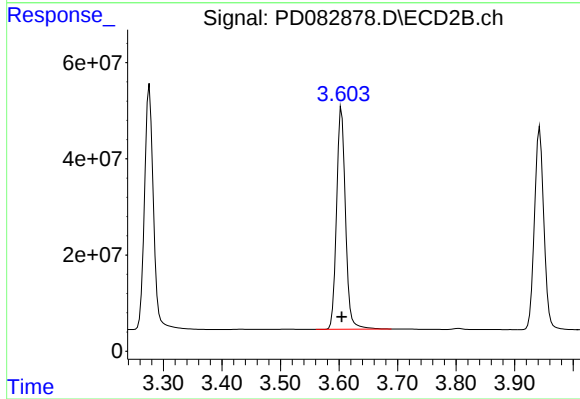


#3 gamma-BHC (Lindane)

R.T.: 3.604 min
Delta R.T.: 0.000 min
Response: 489027228
Conc: 84.69 ng/ml

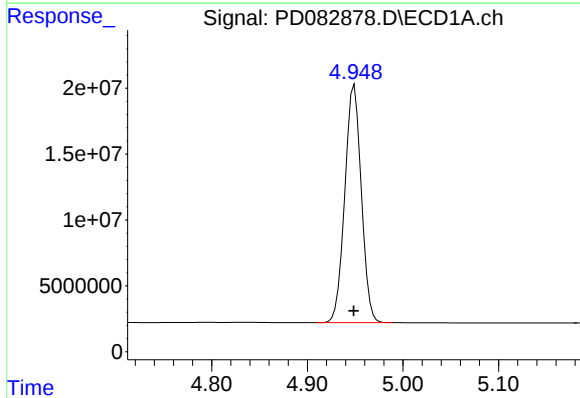


#4 Heptachlor

R.T.: 4.949 min
Delta R.T.: 0.000 min
Response: 217370145
Conc: 86.00 ng/ml

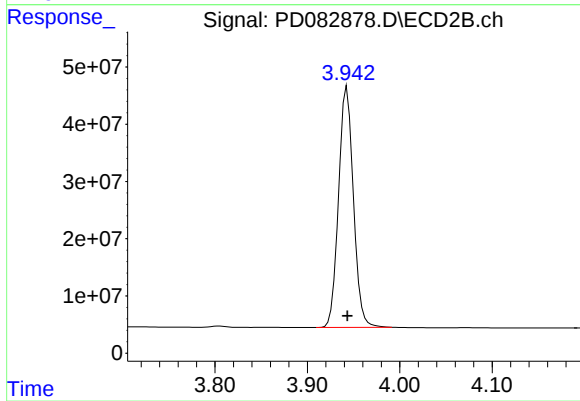


#4 Heptachlor

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 469676106
Conc: 84.41 ng/ml

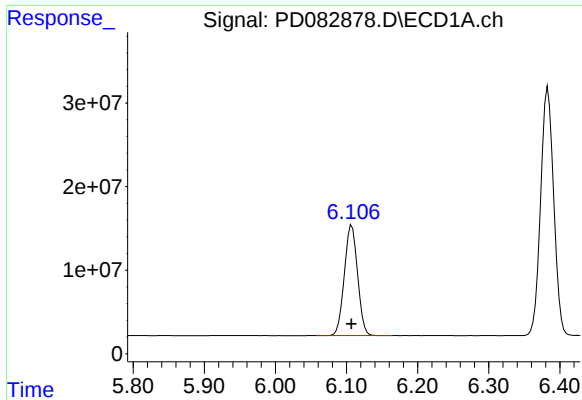


#9 Endosulfan I

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 171185427
Conc: 82.15 ng/ml

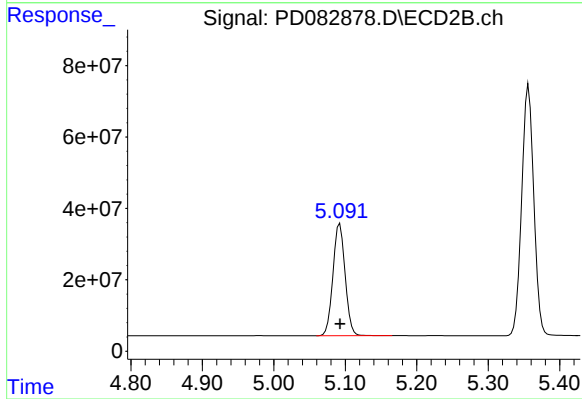


#9 Endosulfan I

R.T.: 5.092 min
Delta R.T.: 0.000 min
Response: 371776839
Conc: 82.46 ng/ml

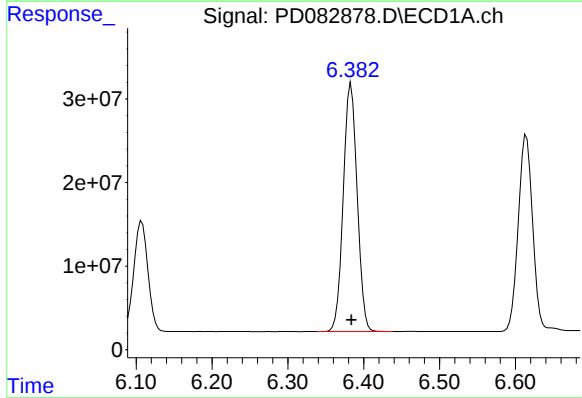


#13 Dieldrin

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 378330905
Conc: 172.29 ng/ml

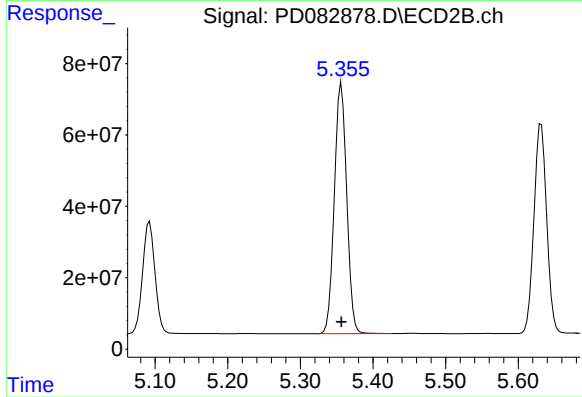


#13 Dieldrin

R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 831132459
Conc: 165.47 ng/ml

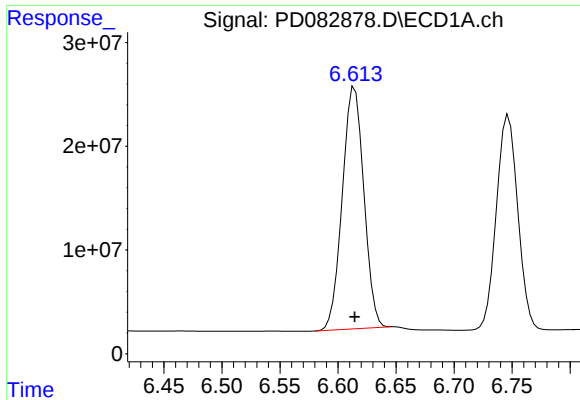


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 302047605
Conc: 168.45 ng/ml

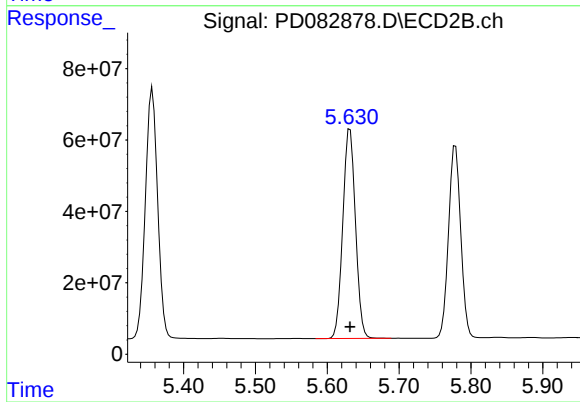


#14 Endrin

R.T.: 5.632 min
Delta R.T.: 0.000 min
Response: 717756339
Conc: 164.15 ng/ml

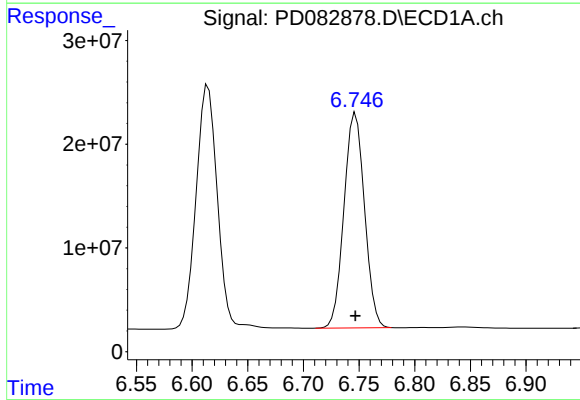


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 265983973
Conc: 169.55 ng/ml

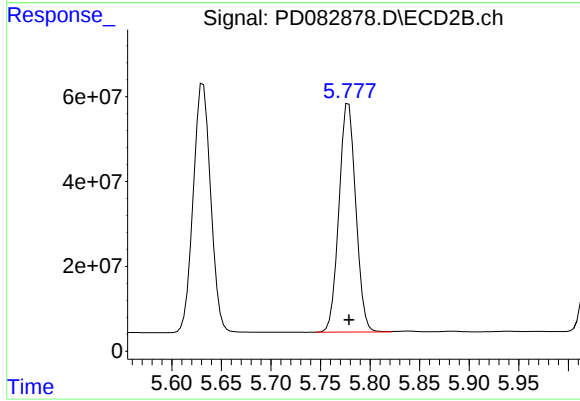


#16 4,4'-DDD

R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 637076259
Conc: 168.76 ng/ml

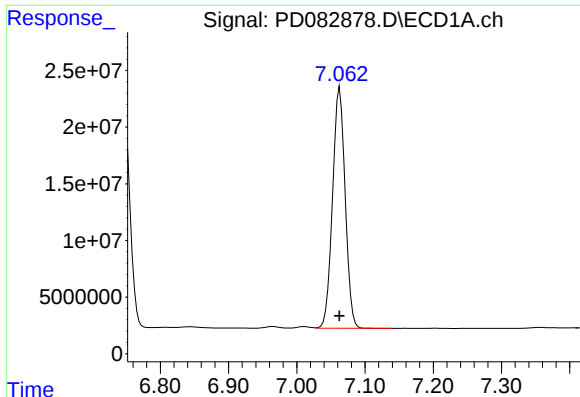


#17 4,4'-DDT

R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 272834047
Conc: 166.78 ng/ml

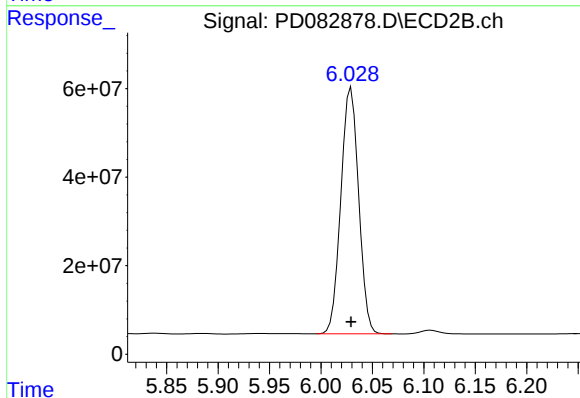


#17 4,4'-DDT

R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 669842216
Conc: 174.08 ng/ml

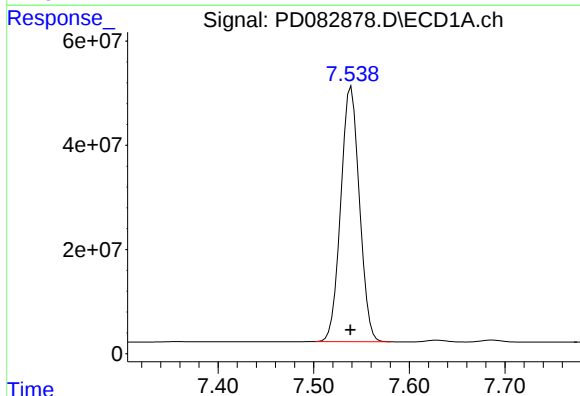


#20 Methoxychlor

R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 664492341
Conc: 755.33 ng/ml

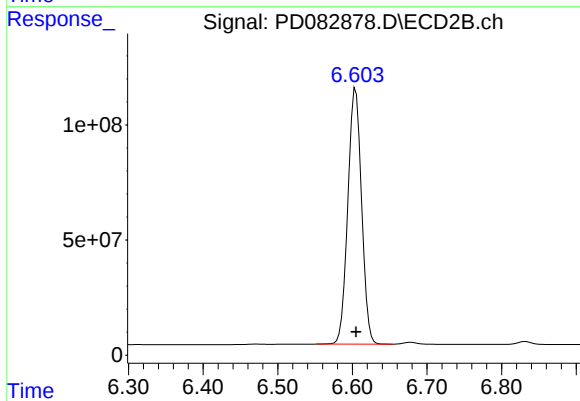


#20 Methoxychlor

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 1419868939
Conc: 712.03 ng/ml

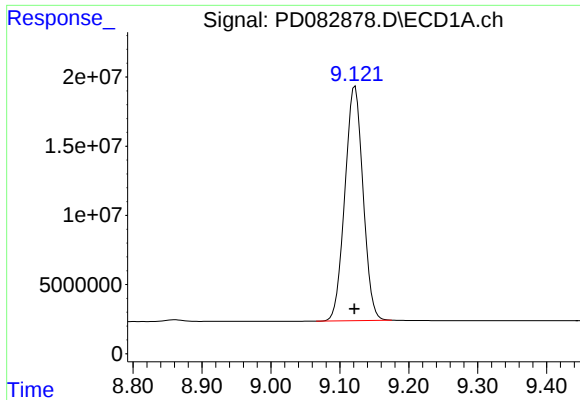

#27 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.001 min
Response: 310130375
Conc: 156.02 ng/ml

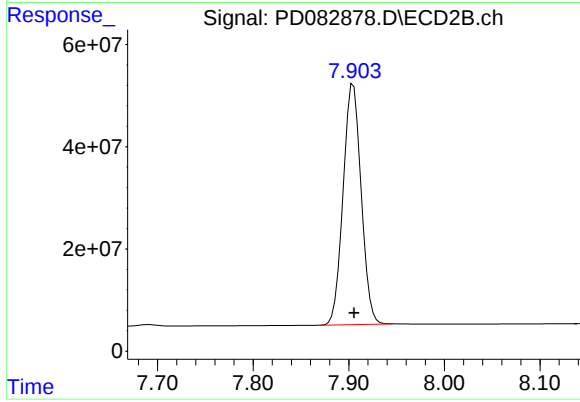

#27 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: 0.000 min
Response: 620048719
Conc: 158.24 ng/ml