

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
 Data File : PD082863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2024 14:22
 Operator : AR\AJ
 Sample : RESC031
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC033

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 05:20:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.777	28567642	79355791	19.099	20.407
27)	SA Decachlor...	9.126	7.907	81774821	158.6E6	40.798	40.080
Target Compounds							
2)	A alpha-BHC	4.023	3.276	22795245	61305931	8.935	9.862
3)	MA gamma-BHC...	4.357	3.605	22685354	56958262	9.193	9.844
4)	MA Heptachlor	4.949	3.943	23031905	55928070	9.147	10.044
5)	MB Aldrin	5.293	4.223	21646851	54423331	8.940	9.846
6)	B beta-BHC	4.553	3.900	10160154	24538316	9.365	9.784
7)	B delta-BHC	4.802	4.130	20651783	55540327	8.434	9.388
8)	B Heptachlo...	5.721	4.724	20851805	49141293	9.337	9.619
9)	A Endosulfan I	6.108	5.093	20709019	46512525	9.952	10.313
10)	B trans-Chl...	5.977	4.973	20239124	47915143	9.350	9.622
11)	B cis-Chlor...	6.057	5.037	20915992	48710761	9.365	9.590
12)	B 4,4'-DDE	6.229	5.226	40462496	90739720	18.554	19.028
13)	MA Dieldrin	6.384	5.357	42289319	100.7E6	19.241	20.142
14)	MA Endrin	6.615	5.633	35129505	88554657	19.700	20.247
15)	B Endosulfa...	6.834	5.926	36774913	80930896	19.089	19.204
16)	A 4,4'-DDD	6.748	5.780	30161473	74978728	19.448	19.926
17)	MA 4,4'-DDT	7.064	6.031	32811671	76025332	20.401	19.800
18)	B Endrin al...	6.965	6.106	26477512	60999168	19.061	19.342
19)	B Endosulfa...	7.200	6.328	34703283	77888124	19.663	19.374
20)	A Methoxychlor	7.540	6.606	94049001	212.9E6	108.716	108.484
21)	B Endrin ke...	7.688	6.834	38617281	89198829	20.485	19.834

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 14:22
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 05:20:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

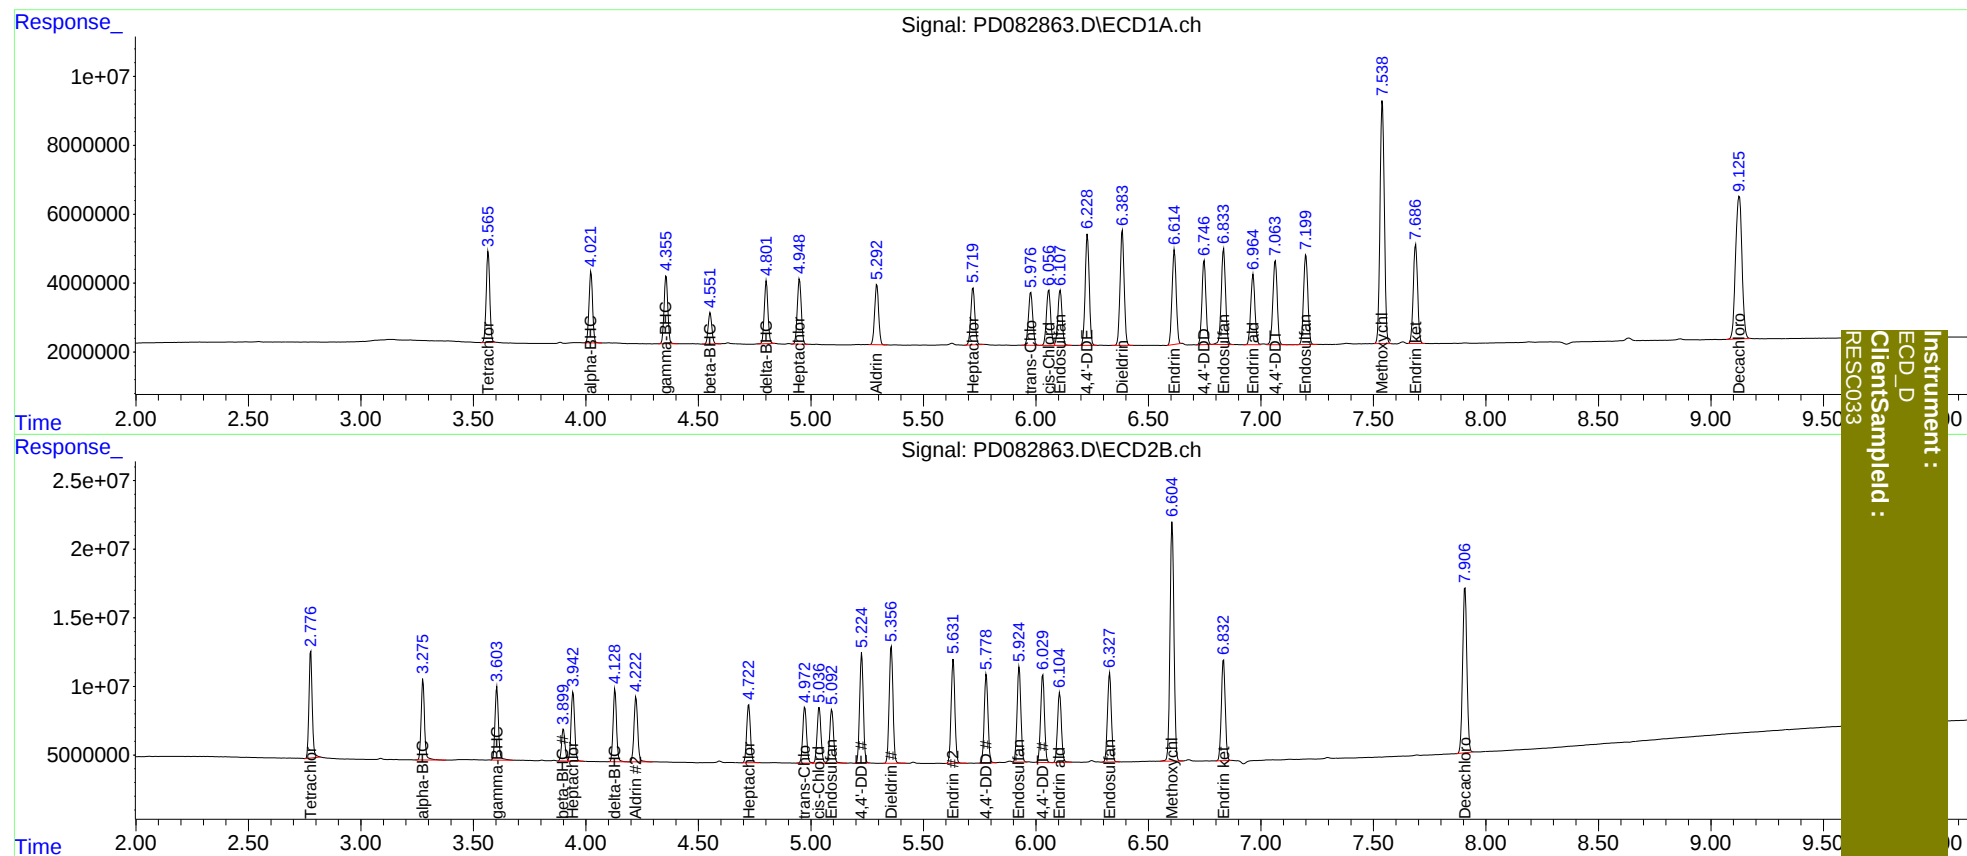

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082863.D
Acq On : 16 May 2024 14:22
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Title : GC Extractables
Last Update : Fri May 17 05:17:58 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.566	4.023	100.00%
4.023	4.357	100.00%
4.357	4.553	100.00%
4.553	4.802	100.00%
4.802	4.949	100.00%
4.949	5.293	100.00%
5.293	5.721	100.00%
5.721	5.977	100.00%
5.977	6.057	100.00%
6.057	6.108	97.85%
6.108	6.229	100.00%
6.229	6.384	100.00%
6.384	6.615	100.00%
6.615	6.748	100.00%
6.748	6.834	100.00%
6.834	6.965	100.00%
6.965	7.064	100.00%
7.064	7.200	100.00%
7.200	7.540	100.00%
7.540	7.688	100.00%
7.688	8.635	100.00%
8.635	9.126	100.00%

Signal #2


2.777	3.276	100.00%
3.276	3.605	100.00%
3.605	3.900	100.00%
3.900	3.943	95.17%
3.943	4.130	100.00%
4.130	4.223	100.00%
4.223	4.724	100.00%
4.724	4.973	100.00%
4.973	5.037	99.39%
5.037	5.093	99.23%
5.093	5.226	100.00%
5.226	5.357	100.00%
5.357	5.633	100.00%
5.633	5.780	100.00%
5.780	5.926	100.00%
5.926	6.031	100.00%
6.031	6.106	100.00%
6.106	6.328	100.00%
6.328	6.606	100.00%
6.606	6.834	100.00%
6.834	7.907	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 14:22
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 05:20:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

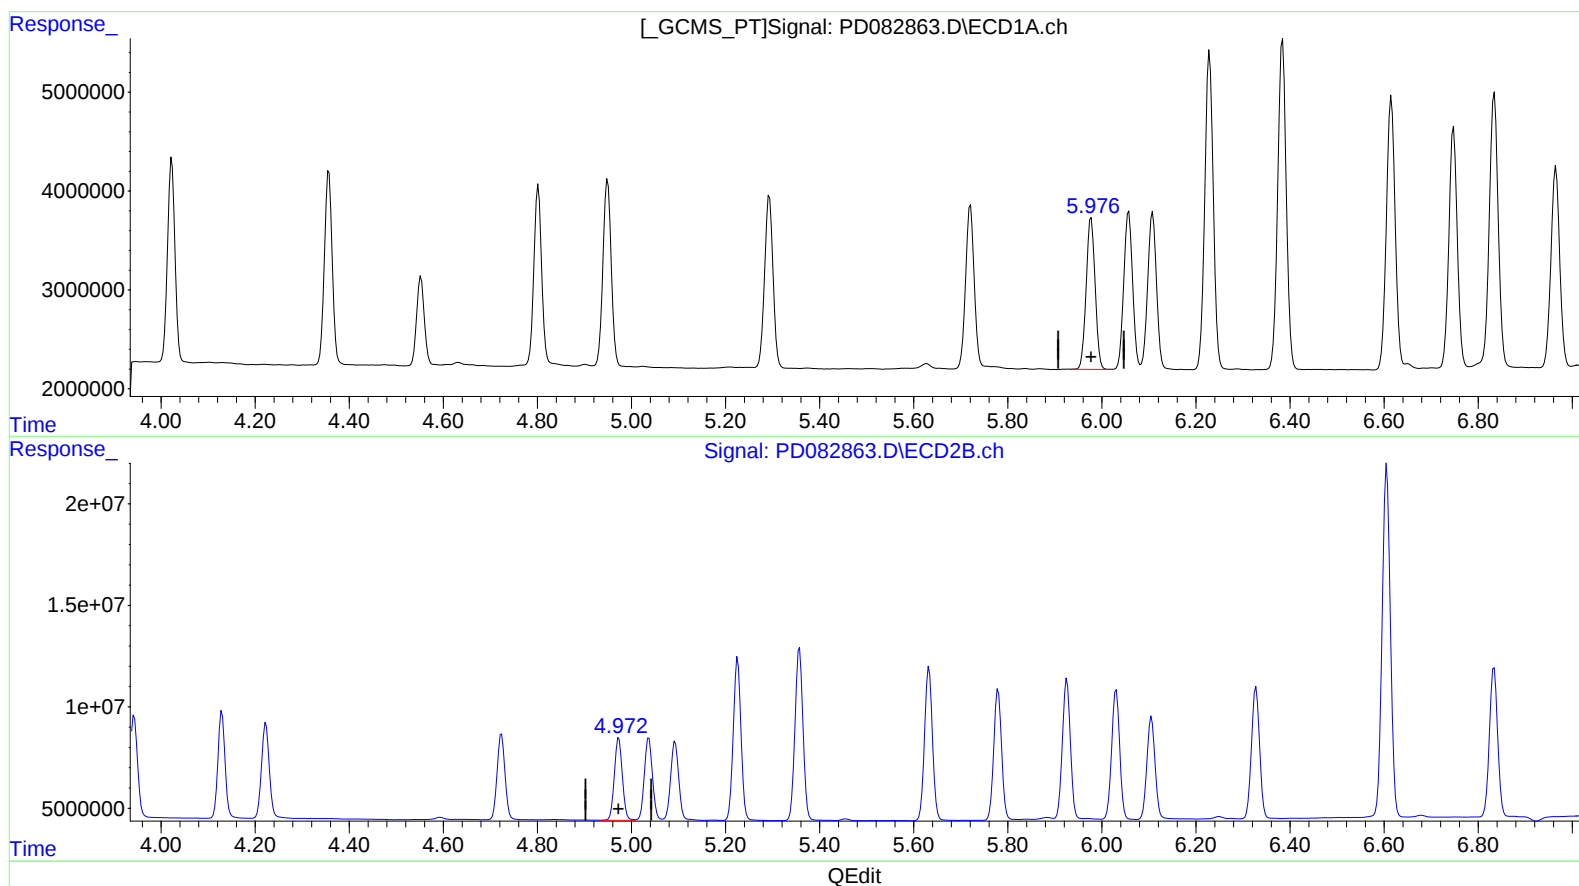

(10) trans-Chlordane (B)

5.977min 9.350 ng/ml

response 20239124

(10) trans-Chlordane #2 (B)

4.973min 9.622 ng/ml


response 47915143

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 14:22
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 05:20:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

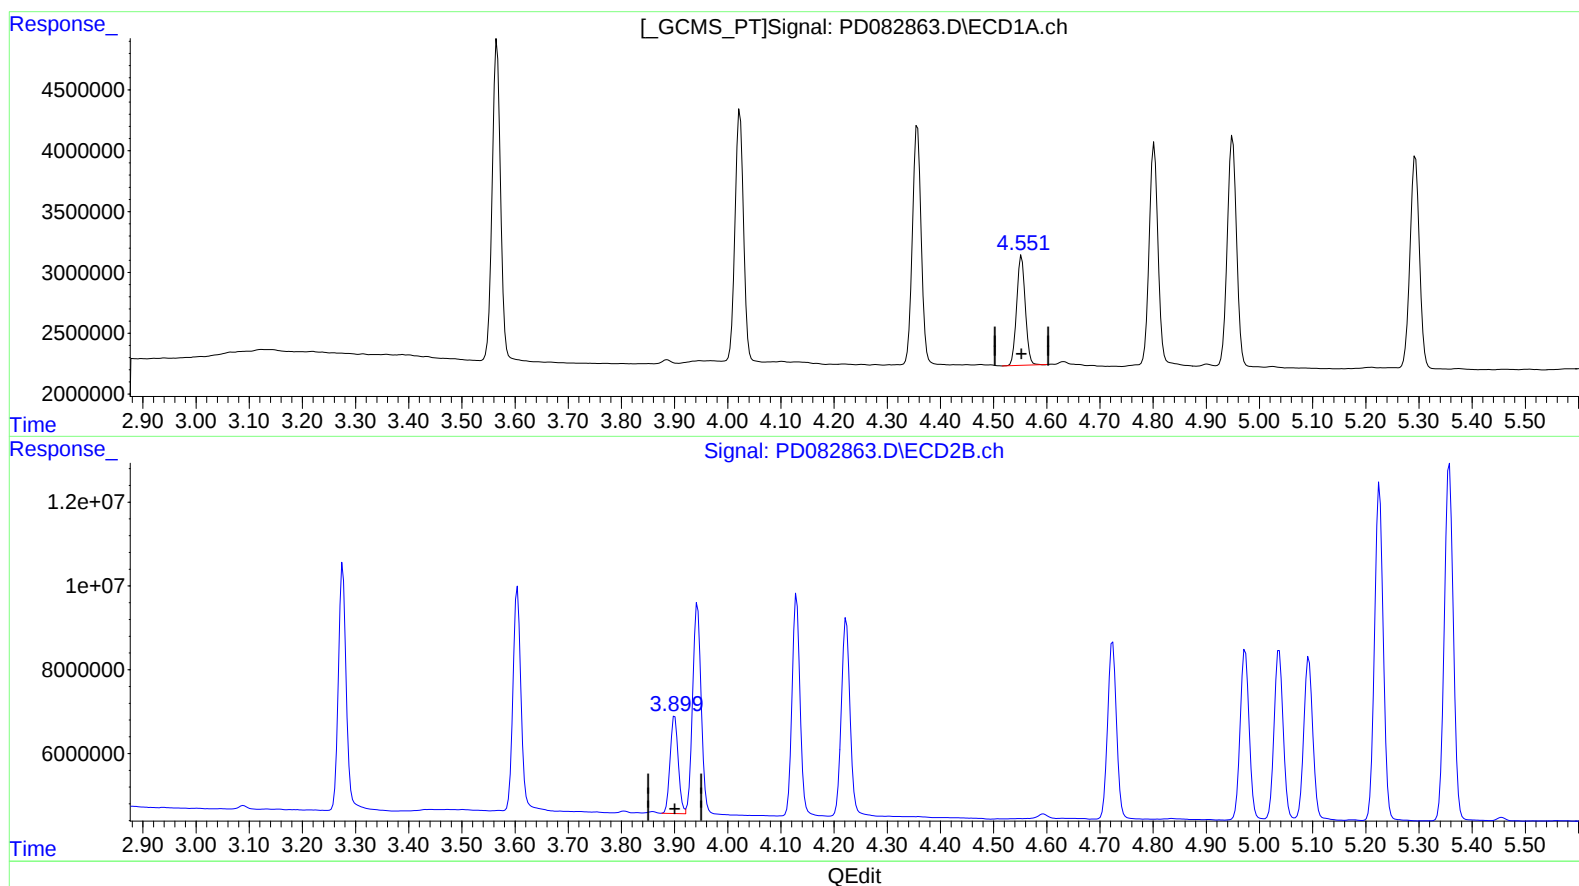

(6) beta-BHC (B)

4.553min 9.365 ng/ml

response 10160154

(6) beta-BHC #2 (B)

3.900min 9.784 ng/ml


response 24538316

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051924\
Data File : PD082863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 14:22
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 05:20:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

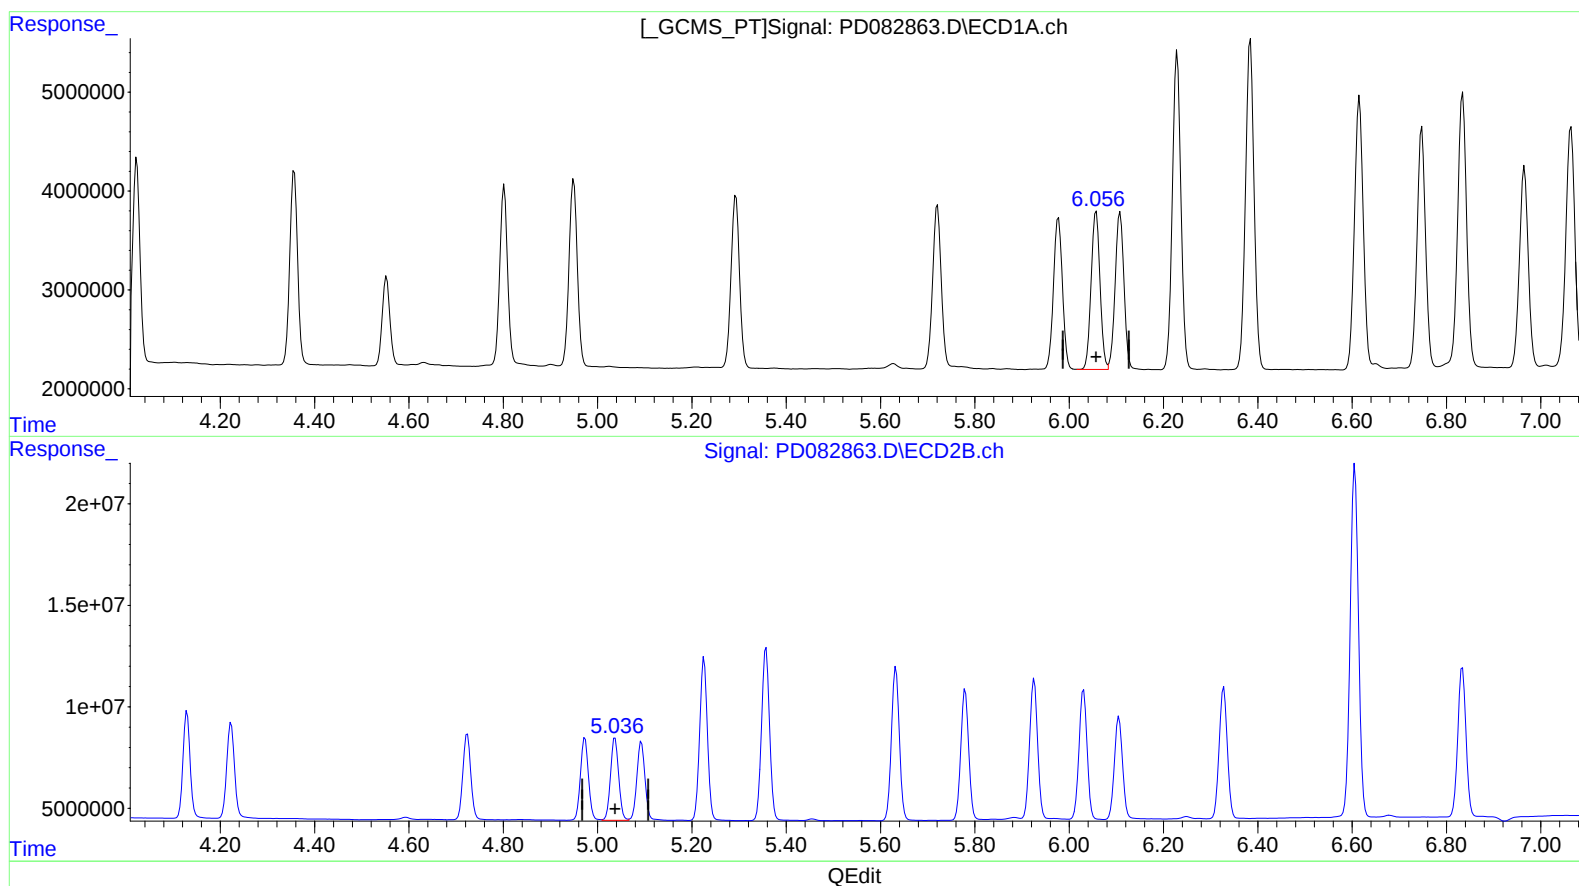

(11) cis-Chlordane (B)

6.057min 9.365 ng/ml

response 20915992

(11) cis-Chlordane #2 (B)

5.037min 9.590 ng/ml

response 48710761