

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052021\
 Data File : PD063115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2021 11:53
 Operator : AR\AJ
 Sample : M2436-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-2A

Manual Integrations
 APPROVED

Ankita
 5/20/2021 1:51:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 07:12:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.969	15993696	164.7E6	14.520	14.209m
28)	SA Decachlor...	8.195	9.024	15355542	148.6E6	12.201	14.566
Target Compounds							
12)	B 4,4'-DDE	5.598	6.302	9458026	123.6E6	6.593m	8.186

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052021\
Data File : PD063115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2021 11:53
Operator : AR\AJ
Sample : M2436-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleID :
TP-2A


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 07:12:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

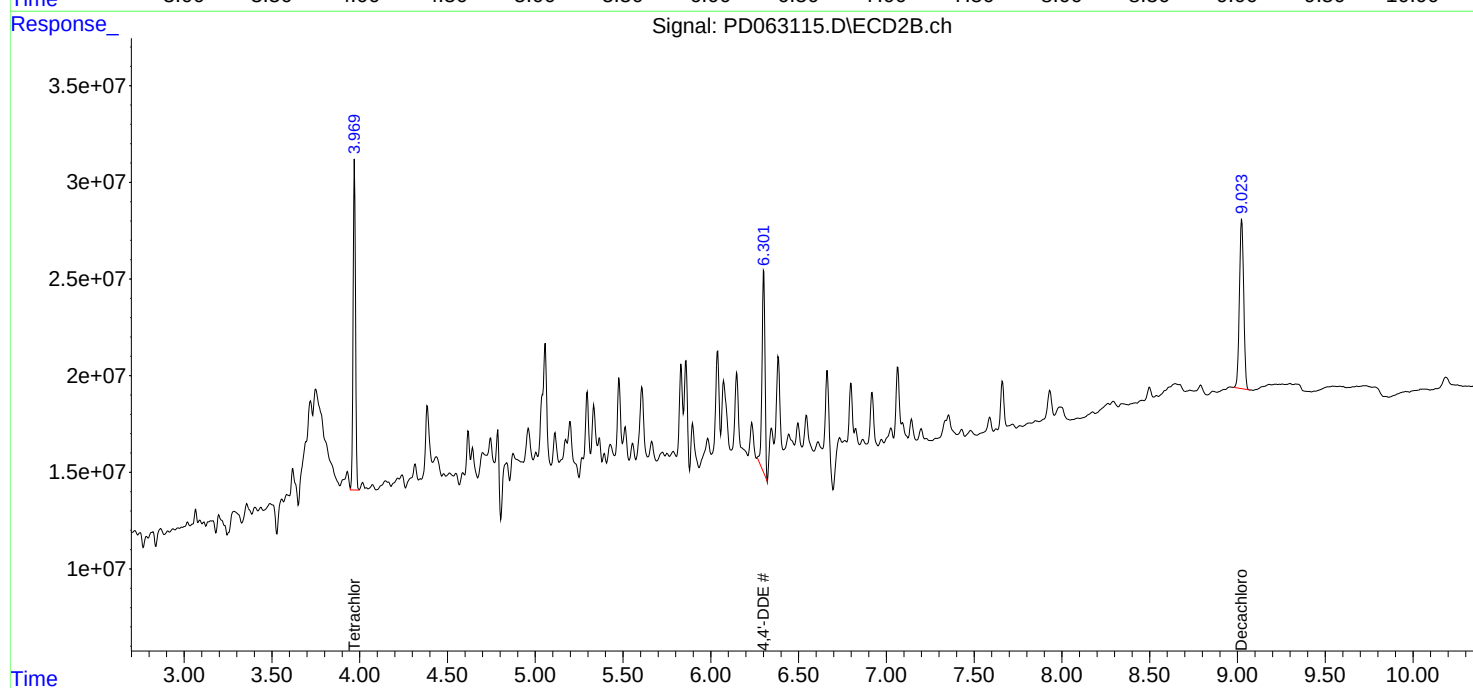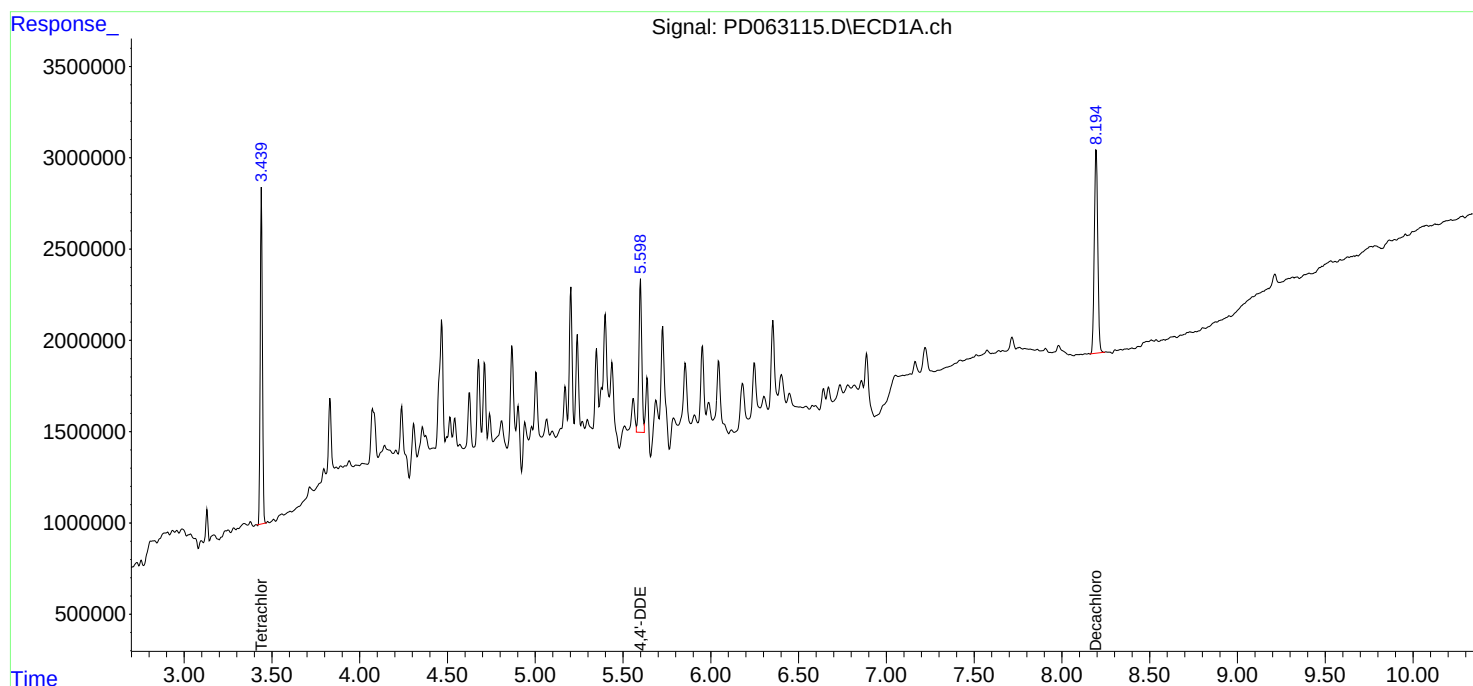

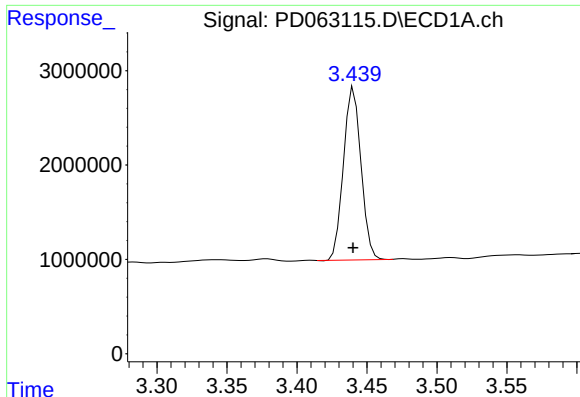


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 15993696
Conc: 14.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-2A


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:06 PM

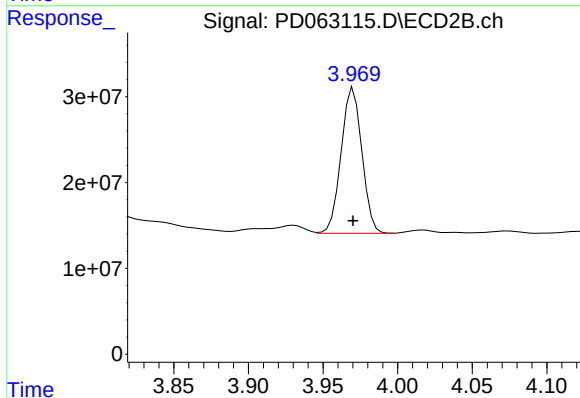


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 164653617
Conc: 14.21 ng/ml m

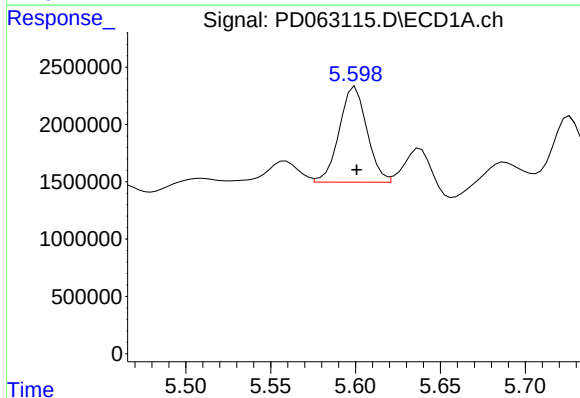


#12 4,4'-DDE

R.T.: 5.598 min
Delta R.T.: -0.002 min
Response: 9458026
Conc: 6.59 ng/ml m

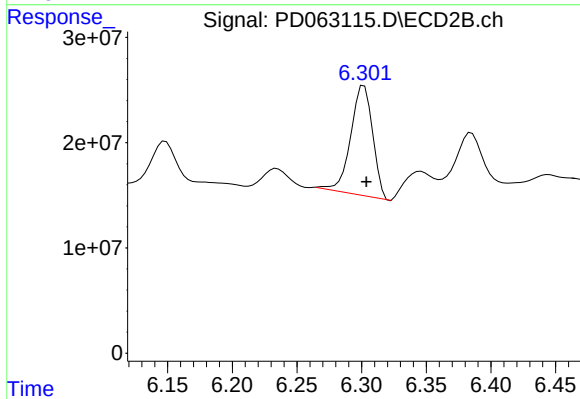

#12 4,4'-DDE

R.T.: 6.302 min
Delta R.T.: -0.002 min
Response: 123565699
Conc: 8.19 ng/ml

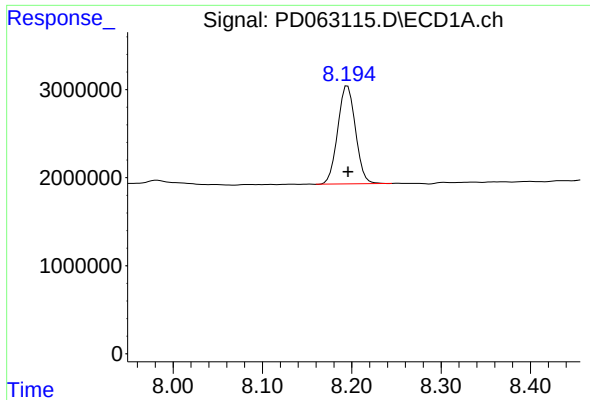


#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 15355542
Conc: 12.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-2A

Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:06 PM

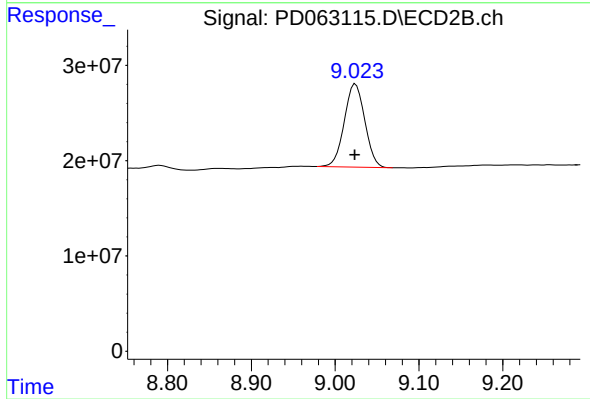

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 148599681
Conc: 14.57 ng/ml