

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052021\
 Data File : PD063116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2021 12:21
 Operator : AR\AJ
 Sample : M2383-06RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DUP-01-05112021RE

Manual Integrations
 APPROVED

Ankita
 5/20/2021 1:51:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 07:12:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.969	19255394	202.4E6	17.481	17.462m
28)	SA Decachlor...	8.195	9.024	18631969	168.5E6	14.804	16.516

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052021\
Data File : PD063116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2021 12:21
Operator : AR\AJ
Sample : M2383-06RE
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
DUP-01-05112021RE


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 07:12:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

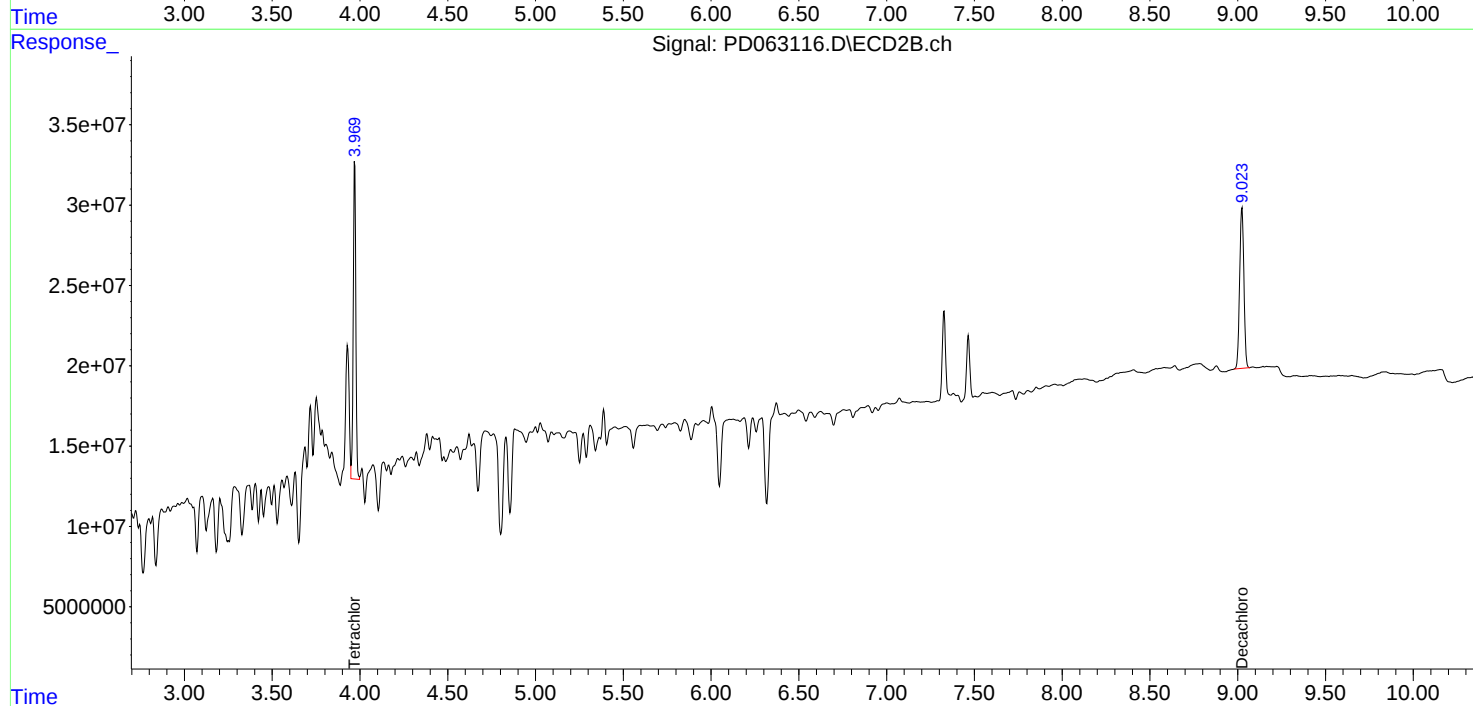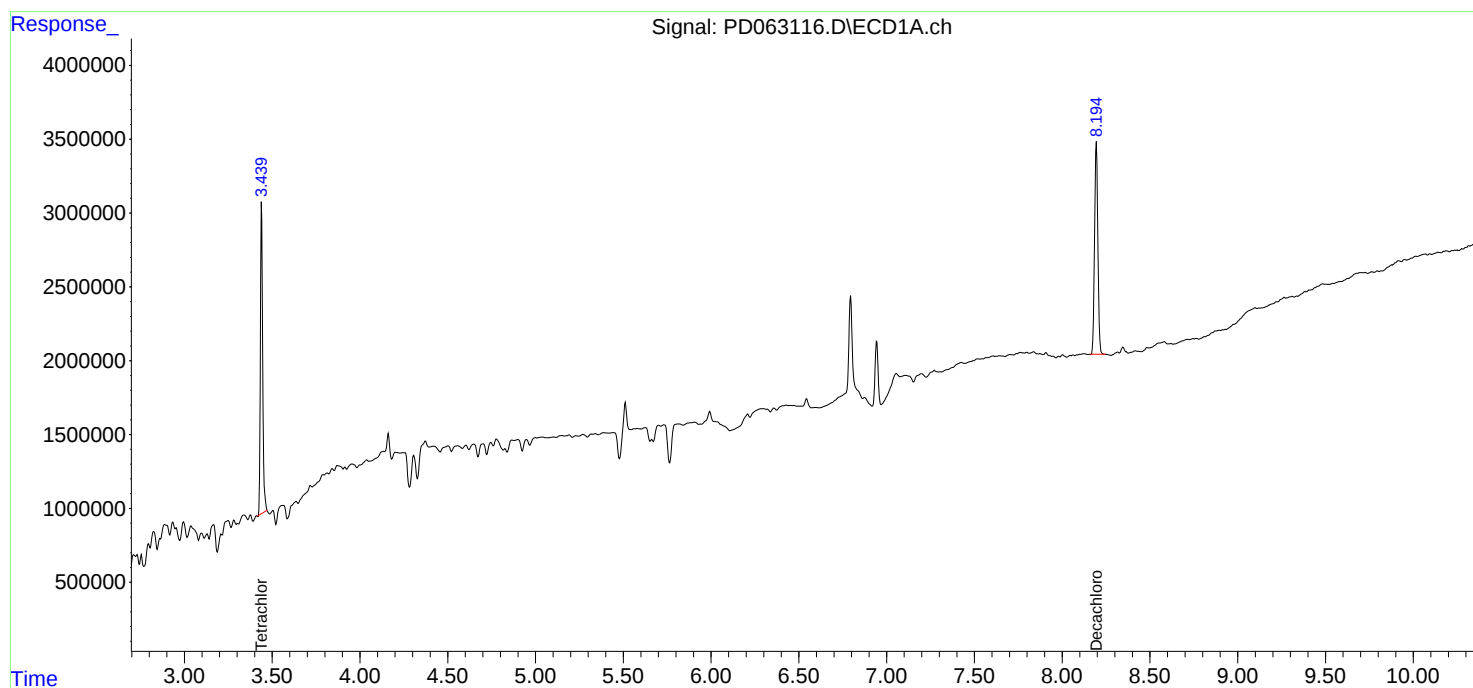

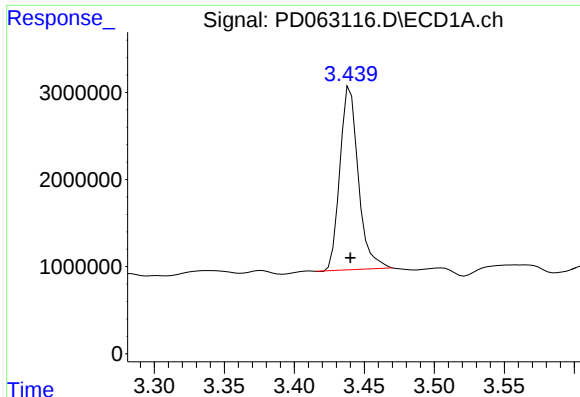


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 19255394
Conc: 17.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-01-05112021RE


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:08 PM

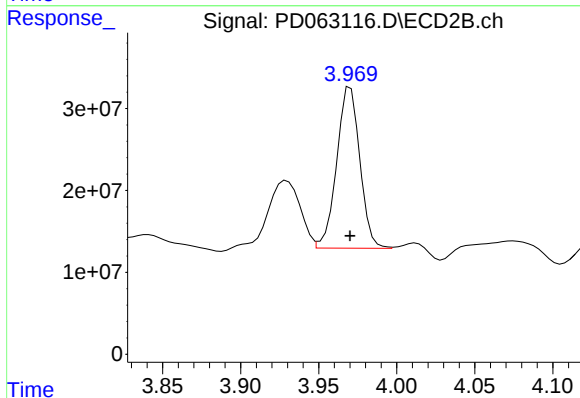


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 202357829
Conc: 17.46 ng/ml m

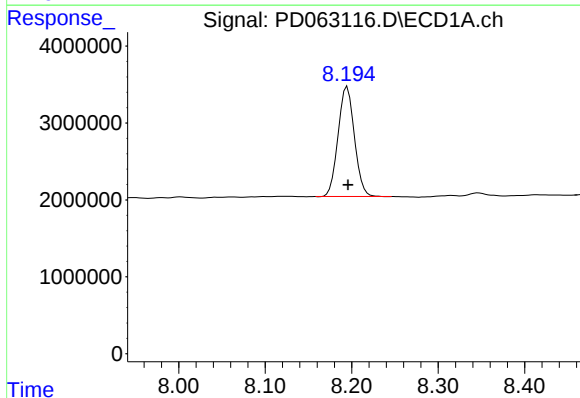

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 18631969
Conc: 14.80 ng/ml

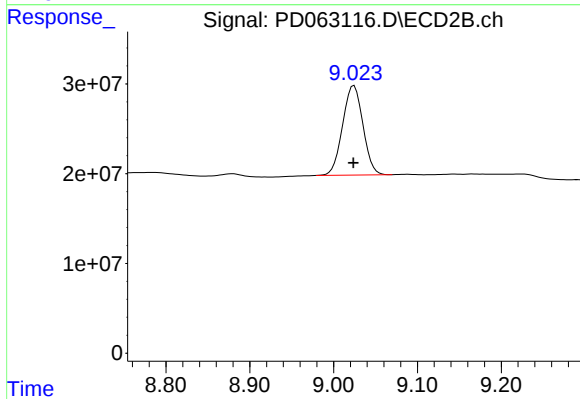

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 168492844
Conc: 16.52 ng/ml