

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052021\
 Data File : PD063134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2021 17:14
 Operator : AR\AJ
 Sample : M2437-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Ankita
 5/20/2021 1:51:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 07:17:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.970	15255010	129.3E6	13.849	11.158m
28)	SA Decachlor...	8.195	9.025	93473567	855.9E6	74.271	83.898
Target Compounds							
12)	B 4,4'-DDE	5.599	6.298	5404521	45081336	3.767m	2.987m
17)	MA 4,4'-DDT	6.354	7.092	15675628	44743052	13.715	3.968m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052021\
Data File : PD063134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2021 17:14
Operator : AR\AJ
Sample : M2437-08
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 07:17:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

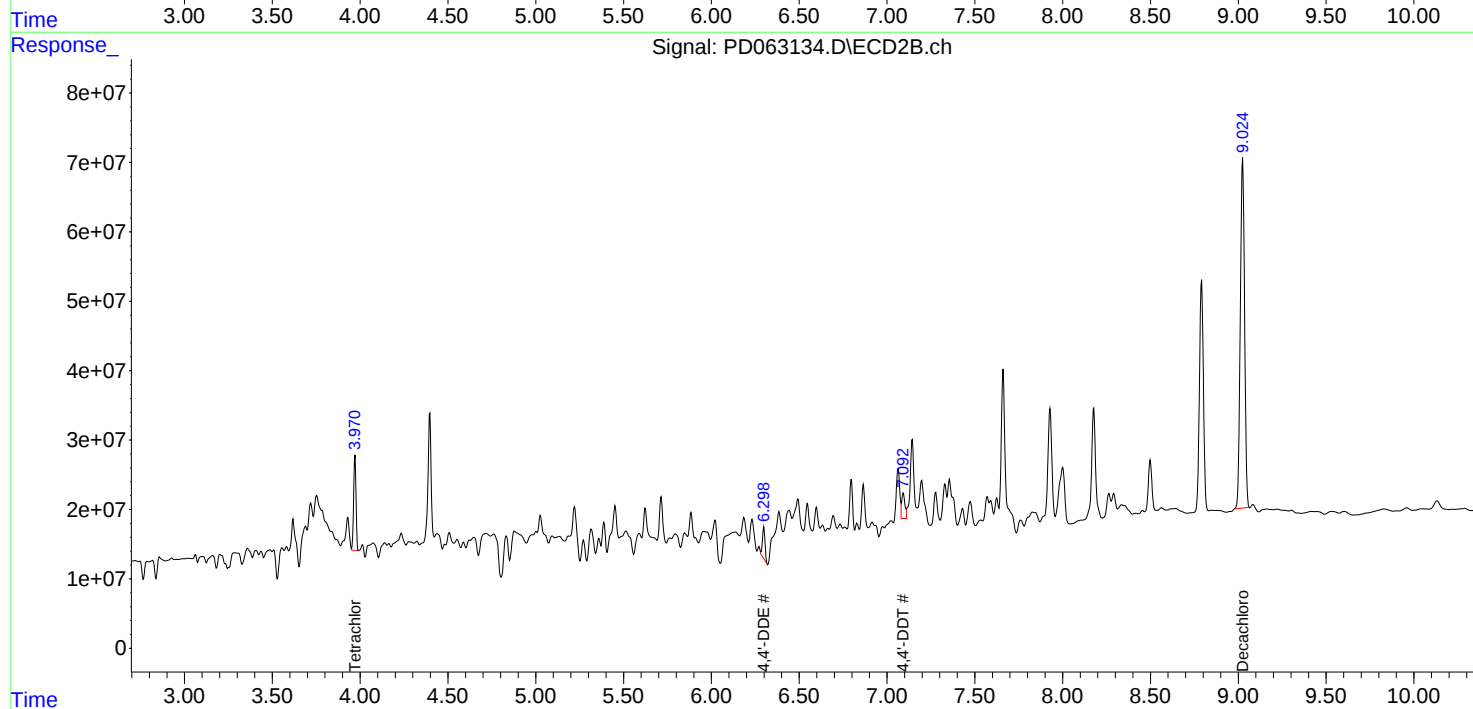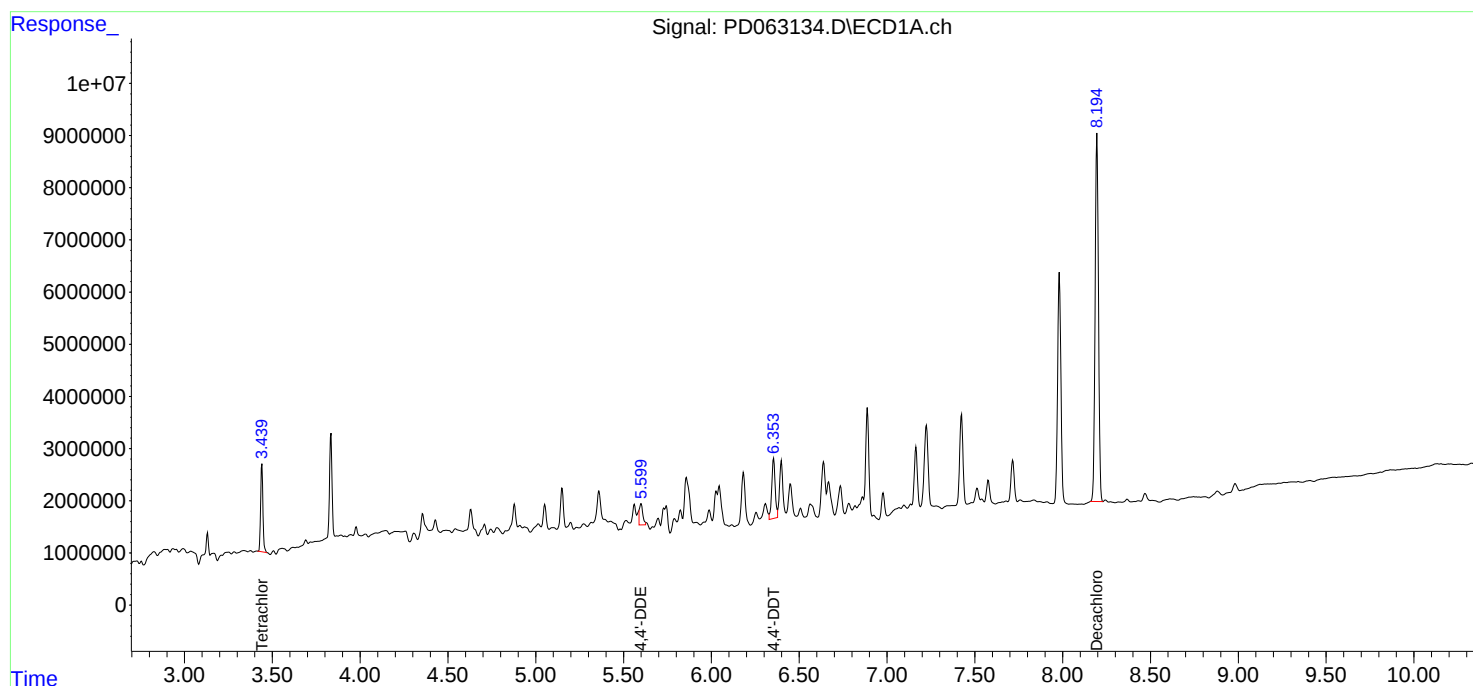

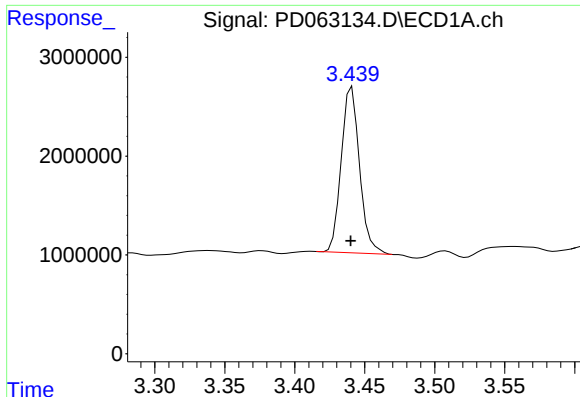


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 15255010
Conc: 13.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:28 PM

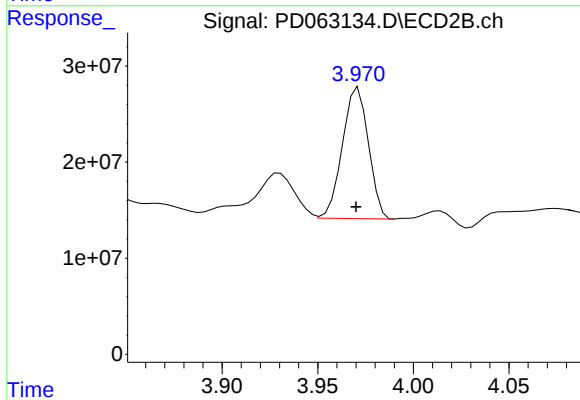


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 129299339
Conc: 11.16 ng/ml m

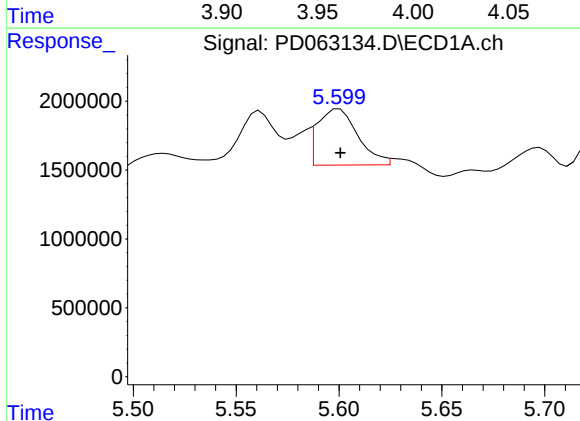


#12 4,4'-DDE

R.T.: 5.599 min
Delta R.T.: -0.002 min
Response: 5404521
Conc: 3.77 ng/ml m

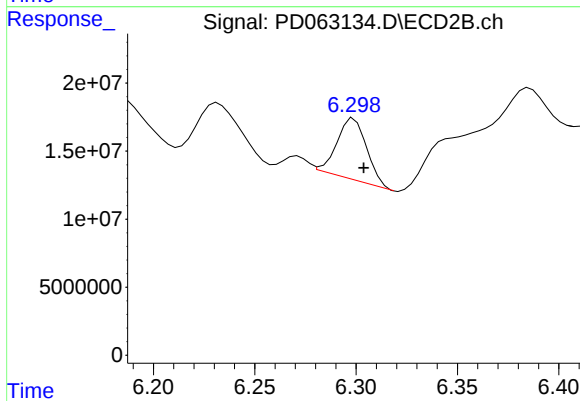

#12 4,4'-DDE

R.T.: 6.298 min
Delta R.T.: -0.006 min
Response: 45081336
Conc: 2.99 ng/ml m

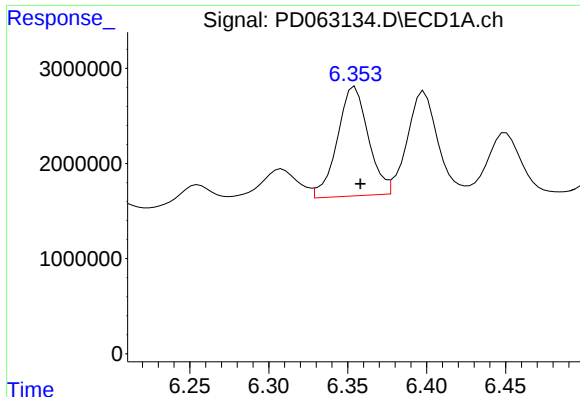


#17 4,4'-DDT

R.T.: 6.354 min
Delta R.T.: -0.003 min
Response: 15675628
Conc: 13.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:28 PM

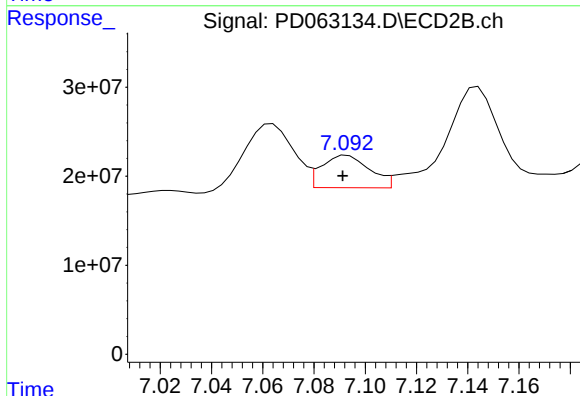


#17 4,4'-DDT

R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 44743052
Conc: 3.97 ng/ml m

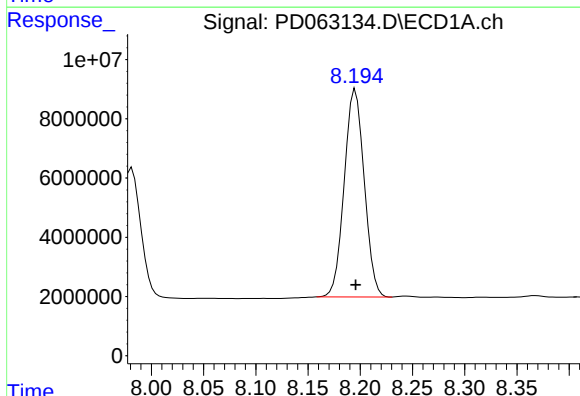

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 93473567
Conc: 74.27 ng/ml

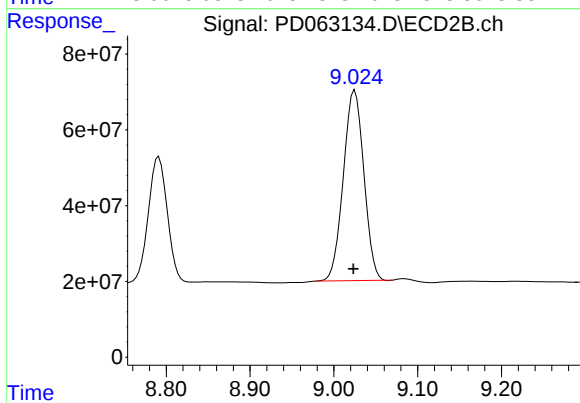

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.001 min
Response: 855929447
Conc: 83.90 ng/ml