

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052021\
 Data File : PD063137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2021 19:40
 Operator : AR\AJ
 Sample : M2438-01 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PL-02-051821

Manual Integrations
 APPROVED

Ankita
 5/20/2021 1:51:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 07:18:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.440	3.969	1904900	18277444	1.729	1.577m
28) SA Decachlor...	8.195	9.024	2198095	23188578	1.747	2.273 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052021\
Data File : PD063137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2021 19:40
Operator : AR\AJ
Sample : M2438-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PL-02-051821


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 07:18:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

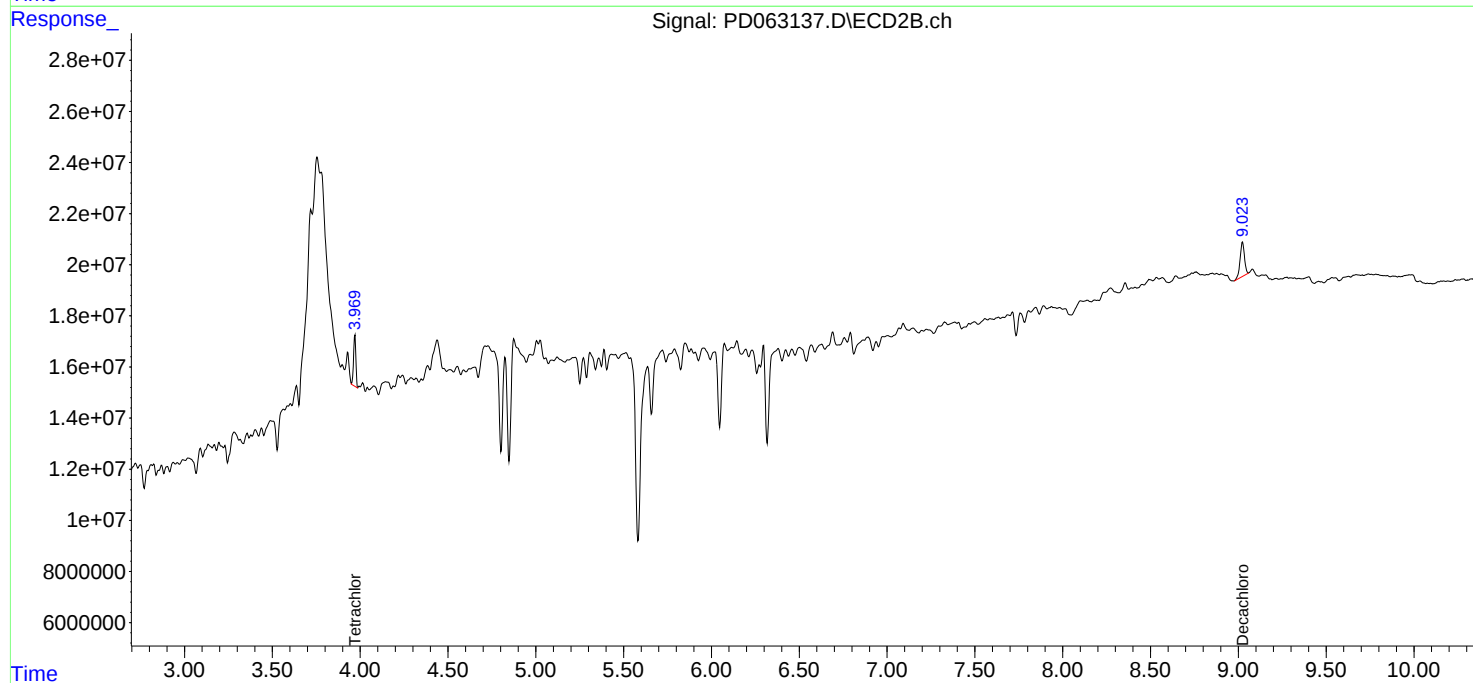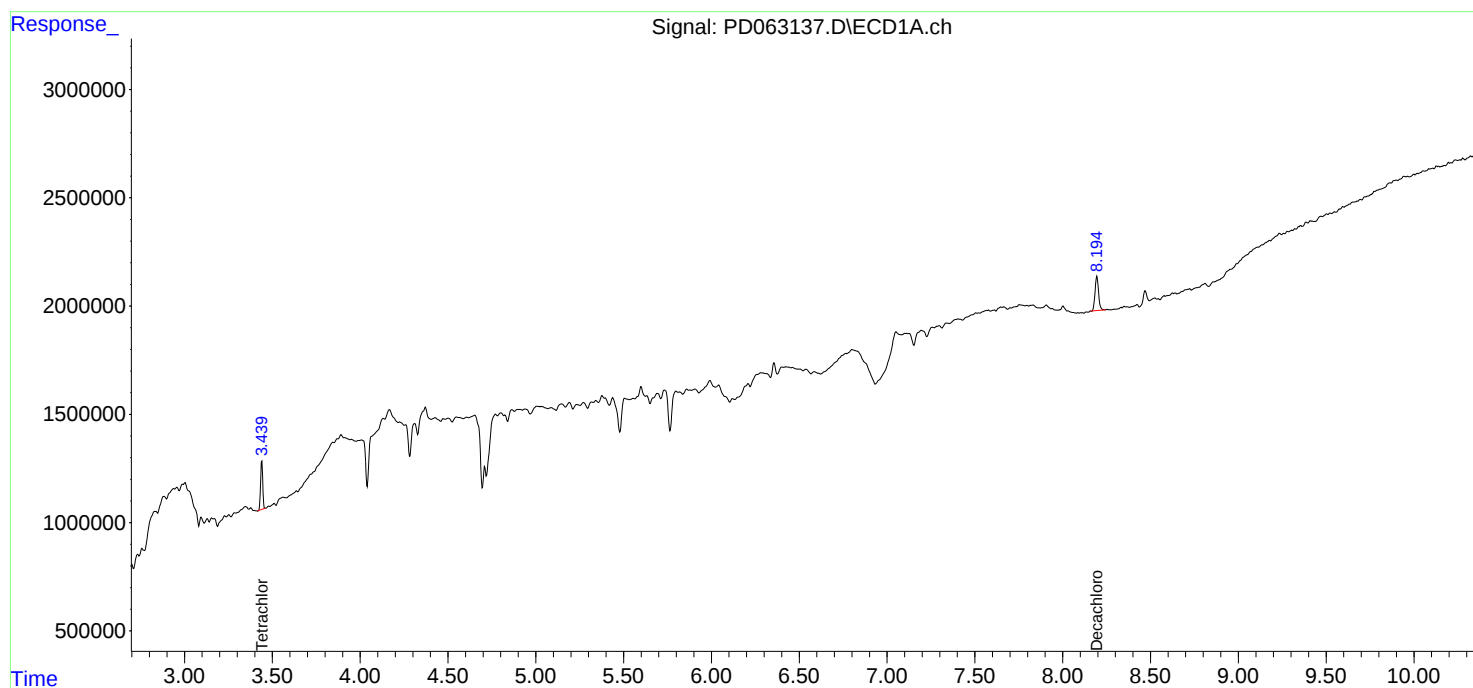

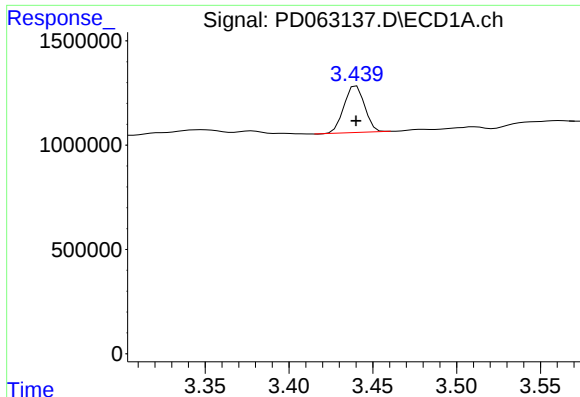


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 1904900
Conc: 1.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PL-02-051821


Manual Integrations
APPROVED

Ankita
5/20/2021 1:51:30 PM

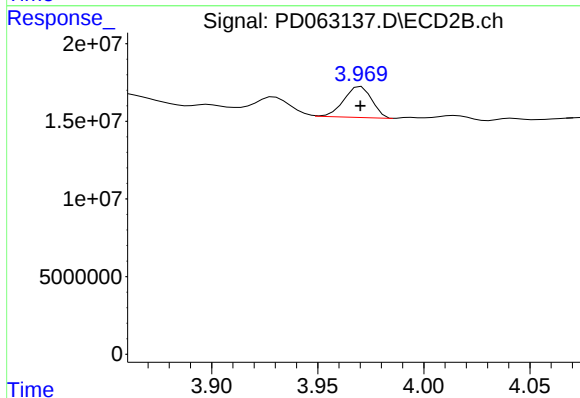


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 18277444
Conc: 1.58 ng/ml m

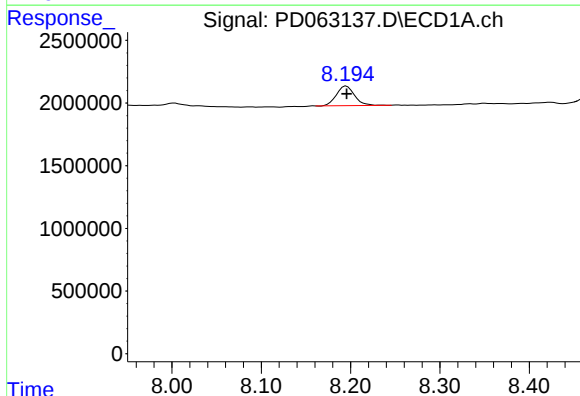

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 2198095
Conc: 1.75 ng/ml

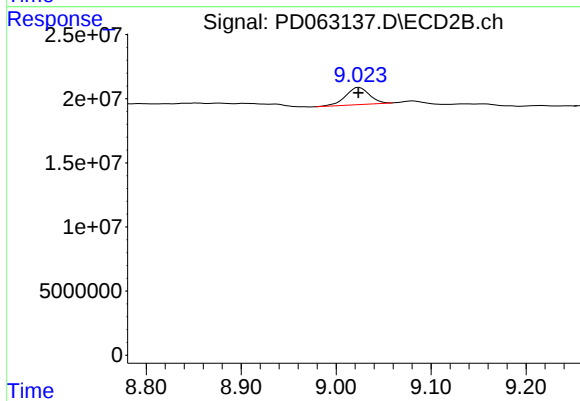

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 23188578
Conc: 2.27 ng/ml