

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
 Data File : PD069718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 19:44
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 01:53:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Fri May 20 01:35:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.173	5838265	56047810	4.744	5.514
28)	SA Decachlor...	8.199	9.370	6481113	34895209	5.530	5.465
Target Compounds							
23)	Chlordane-1	4.313	5.194	2170260	23288802	54.165	56.722
24)	Chlordane-2	4.815	5.667	2498096	23025046	53.128	55.851
25)	Chlordane-3	5.381	6.324	6230761	97966126	48.669	66.129 #
26)	Chlordane-4	5.439	6.402	5519770	109.3E6	51.112	63.199
27)	Chlordane-5	6.278	7.213	1891950	18926360	44.656	55.233



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
Data File : PD069718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 19:44
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 01:53:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Fri May 20 01:35:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

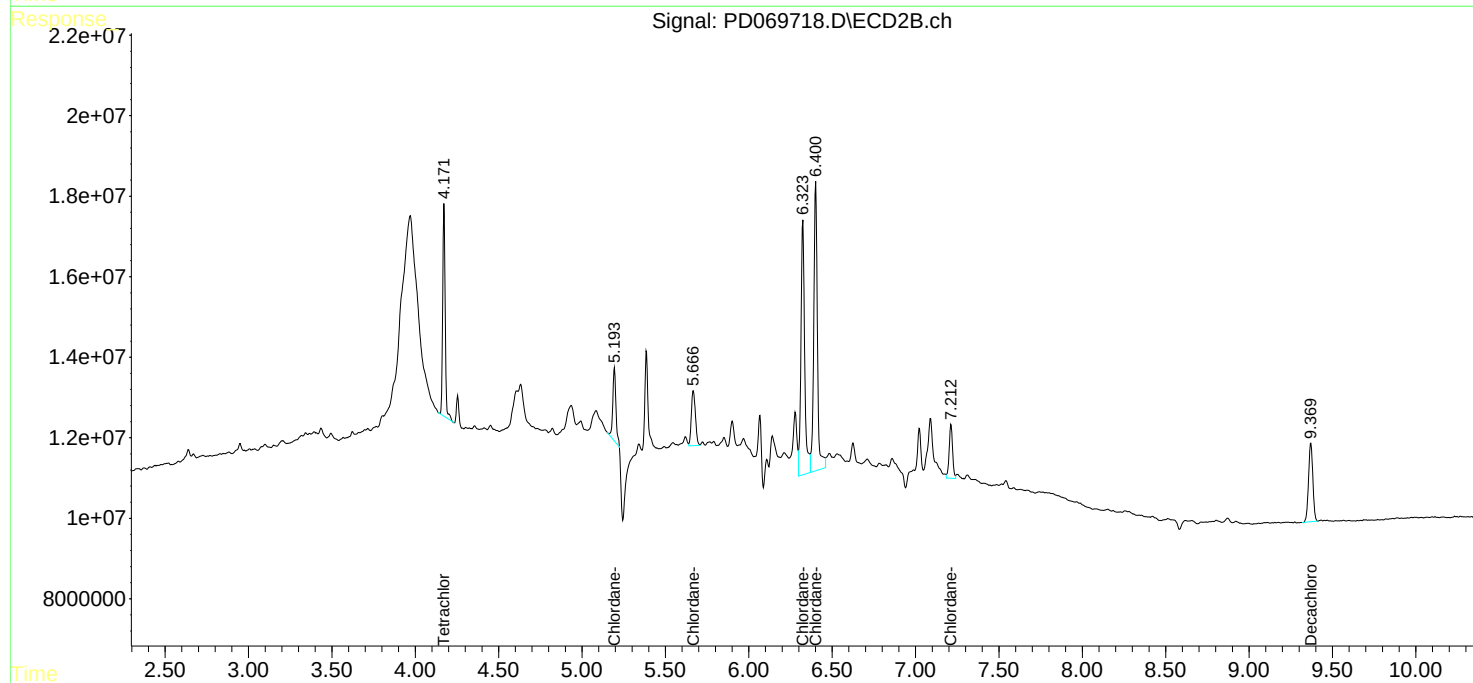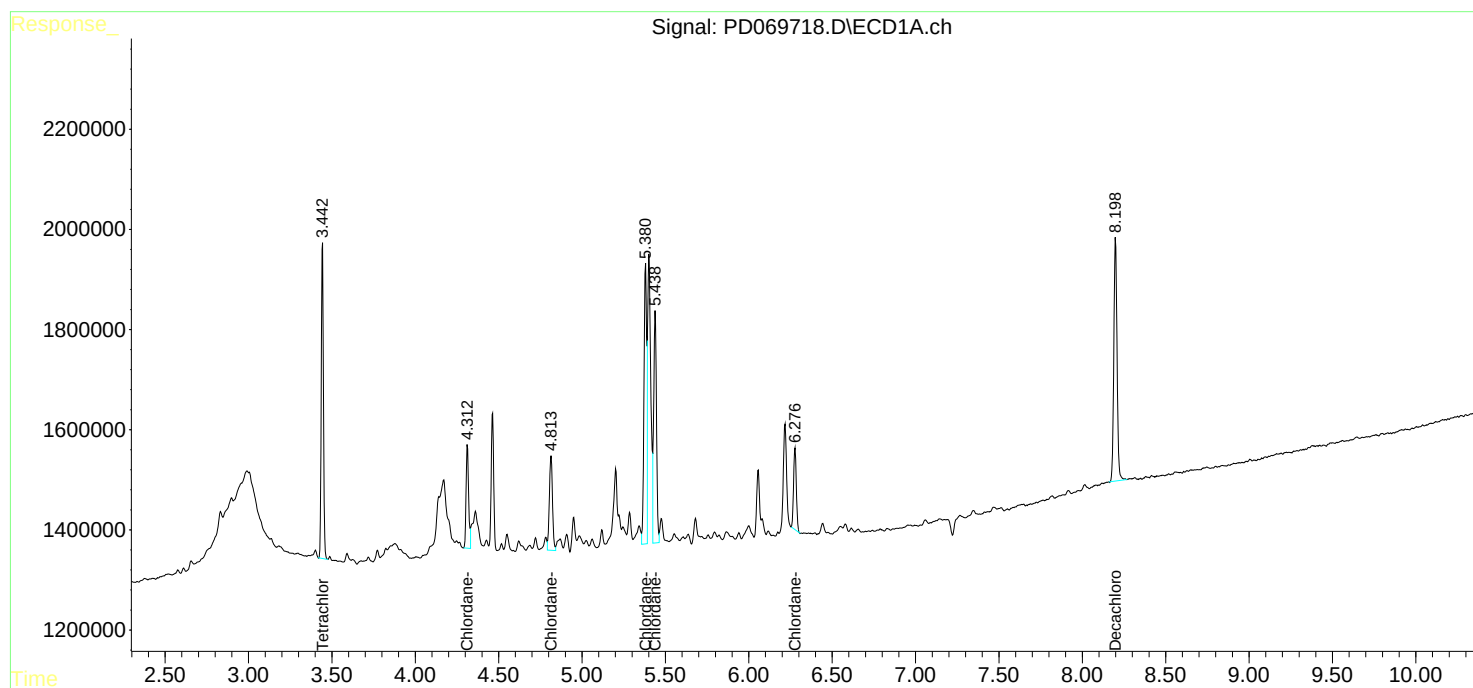


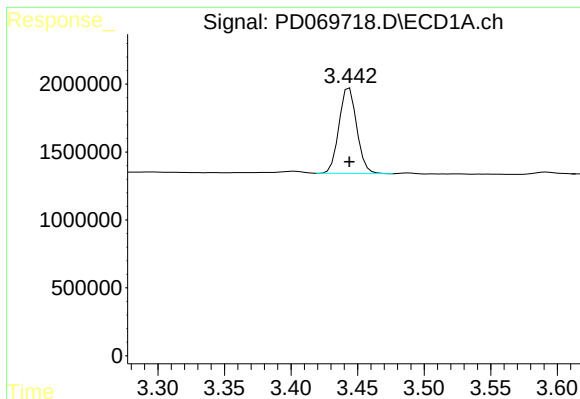

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 5838265
Conc: 4.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

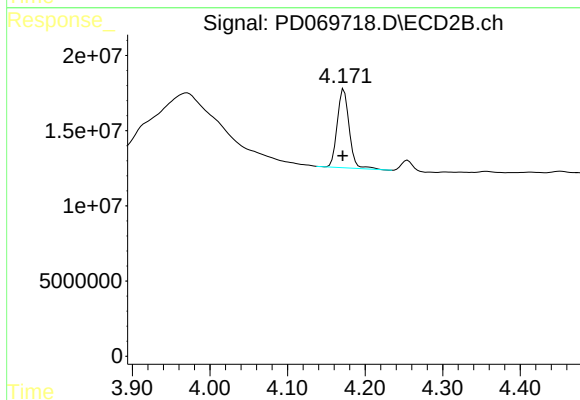


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: 0.002 min
Response: 56047810
Conc: 5.51 ng/ml

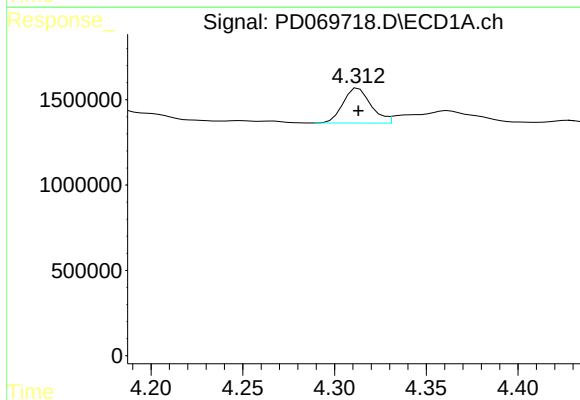


#23 Chlordane-1

R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 2170260
Conc: 54.17 ng/ml

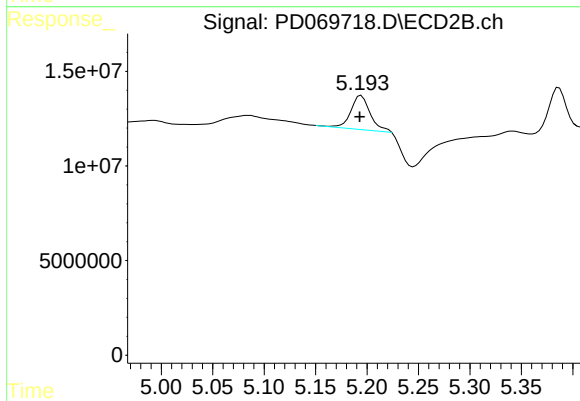

#23 Chlordane-1


R.T.: 5.194 min
Delta R.T.: 0.001 min
Response: 23288802
Conc: 56.72 ng/ml

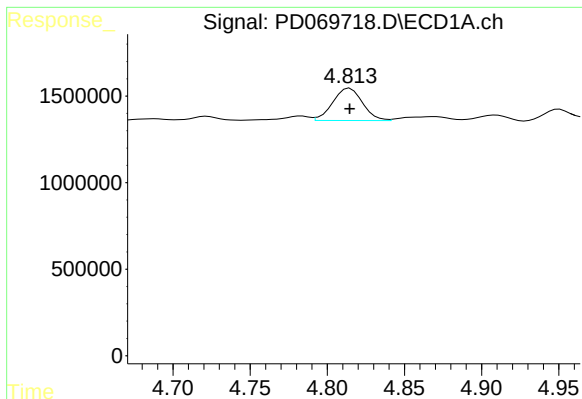

#24 Chlordane-2


R.T.: 4.815 min
Delta R.T.: 0.000 min
Response: 2498096
Conc: 53.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

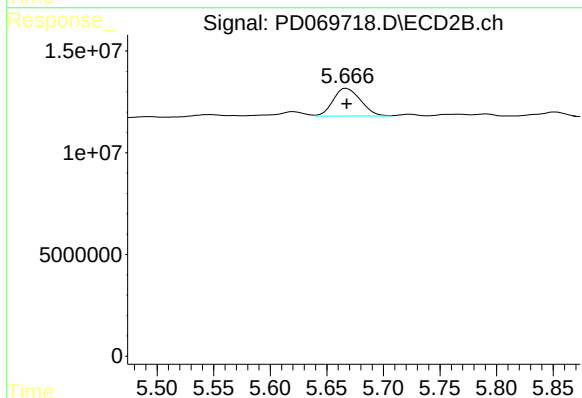


#24 Chlordane-2

R.T.: 5.667 min
Delta R.T.: 0.000 min
Response: 23025046
Conc: 55.85 ng/ml

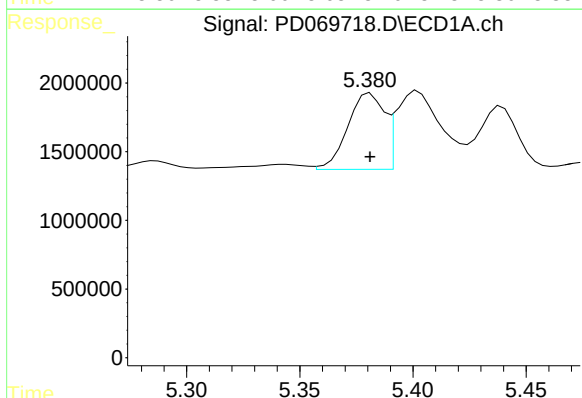


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 6230761
Conc: 48.67 ng/ml

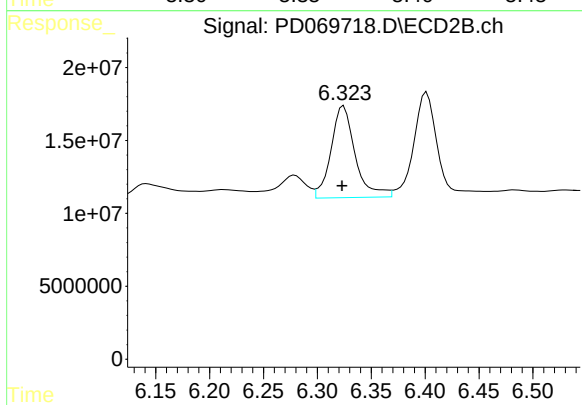

#25 Chlordane-3


R.T.: 6.324 min
Delta R.T.: 0.001 min
Response: 97966126
Conc: 66.13 ng/ml

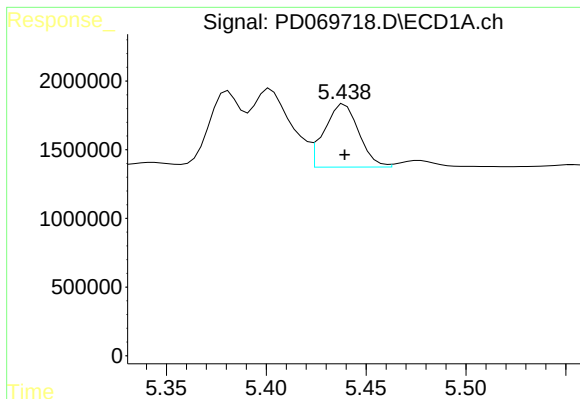

#26 Chlordane-4


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 5519770
Conc: 51.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

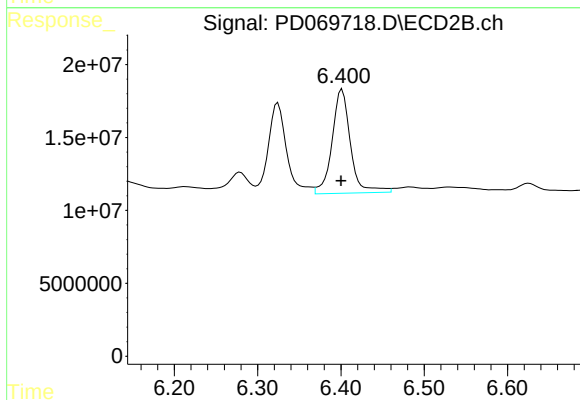


#26 Chlordane-4

R.T.: 6.402 min
Delta R.T.: 0.001 min
Response: 109306830
Conc: 63.20 ng/ml

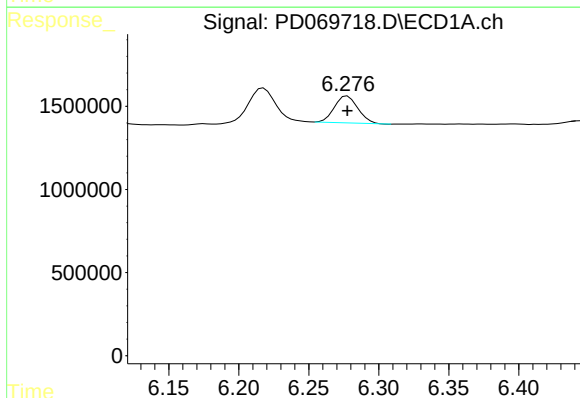


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 1891950
Conc: 44.66 ng/ml

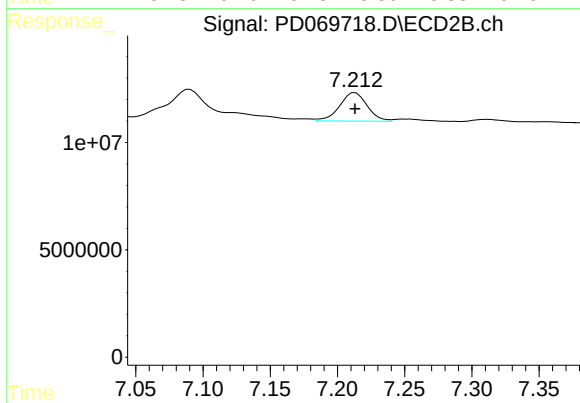

#27 Chlordane-5


R.T.: 7.213 min
Delta R.T.: 0.000 min
Response: 18926360
Conc: 55.23 ng/ml

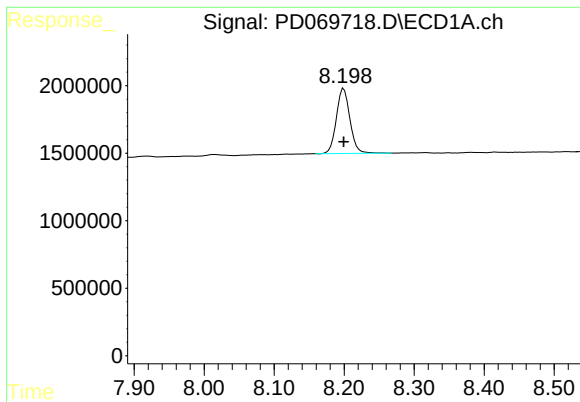

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 6481113
Conc: 5.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

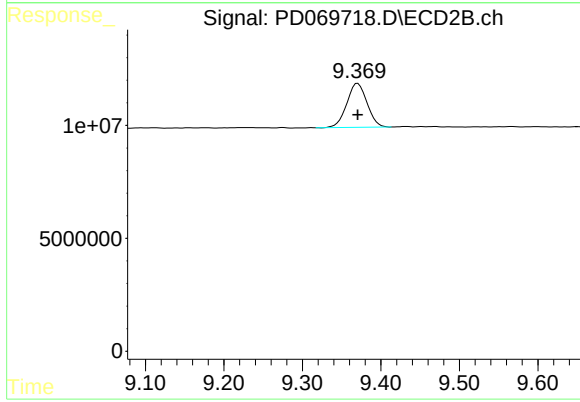

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: 0.000 min
Response: 34895209
Conc: 5.47 ng/ml