

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
 Data File : PD069708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 17:24
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 02:40:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.172	24261033	236.0E6	24.211	24.702
28)	SA Decachlor...	8.199	9.370	25568959	144.8E6	23.705	24.162
Target Compounds							
9)	A Endosulfan I	5.493	6.450	14000695	123.9E6	11.804	12.502
10)	B gamma-Chl...	5.380	6.324	15070119	131.9E6	11.782	12.326
12)	B 4,4'-DDE	5.605	6.549	26431413	235.0E6	22.837	23.672
13)	MA Dieldrin	5.737	6.709	28697479	249.5E6	23.213	24.373
19)	B Endosulfa...	6.651	7.484	23750472	178.1E6	21.592	22.296
20)	A Methoxychlor	6.912	7.797	60436748	408.4E6	104.854	99.054
21)	B Endrin ke...	7.145	7.959	28561379	200.6E6	22.799	24.018



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
Data File : PD069708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 17:24
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 02:40:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

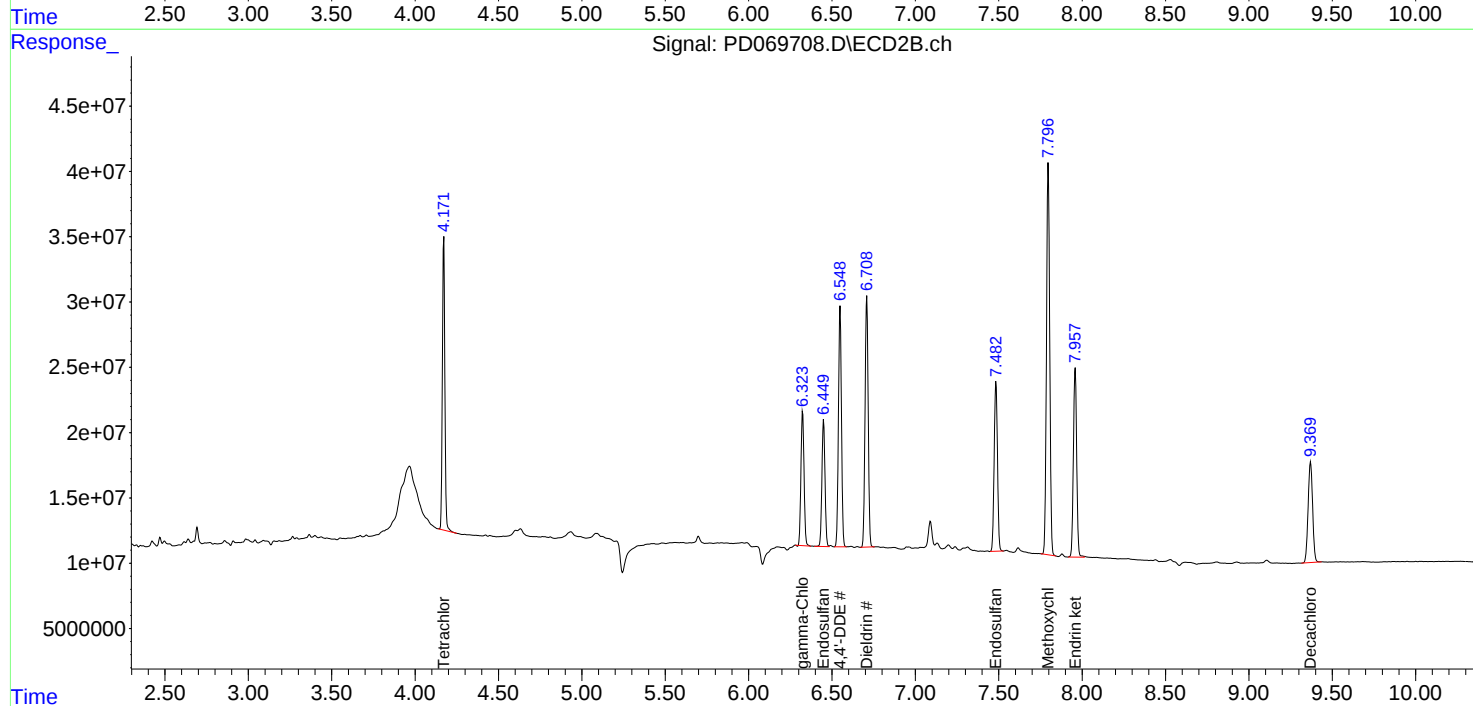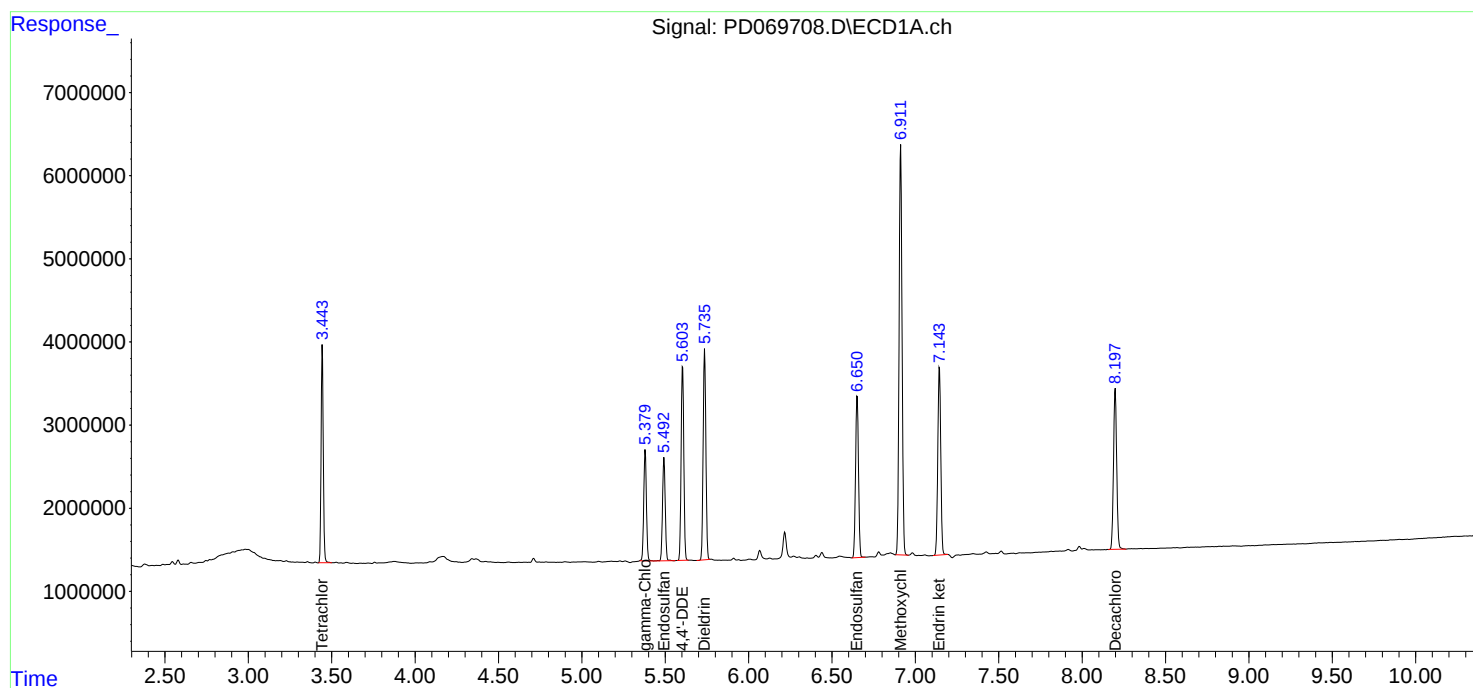


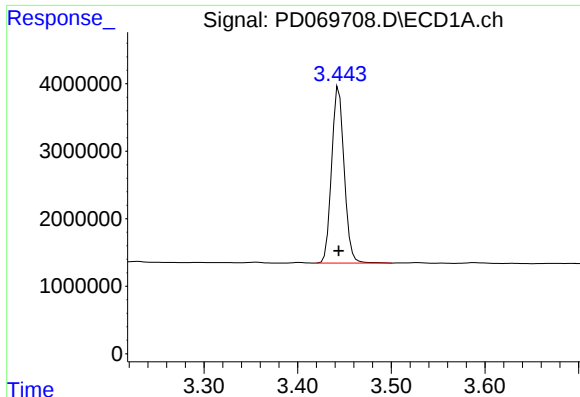

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 24261033
Conc: 24.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

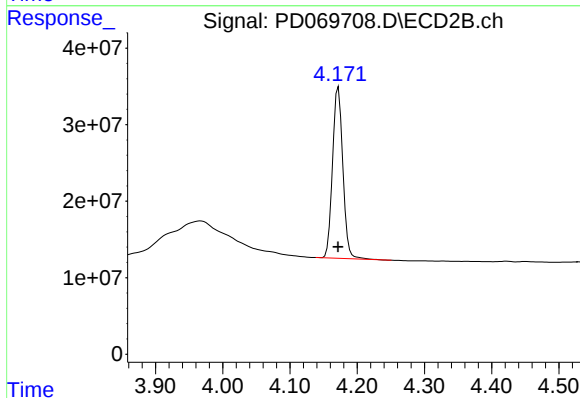


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 236003921
Conc: 24.70 ng/ml

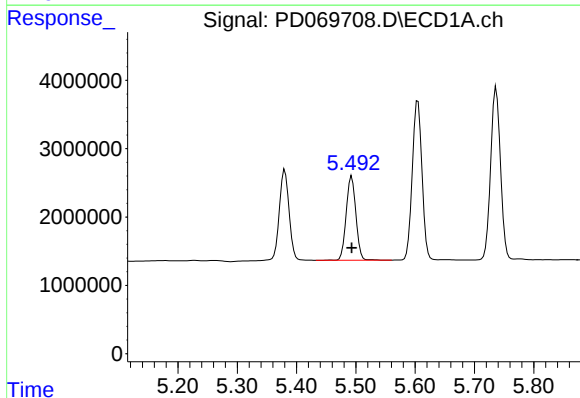


#9 Endosulfan I

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 14000695
Conc: 11.80 ng/ml

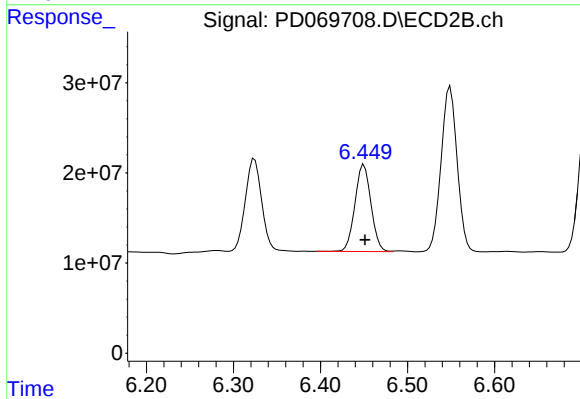

#9 Endosulfan I


R.T.: 6.450 min
Delta R.T.: -0.001 min
Response: 123911128
Conc: 12.50 ng/ml

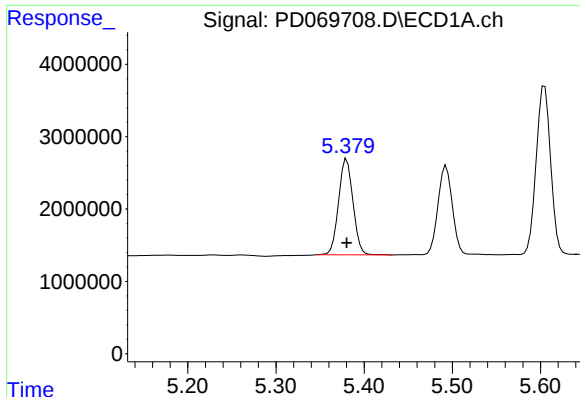

#10 gamma-Chlordane


R.T.: 5.380 min
Delta R.T.: 0.000 min
Response: 15070119
Conc: 11.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

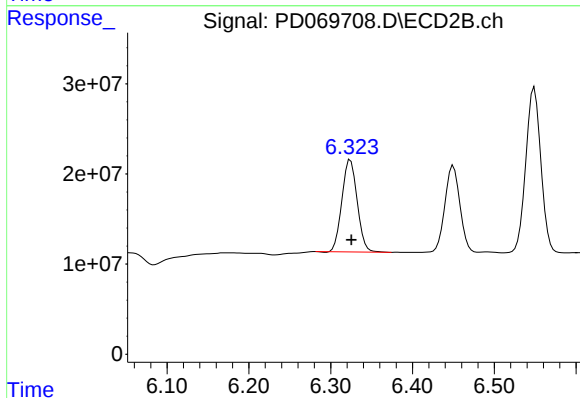


#10 gamma-Chlordane

R.T.: 6.324 min
Delta R.T.: -0.001 min
Response: 131923947
Conc: 12.33 ng/ml

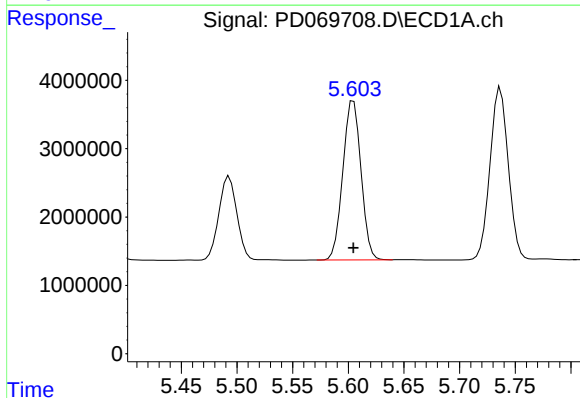


#12 4,4'-DDE

R.T.: 5.605 min
Delta R.T.: 0.000 min
Response: 26431413
Conc: 22.84 ng/ml

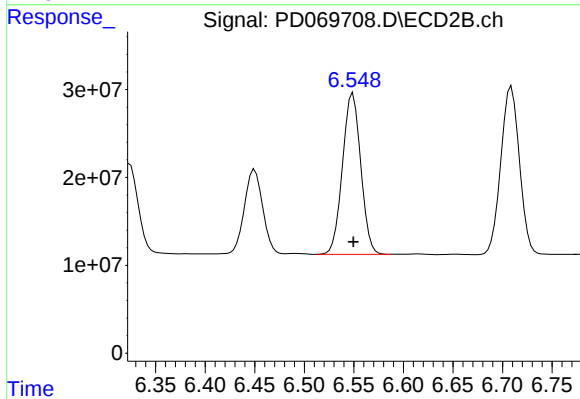

#12 4,4'-DDE


R.T.: 6.549 min
Delta R.T.: 0.000 min
Response: 234976993
Conc: 23.67 ng/ml

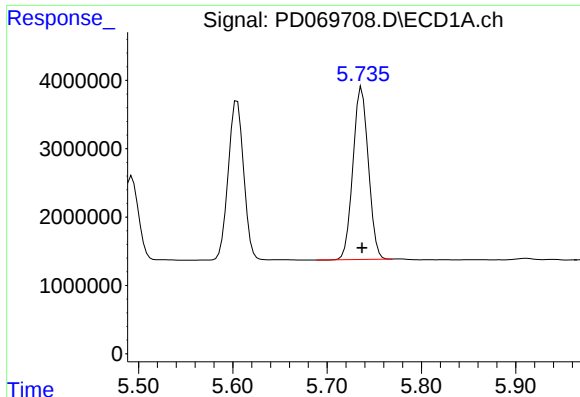

#13 Dieldrin


R.T.: 5.737 min
Delta R.T.: 0.000 min
Response: 28697479
Conc: 23.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

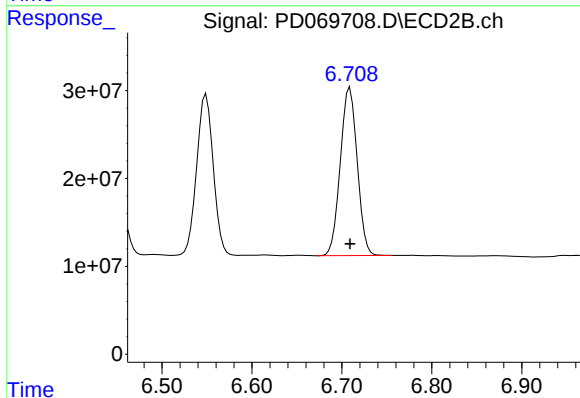


#13 Dieldrin

R.T.: 6.709 min
Delta R.T.: 0.000 min
Response: 249527367
Conc: 24.37 ng/ml

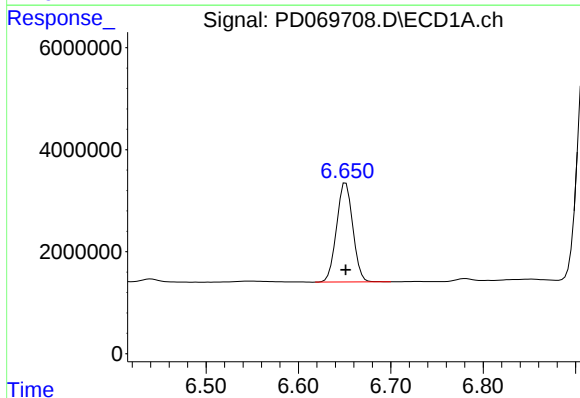


#19 Endosulfan Sulfate

R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 23750472
Conc: 21.59 ng/ml

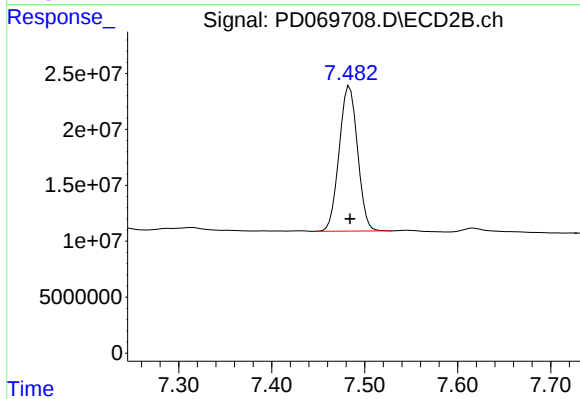

#19 Endosulfan Sulfate


R.T.: 7.484 min
Delta R.T.: 0.000 min
Response: 178123808
Conc: 22.30 ng/ml

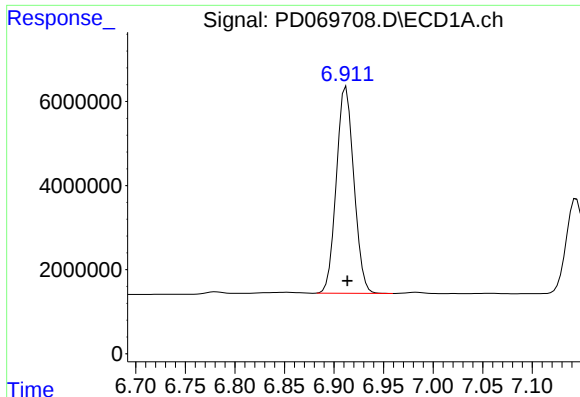

#20 Methoxychlor


R.T.: 6.912 min
Delta R.T.: -0.001 min
Response: 60436748
Conc: 104.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

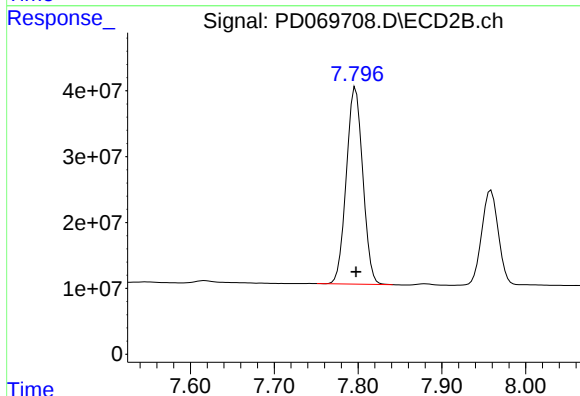


#20 Methoxychlor

R.T.: 7.797 min
Delta R.T.: 0.000 min
Response: 408437894
Conc: 99.05 ng/ml

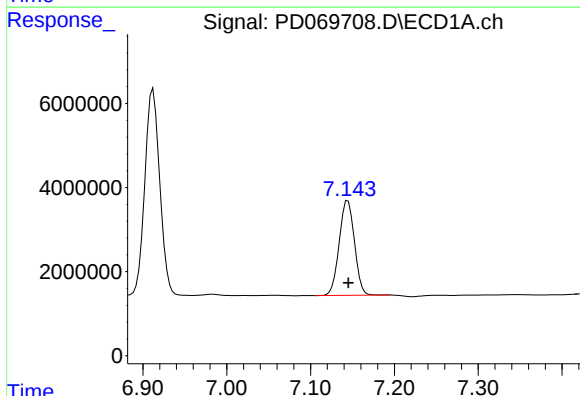


#21 Endrin ketone

R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 28561379
Conc: 22.80 ng/ml

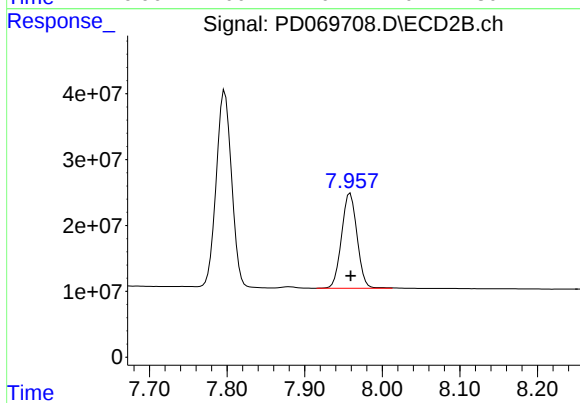

#21 Endrin ketone


R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 200645303
Conc: 24.02 ng/ml

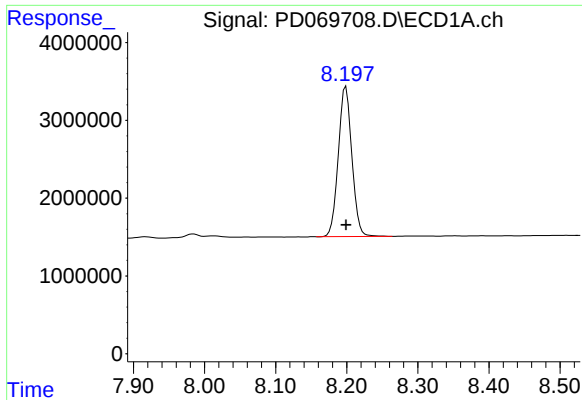

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 25568959
Conc: 23.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

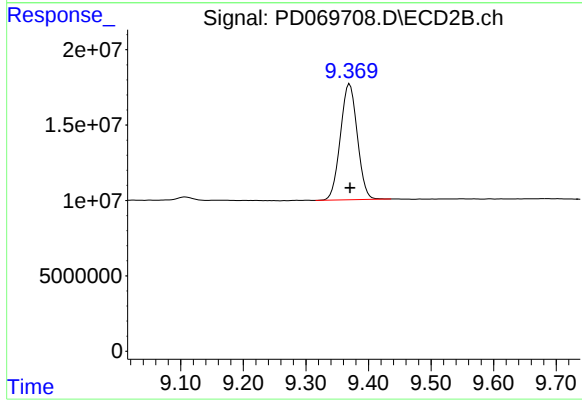

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: 0.000 min
Response: 144803288
Conc: 24.16 ng/ml