

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
 Data File : PD069714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 18:48
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 01:40:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Fri May 20 01:35:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.173	127.0E6	984.1E6	99.786	97.737
28)	SA Decachlor...	8.199	9.370	111.1E6	598.0E6	97.207	96.443
Target Compounds							
23)	Chlordane-1	4.313	5.195	38856545	399.9E6	987.333	963.912
24)	Chlordane-2	4.814	5.669	44349479	377.8E6	961.704	953.862
25)	Chlordane-3	5.381	6.325	131.9E6	1423.9E6	1002.893	978.779
26)	Chlordane-4	5.440	6.402	108.0E6	1648.3E6	988.192	974.654
27)	Chlordane-5	6.278	7.214	44195535	319.4E6	996.311	968.167



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
Data File : PD069714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 18:48
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 01:40:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Fri May 20 01:35:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

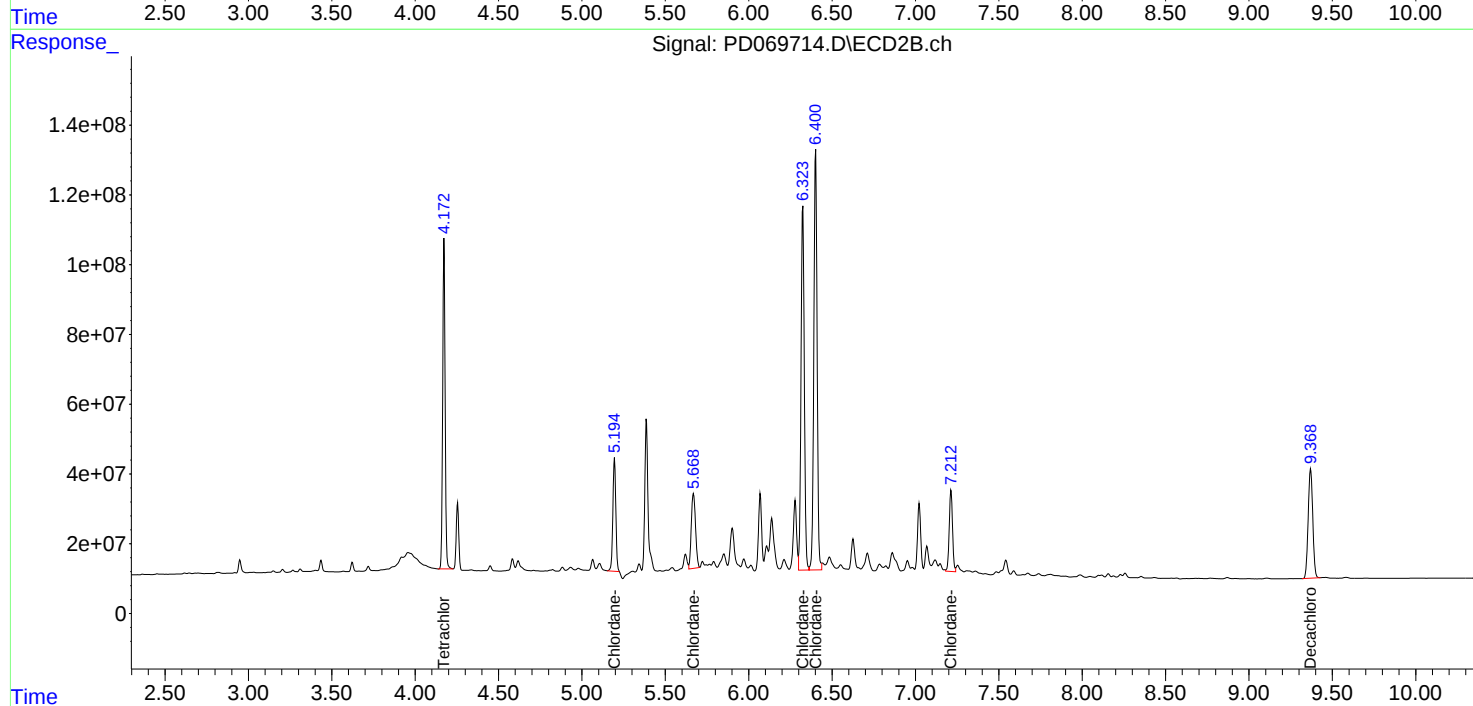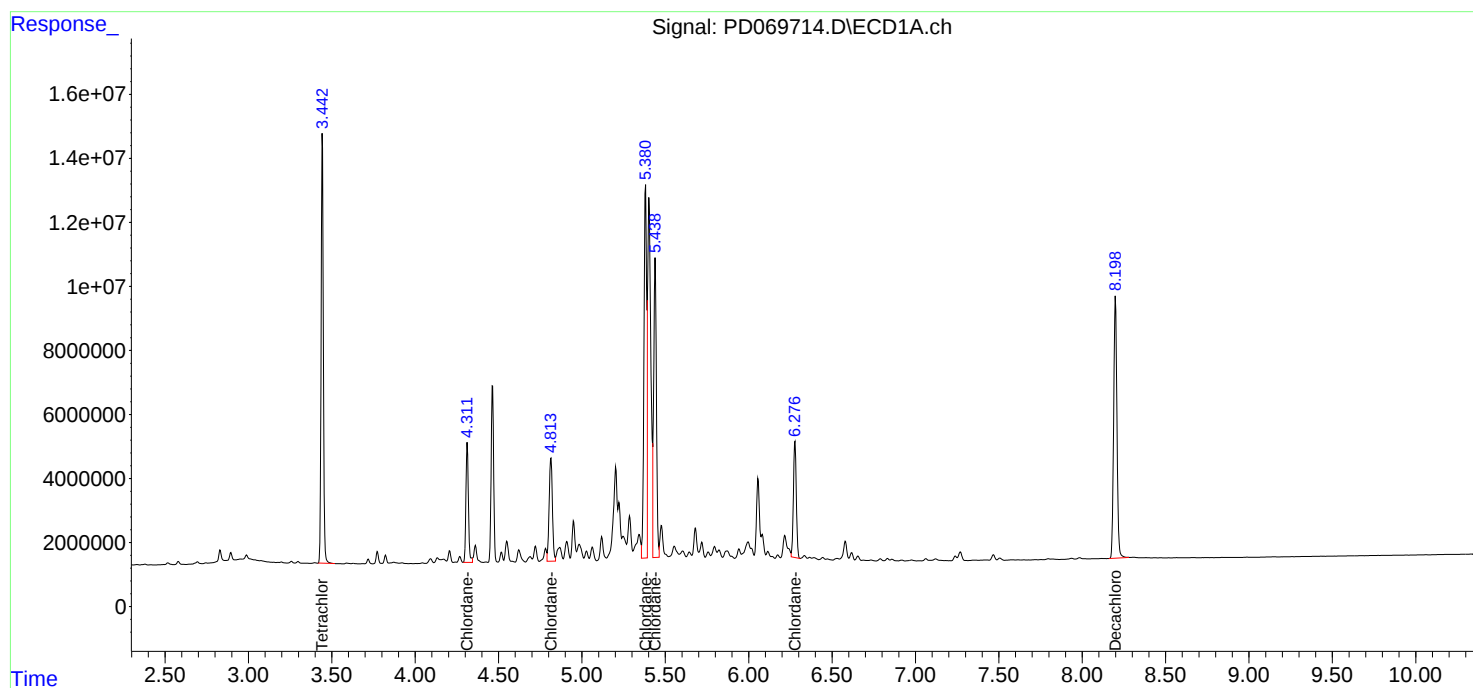


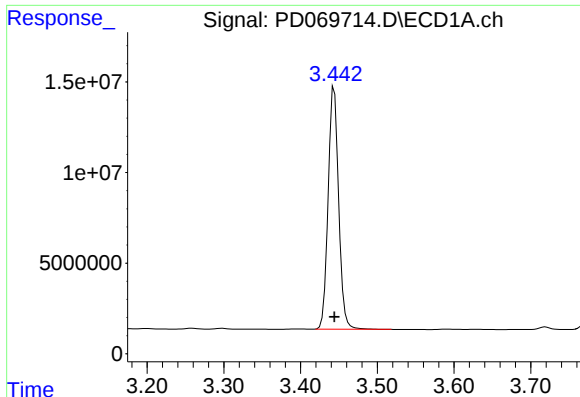

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 127014714
Conc: 99.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

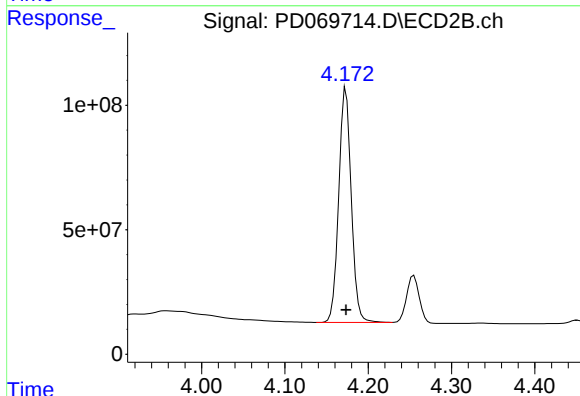


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 984095349
Conc: 97.74 ng/ml

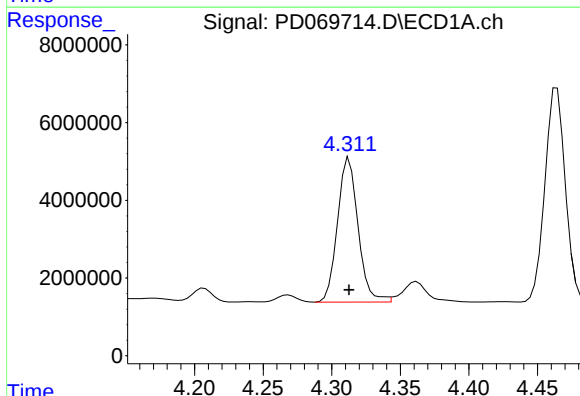


#23 Chlordane-1

R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 38856545
Conc: 987.33 ng/ml

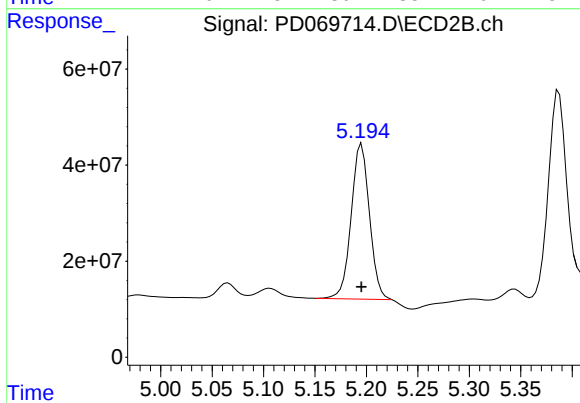

#23 Chlordane-1


R.T.: 5.195 min
Delta R.T.: 0.000 min
Response: 399929437
Conc: 963.91 ng/ml

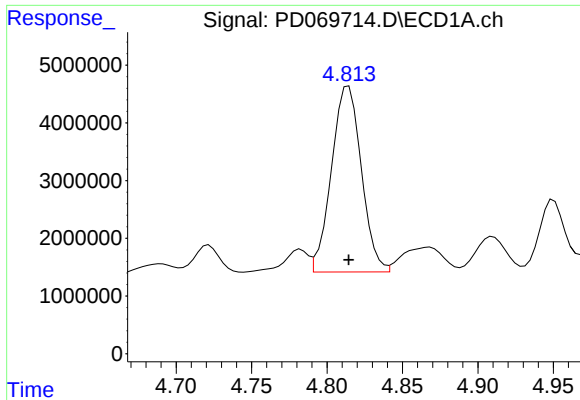

#24 Chlordane-2


R.T.: 4.814 min
Delta R.T.: 0.000 min
Response: 44349479
Conc: 961.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

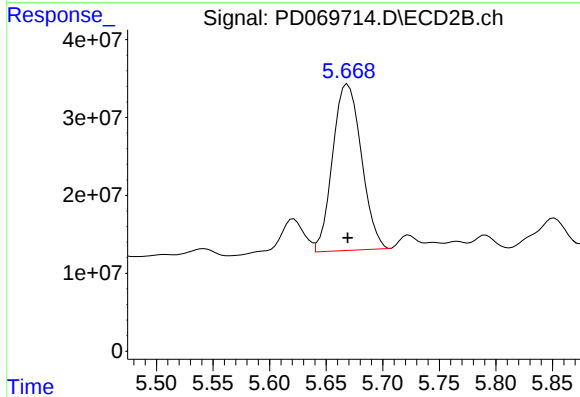


#24 Chlordane-2

R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 377809973
Conc: 953.86 ng/ml

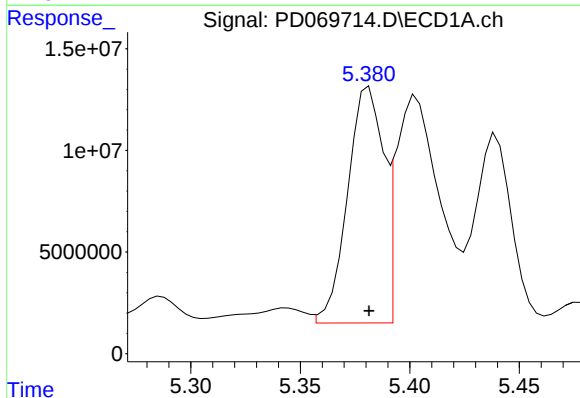


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 131932193
Conc: 1002.89 ng/ml

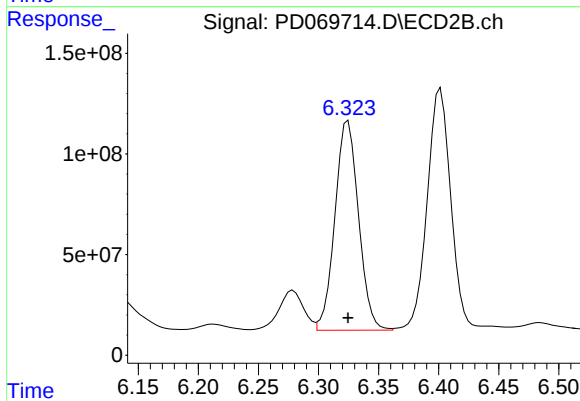

#25 Chlordane-3


R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 1423900398
Conc: 978.78 ng/ml

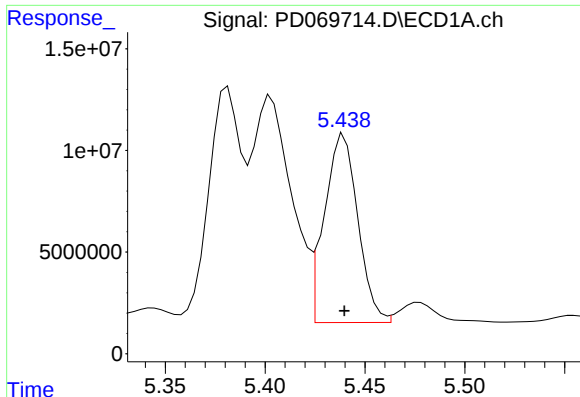

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 107966303
Conc: 988.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

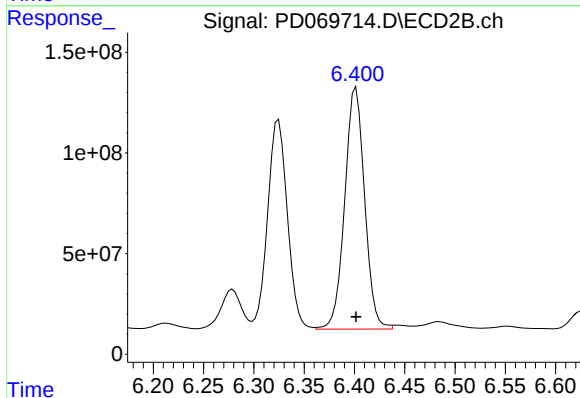


#26 Chlordane-4

R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 1648312860
Conc: 974.65 ng/ml

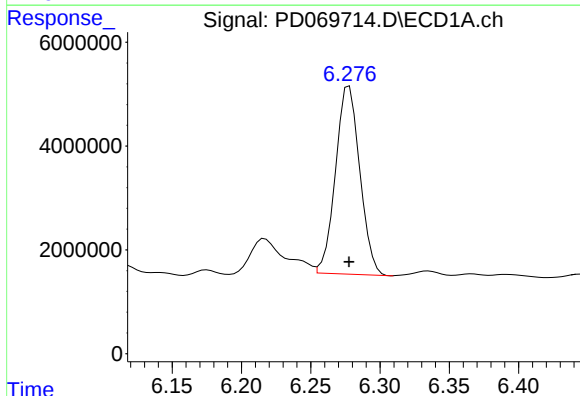


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 44195535
Conc: 996.31 ng/ml

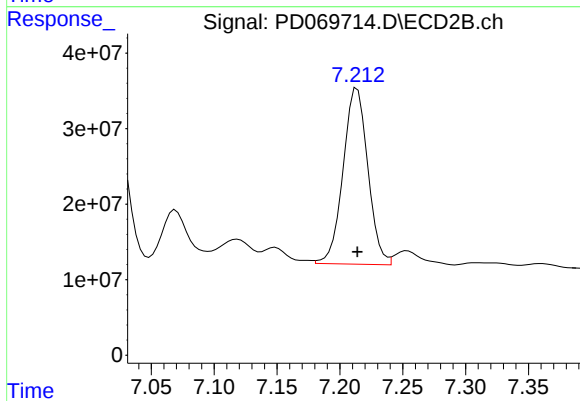

#27 Chlordane-5


R.T.: 7.214 min
Delta R.T.: 0.000 min
Response: 319448287
Conc: 968.17 ng/ml

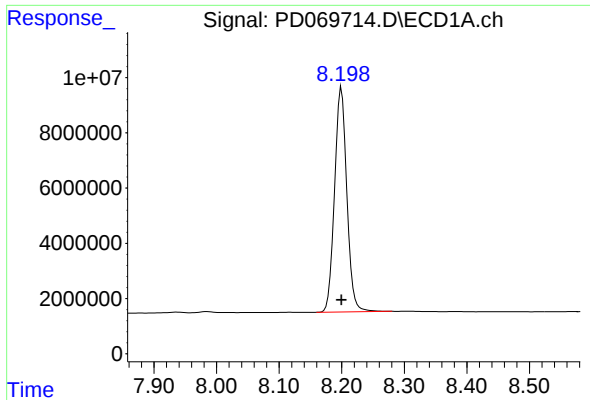

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 111107917
Conc: 97.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

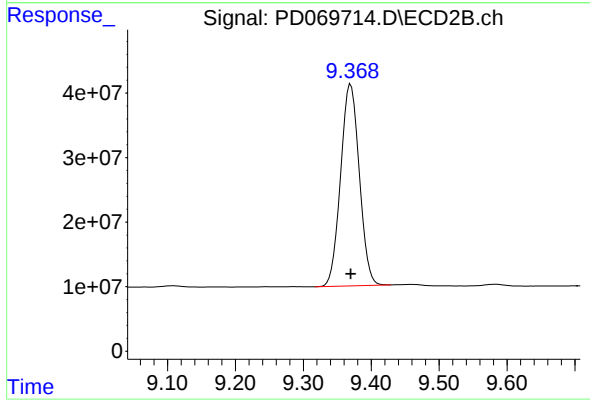

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: 0.000 min
Response: 597960617
Conc: 96.44 ng/ml