

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
 Data File : PD069715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 19:02
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 01:46:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Fri May 20 01:35:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.173	91791537	725.3E6	73.051	72.993
28)	SA Decachlor...	8.199	9.372	81720597	445.2E6	72.627	72.837
Target Compounds							
23)	Chlordane-1	4.312	5.195	28488368	294.7E6	732.383	722.983
24)	Chlordane-2	4.814	5.669	32995066	283.3E6	726.633	726.526
25)	Chlordane-3	5.382	6.325	95258557	1046.2E6	732.543	729.132
26)	Chlordane-4	5.440	6.402	77868653	1231.3E6	724.724	735.256
27)	Chlordane-5	6.277	7.214	31791270	236.8E6	727.452	728.156



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
Data File : PD069715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 19:02
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 01:46:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Fri May 20 01:35:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

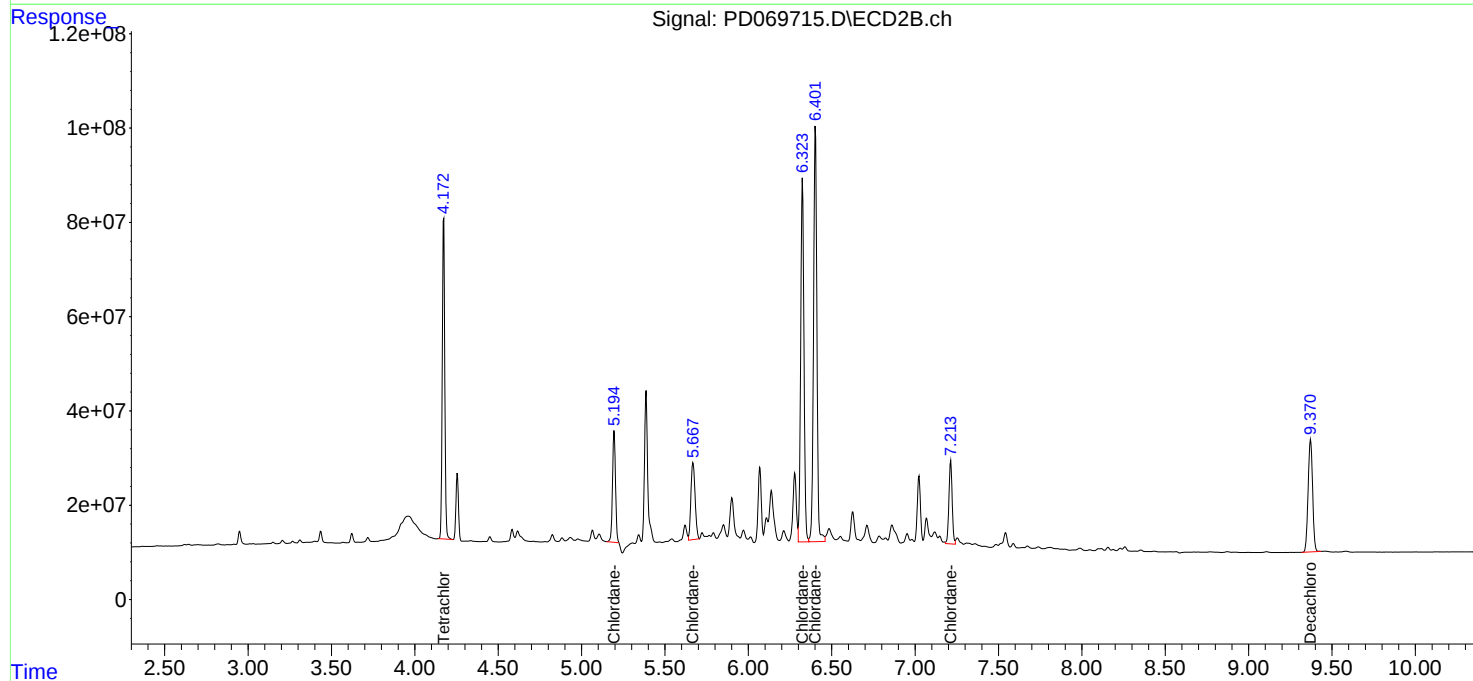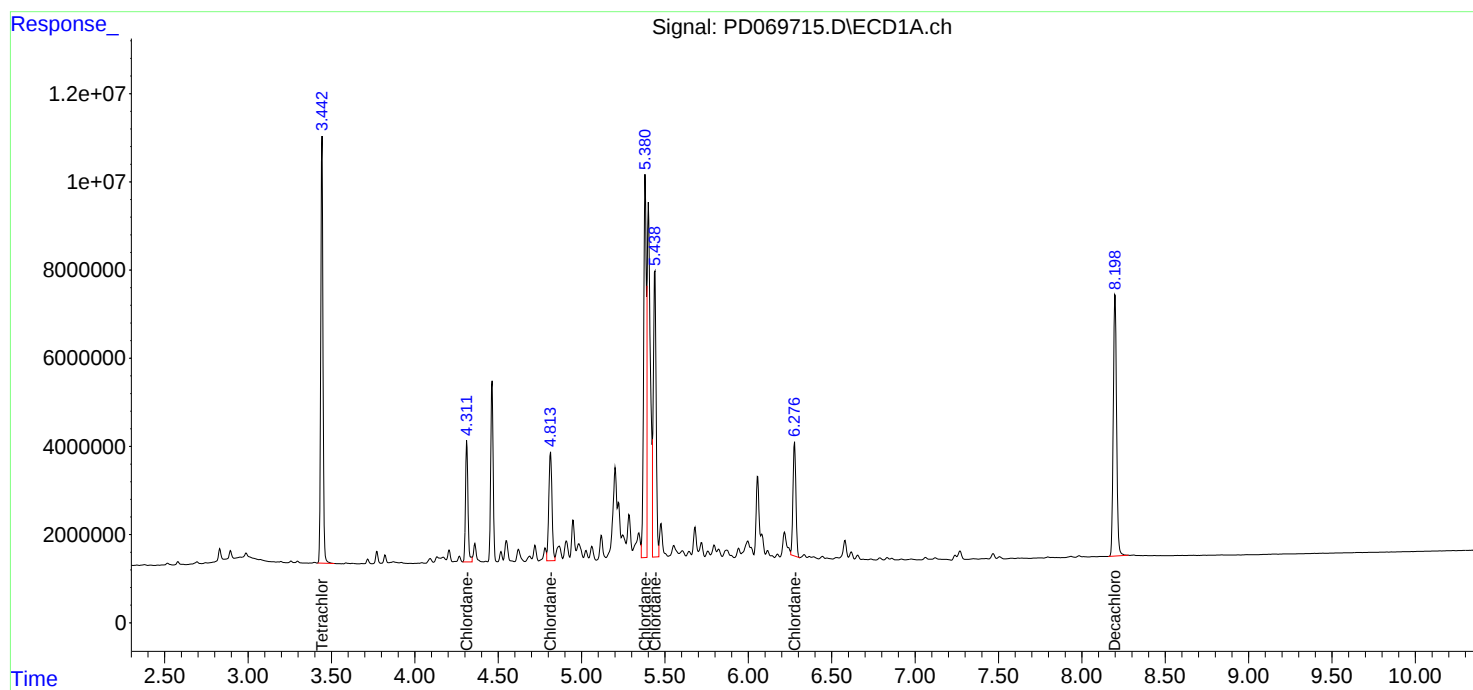


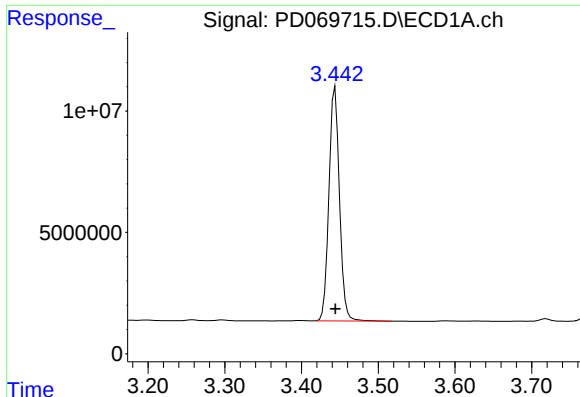

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 91791537
Conc: 73.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

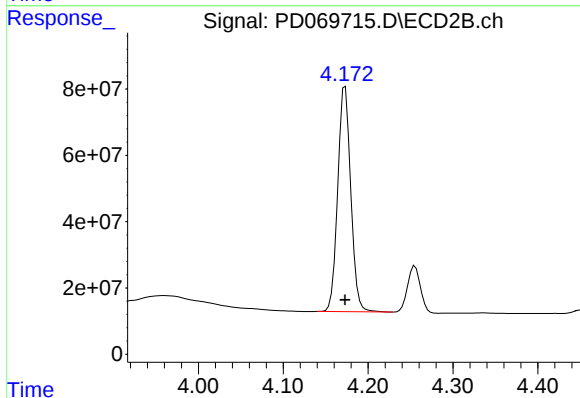


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 725254364
Conc: 72.99 ng/ml

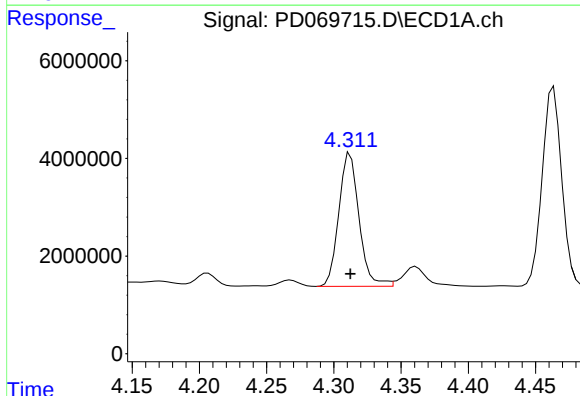


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 28488368
Conc: 732.38 ng/ml

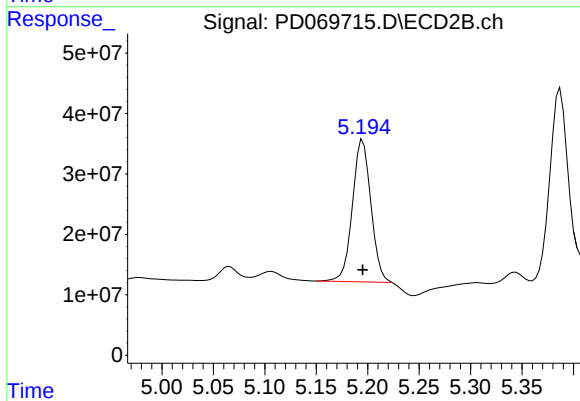

#23 Chlordane-1


R.T.: 5.195 min
Delta R.T.: 0.000 min
Response: 294659974
Conc: 722.98 ng/ml

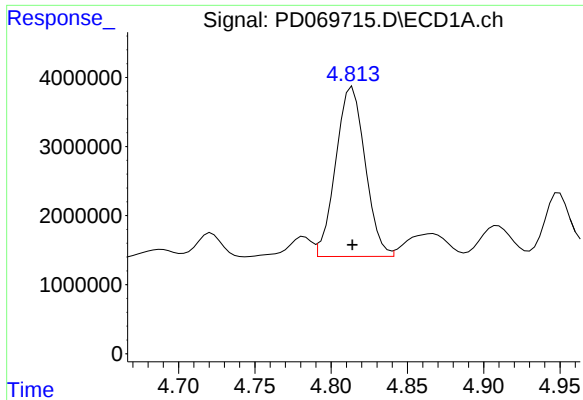

#24 Chlordane-2


R.T.: 4.814 min
Delta R.T.: 0.000 min
Response: 32995066
Conc: 726.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

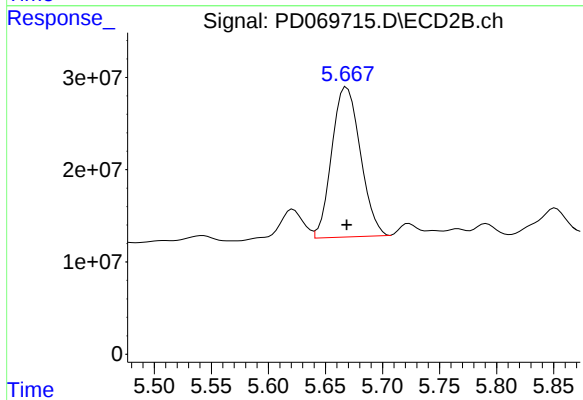


#24 Chlordane-2

R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 283331631
Conc: 726.53 ng/ml

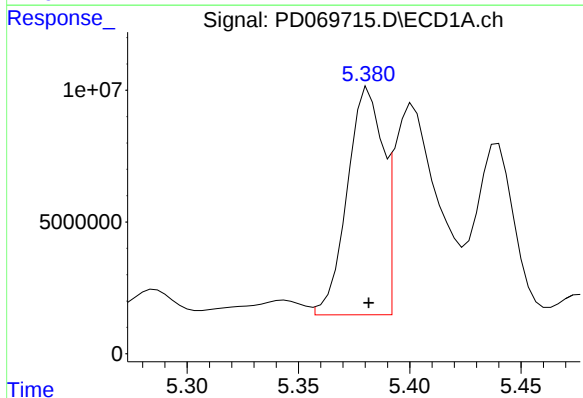


#25 Chlordane-3

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 95258557
Conc: 732.54 ng/ml

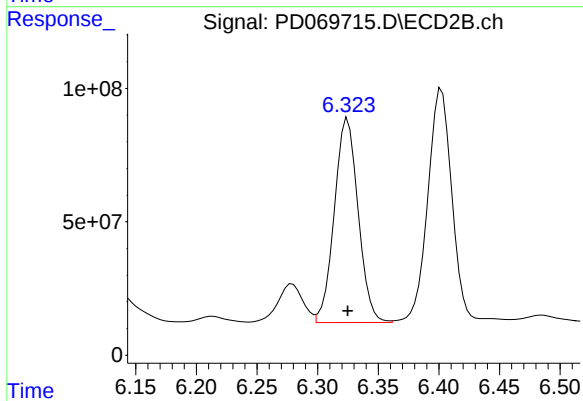

#25 Chlordane-3


R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 1046165175
Conc: 729.13 ng/ml

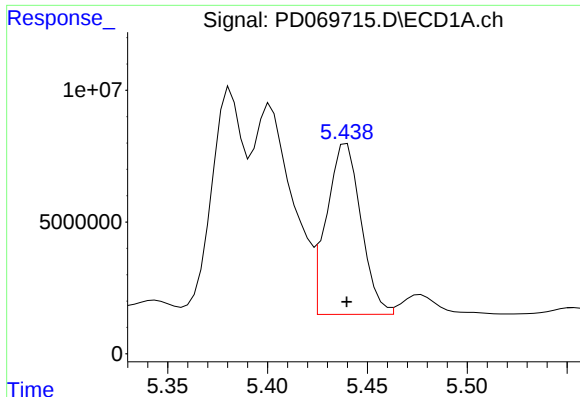

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 77868653
Conc: 724.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

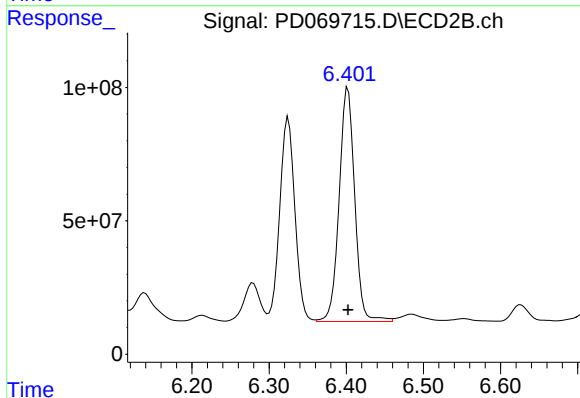


#26 Chlordane-4

R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 1231346152
Conc: 735.26 ng/ml

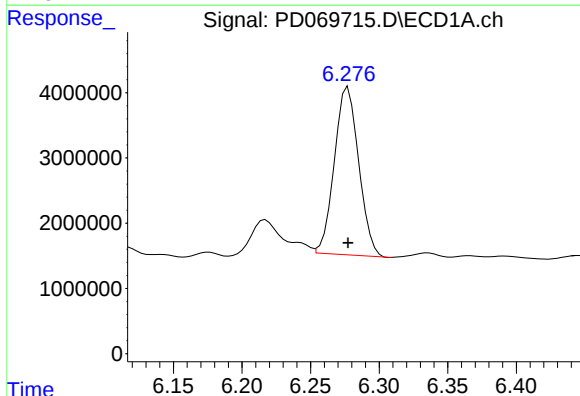


#27 Chlordane-5

R.T.: 6.277 min
Delta R.T.: 0.000 min
Response: 31791270
Conc: 727.45 ng/ml

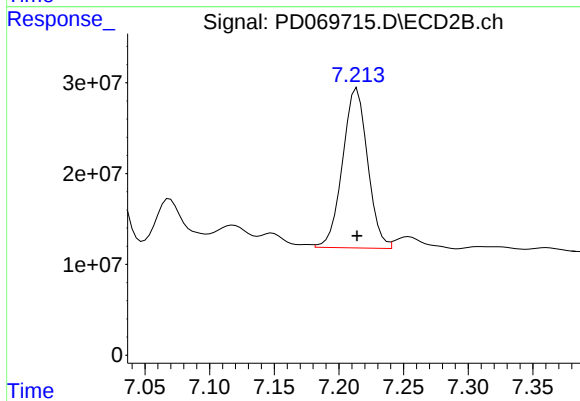

#27 Chlordane-5


R.T.: 7.214 min
Delta R.T.: 0.000 min
Response: 236807437
Conc: 728.16 ng/ml

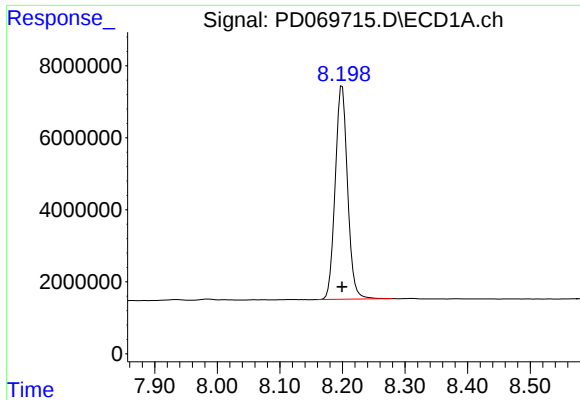

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 81720597
Conc: 72.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

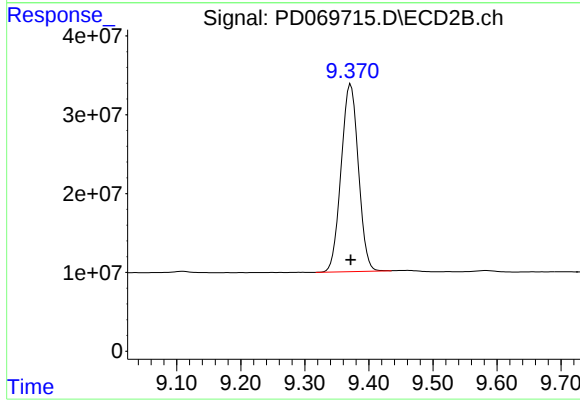

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 445176494
Conc: 72.84 ng/ml