

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
 Data File : PD069716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 19:16
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 01:36:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Fri May 20 01:35:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.172	63779395	514.8E6	50.000	50.000
28)	SA Decachlor...	8.200	9.370	58746442	321.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.313	5.195	19926774	214.9E6	500.000	500.000
24)	Chlordane-2	4.814	5.669	23940776	207.2E6	500.000	500.000
25)	Chlordane-3	5.382	6.325	65585558	742.8E6	500.000	500.000
26)	Chlordane-4	5.440	6.402	55273292	867.0E6	500.000	500.000
27)	Chlordane-5	6.277	7.213	22261413	170.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
Data File : PD069716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 19:16
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 01:36:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Fri May 20 01:35:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

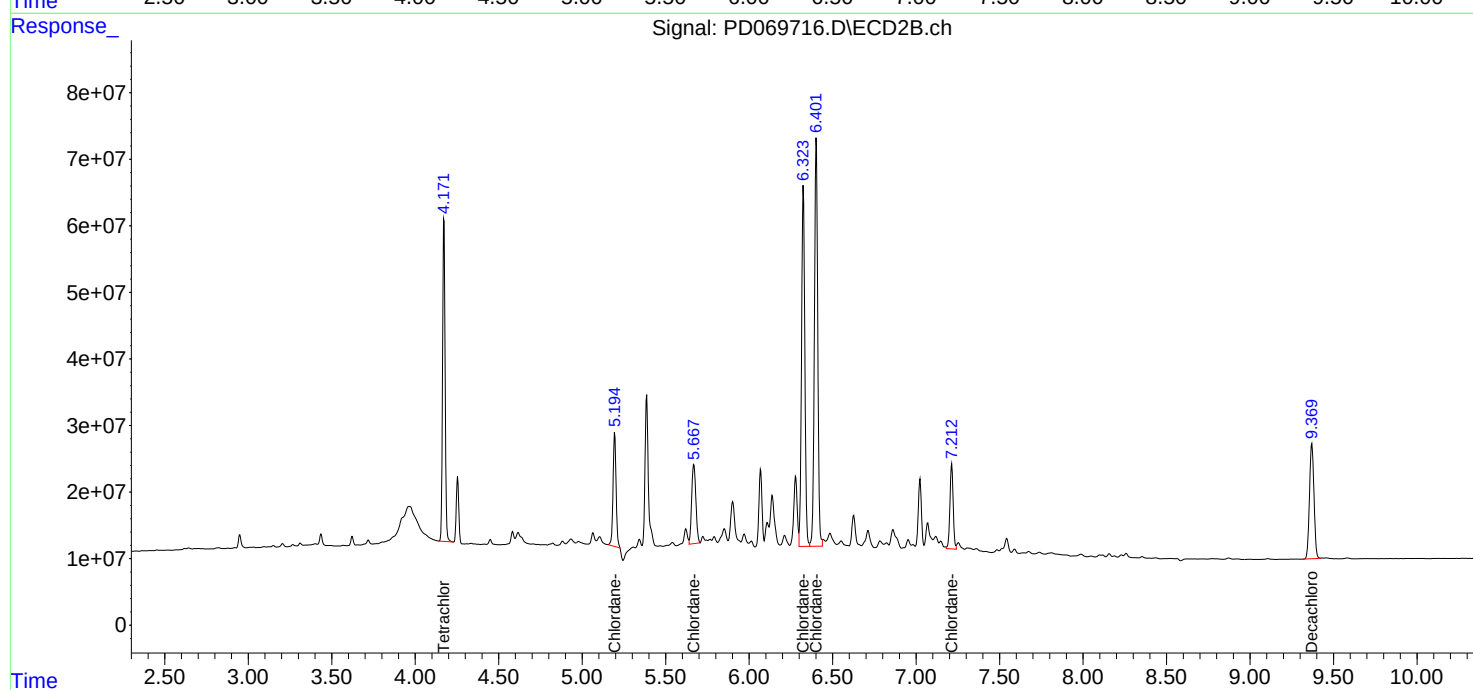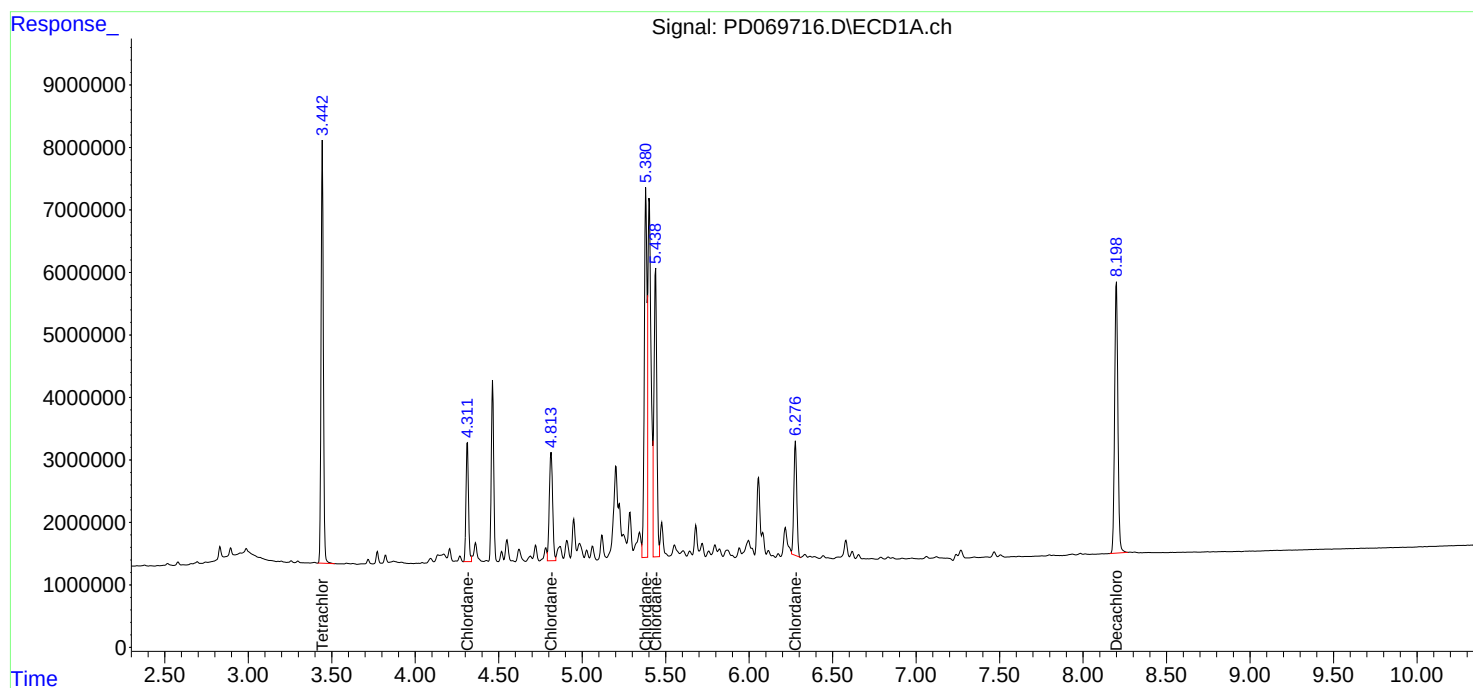


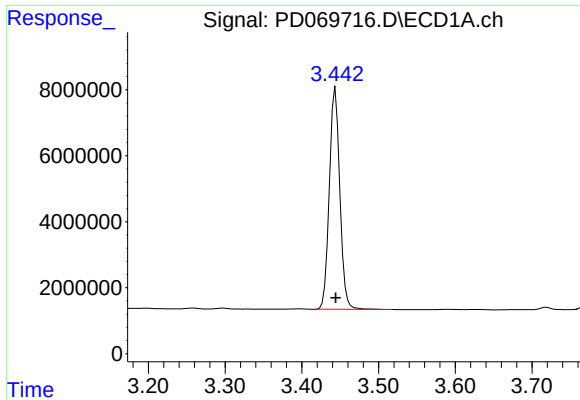

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 63779395
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

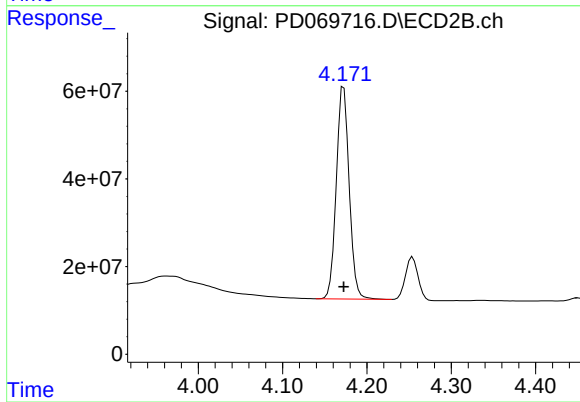


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 514832906
Conc: 50.00 ng/ml

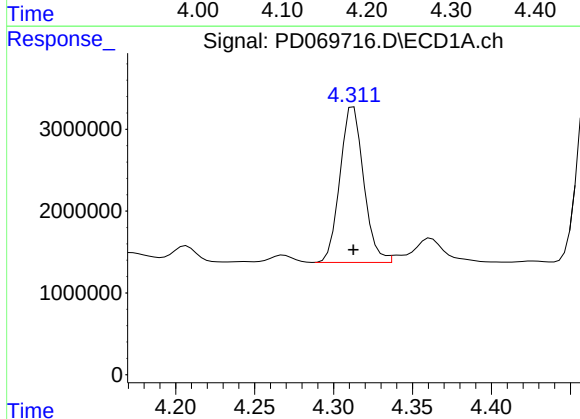


#23 Chlordane-1

R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 19926774
Conc: 500.00 ng/ml

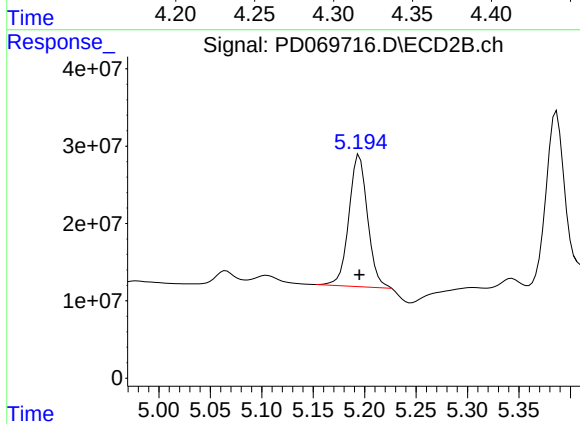

#23 Chlordane-1


R.T.: 5.195 min
Delta R.T.: 0.000 min
Response: 214937560
Conc: 500.00 ng/ml

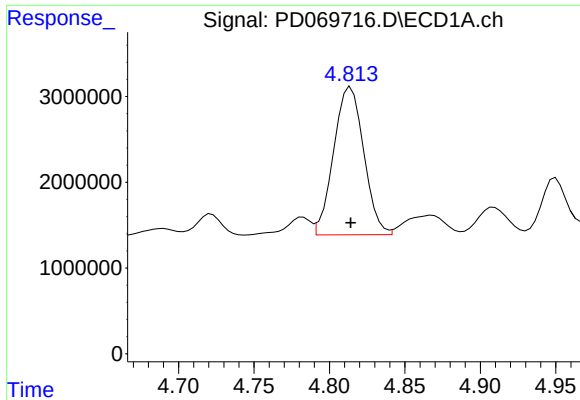

#24 Chlordane-2


R.T.: 4.814 min
Delta R.T.: 0.000 min
Response: 23940776
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

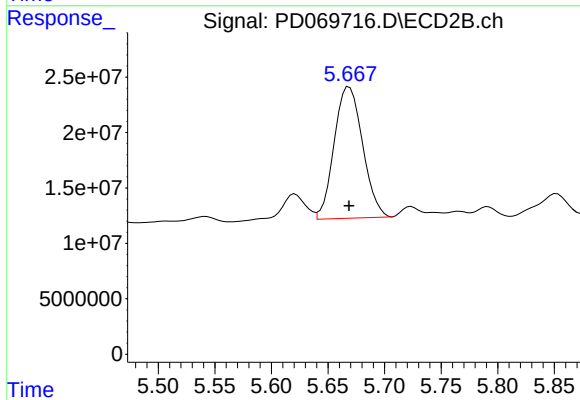


#24 Chlordane-2

R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 207179354
Conc: 500.00 ng/ml

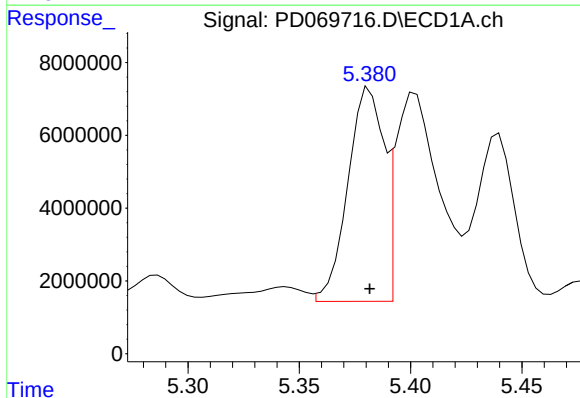


#25 Chlordane-3

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 65585558
Conc: 500.00 ng/ml

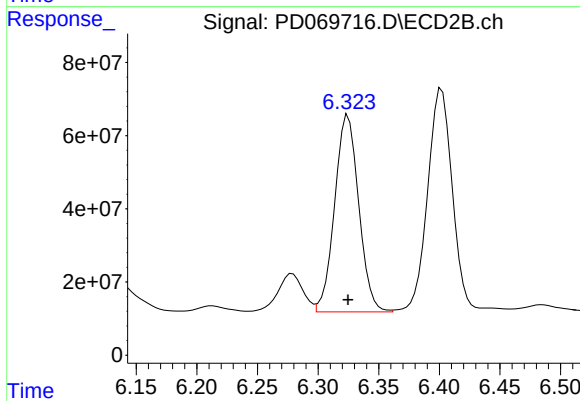

#25 Chlordane-3


R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 742821252
Conc: 500.00 ng/ml

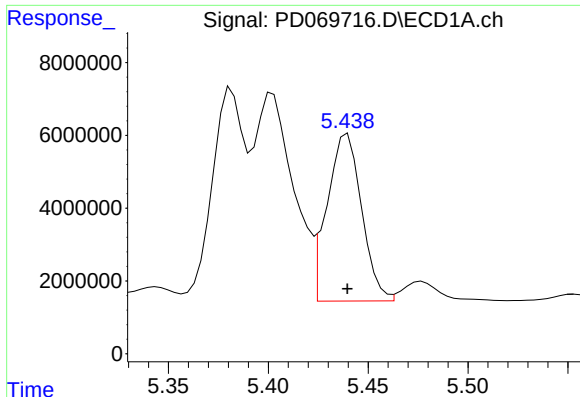

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 55273292
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

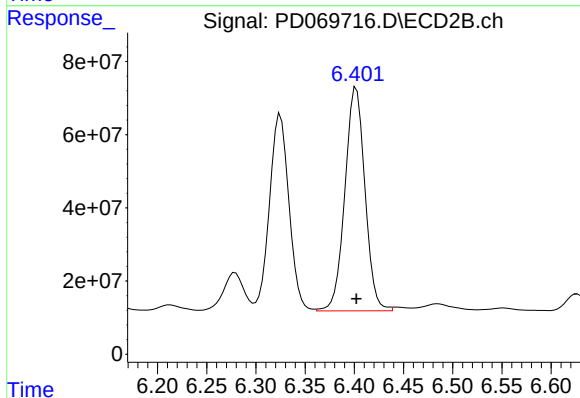


#26 Chlordane-4

R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 867021738
Conc: 500.00 ng/ml

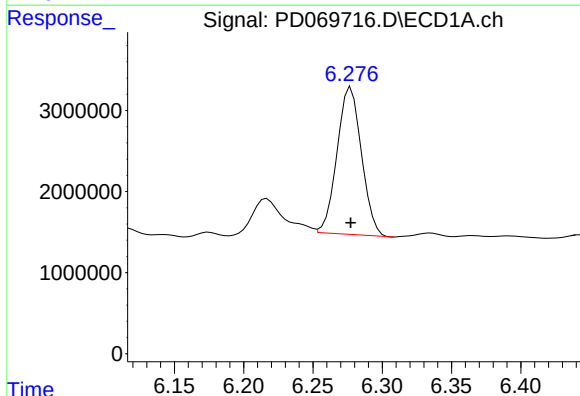


#27 Chlordane-5

R.T.: 6.277 min
Delta R.T.: 0.000 min
Response: 22261413
Conc: 500.00 ng/ml

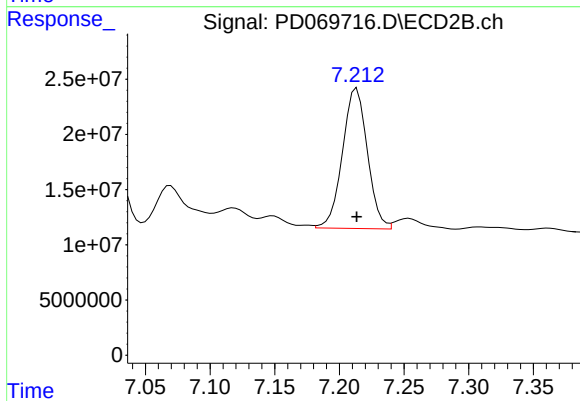

#27 Chlordane-5


R.T.: 7.213 min
Delta R.T.: 0.000 min
Response: 170227432
Conc: 500.00 ng/ml

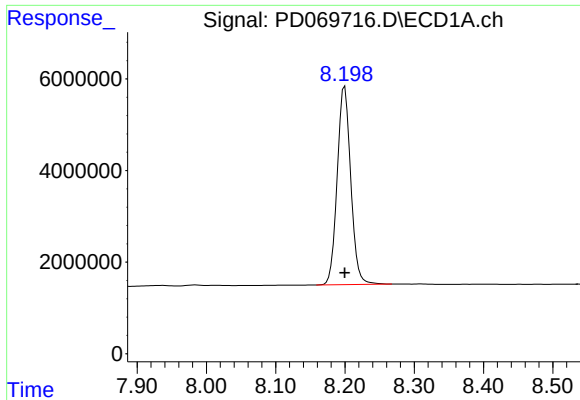

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: 0.000 min
Response: 58746442
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

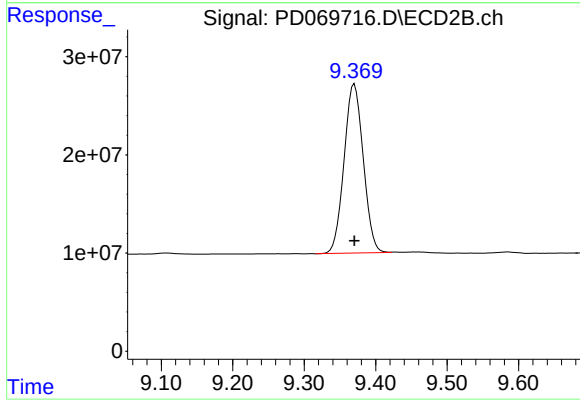

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: 0.000 min
Response: 321032501
Conc: 50.00 ng/ml