

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
 Data File : PD069717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 19:30
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 01:49:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Fri May 20 01:35:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.173	30404859	261.7E6	24.393	25.989
28)	SA Decachlor...	8.199	9.370	29695574	165.2E6	26.029	26.495
Target Compounds							
23)	Chlordane-1	4.313	5.195	10059518	108.2E6	256.403	261.479
24)	Chlordane-2	4.815	5.668	12229077	107.7E6	264.211	269.140
25)	Chlordane-3	5.381	6.325	31347975	374.8E6	243.240	258.320
26)	Chlordane-4	5.440	6.402	26807476	446.5E6	249.623	262.240
27)	Chlordane-5	6.278	7.214	10722367	89786050	246.497	269.064



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052022\
Data File : PD069717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 19:30
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 01:49:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Fri May 20 01:35:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

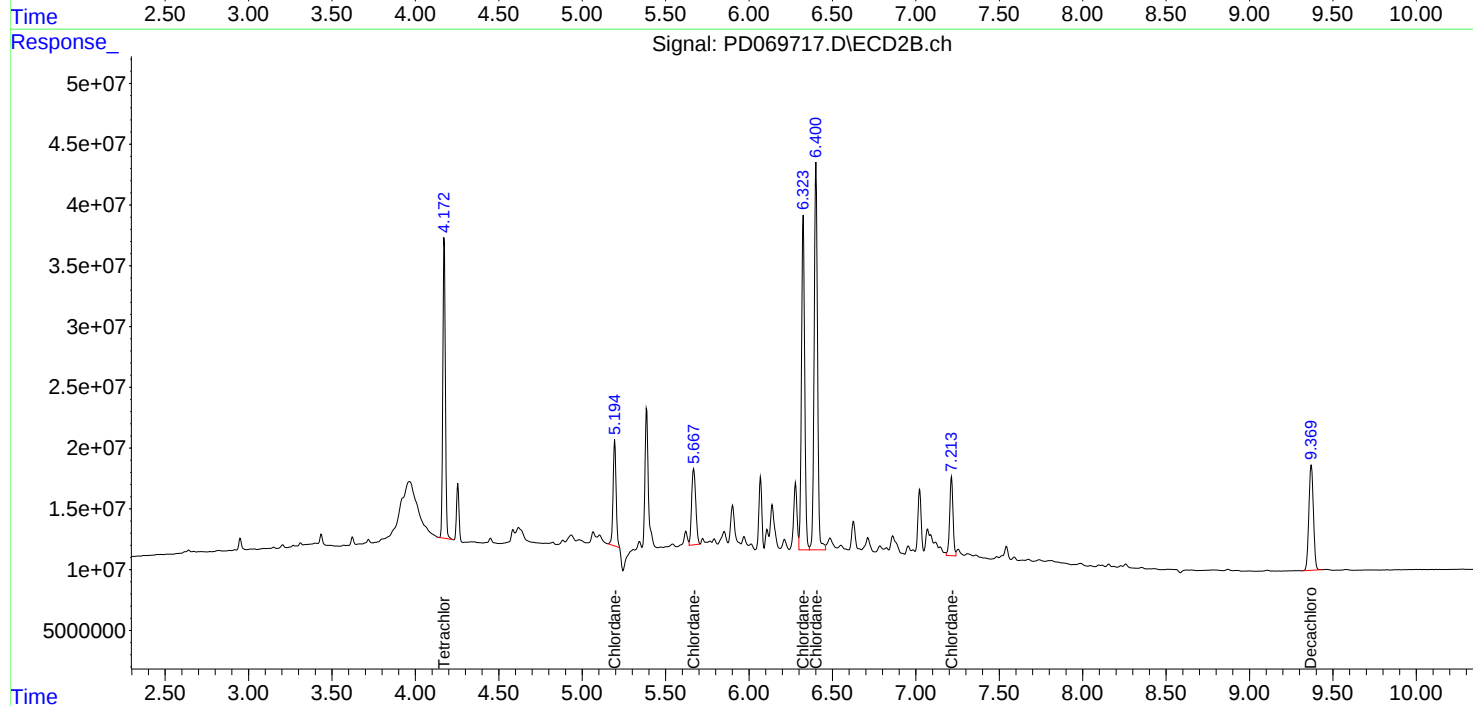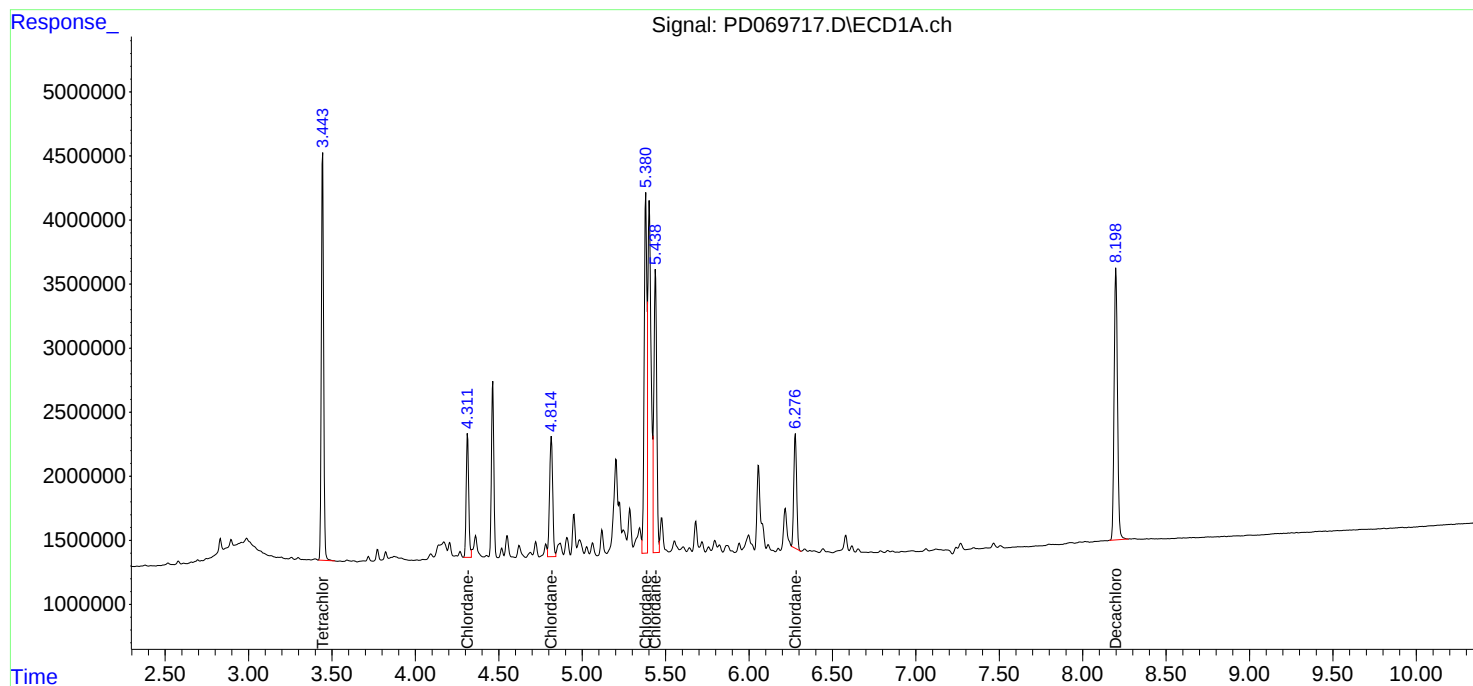


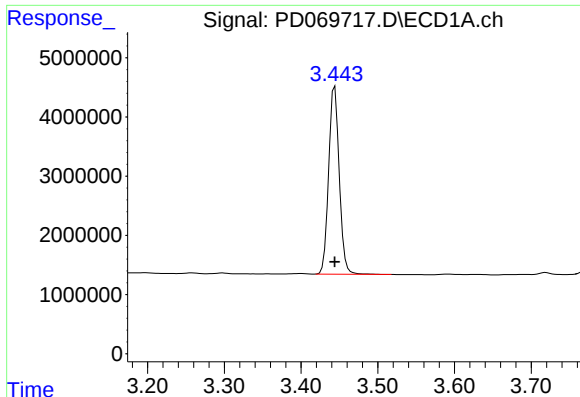

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 30404859
Conc: 24.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

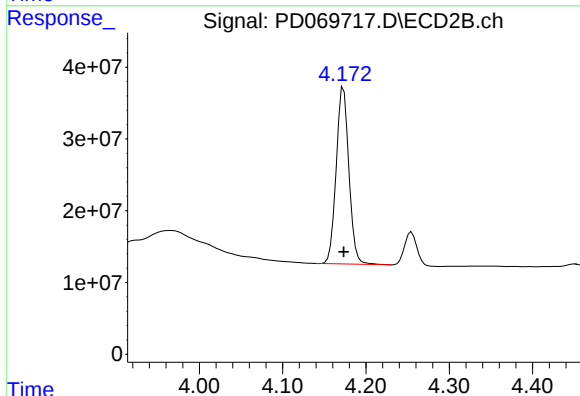


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 261680467
Conc: 25.99 ng/ml

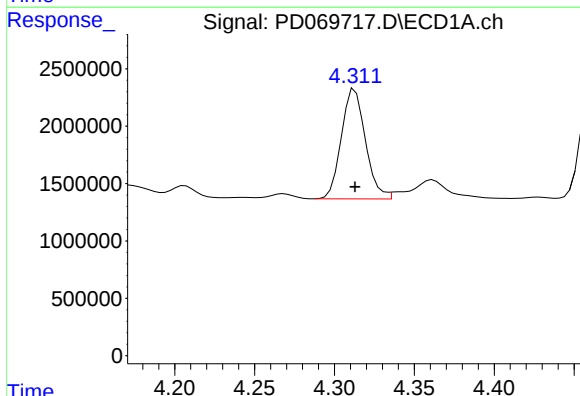


#23 Chlordane-1

R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 10059518
Conc: 256.40 ng/ml

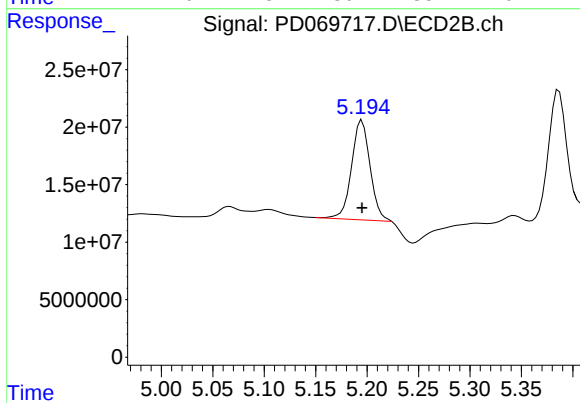

#23 Chlordane-1


R.T.: 5.195 min
Delta R.T.: 0.000 min
Response: 108225149
Conc: 261.48 ng/ml

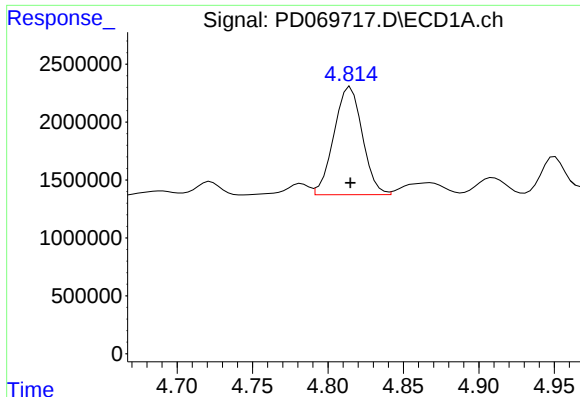

#24 Chlordane-2


R.T.: 4.815 min
Delta R.T.: 0.000 min
Response: 12229077
Conc: 264.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

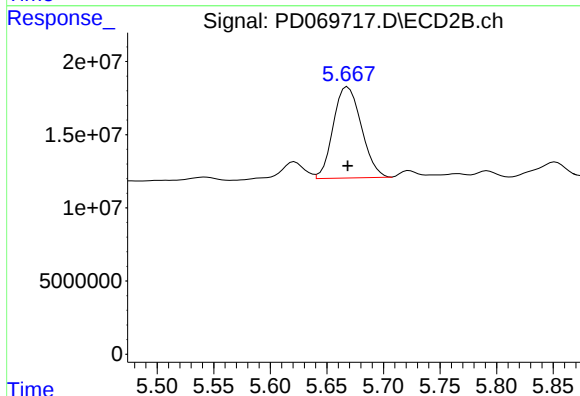


#24 Chlordane-2

R.T.: 5.668 min
Delta R.T.: 0.000 min
Response: 107708317
Conc: 269.14 ng/ml

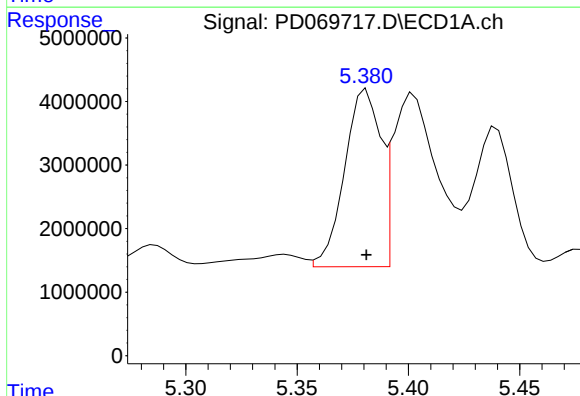


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 31347975
Conc: 243.24 ng/ml

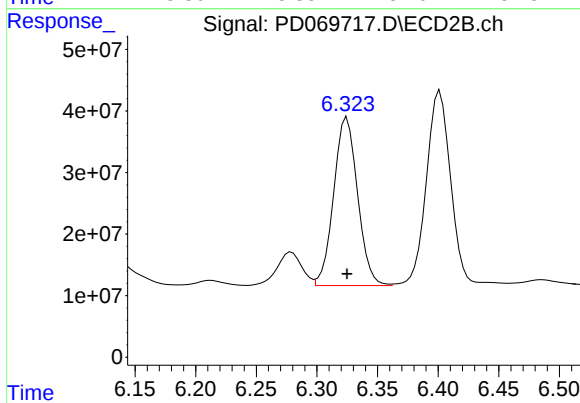

#25 Chlordane-3


R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 374797224
Conc: 258.32 ng/ml

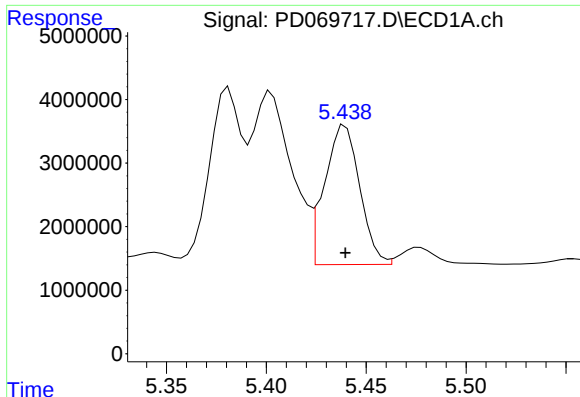

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 26807476
Conc: 249.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

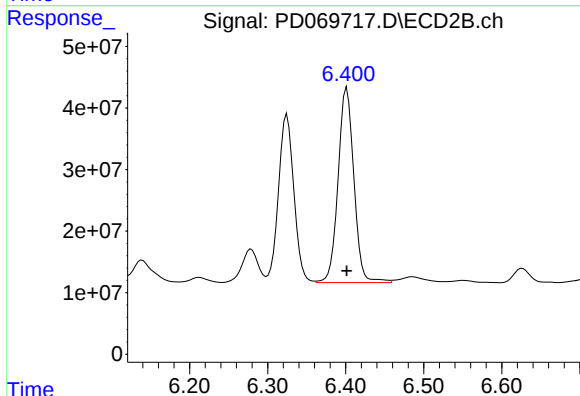


#26 Chlordane-4

R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 446464048
Conc: 262.24 ng/ml

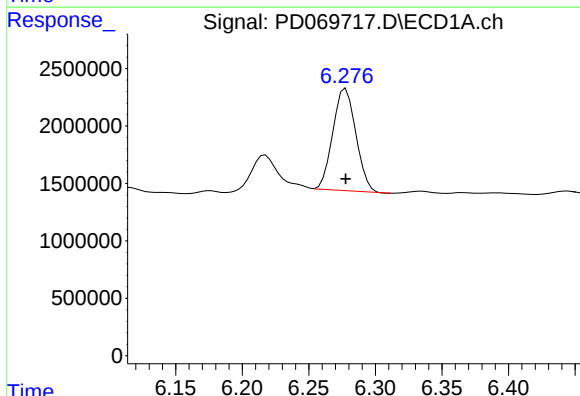


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 10722367
Conc: 246.50 ng/ml

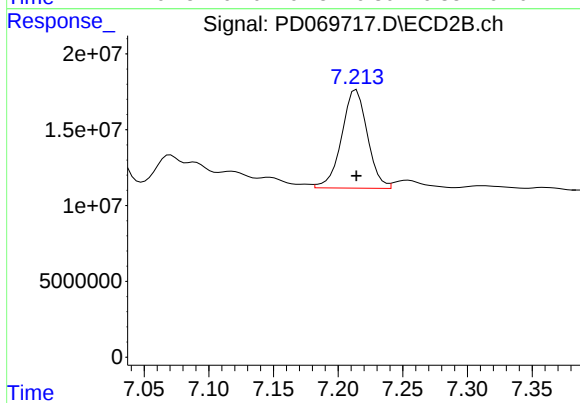

#27 Chlordane-5


R.T.: 7.214 min
Delta R.T.: 0.000 min
Response: 89786050
Conc: 269.06 ng/ml

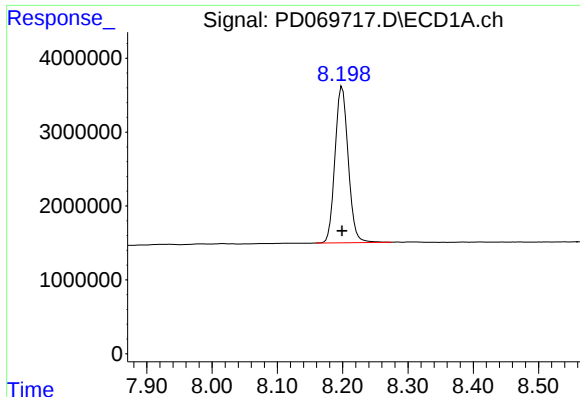

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 29695574
Conc: 26.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

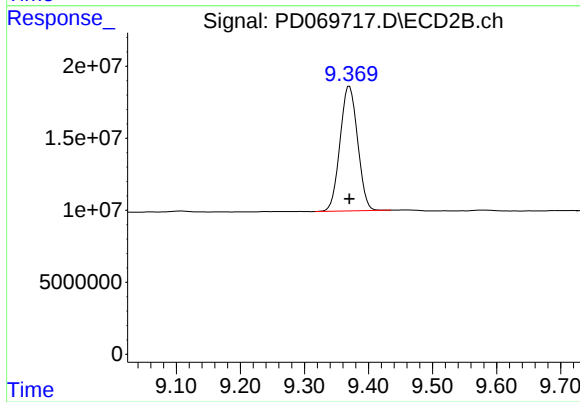

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: 0.000 min
Response: 165227532
Conc: 26.49 ng/ml