

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

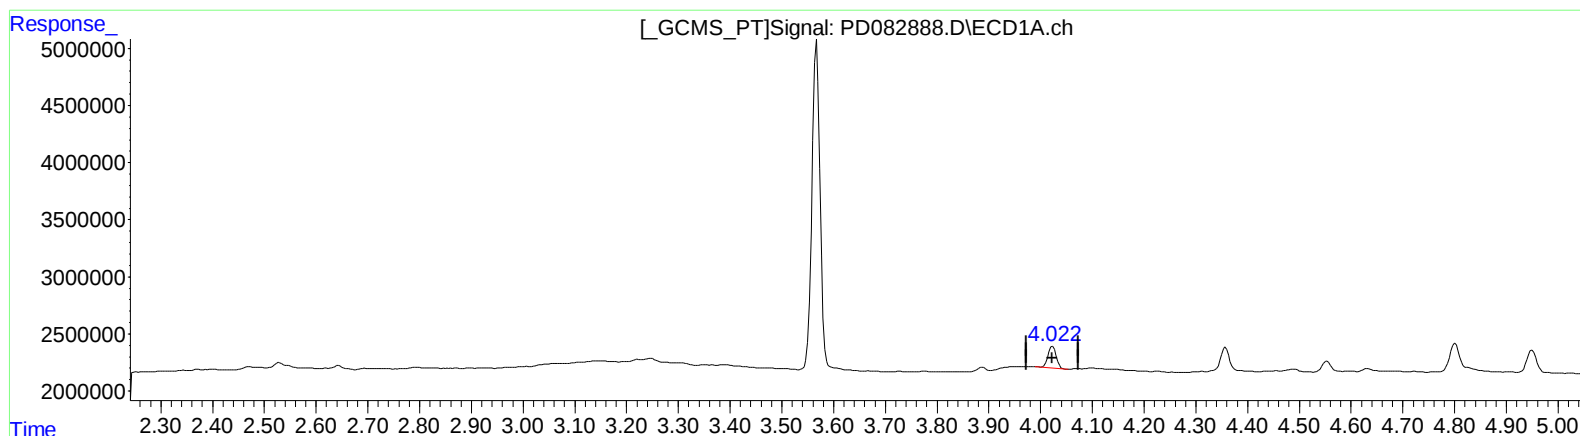

(2) alpha-BHC (A)
4.023min 0.841 ng/ml
response 2146058

(2) alpha-BHC #2 (A)
3.276min 0.866 ng/ml
response 5383651

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

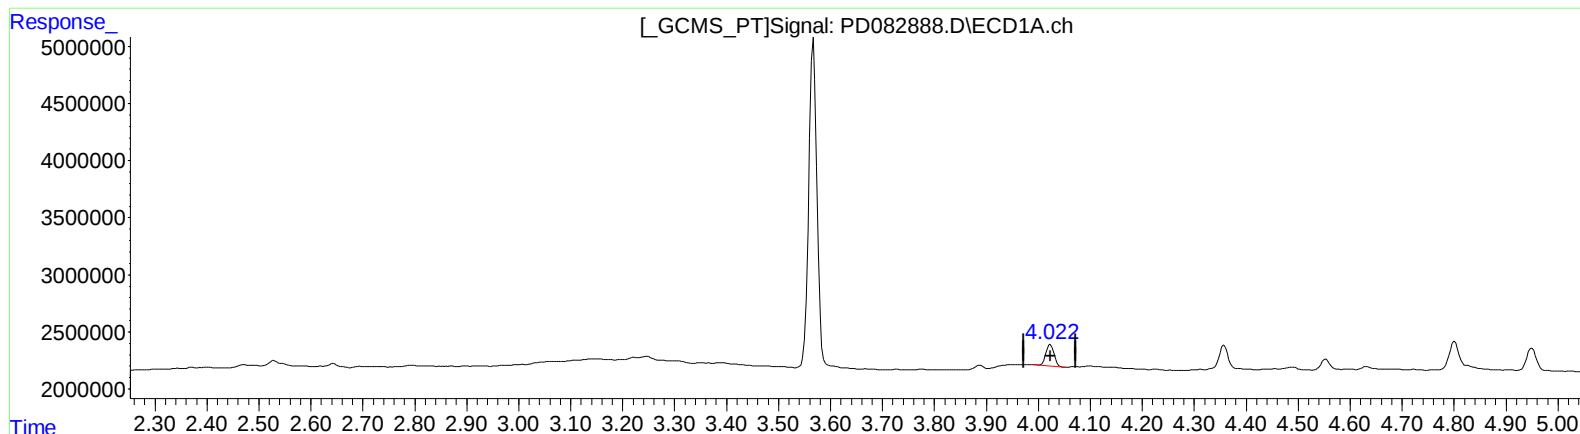

(2) alpha-BHC (A)
4.023min 0.841 ng/ml
response 2146058

(2) alpha-BHC #2 (A)
3.274min 0.774 ng/ml m
response 4810273

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

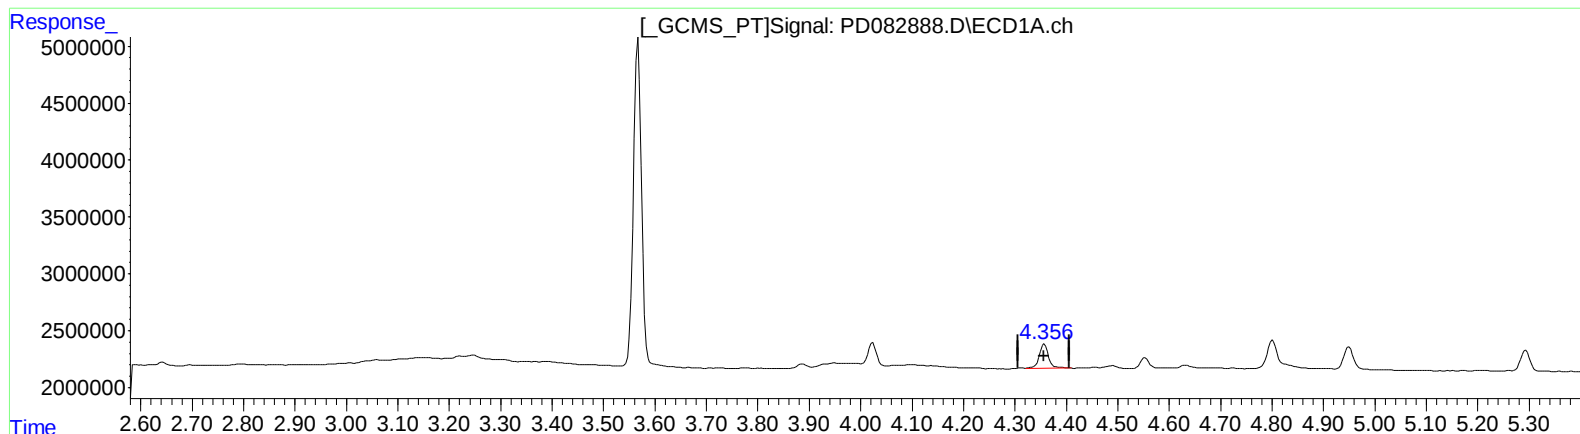

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

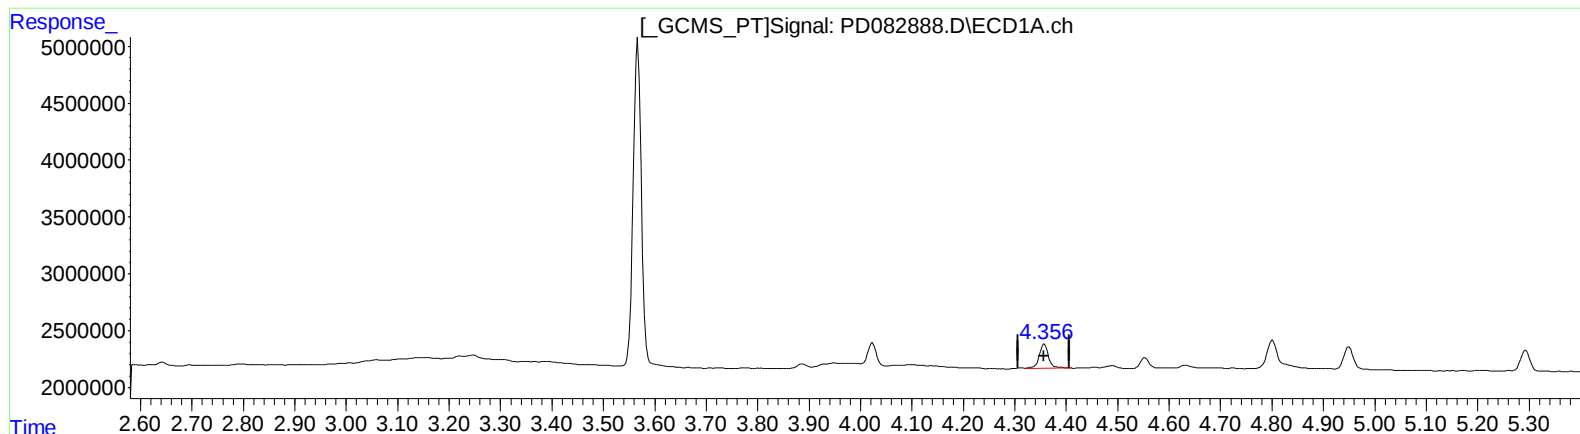

(3) gamma-BHC (Lindane) (MA)

4.357min 1.063 ng/ml

response 2622929

(3) gamma-BHC (Lindane) #2 (MA)

3.603min 0.853 ng/ml m

response 4935788

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

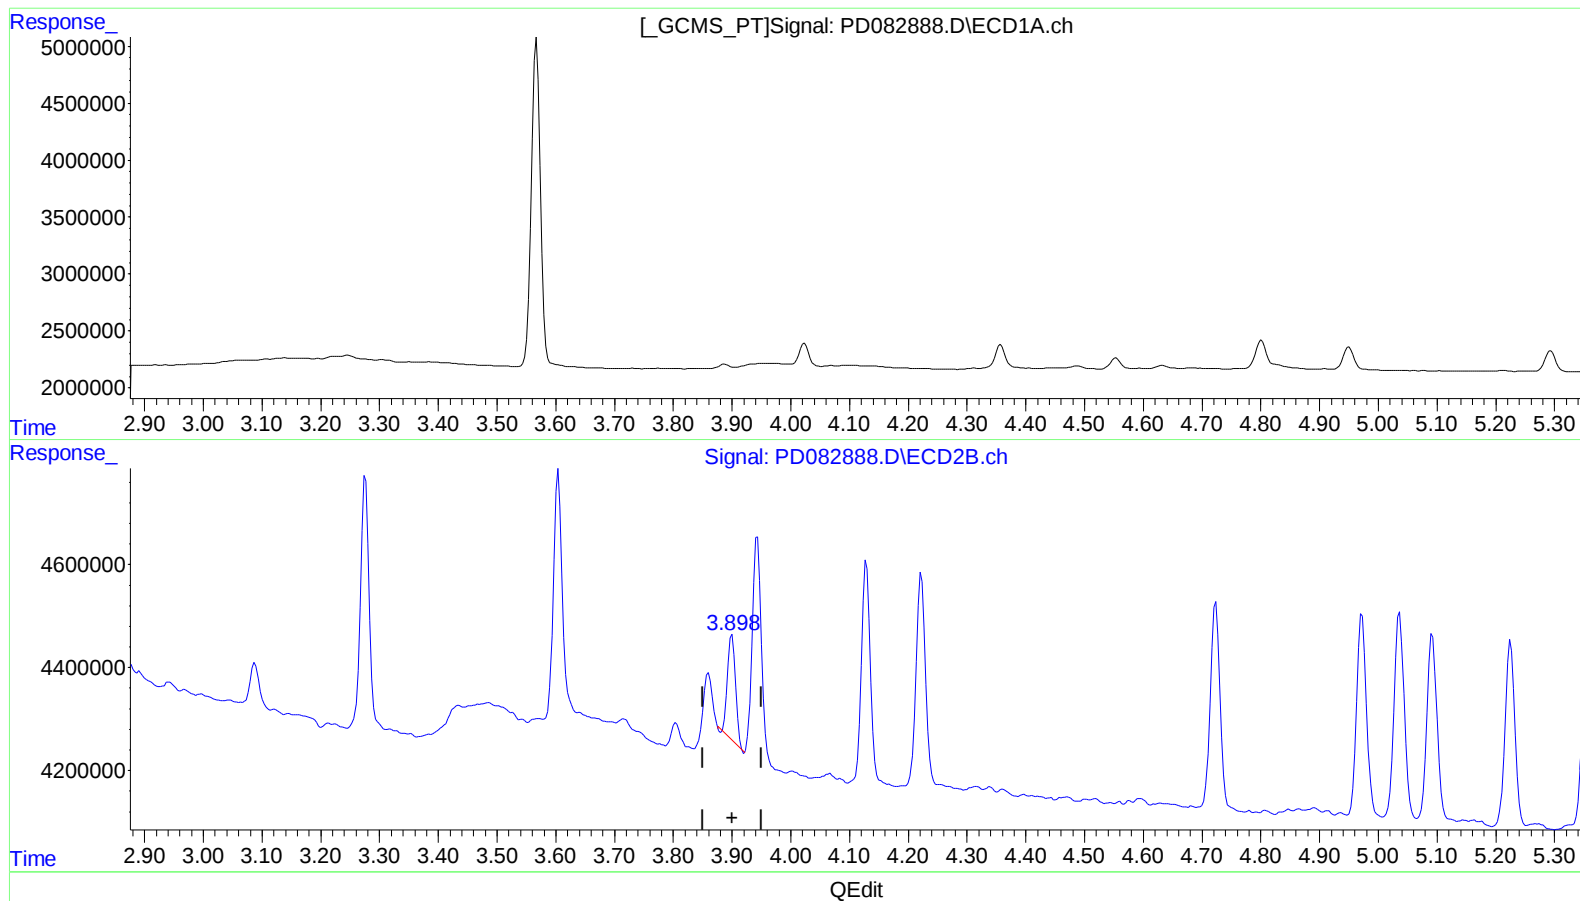

(6) beta-BHC (B)

0.000min 0.000 ng/ml

response 0

(6) beta-BHC #2 (B)

3.900min 0.792 ng/ml

response 1985766

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

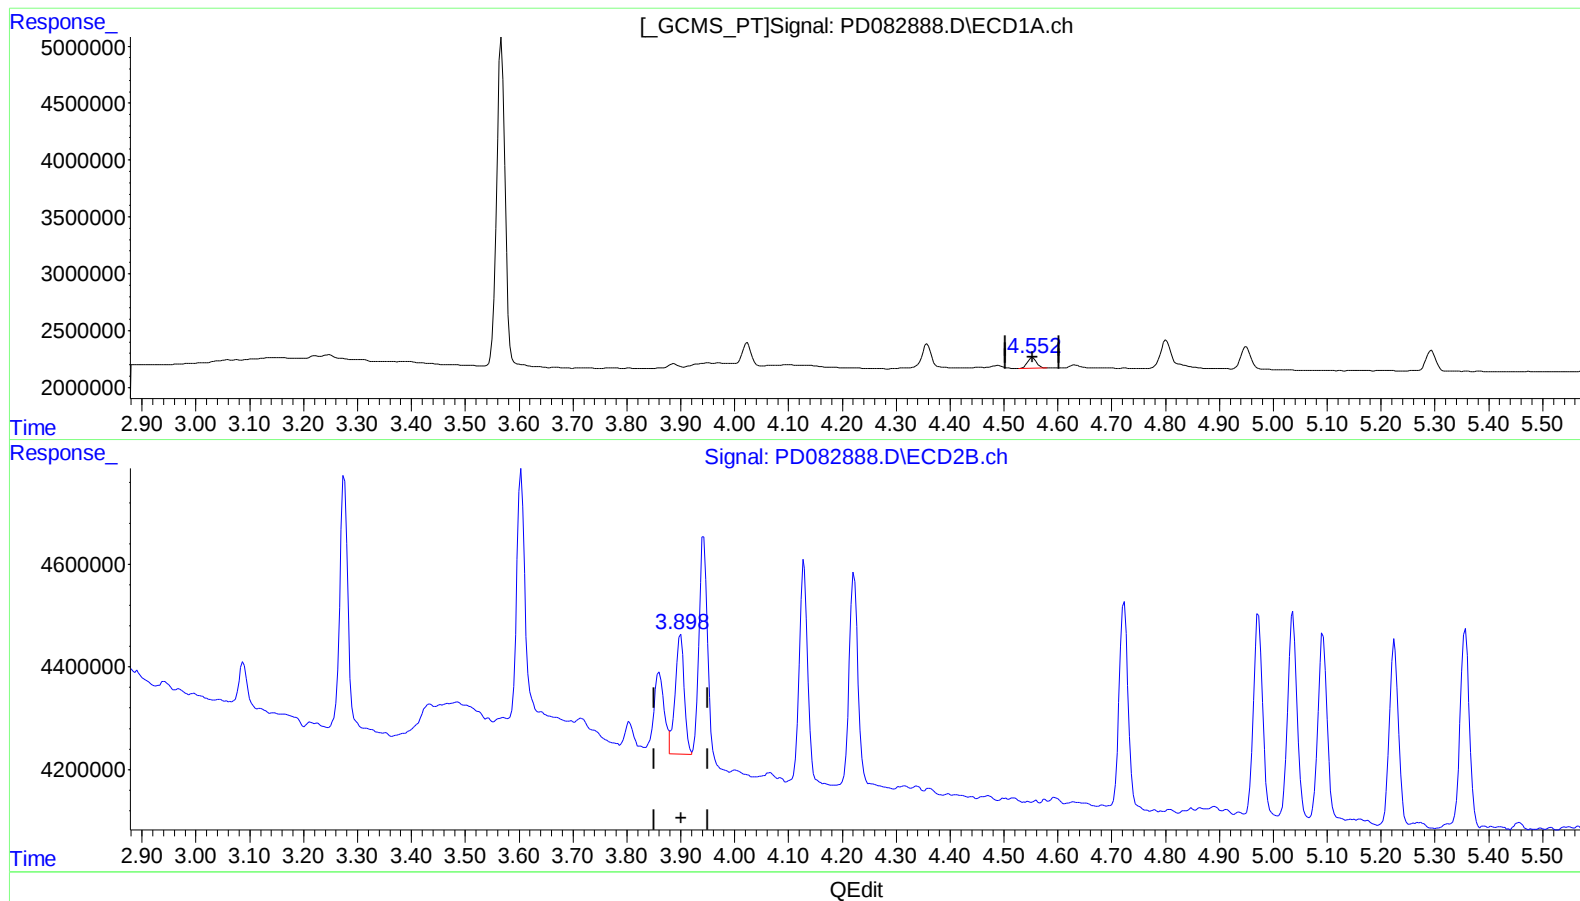

(6) beta-BHC (B)

4.552min 0.980 ng/ml m

response 1063134

(6) beta-BHC #2 (B)

3.898min 1.081 ng/ml m

response 2710792

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

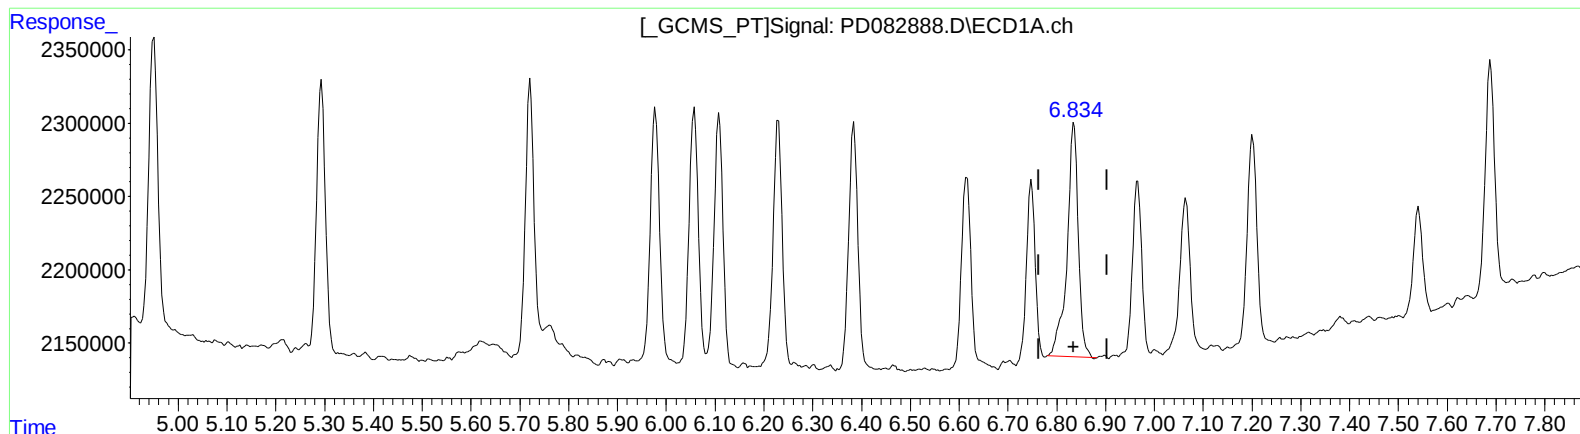

QEdit

(15) Endosulfan II (B)

6.835min 1.322 ng/ml

response 2546740

(15) Endosulfan II #2 (B)

5.924min 0.965 ng/ml

response 4064997

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

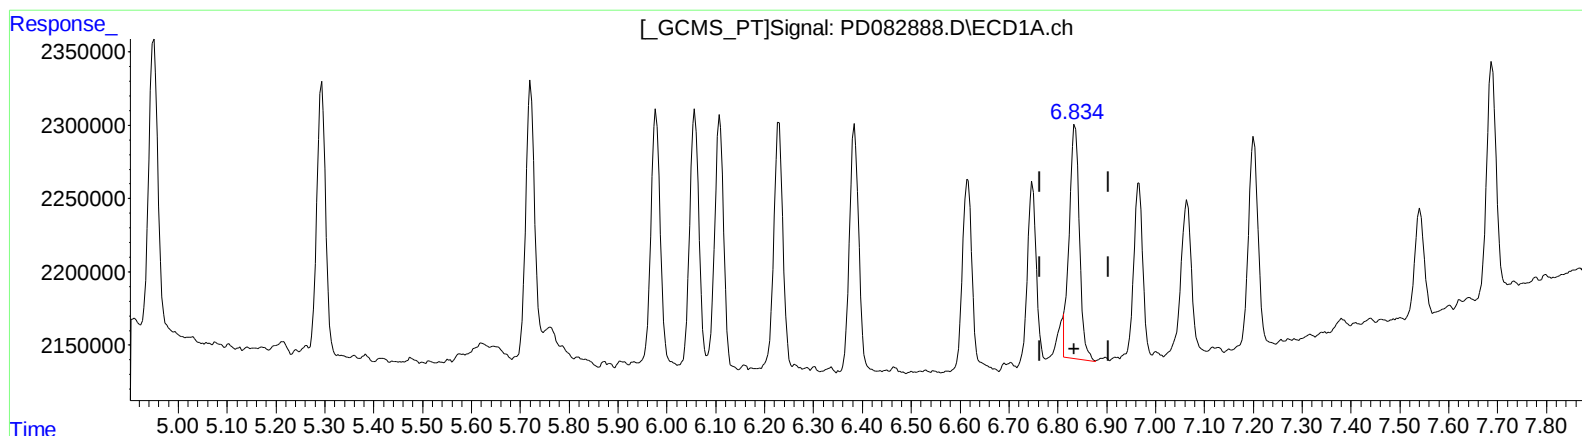

(15) Endosulfan II (B)
6.834min 1.202 ng/ml m
response 2316097

(15) Endosulfan II #2 (B)
5.924min 0.965 ng/ml
response 4064997

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

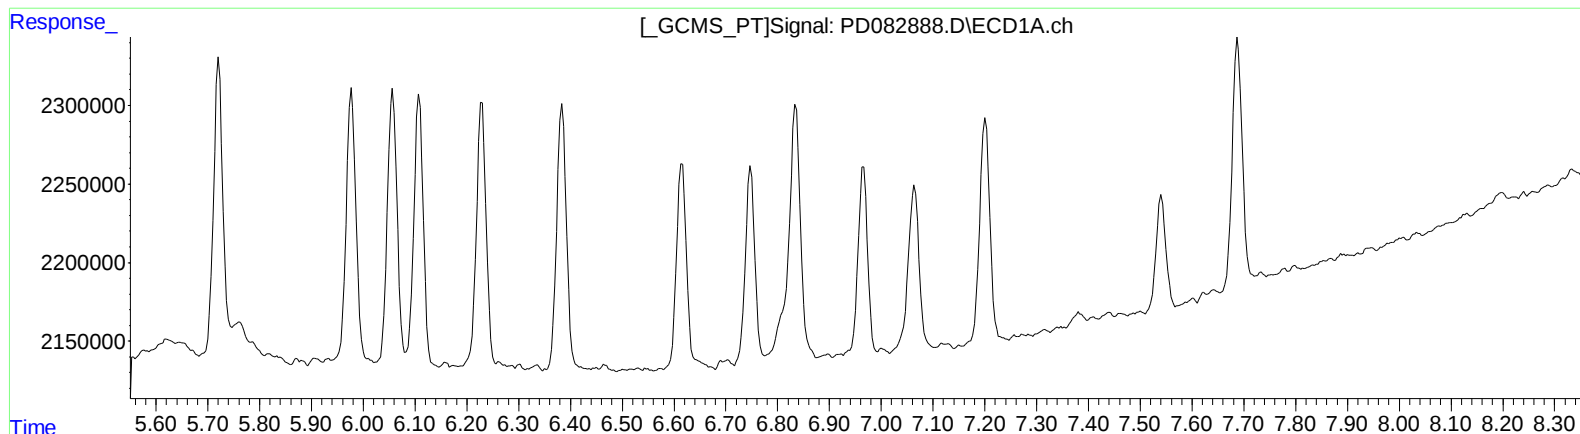

(20) Methoxychlor (A)

0.000min 0.000 ng/ml

response 0

(20) Methoxychlor #2 (A)

6.605min 0.931 ng/ml

response 1825900

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052024\
Data File : PD082888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:57
Operator : AR\AJ
Sample : P2409-01
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-03

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:50:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

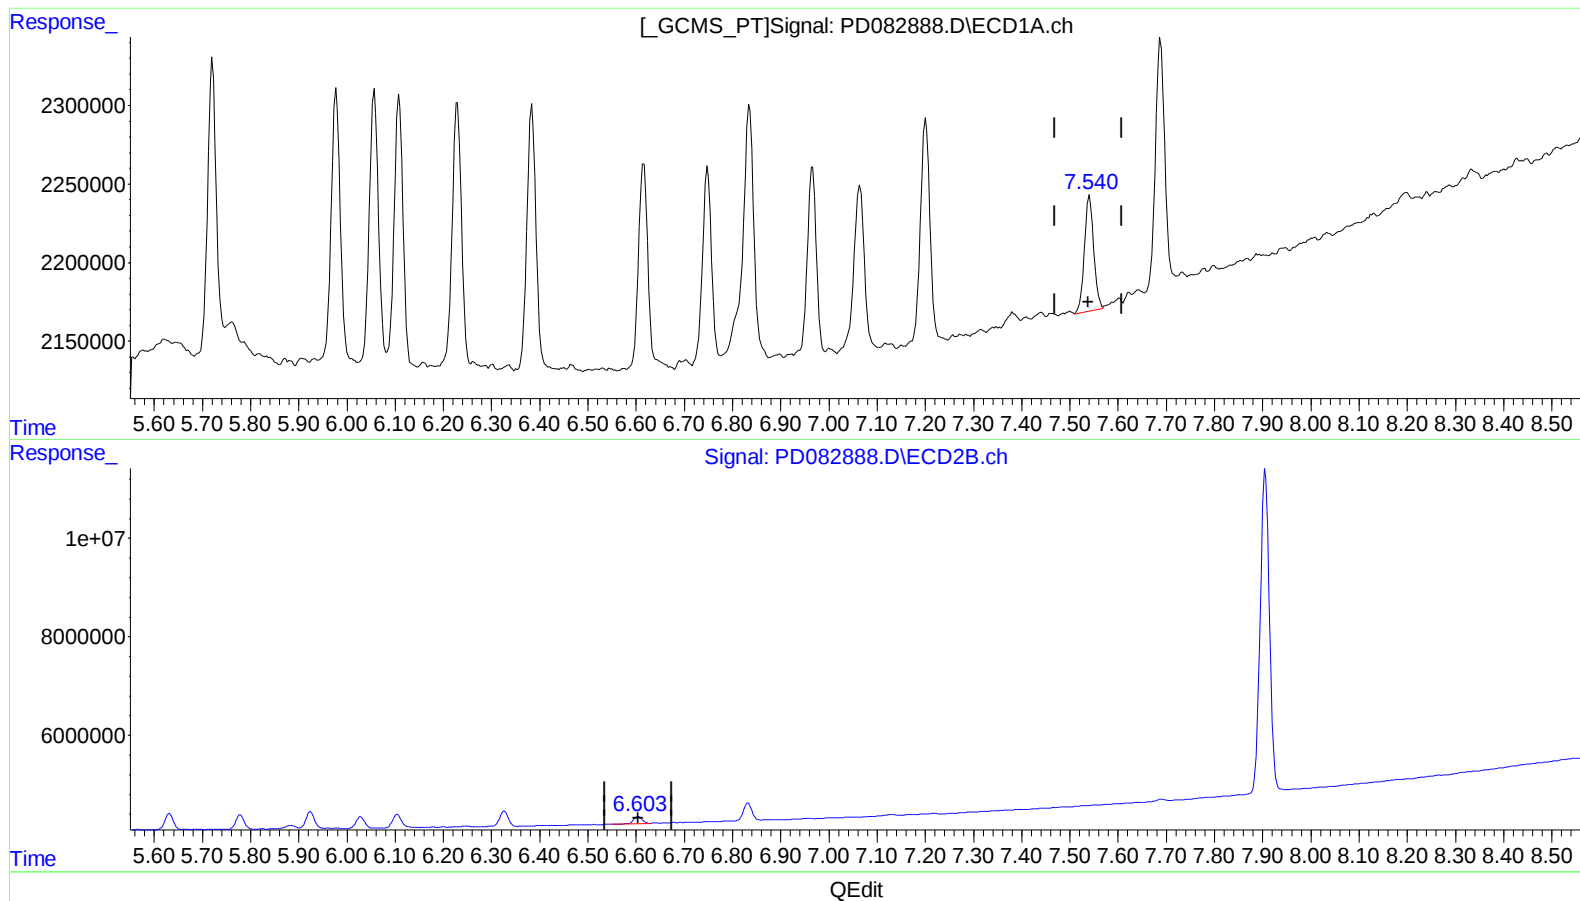

(20) Methoxychlor (A)
7.540min 1.140 ng/ml m
response 986137

(20) Methoxychlor #2 (A)
6.605min 0.931 ng/ml
response 1825900