

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
 Data File : PD058056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 10:35
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 14:48:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.217	3.866	16864782	25144745	21.579	22.078
28)	SA Decachlor...	7.858	8.853	18186959	23653860	22.746	22.816
Target Compounds							
5)	MB Aldrin	4.419	0.000	258009	0	0.246	N.D. #
7)	B delta-BHC	4.371f	0.000	229939	0	0.201	N.D. #
8)	B Heptachlo...	4.826f	0.000	200464	0	0.205	N.D. #
10)	B gamma-Chl...	5.065	0.000	145887	0	0.147	N.D. #
11)	B alpha-Chl...	5.117	0.000	31857	0	0.032	N.D. #
14)	MA Endrin	5.639f	0.000	407196	0	0.509	N.D. #
25)	Chlordane-3	5.065	0.000	145887	0	1.628	N.D. #
26)	Chlordane-4	5.117	0.000	31857	0	0.373	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
Data File : PD058056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 10:35
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 14:48:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

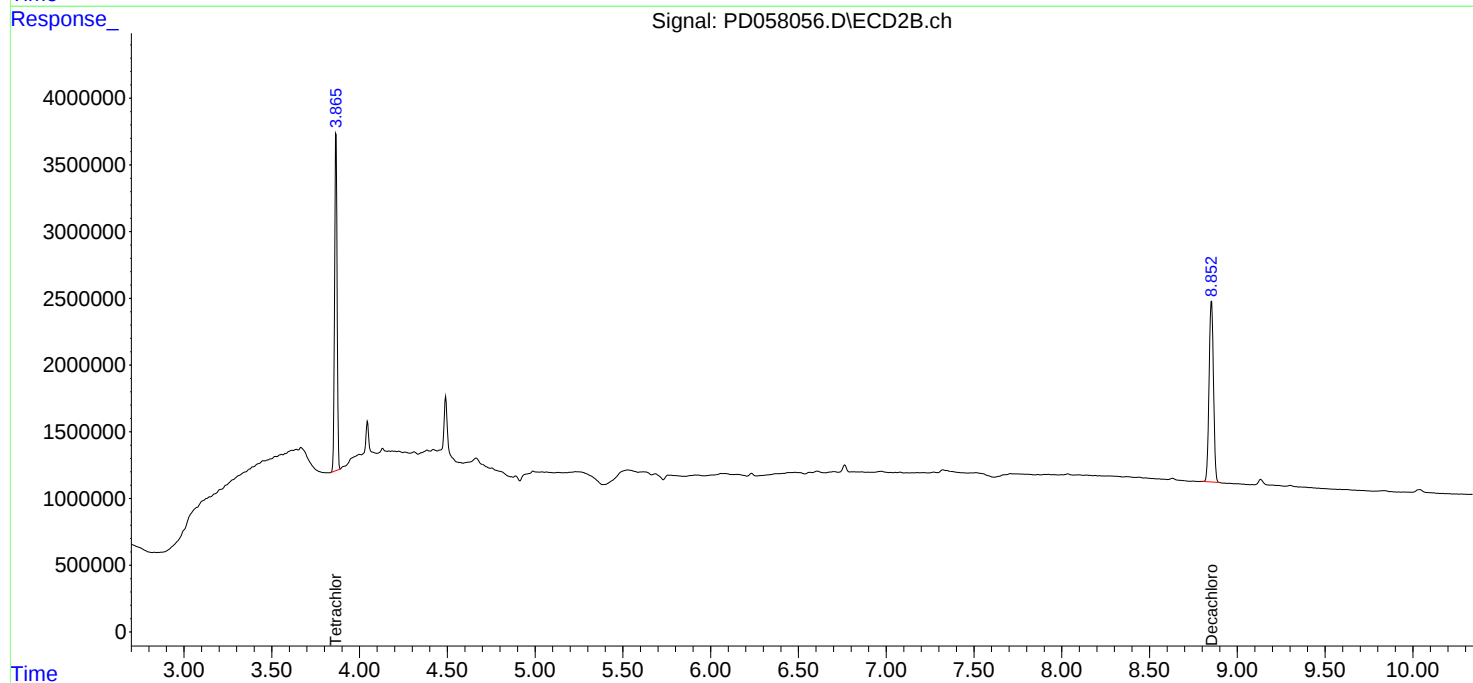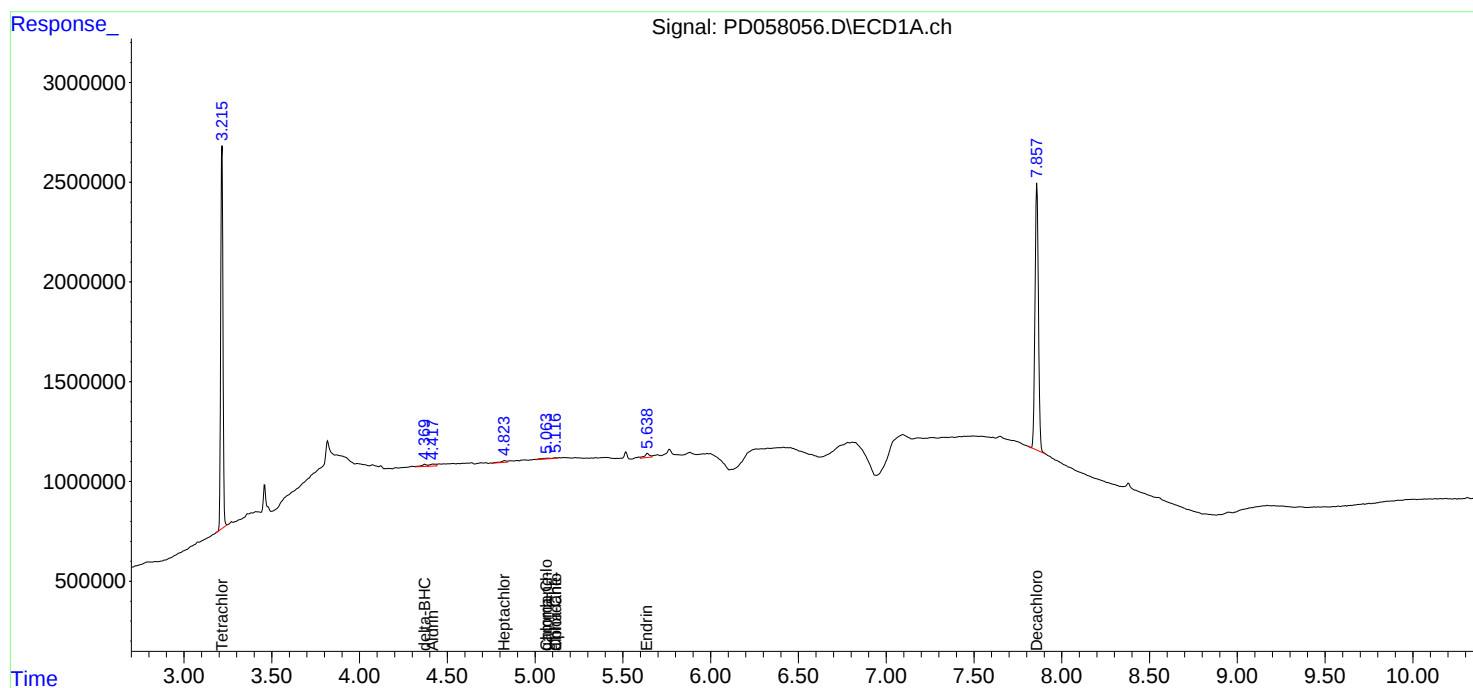


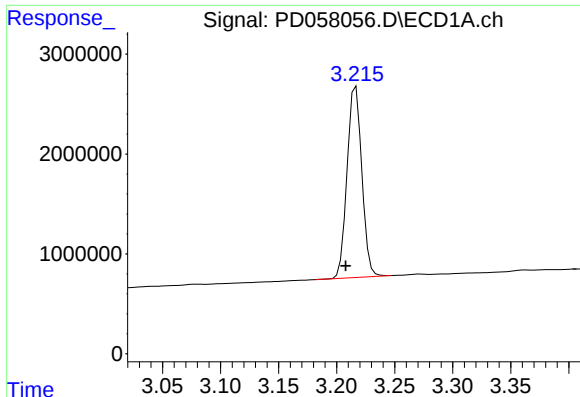

#1 Tetrachloro-m-xylene


R.T.: 3.217 min
Delta R.T.: 0.009 min
Response: 16864782
Conc: 21.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

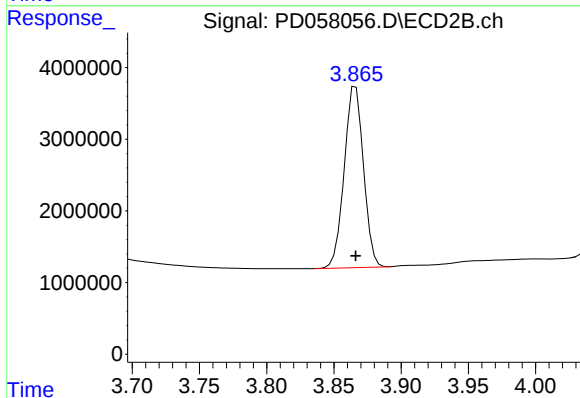


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 25144745
Conc: 22.08 ng/ml

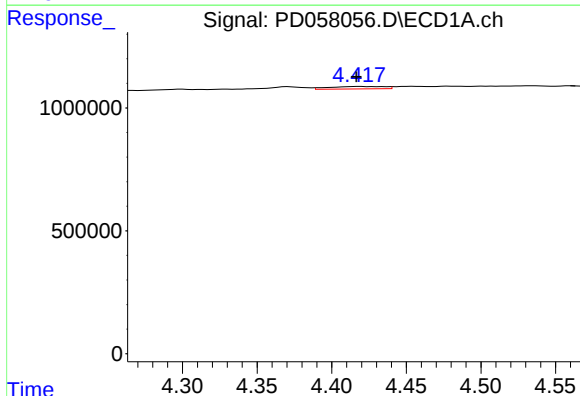


#5 Aldrin

R.T.: 4.419 min
Delta R.T.: 0.002 min
Response: 258009
Conc: 0.25 ng/ml

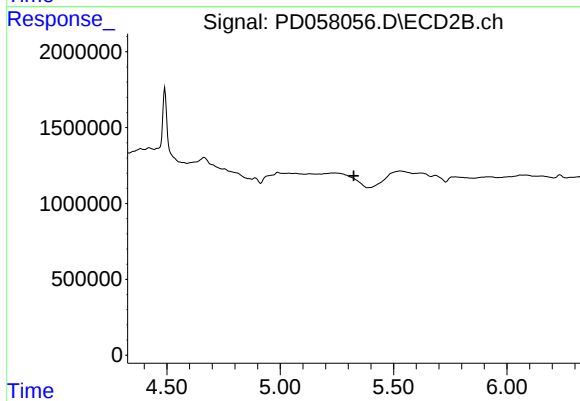

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.325 min
Response: 0
Conc: N.D.

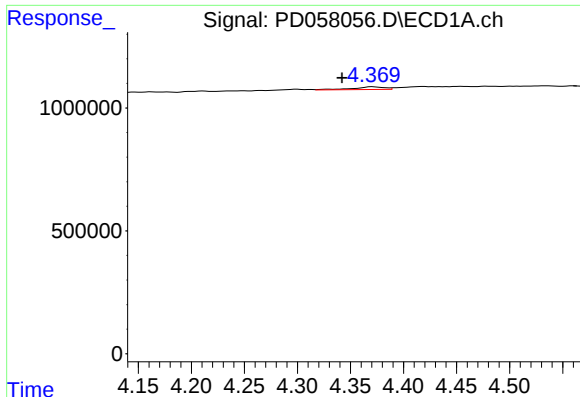

#7 delta-BHC


R.T.: 4.371 min
Delta R.T.: 0.029 min
Response: 229939
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

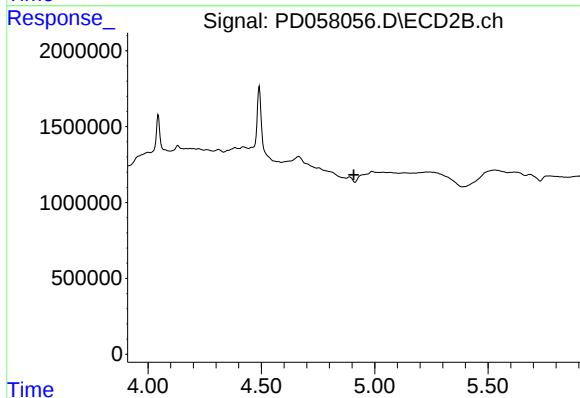


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

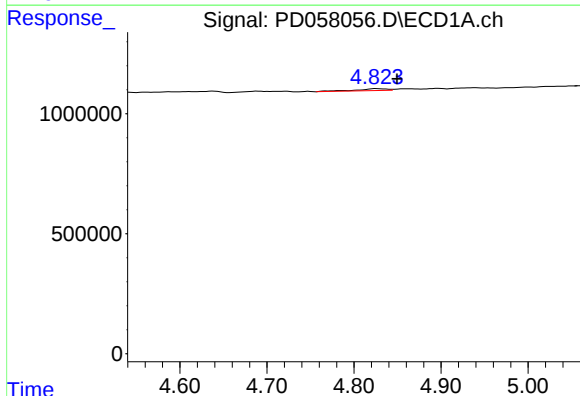


#8 Heptachlor epoxide

R.T.: 4.826 min
Delta R.T.: -0.023 min
Response: 200464
Conc: 0.21 ng/ml

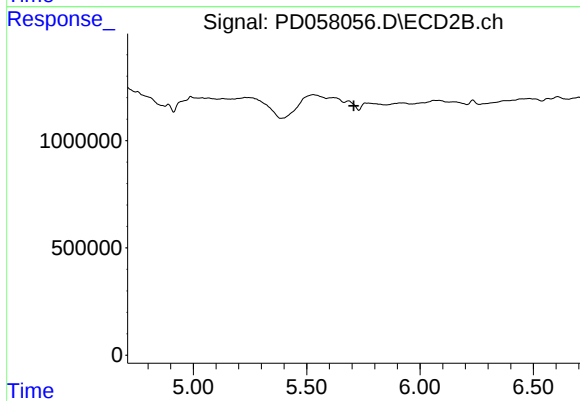

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.708 min
Response: 0
Conc: N.D.

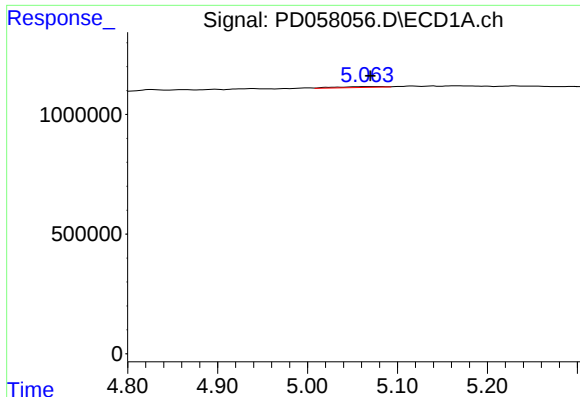

#10 gamma-Chlordane


R.T.: 5.065 min
Delta R.T.: -0.005 min
Response: 145887
Conc: 0.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

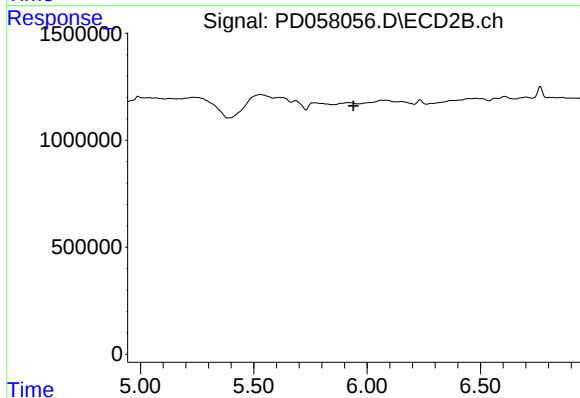


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.940 min
Response: 0
Conc: N.D.

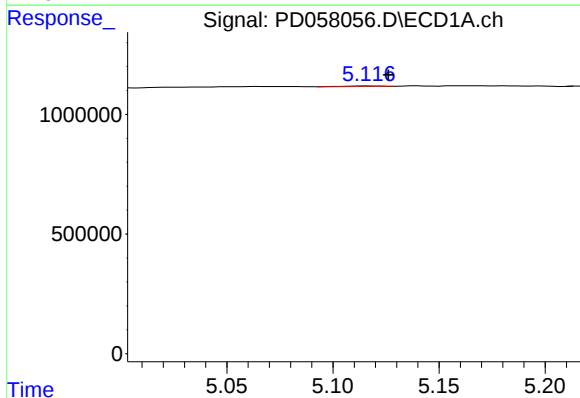


#11 alpha-Chlordane

R.T.: 5.117 min
Delta R.T.: -0.009 min
Response: 31857
Conc: 0.03 ng/ml

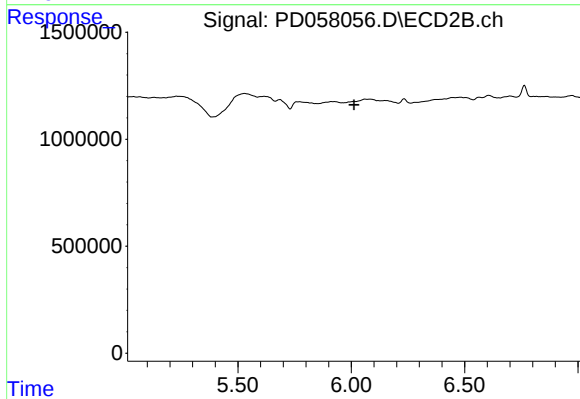

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

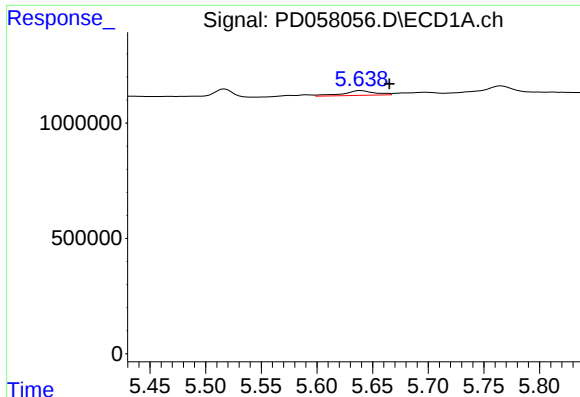

#14 Endrin


R.T.: 5.639 min
Delta R.T.: -0.026 min
Response: 407196
Conc: 0.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

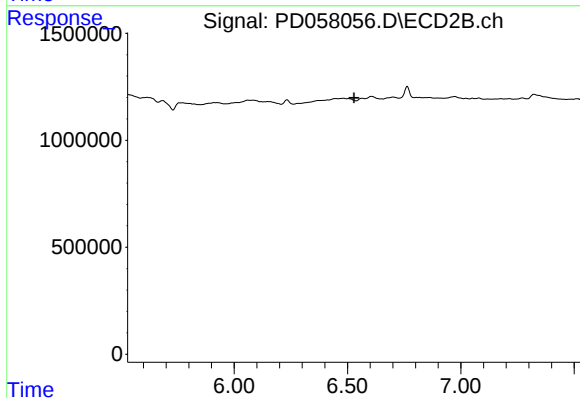


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.530 min
Response: 0
Conc: N.D.

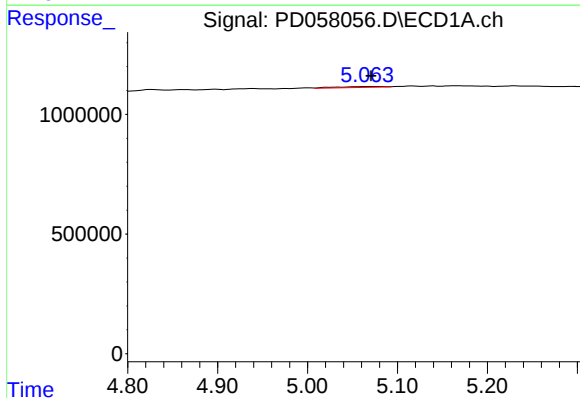


#25 Chlordane-3

R.T.: 5.065 min
Delta R.T.: -0.005 min
Response: 145887
Conc: 1.63 ng/ml

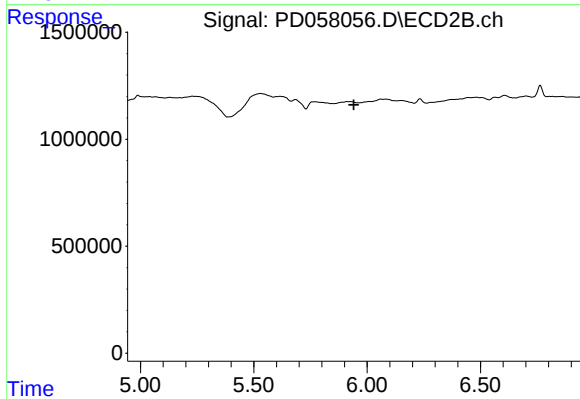

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.941 min
Response: 0
Conc: N.D.

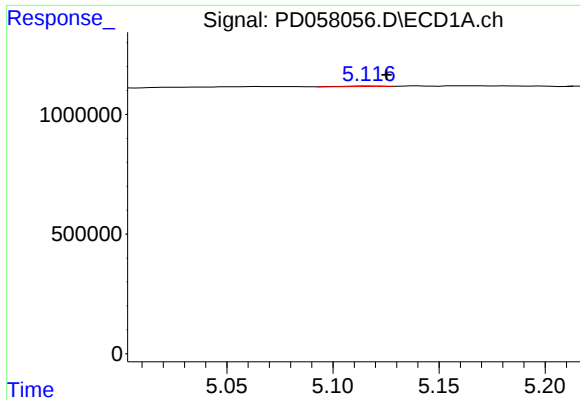

#26 Chlordane-4


R.T.: 5.117 min
Delta R.T.: -0.008 min
Response: 31857
Conc: 0.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

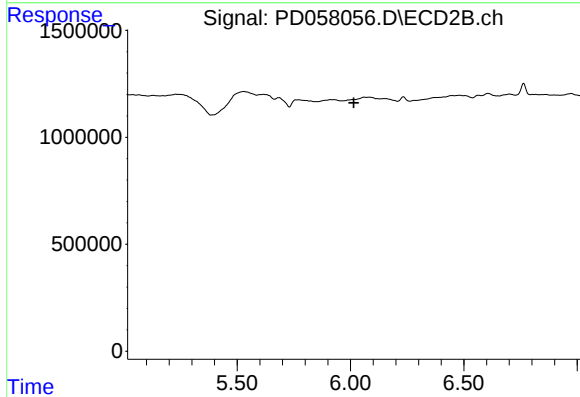


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

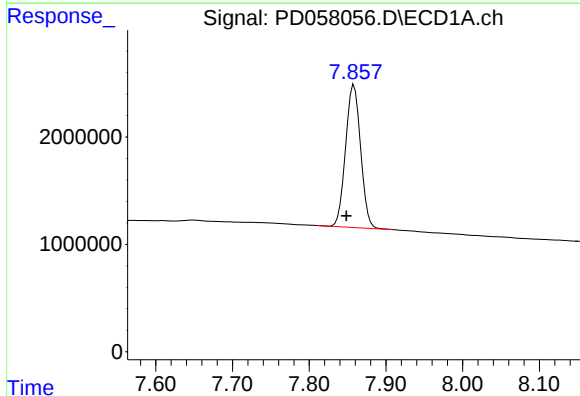

#28 Decachlorobiphenyl

R.T.: 7.858 min
Delta R.T.: 0.010 min
Response: 18186959
Conc: 22.75 ng/ml

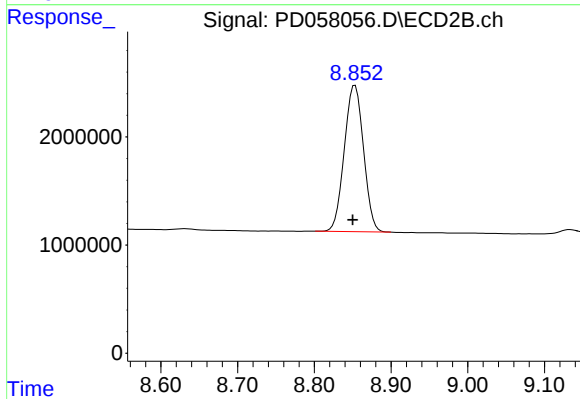

#28 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.003 min
Response: 23653860
Conc: 22.82 ng/ml