

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
 Data File : PD058064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 12:28
 Operator : AJ\MA
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 13:36:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:16:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	85140786	108.4E6	102.178	100.469
28)	SA Decachlor...	7.848	8.849	73629427	89285313	95.283	92.407
Target Compounds							
23)	Chlordane-1	4.036	4.839	24948314	40185690	995.779	1004.409
24)	Chlordane-2	4.522	5.301	29320916	43896226	949.648	938.877
25)	Chlordane-3	5.070	5.940	90922896	173.1E6	1033.298	1009.147
26)	Chlordane-4	5.126	6.014	84841181	206.8E6	1014.977	996.419
27)	Chlordane-5	5.942	6.809	28701837	38133953	1038.465	1027.143



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
Data File : PD058064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 12:28
Operator : AJ\MA
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 13:36:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:16:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

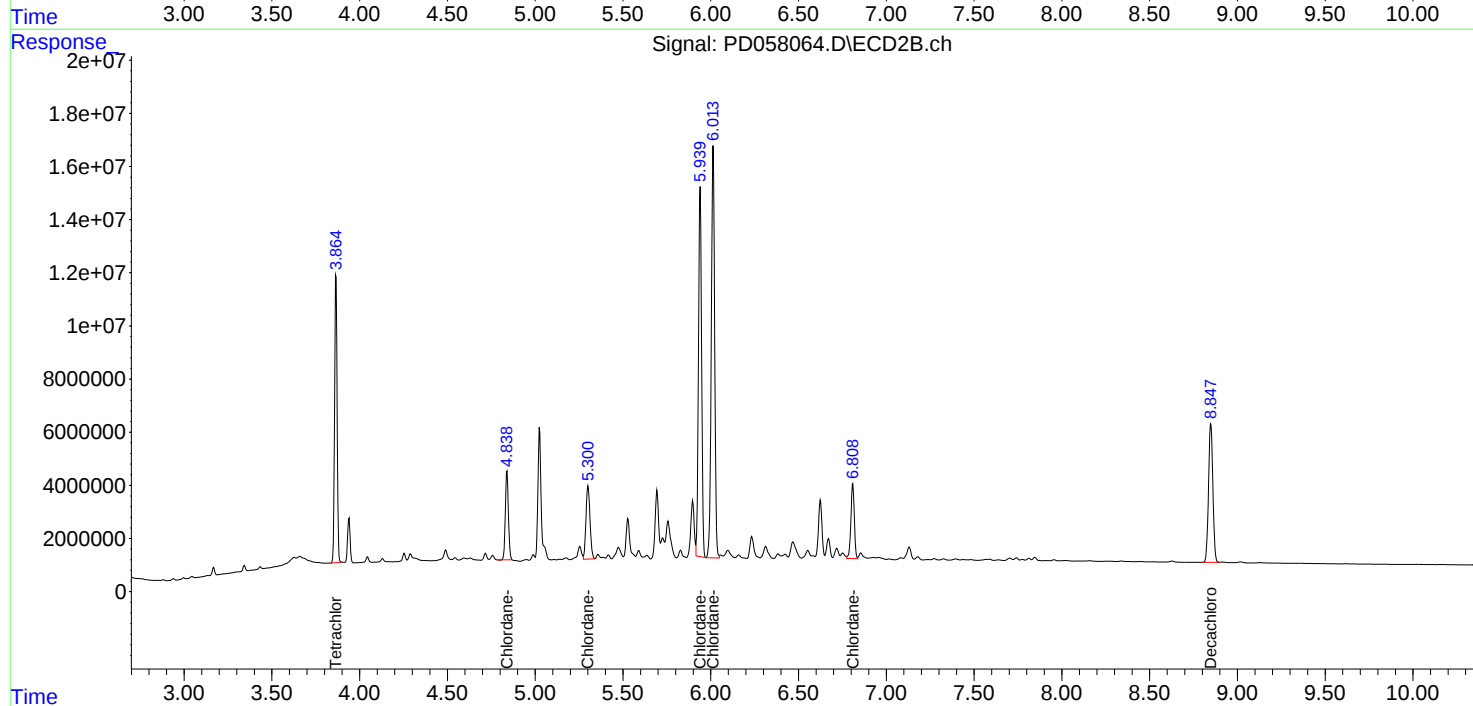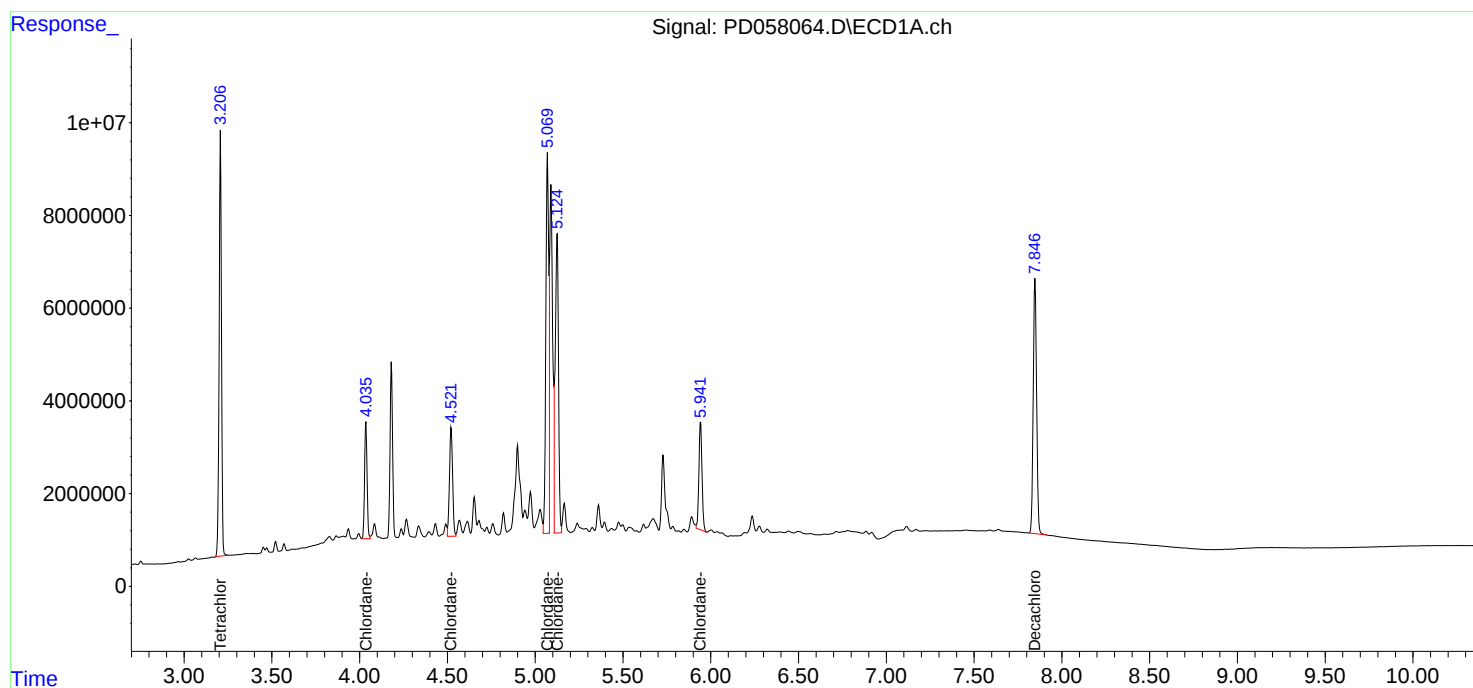


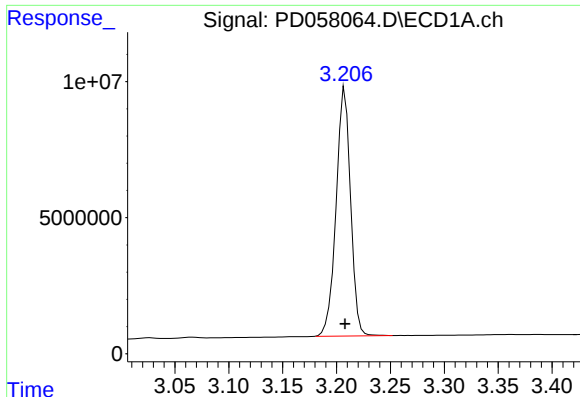

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 85140786
Conc: 102.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

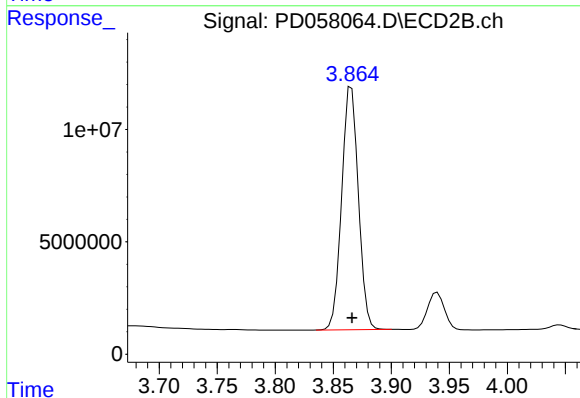


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 108354894
Conc: 100.47 ng/ml

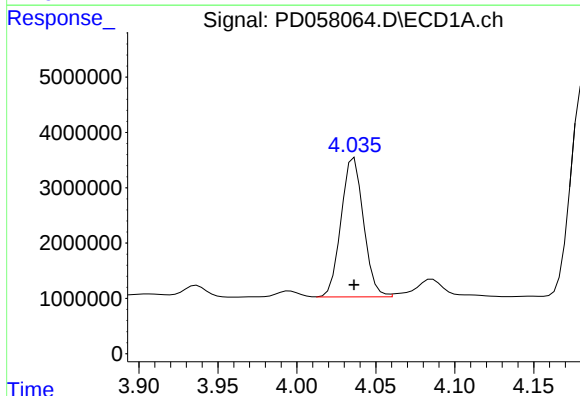


#23 Chlordane-1

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 24948314
Conc: 995.78 ng/ml

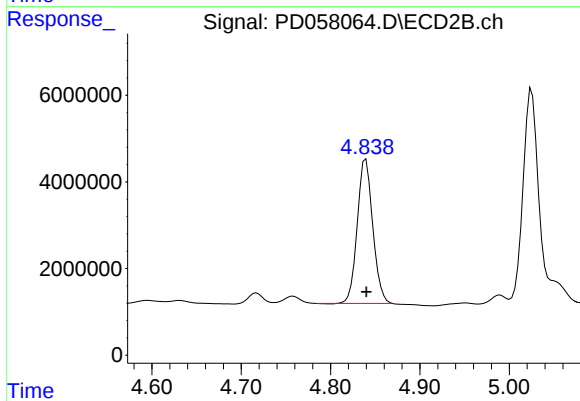

#23 Chlordane-1


R.T.: 4.839 min
Delta R.T.: 0.000 min
Response: 40185690
Conc: 1004.41 ng/ml

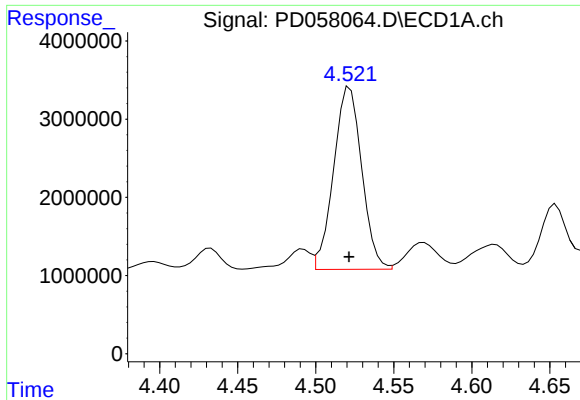

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 29320916
Conc: 949.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

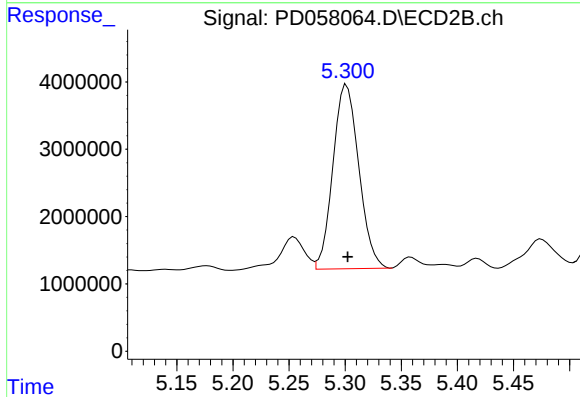


#24 Chlordane-2

R.T.: 5.301 min
Delta R.T.: 0.000 min
Response: 43896226
Conc: 938.88 ng/ml

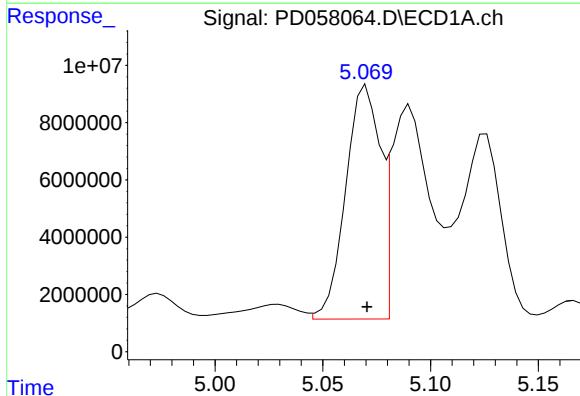


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 90922896
Conc: 1033.30 ng/ml

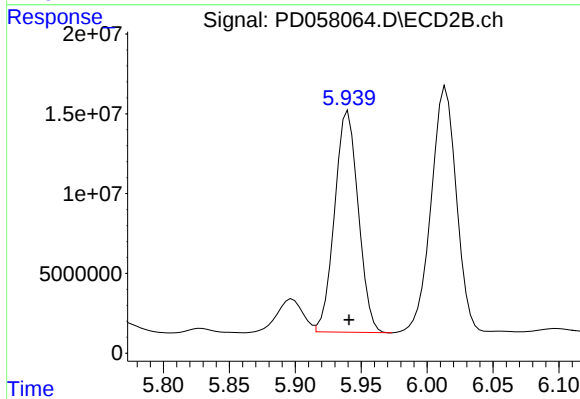

#25 Chlordane-3


R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 173099266
Conc: 1009.15 ng/ml

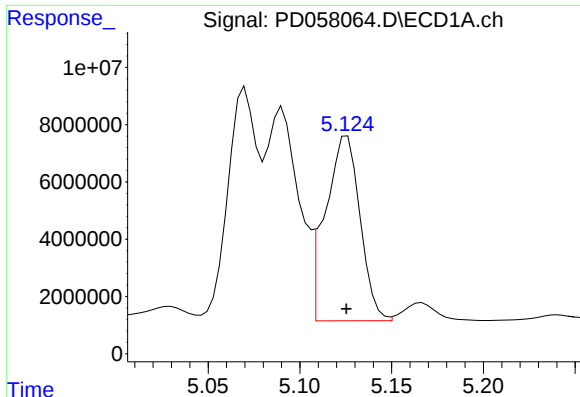

#26 Chlordane-4


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 84841181
Conc: 1014.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

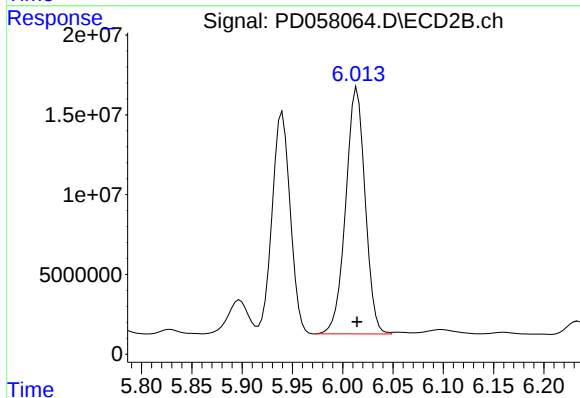


#26 Chlordane-4

R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 206809159
Conc: 996.42 ng/ml

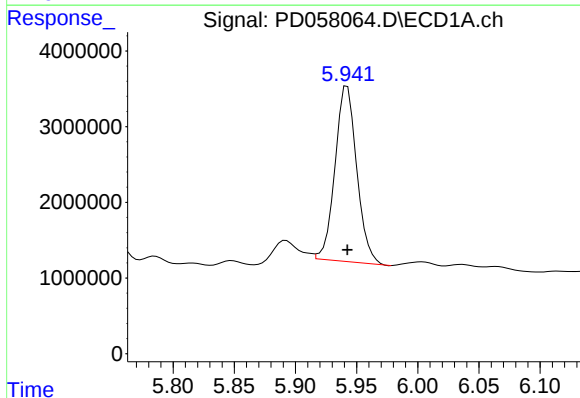


#27 Chlordane-5

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 28701837
Conc: 1038.46 ng/ml

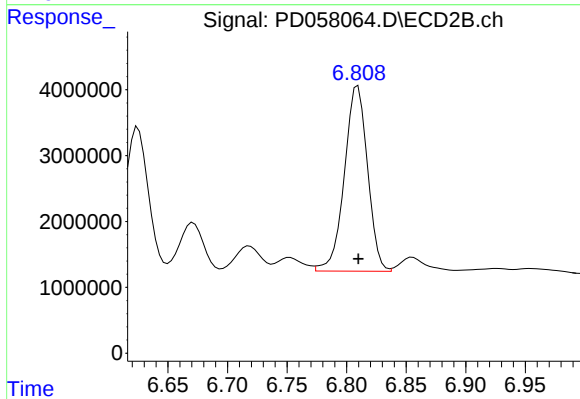

#27 Chlordane-5


R.T.: 6.809 min
Delta R.T.: 0.000 min
Response: 38133953
Conc: 1027.14 ng/ml

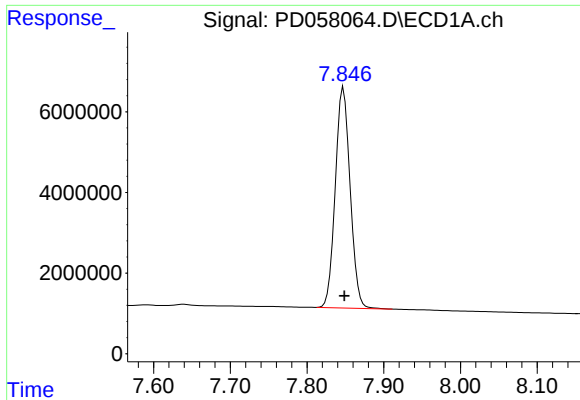

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: -0.001 min
Response: 73629427
Conc: 95.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

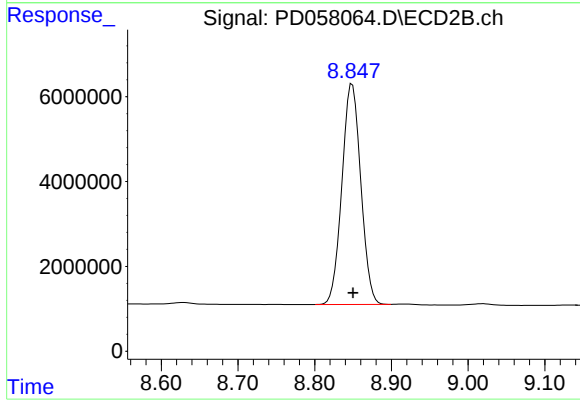

#28 Decachlorobiphenyl

R.T.: 8.849 min
Delta R.T.: 0.000 min
Response: 89285313
Conc: 92.41 ng/ml