

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
 Data File : PD058065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 12:42
 Operator : AJ\MA
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 13:36:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:16:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	63475059	81144711	76.177	75.239
28)	SA Decachlor...	7.849	8.850	57330312	69465642	74.191	71.894
Target Compounds							
23)	Chlordane-1	4.037	4.840	18707860	30114552	746.699	752.689
24)	Chlordane-2	4.522	5.302	22556035	33713710	730.546	721.088
25)	Chlordane-3	5.070	5.941	68962647	130.7E6	783.729	761.837
26)	Chlordane-4	5.126	6.014	65071424	156.5E6	778.466	753.947
27)	Chlordane-5	5.943	6.810	21370603	28728632	773.213	773.809



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
Data File : PD058065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 12:42
Operator : AJ\MA
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 13:36:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:16:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

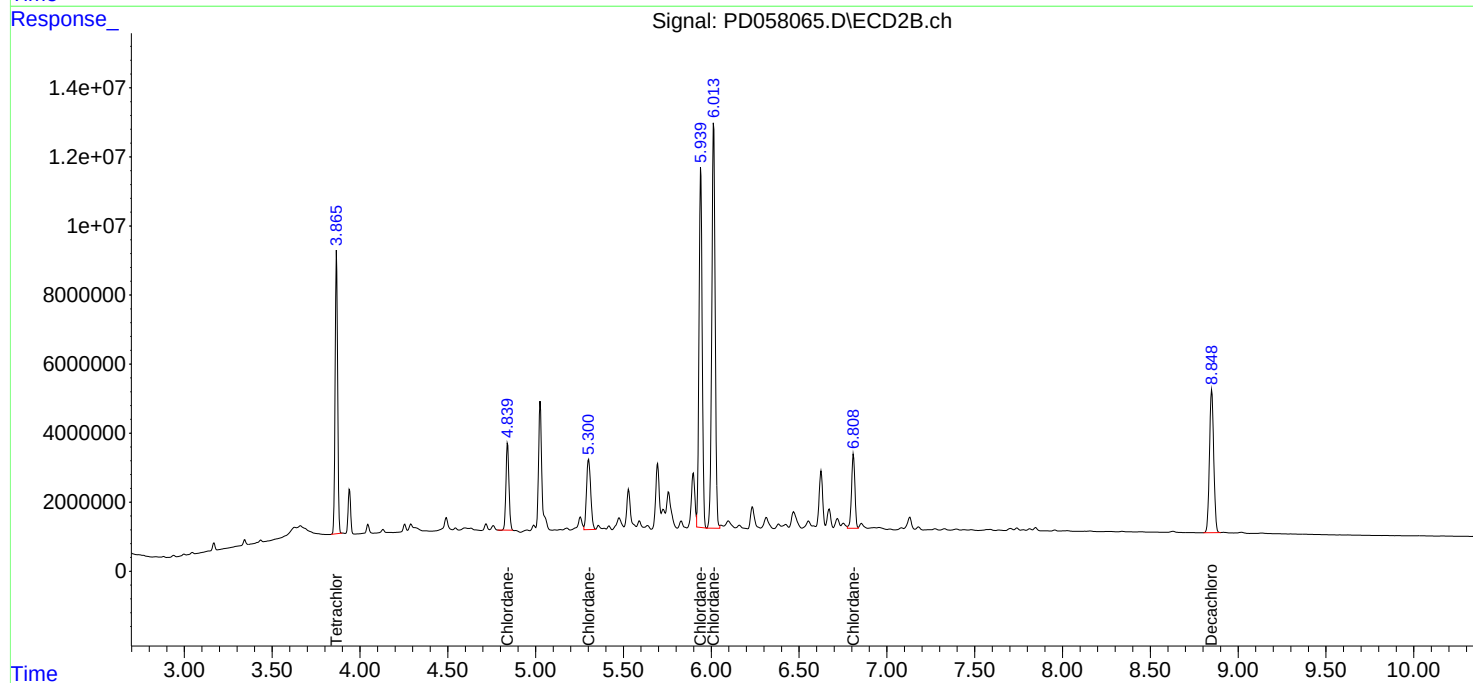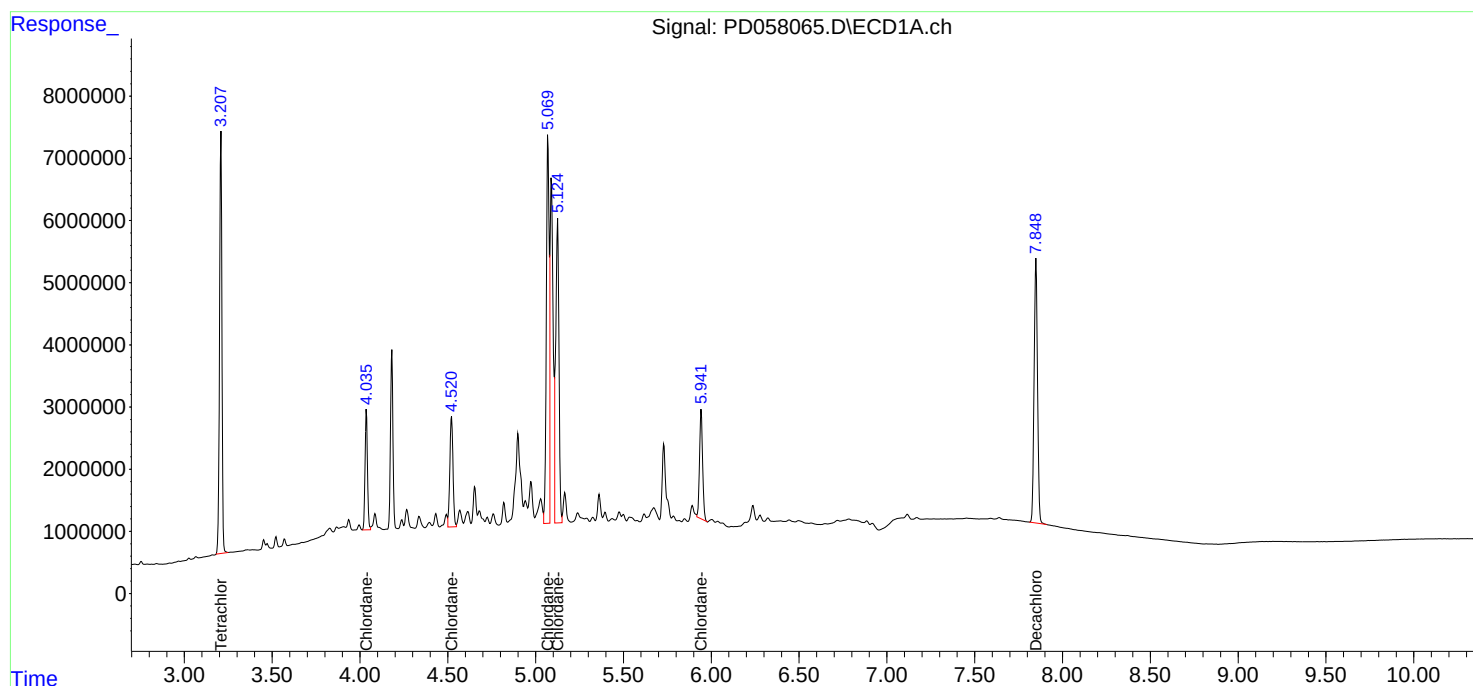


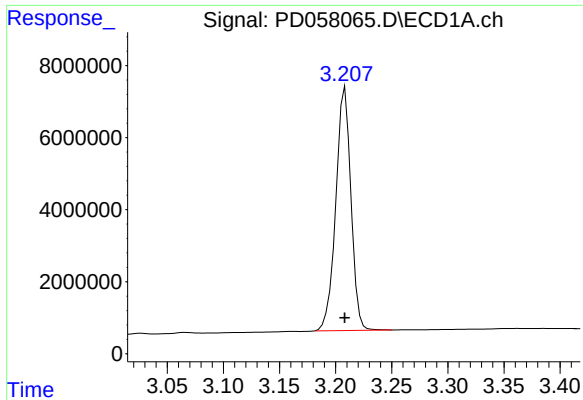

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 63475059
Conc: 76.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

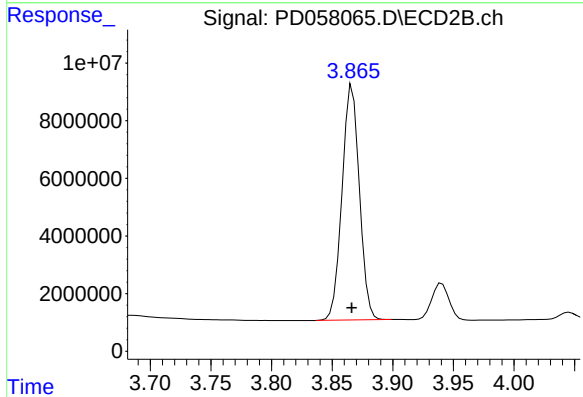


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 81144711
Conc: 75.24 ng/ml

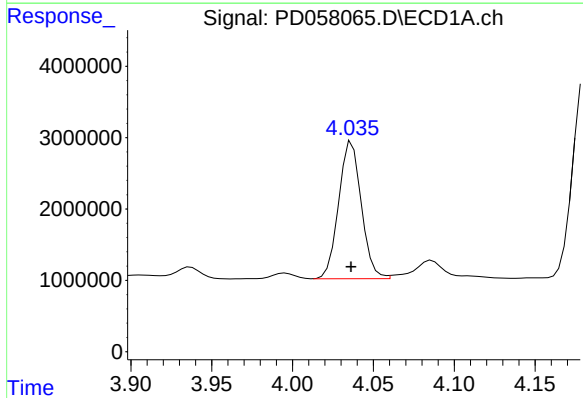


#23 Chlordane-1

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 18707860
Conc: 746.70 ng/ml

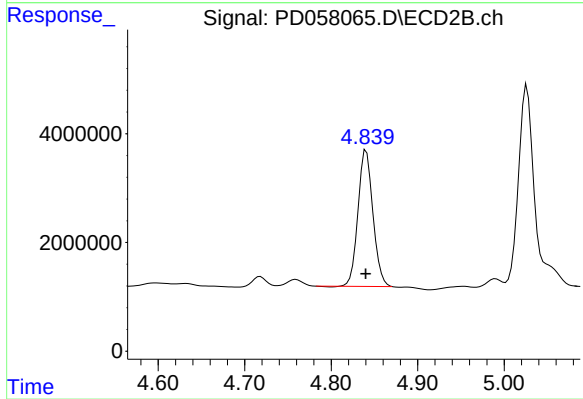

#23 Chlordane-1


R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 30114552
Conc: 752.69 ng/ml

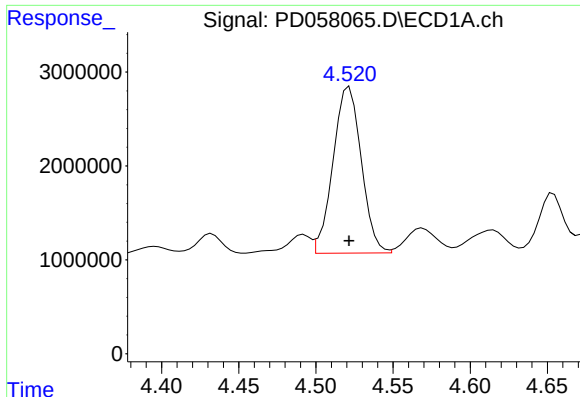

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 22556035
Conc: 730.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

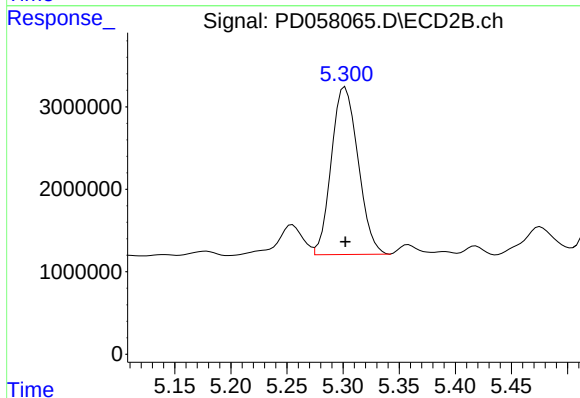


#24 Chlordane-2

R.T.: 5.302 min
Delta R.T.: 0.000 min
Response: 33713710
Conc: 721.09 ng/ml

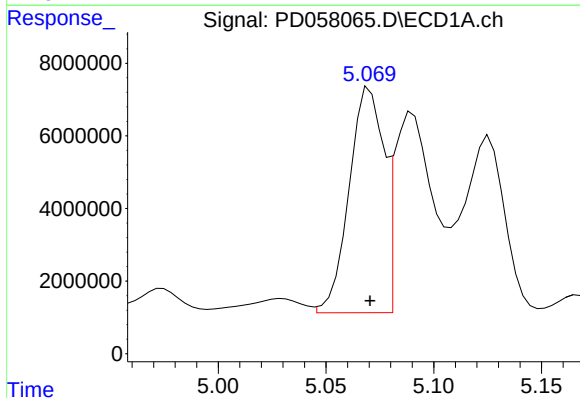


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 68962647
Conc: 783.73 ng/ml

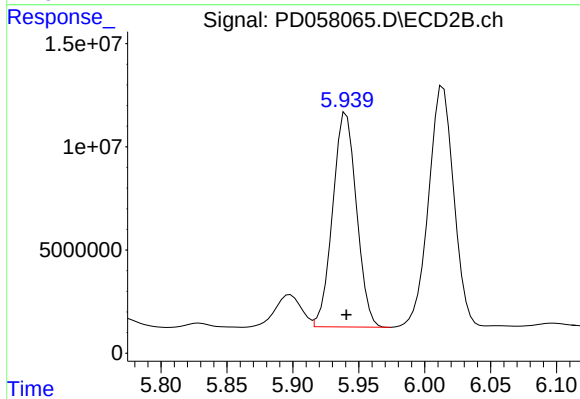

#25 Chlordane-3


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 130678082
Conc: 761.84 ng/ml

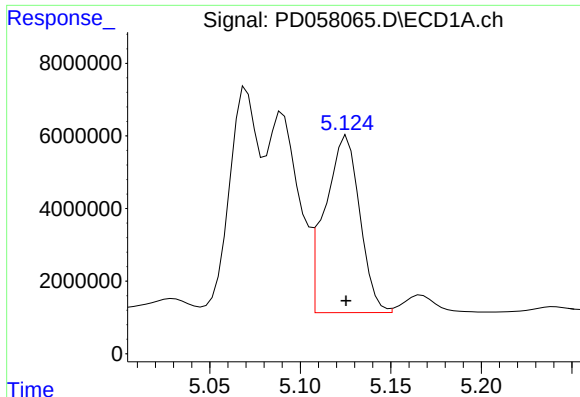

#26 Chlordane-4


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 65071424
Conc: 778.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

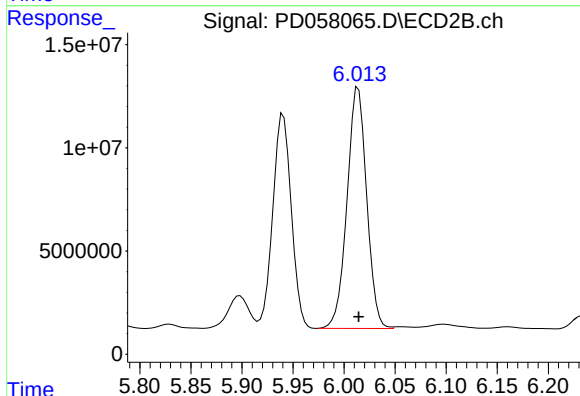


#26 Chlordane-4

R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 156483468
Conc: 753.95 ng/ml

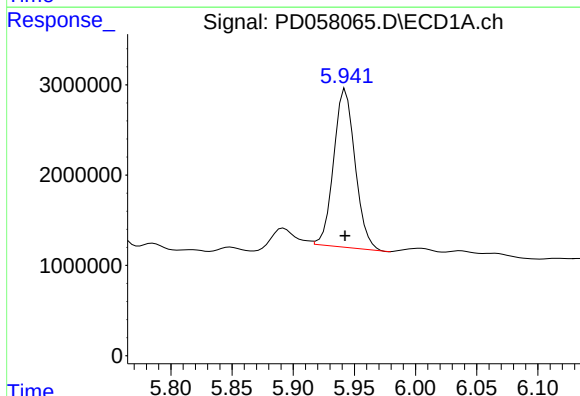


#27 Chlordane-5

R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 21370603
Conc: 773.21 ng/ml

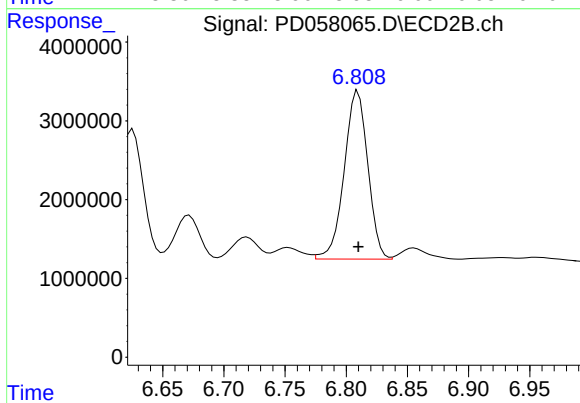

#27 Chlordane-5


R.T.: 6.810 min
Delta R.T.: 0.000 min
Response: 28728632
Conc: 773.81 ng/ml

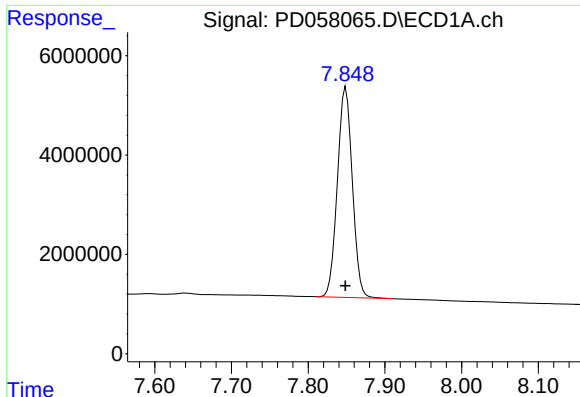

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 57330312
Conc: 74.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

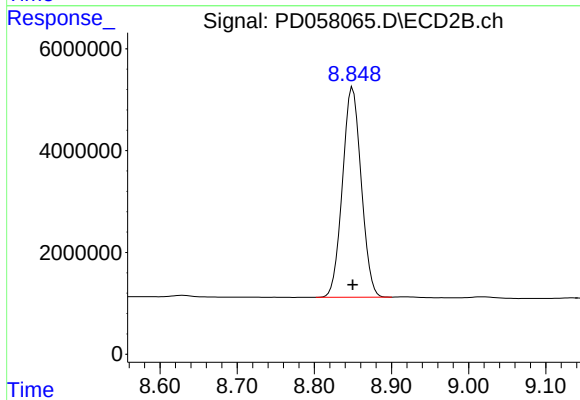

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 69465642
Conc: 71.89 ng/ml