

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
 Data File : PD058066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 12:56
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 13:36:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:16:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	41662991	53924585	50.000	50.000
28)	SA Decachlor...	7.849	8.850	38637180	48311107	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.036	4.840	12527037	20004642	500.000	500.000
24)	Chlordane-2	4.521	5.302	15437787	23376984	500.000	500.000
25)	Chlordane-3	5.070	5.941	43996466	85765141	500.000	500.000
26)	Chlordane-4	5.125	6.015	41794647	103.8E6	500.000	500.000
27)	Chlordane-5	5.942	6.810	13819359	18563119	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
Data File : PD058066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 12:56
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 13:36:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:16:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

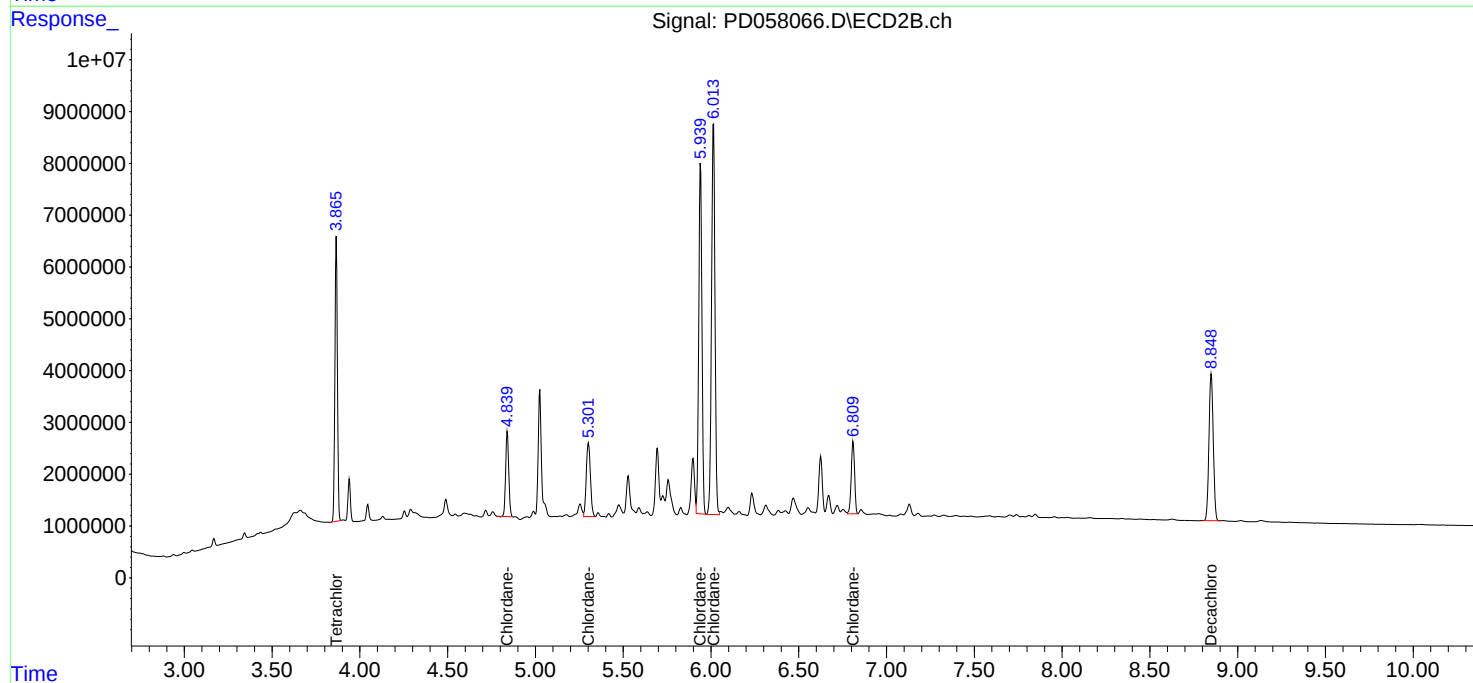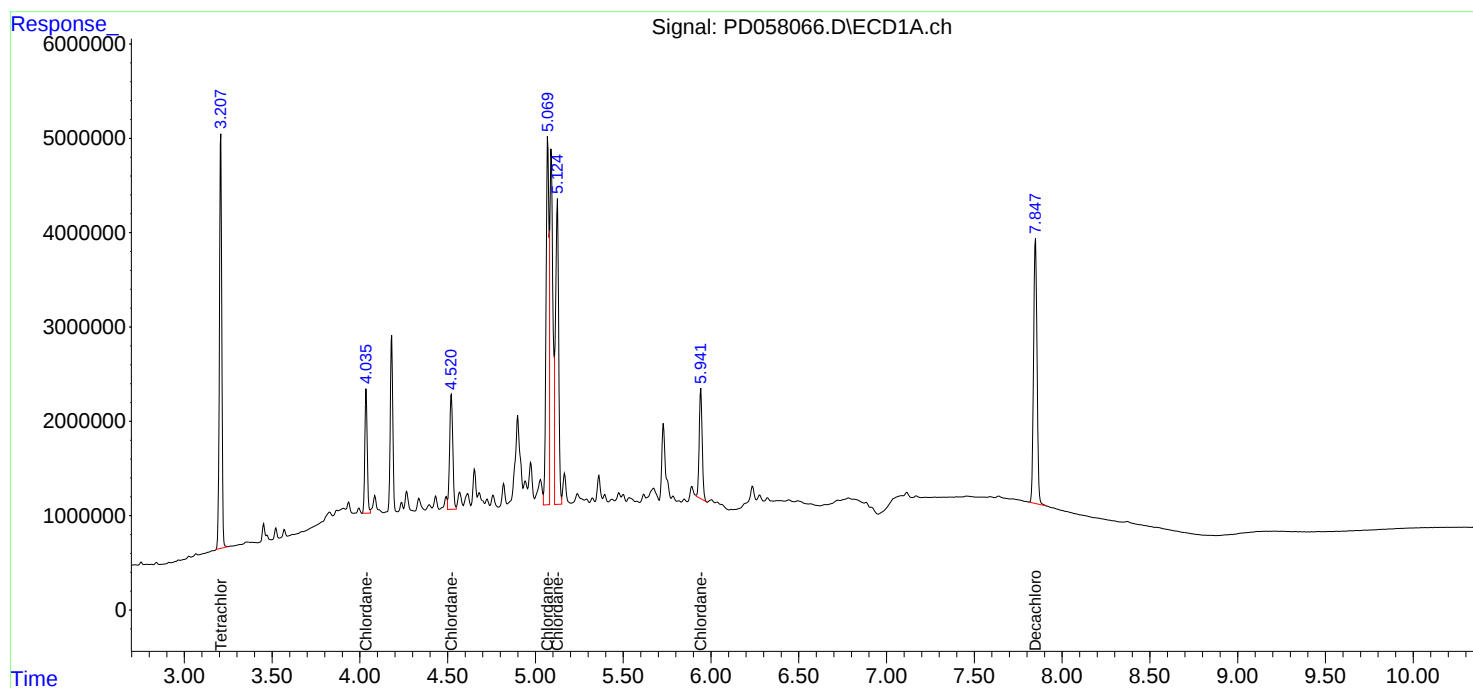


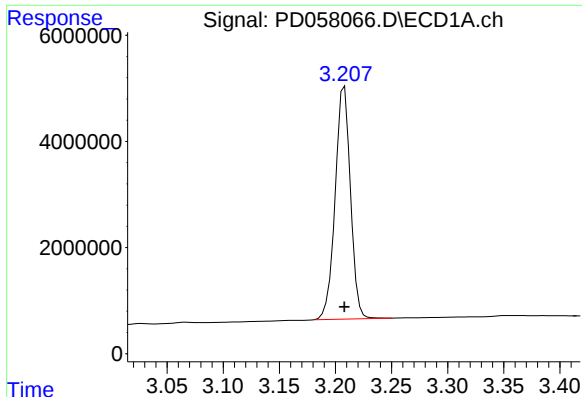

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 41662991
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

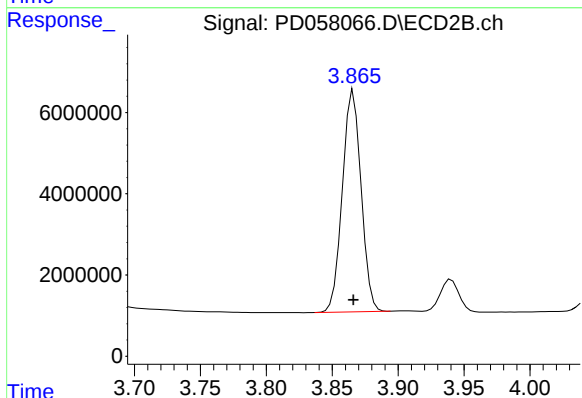


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 53924585
Conc: 50.00 ng/ml

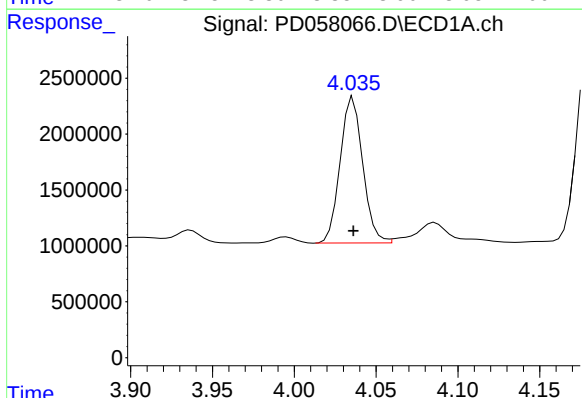


#23 Chlordane-1

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 12527037
Conc: 500.00 ng/ml

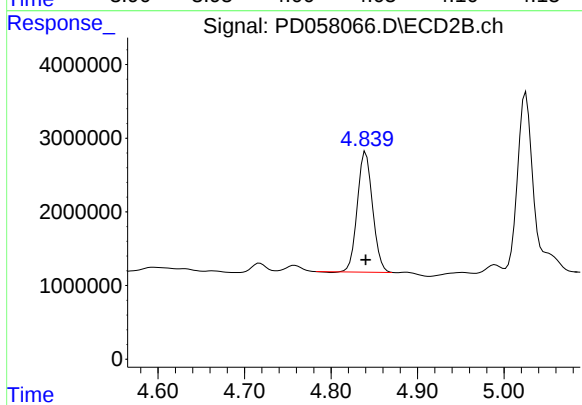

#23 Chlordane-1


R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 20004642
Conc: 500.00 ng/ml

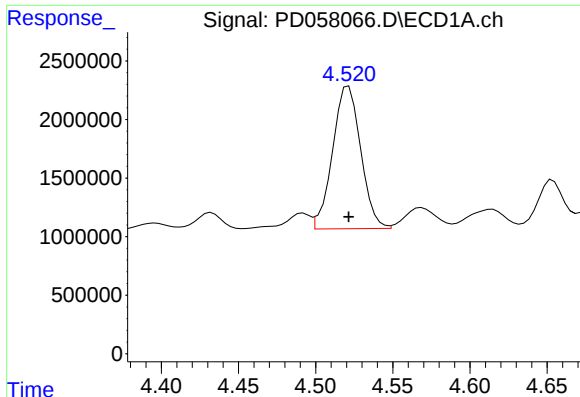

#24 Chlordane-2


R.T.: 4.521 min
Delta R.T.: 0.000 min
Response: 15437787
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

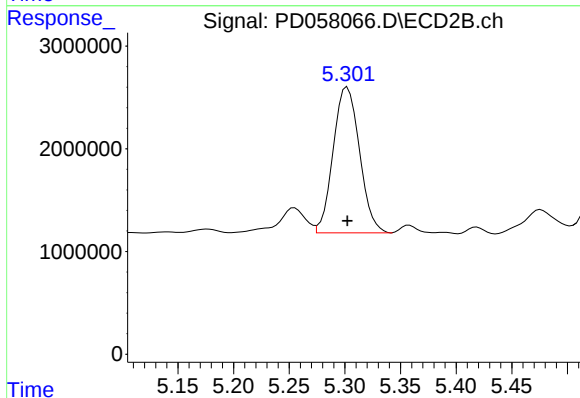


#24 Chlordane-2

R.T.: 5.302 min
Delta R.T.: 0.000 min
Response: 23376984
Conc: 500.00 ng/ml

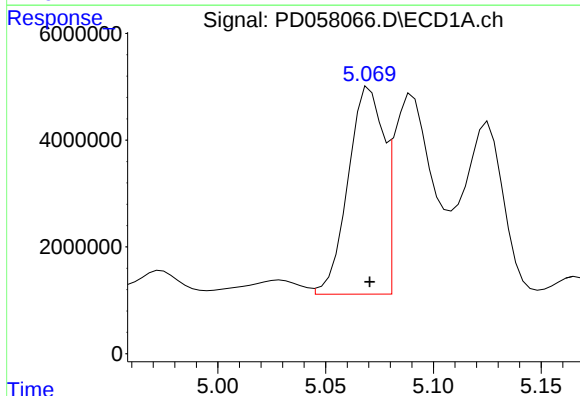


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 43996466
Conc: 500.00 ng/ml

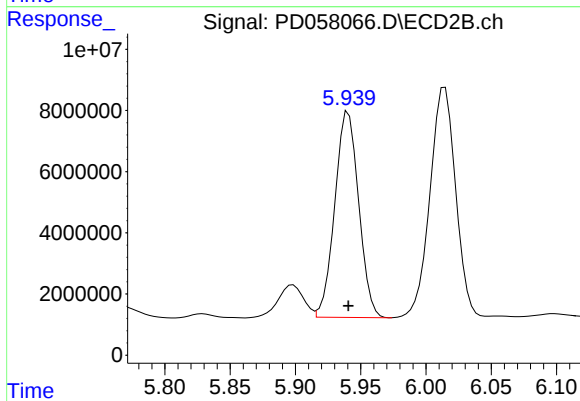

#25 Chlordane-3


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 85765141
Conc: 500.00 ng/ml

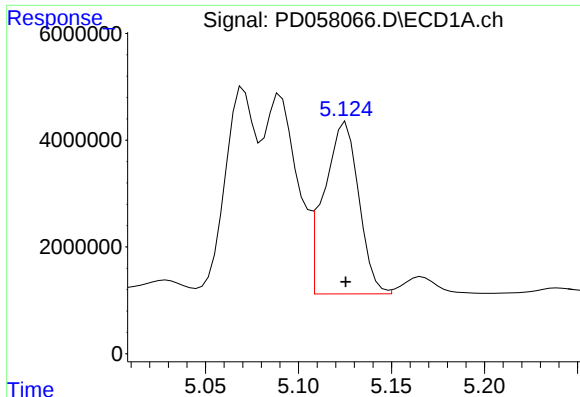

#26 Chlordane-4


R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 41794647
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

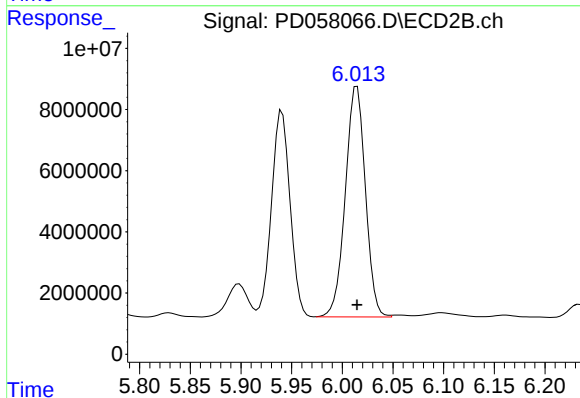


#26 Chlordane-4

R.T.: 6.015 min
Delta R.T.: 0.000 min
Response: 103776187
Conc: 500.00 ng/ml

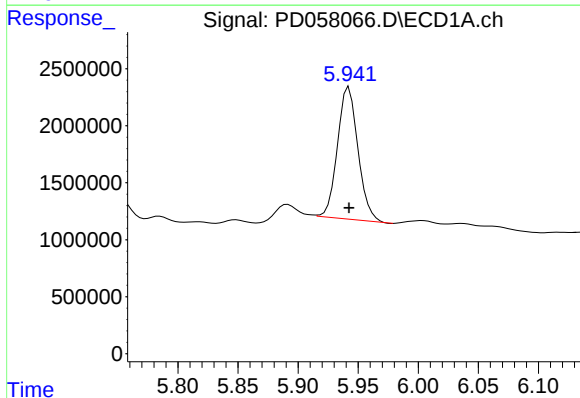


#27 Chlordane-5

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 13819359
Conc: 500.00 ng/ml

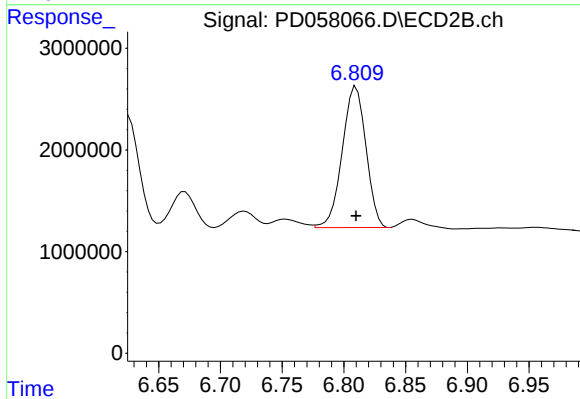

#27 Chlordane-5


R.T.: 6.810 min
Delta R.T.: 0.000 min
Response: 18563119
Conc: 500.00 ng/ml

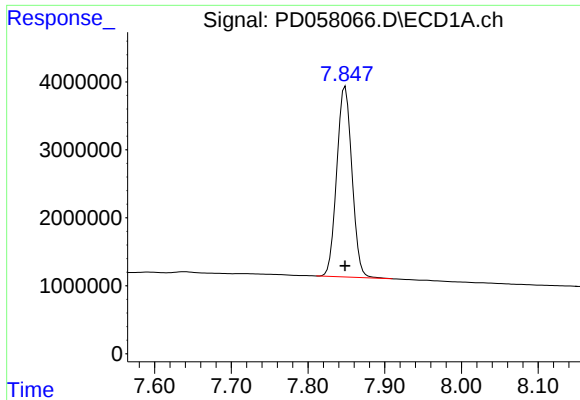

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 38637180
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

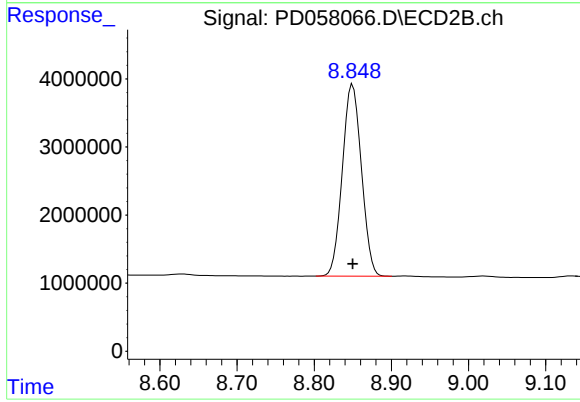

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 48311107
Conc: 50.00 ng/ml