

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
 Data File : PD058067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 13:10
 Operator : AJ\MA
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 13:37:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:16:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.867	20600487	27241001	24.723	25.258
28)	SA Decachlor...	7.848	8.850	20063743	25488249	25.964	26.379
Target Compounds							
23)	Chlordane-1	4.036	4.840	6322325	9963584	252.347	249.032
24)	Chlordane-2	4.521	5.301	8805211	12444714	285.184	266.174
25)	Chlordane-3	5.070	5.941	21998578	42259766	250.004	246.369
26)	Chlordane-4	5.125	6.014	21196284	51768853	253.577	249.425
27)	Chlordane-5	5.942	6.809	6511240	9137057	235.584	246.108



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
Data File : PD058067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 13:10
Operator : AJ\MA
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 13:37:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:16:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

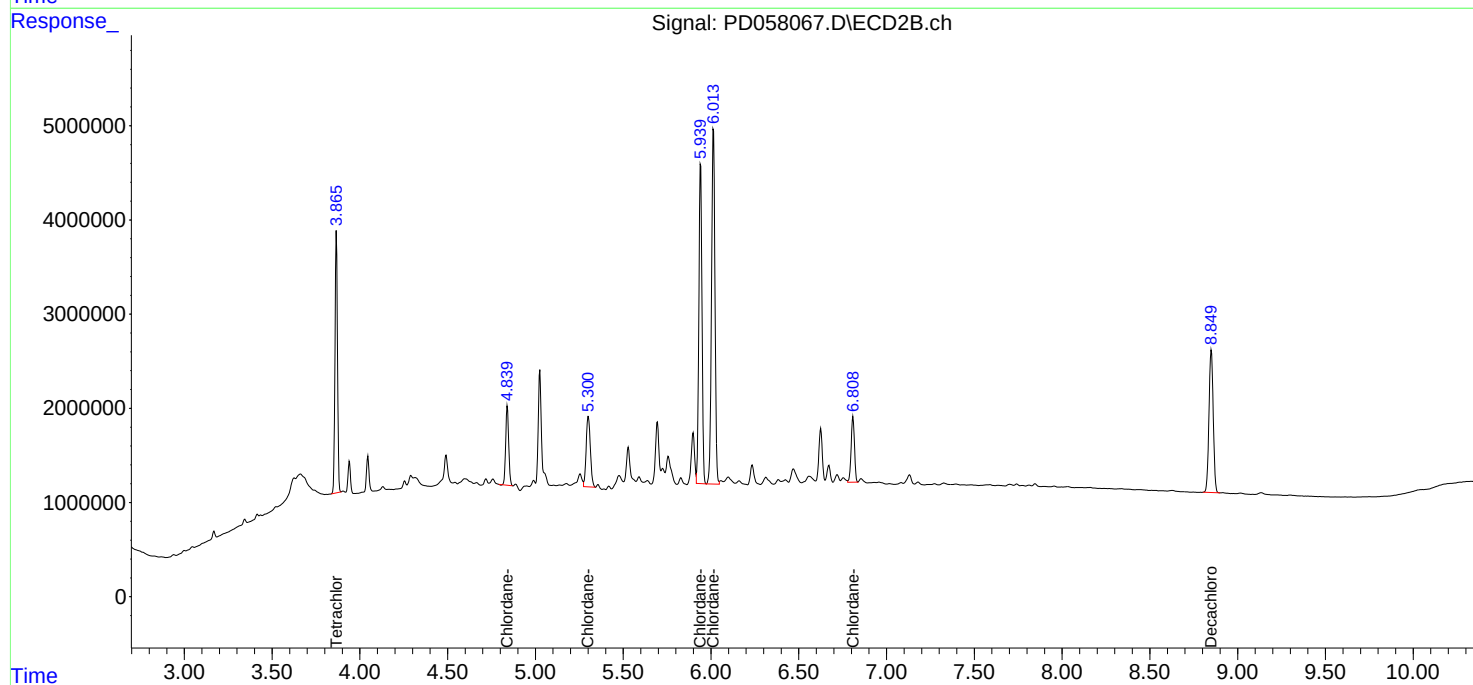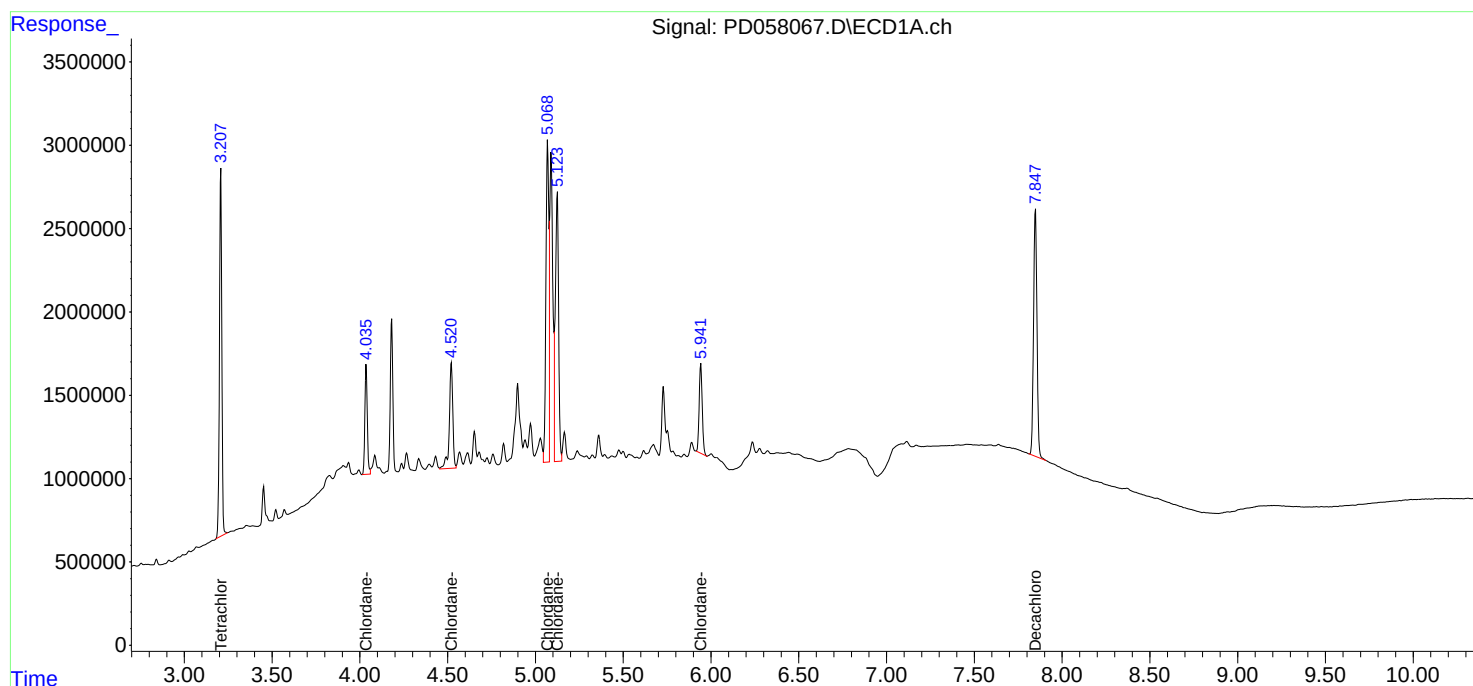


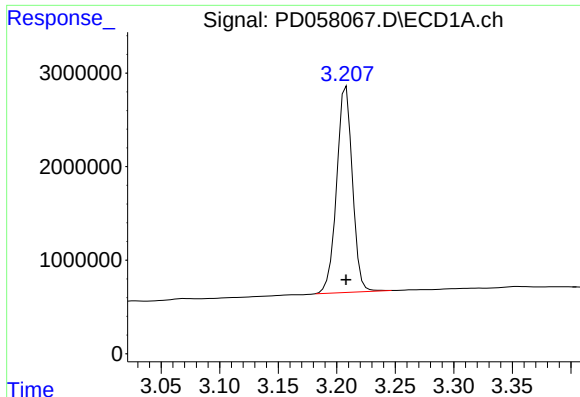

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 20600487
Conc: 24.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

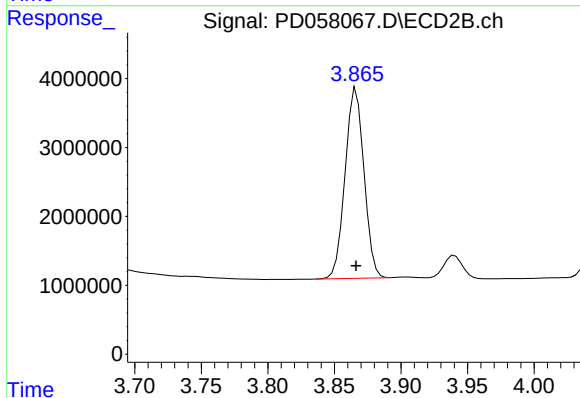


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 27241001
Conc: 25.26 ng/ml

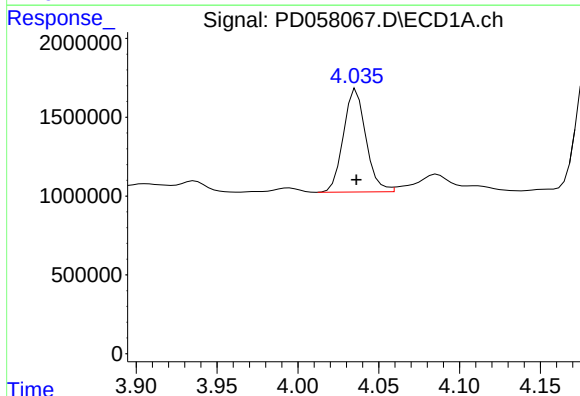


#23 Chlordane-1

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 6322325
Conc: 252.35 ng/ml

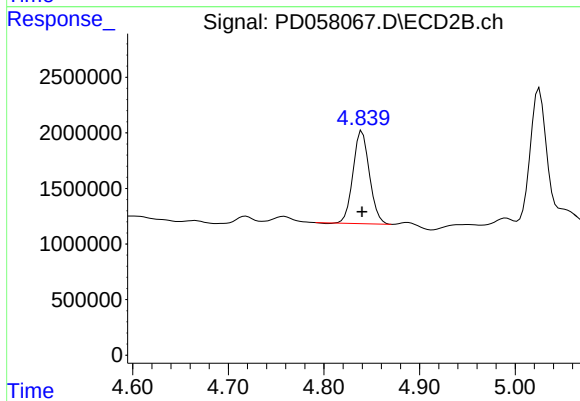

#23 Chlordane-1


R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 9963584
Conc: 249.03 ng/ml

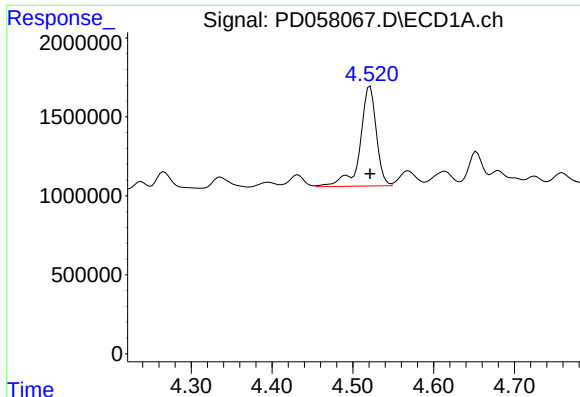

#24 Chlordane-2


R.T.: 4.521 min
Delta R.T.: 0.000 min
Response: 8805211
Conc: 285.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

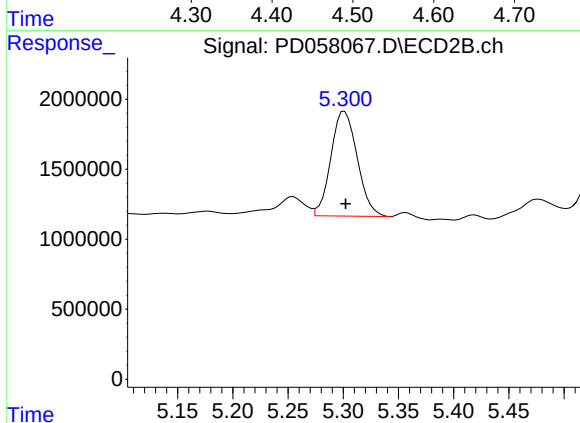


#24 Chlordane-2

R.T.: 5.301 min
Delta R.T.: -0.001 min
Response: 12444714
Conc: 266.17 ng/ml

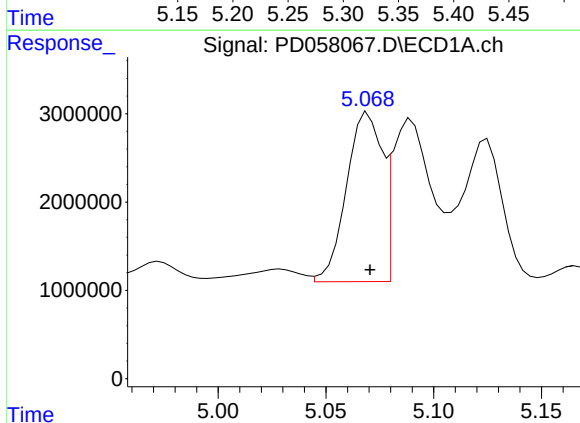


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 21998578
Conc: 250.00 ng/ml

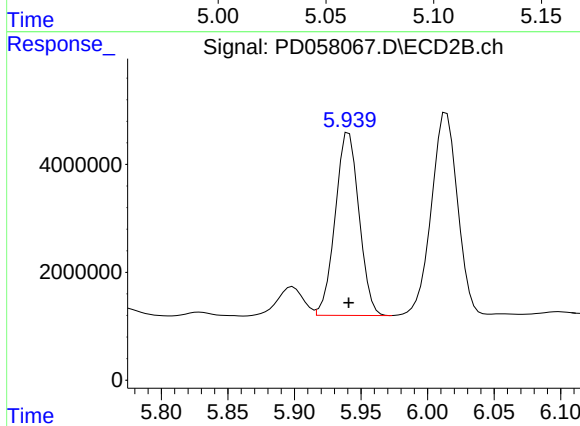

#25 Chlordane-3


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 42259766
Conc: 246.37 ng/ml

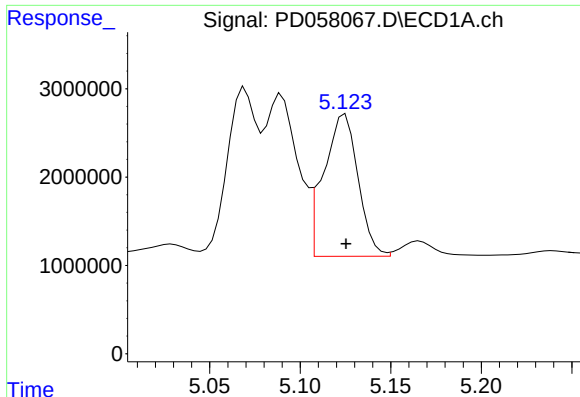

#26 Chlordane-4


R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 21196284
Conc: 253.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

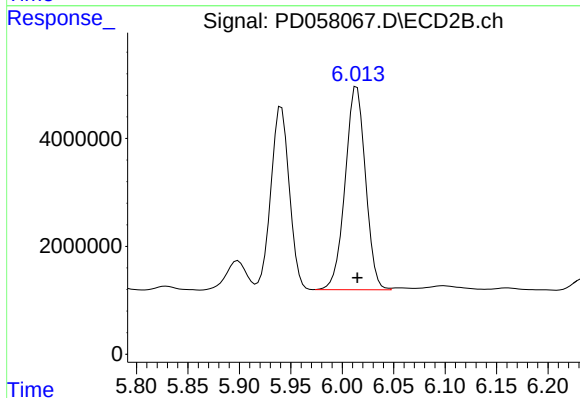


#26 Chlordane-4

R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 51768853
Conc: 249.43 ng/ml

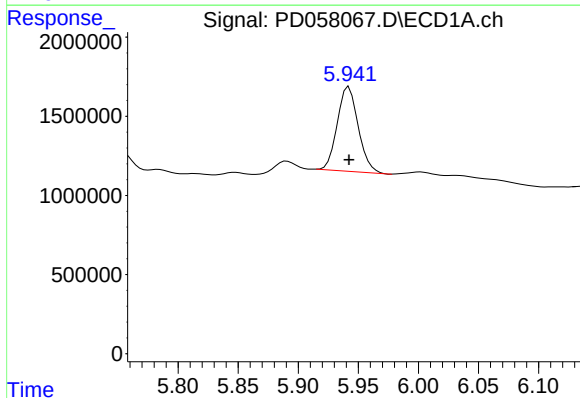


#27 Chlordane-5

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 6511240
Conc: 235.58 ng/ml

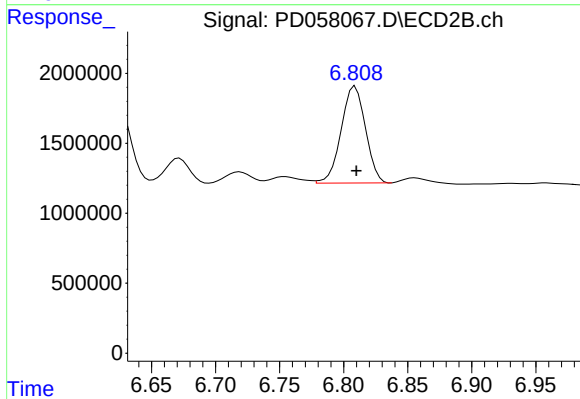

#27 Chlordane-5


R.T.: 6.809 min
Delta R.T.: 0.000 min
Response: 9137057
Conc: 246.11 ng/ml

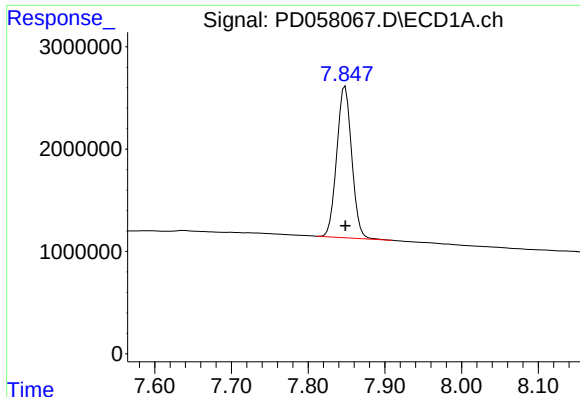

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 20063743
Conc: 25.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

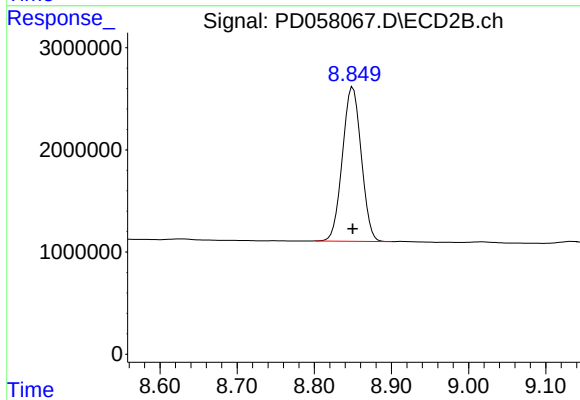

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 25488249
Conc: 26.38 ng/ml