

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
 Data File : PD058075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 15:02
 Operator : AJ\MA
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD052120CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 15:16:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	43441089	56411199	55.584	49.531
28)	SA Decachlor...	7.848	8.851	39769200	49046645	49.738	47.310
Target Compounds							
23)	Chlordane-1	4.037	4.840	13084005	20665855	503.337	522.661
24)	Chlordane-2	4.523	5.302	16070223	23982035	502.673	498.735
25)	Chlordane-3	5.071	5.941	46888488	88625173	523.136	515.404
26)	Chlordane-4	5.126	6.015	44415075	107.0E6	519.848	513.588
27)	Chlordane-5	5.944	6.810	14616448	19095931	541.130	517.976



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052120\
Data File : PD058075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 15:02
Operator : AJ\MA
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD052120CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 15:16:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

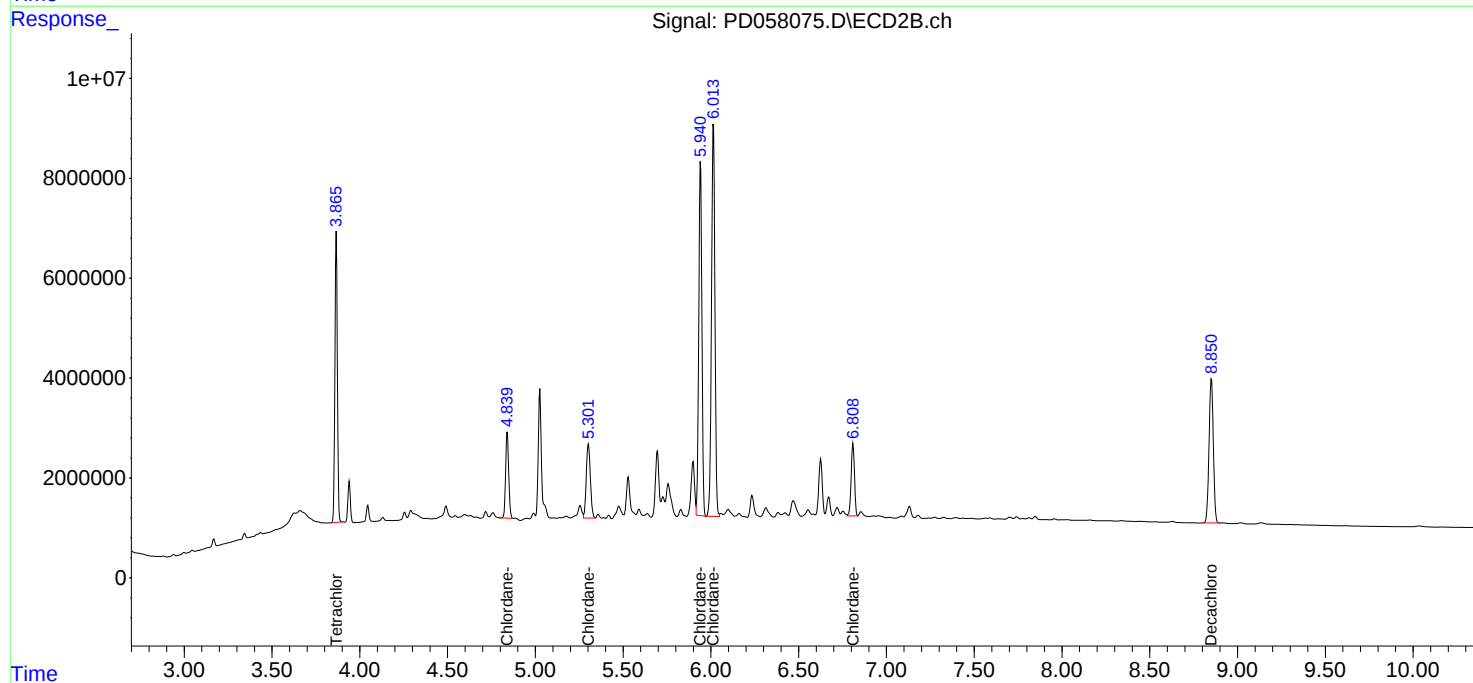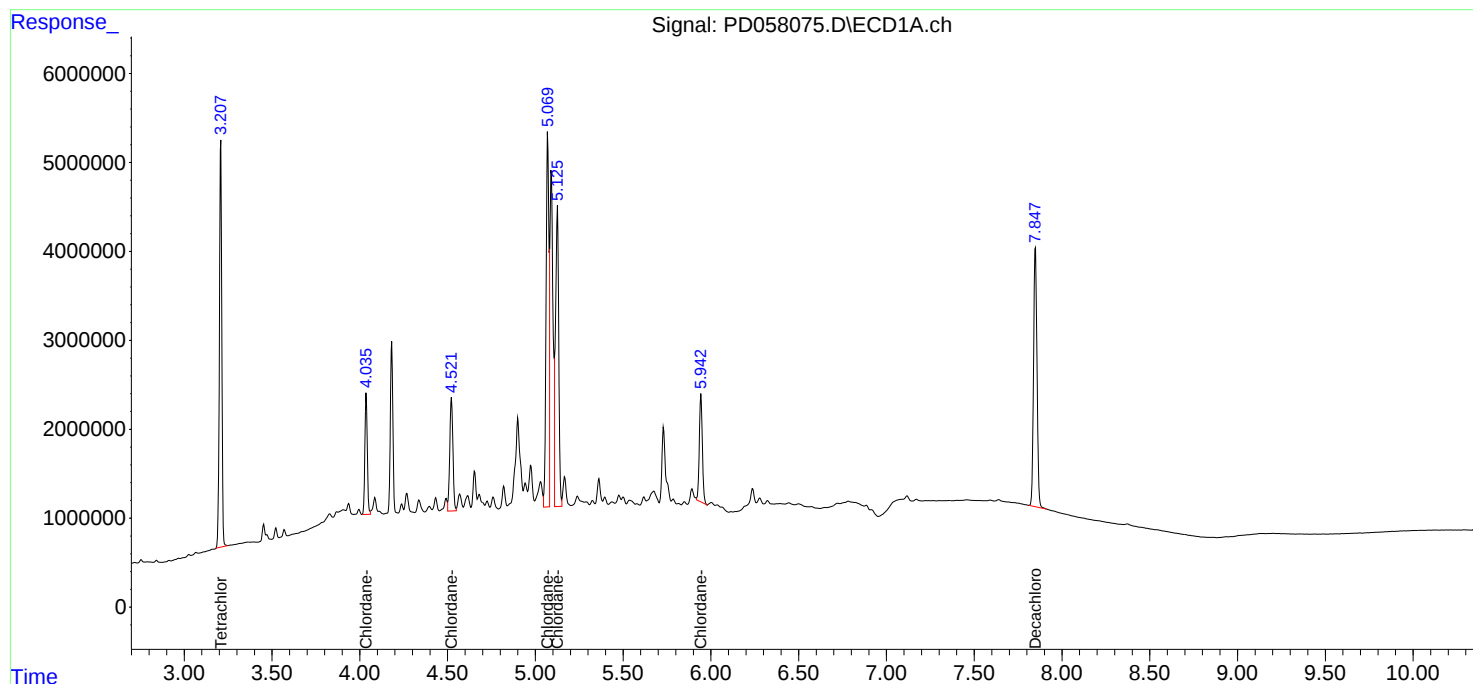


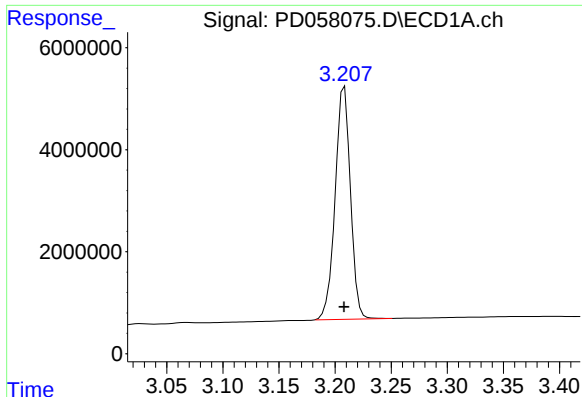

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 43441089
Conc: 55.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD052120CHLOR

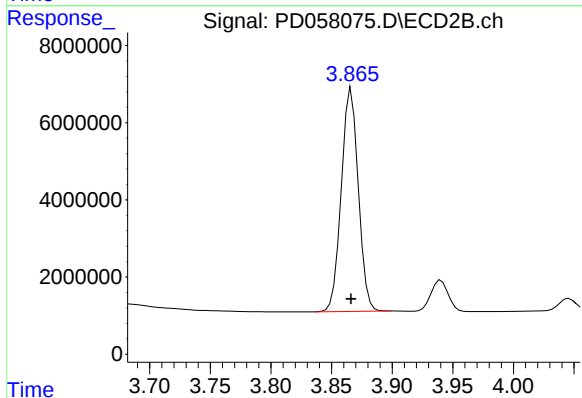


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 56411199
Conc: 49.53 ng/ml

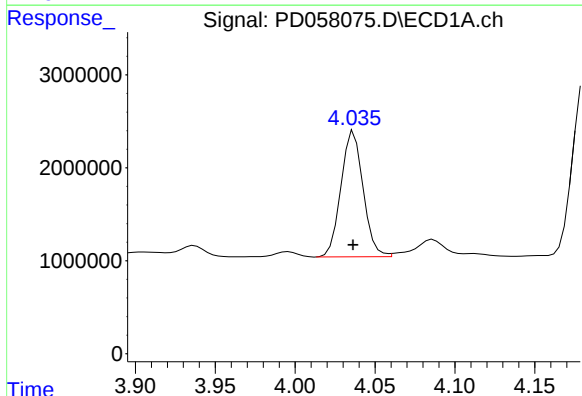


#23 Chlordane-1

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 13084005
Conc: 503.34 ng/ml

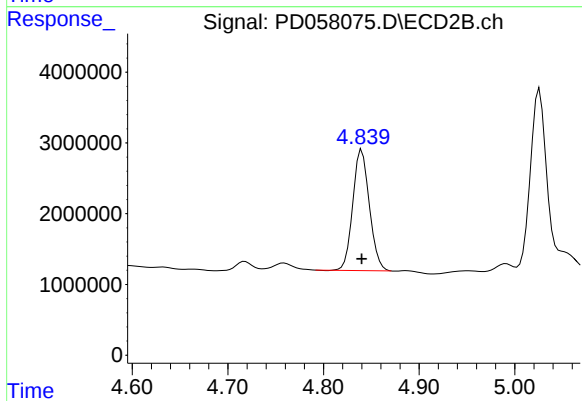

#23 Chlordane-1


R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 20665855
Conc: 522.66 ng/ml

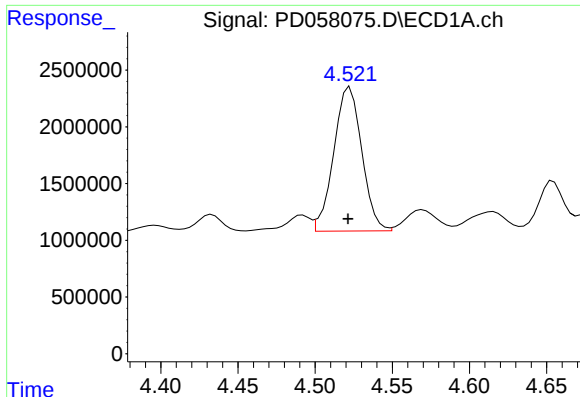

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.001 min
Response: 16070223
Conc: 502.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD052120CHLOR

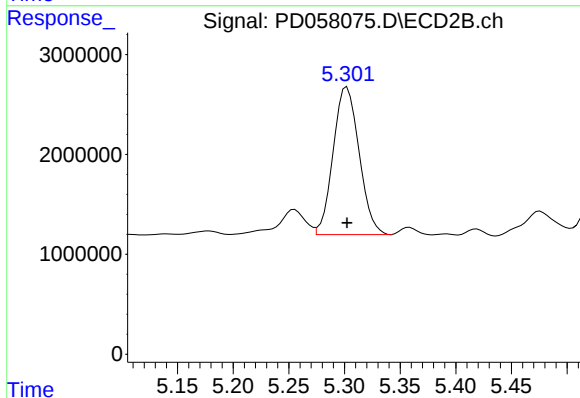


#24 Chlordane-2

R.T.: 5.302 min
Delta R.T.: 0.000 min
Response: 23982035
Conc: 498.73 ng/ml

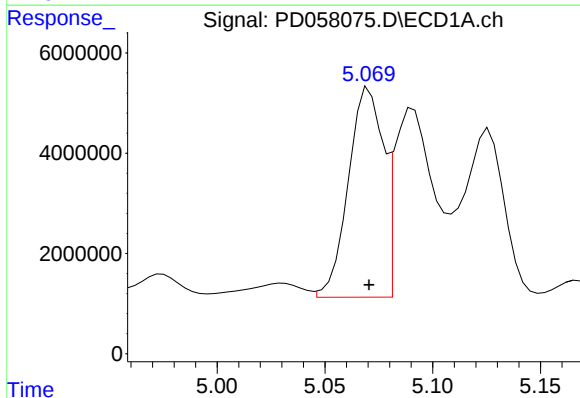


#25 Chlordane-3

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 46888488
Conc: 523.14 ng/ml

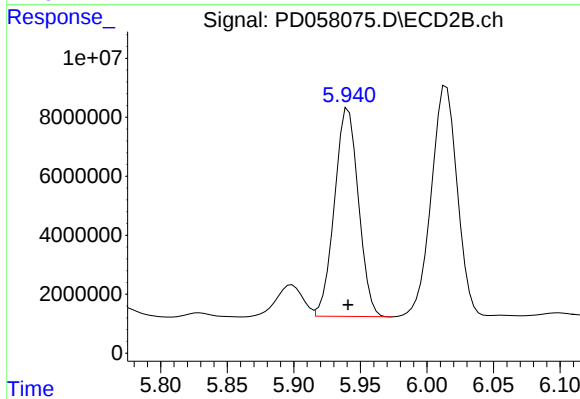

#25 Chlordane-3


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 88625173
Conc: 515.40 ng/ml

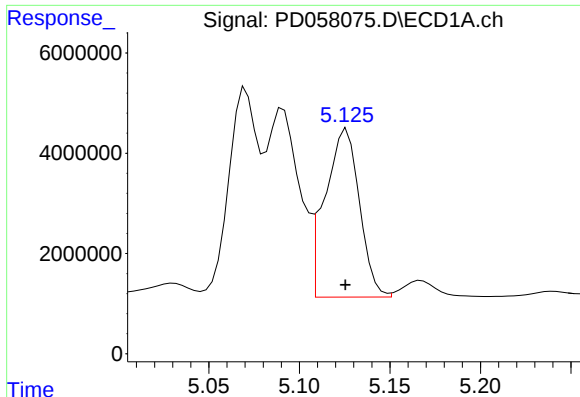

#26 Chlordane-4


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 44415075
Conc: 519.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD052120CHLOR

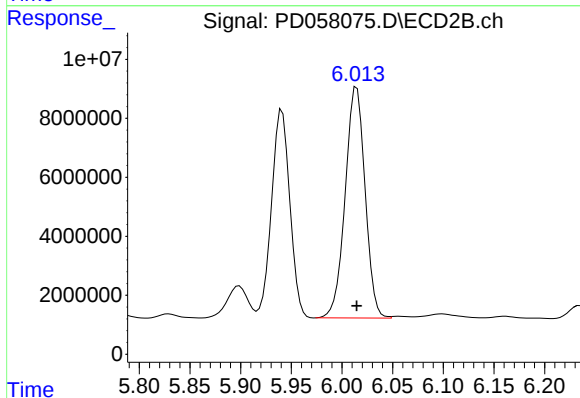


#26 Chlordane-4

R.T.: 6.015 min
Delta R.T.: 0.000 min
Response: 107025086
Conc: 513.59 ng/ml

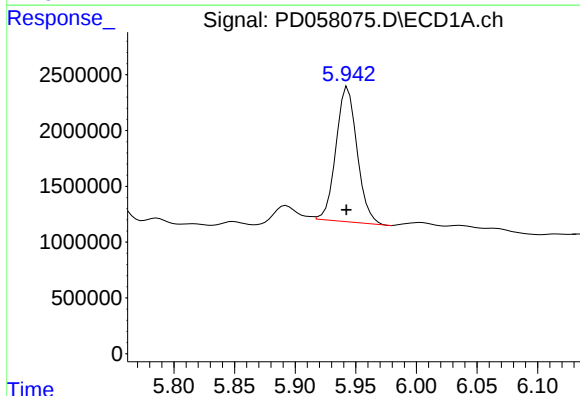


#27 Chlordane-5

R.T.: 5.944 min
Delta R.T.: 0.001 min
Response: 14616448
Conc: 541.13 ng/ml

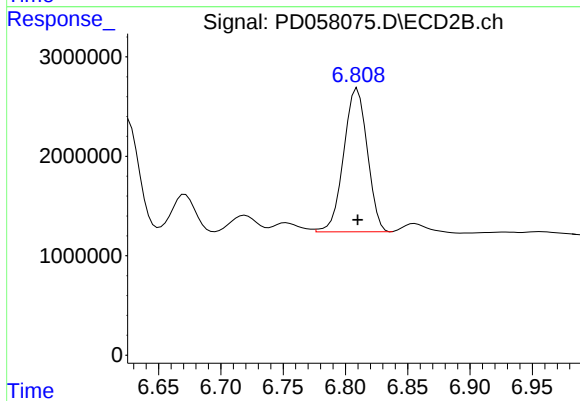

#27 Chlordane-5


R.T.: 6.810 min
Delta R.T.: 0.000 min
Response: 19095931
Conc: 517.98 ng/ml

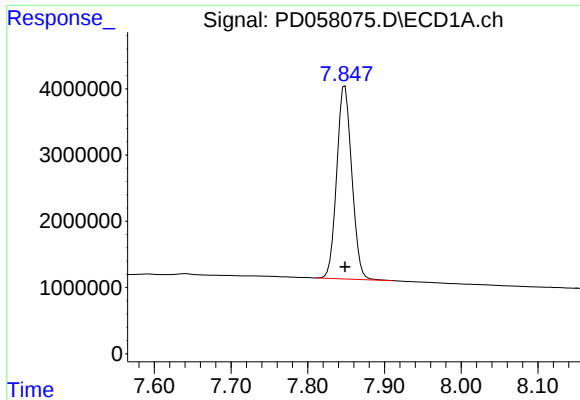

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 39769200
Conc: 49.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD052120CHLOR

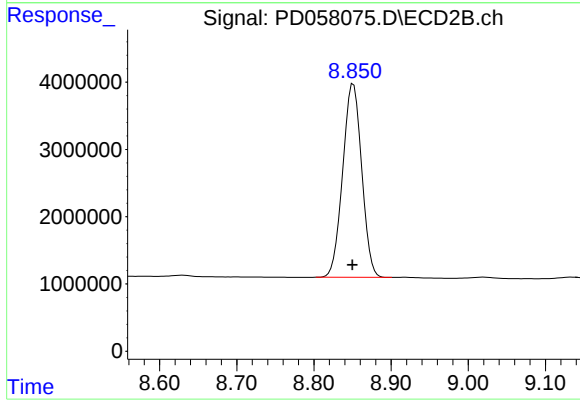

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: 0.001 min
Response: 49046645
Conc: 47.31 ng/ml