

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
 Data File : PD063148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 11:45
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 14:19:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 20 14:10:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	5850344	61977506	5.128	5.116
27)	SA Decachlor...	8.193	9.021	13614835	119.5E6	10.206	10.436
Target Compounds							
2)	A alpha-BHC	3.875	4.357	8063110	87730807	4.801	4.803
3)	MA gamma-BHC...	4.158	4.642	8051104	87767709	5.031	5.067
4)	MA Heptachlor	4.459	5.149	7567012	89083788	4.808	5.074
9)	A Endosulfan I	5.488	6.195	6559758	75942291	4.908	5.158
13)	MA Dieldrin	5.731	6.452	14176362	158.6E6	9.262	10.074
14)	MA Endrin	5.989	6.669	13242329	134.9E6	9.817	10.352
16)	A 4,4'-DDD	6.115	6.792	10956878	124.1E6	9.011	10.053
17)	MA 4,4'-DDT	6.356	7.090	10537310	125.8E6	8.470	10.347
20)	A Methoxychlor	6.902	7.548	35414322	308.7E6	48.786	53.241


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
Data File : PD063148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 11:45
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 14:19:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 20 14:10:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

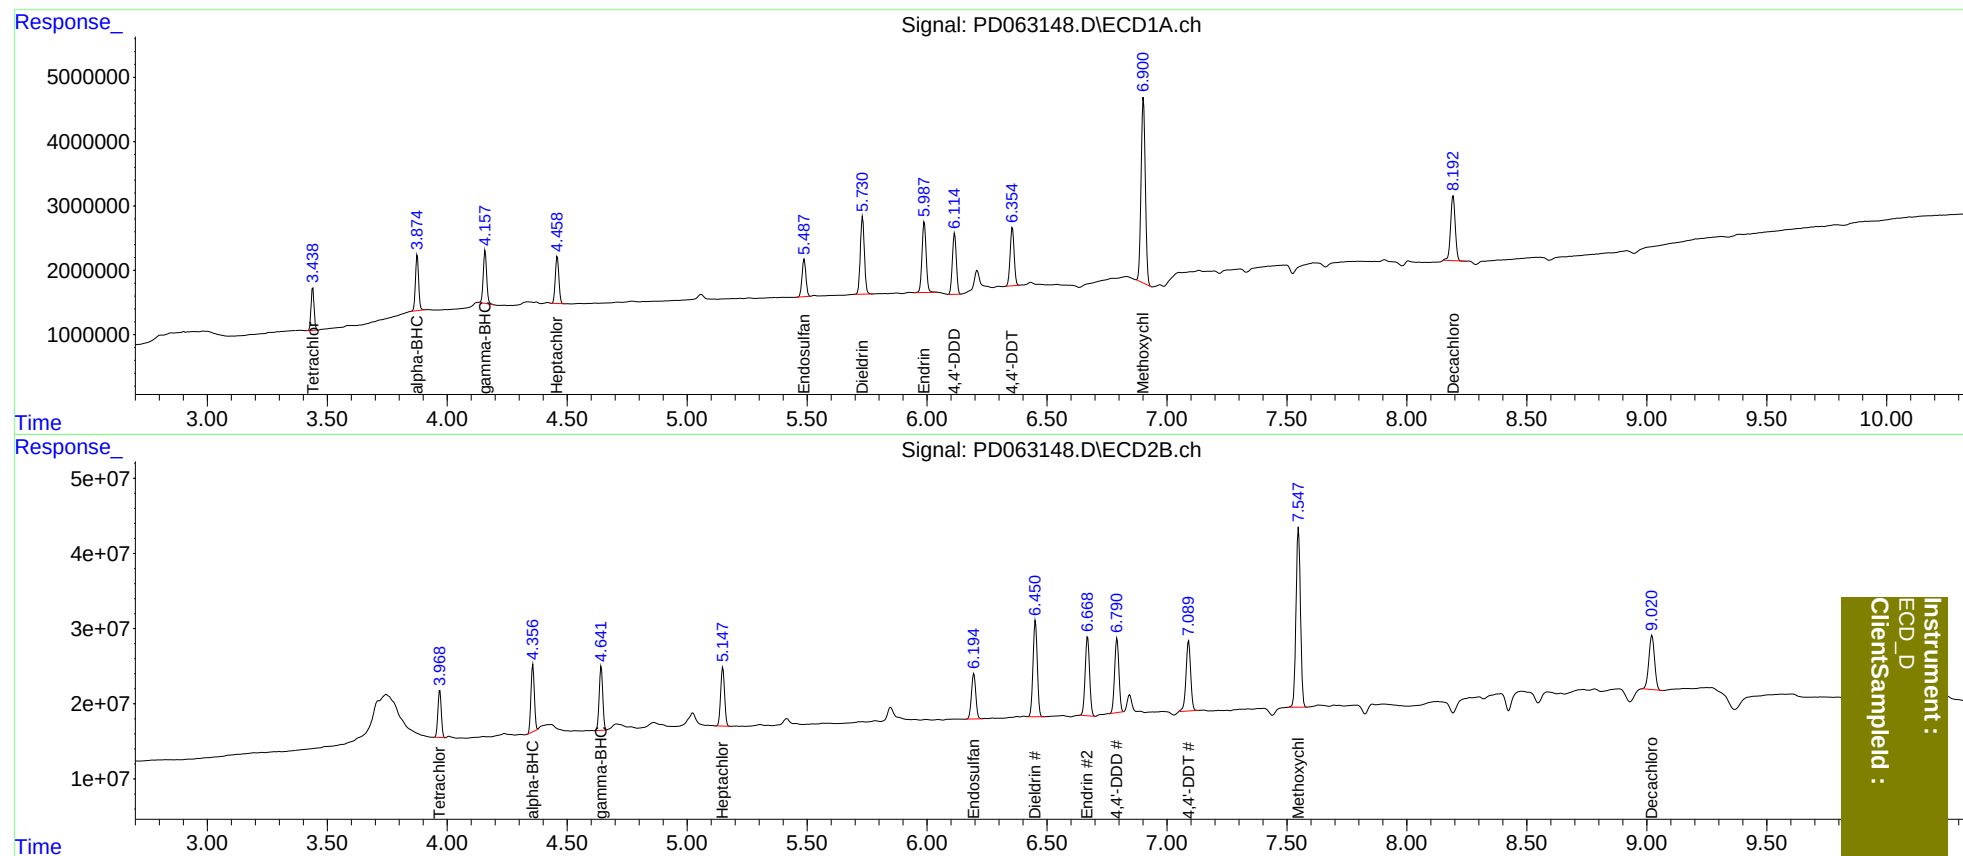


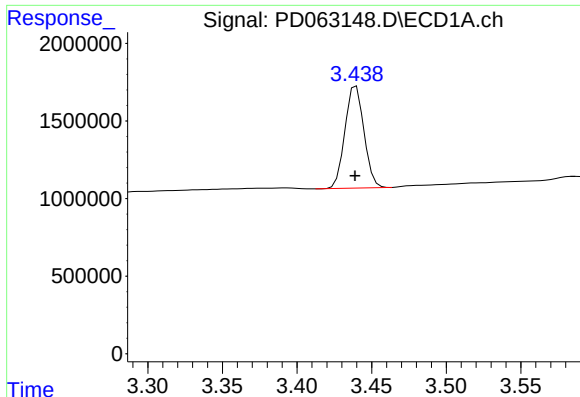

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 5850344
Conc: 5.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

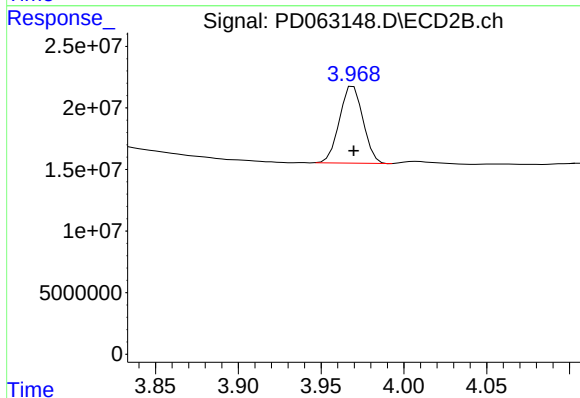


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 61977506
Conc: 5.12 ng/ml

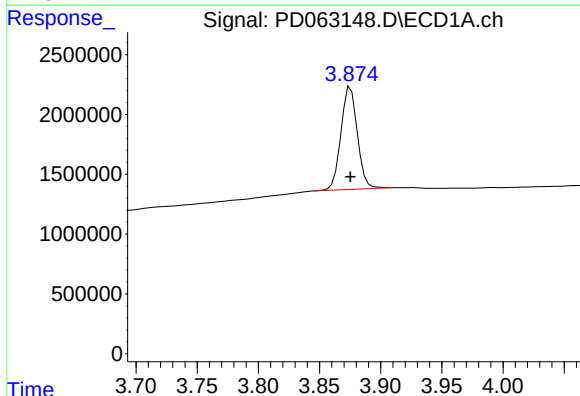


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 8063110
Conc: 4.80 ng/ml

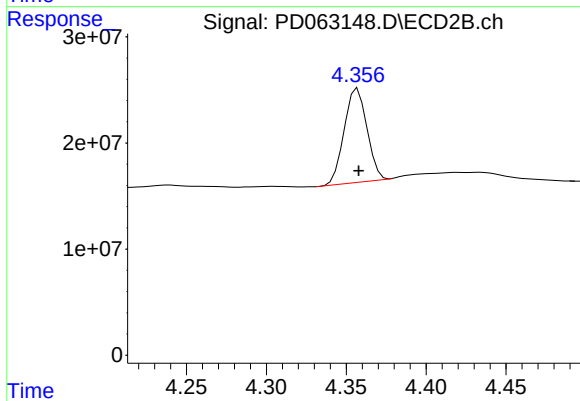

#2 alpha-BHC


R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 87730807
Conc: 4.80 ng/ml

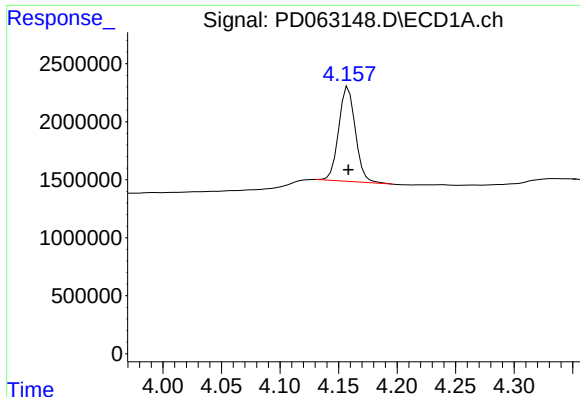

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 8051104
Conc: 5.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

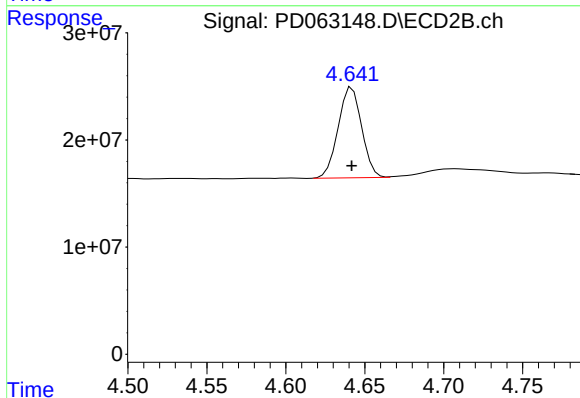


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 87767709
Conc: 5.07 ng/ml

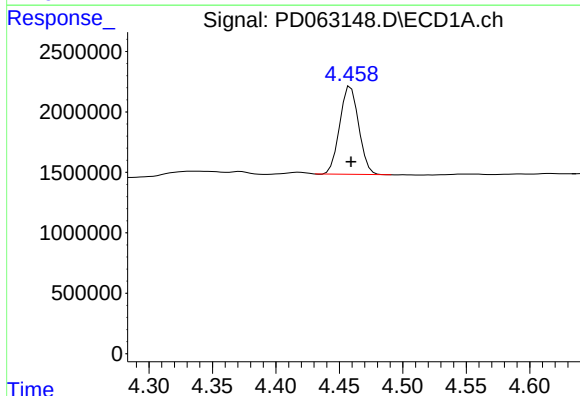


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 7567012
Conc: 4.81 ng/ml

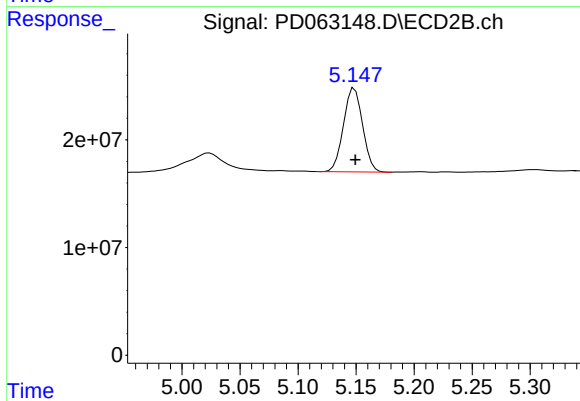

#4 Heptachlor


R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 89083788
Conc: 5.07 ng/ml

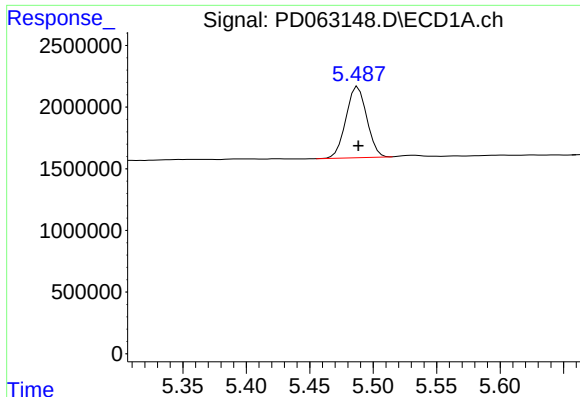

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 6559758
Conc: 4.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

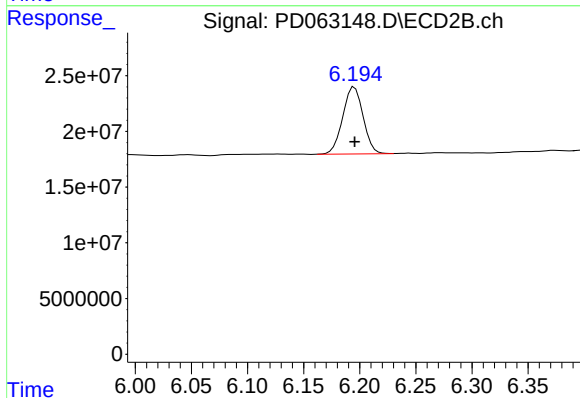


#9 Endosulfan I

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 75942291
Conc: 5.16 ng/ml

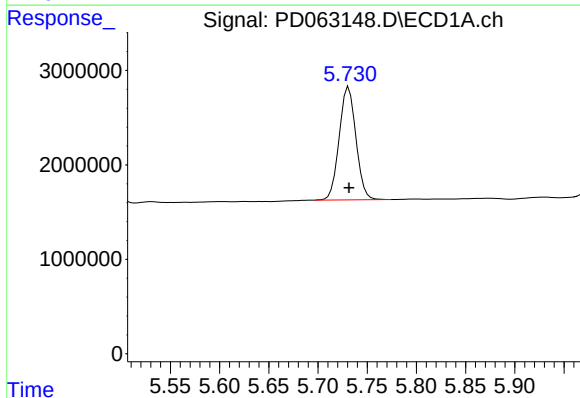


#13 Dieldrin

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 14176362
Conc: 9.26 ng/ml

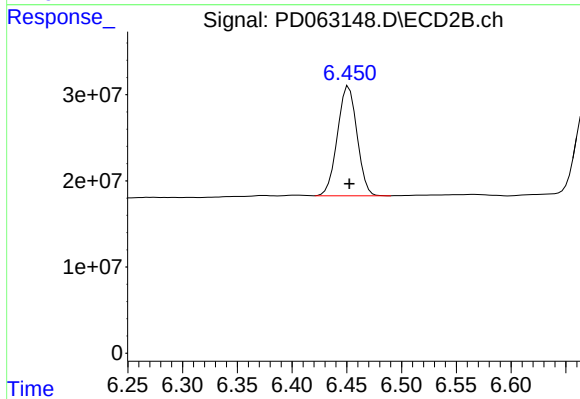

#13 Dieldrin


R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 158611572
Conc: 10.07 ng/ml

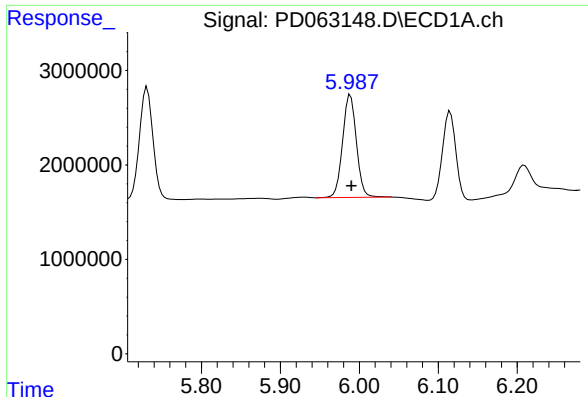

#14 Endrin


R.T.: 5.989 min
Delta R.T.: -0.001 min
Response: 13242329
Conc: 9.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

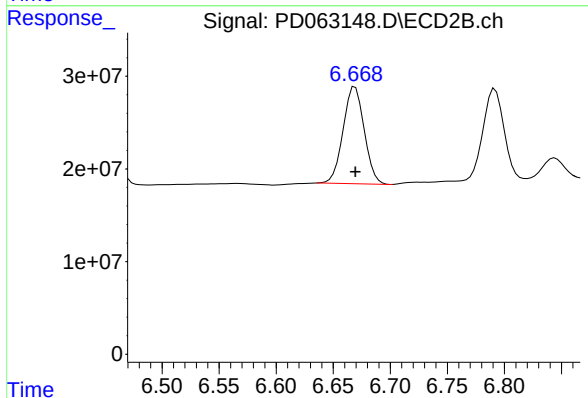


#14 Endrin

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 134869468
Conc: 10.35 ng/ml

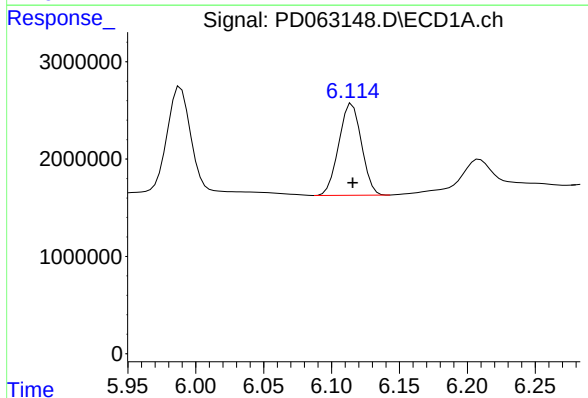


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 10956878
Conc: 9.01 ng/ml

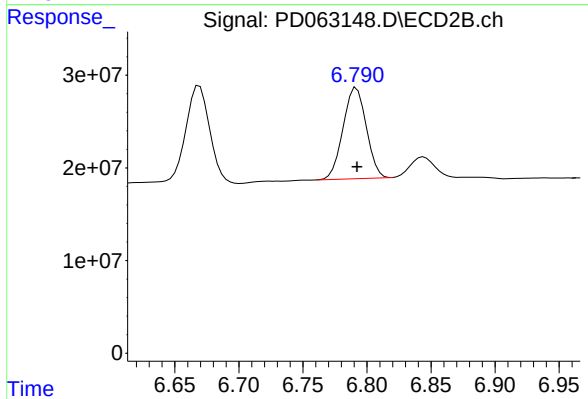

#16 4,4'-DDD


R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 124062644
Conc: 10.05 ng/ml

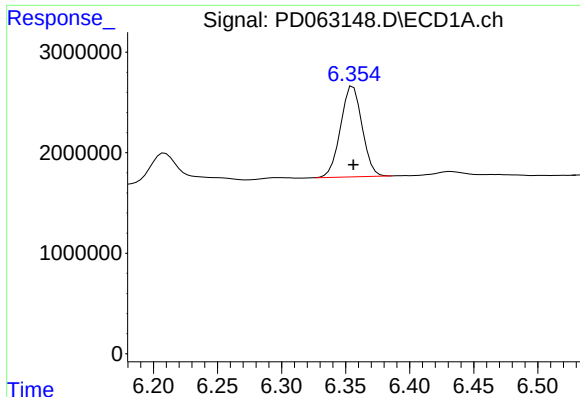

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 10537310
Conc: 8.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

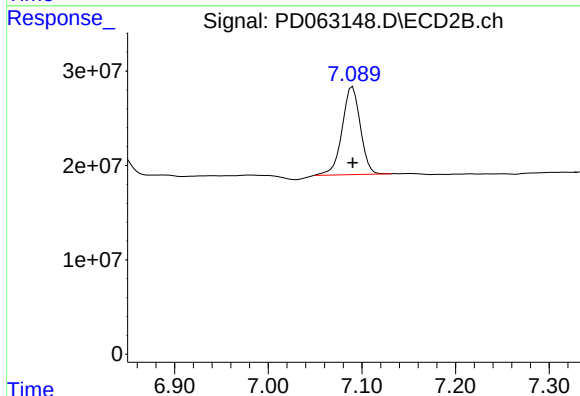


#17 4,4'-DDT

R.T.: 7.090 min
Delta R.T.: 0.000 min
Response: 125840603
Conc: 10.35 ng/ml

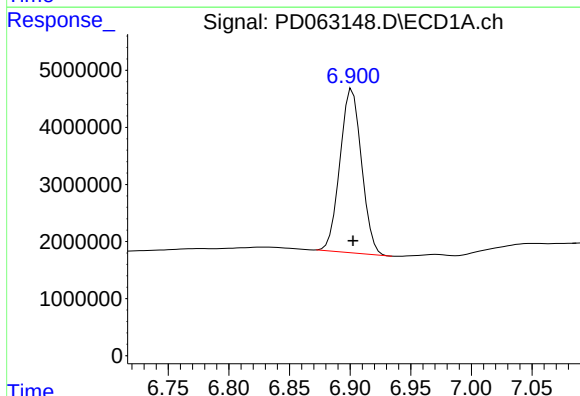


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 35414322
Conc: 48.79 ng/ml

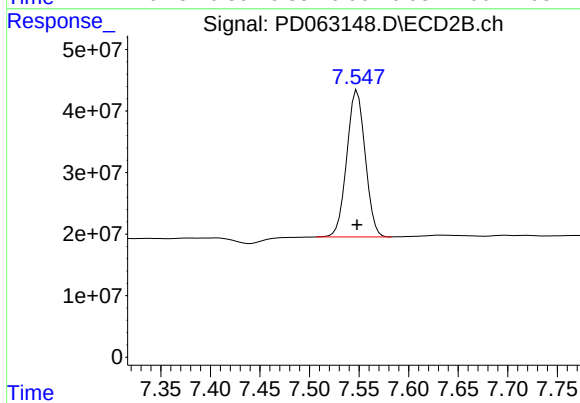

#20 Methoxychlor


R.T.: 7.548 min
Delta R.T.: 0.000 min
Response: 308719293
Conc: 53.24 ng/ml

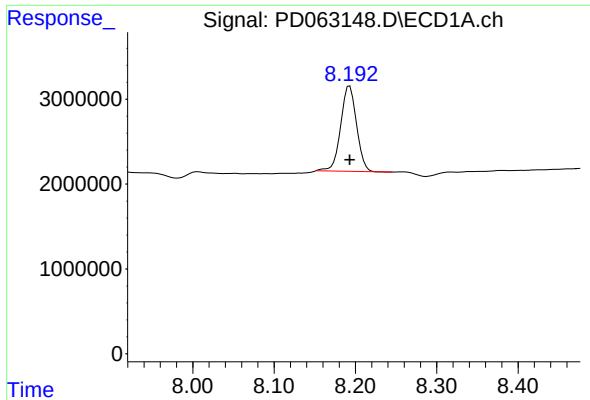

#27 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 13614835
Conc: 10.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

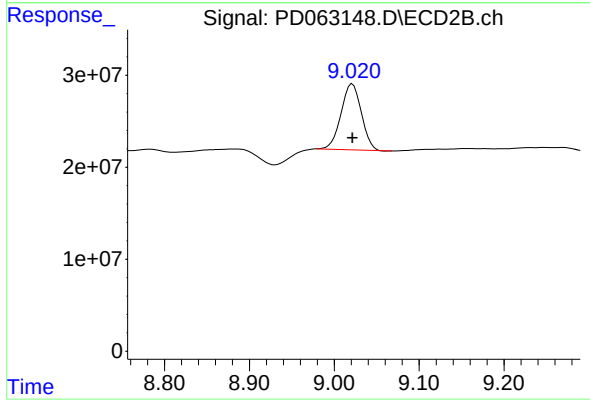

#27 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 119518029
Conc: 10.44 ng/ml