

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
 Data File : PD063150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 12:13
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 14:20:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 20 14:10:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	11578485	126.1E6	10.150	10.407
27)	SA Decachlor...	8.194	9.022	26935866	230.7E6	20.191	20.148
Target Compounds							
2)	A alpha-BHC	3.875	4.358	16330032	182.9E6	9.723	10.012
3)	MA gamma-BHC...	4.158	4.642	15902427	177.5E6	9.937	10.247
4)	MA Heptachlor	4.459	5.149	15514666	180.4E6	9.858	10.277
9)	A Endosulfan I	5.489	6.195	13231495	151.6E6	9.900	10.296
13)	MA Dieldrin	5.732	6.452	29510434	324.7E6	19.280	20.625
14)	MA Endrin	5.989	6.669	26458843	268.2E6	19.615	20.588
16)	A 4,4'-DDD	6.115	6.792	23249291	253.4E6	19.120	20.529
17)	MA 4,4'-DDT	6.356	7.090	23138062	247.4E6	18.598	20.342
20)	A Methoxychlor	6.903	7.549	72401577	611.6E6	99.738	105.478

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
Data File : PD063150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 12:13
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 14:20:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 20 14:10:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

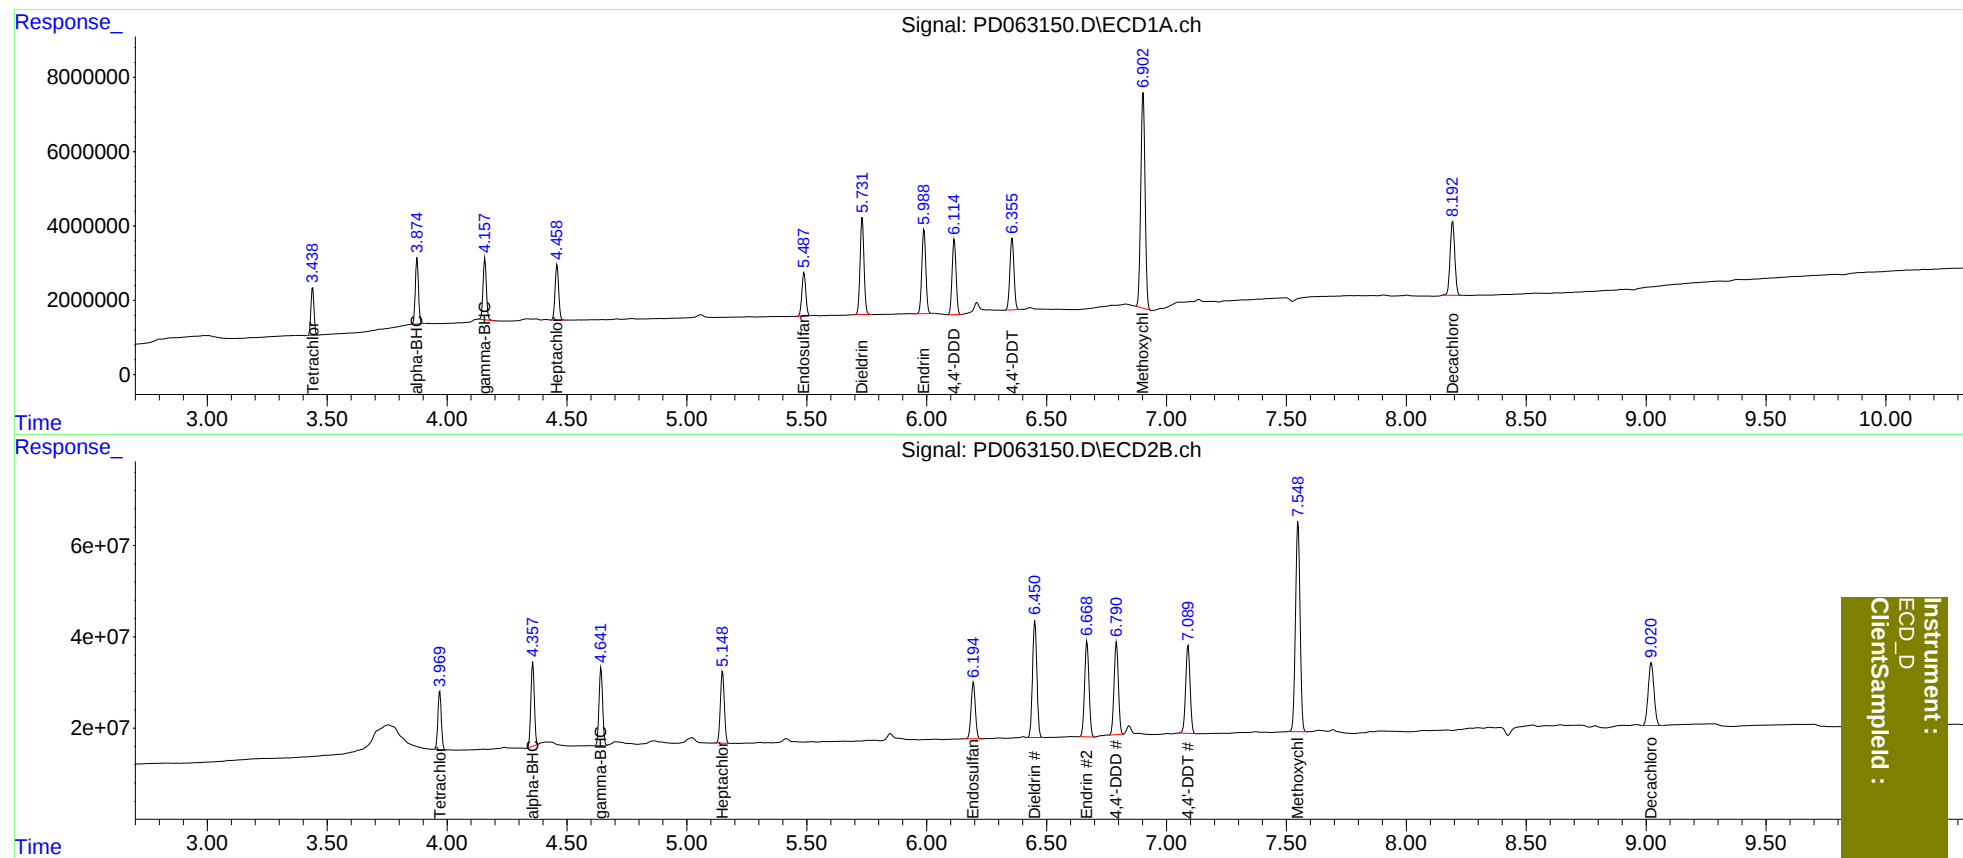


Instrument :
ECD_D
ClientSampled :

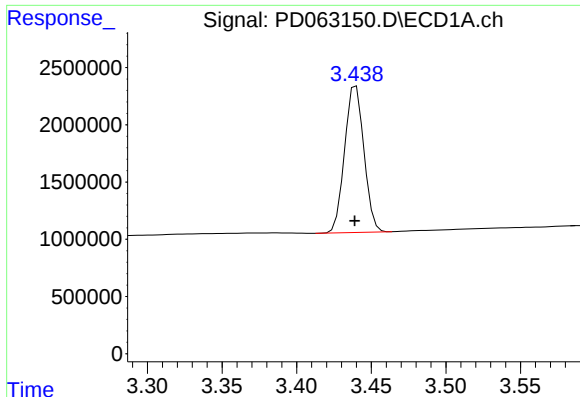

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 11578485
Conc: 10.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

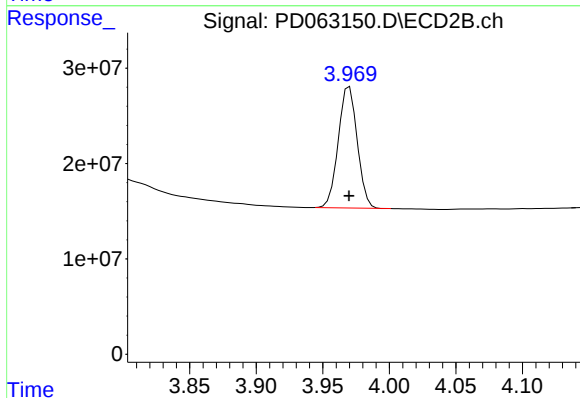


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 126070590
Conc: 10.41 ng/ml

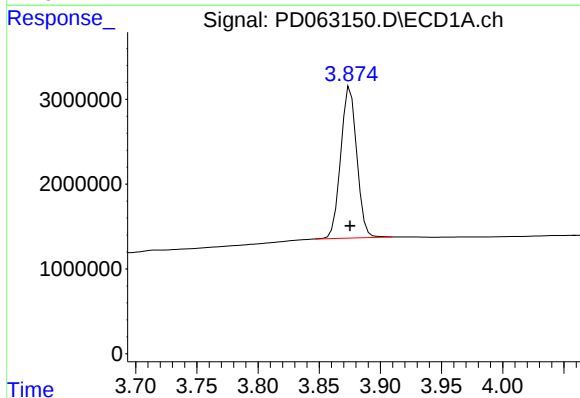


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 16330032
Conc: 9.72 ng/ml

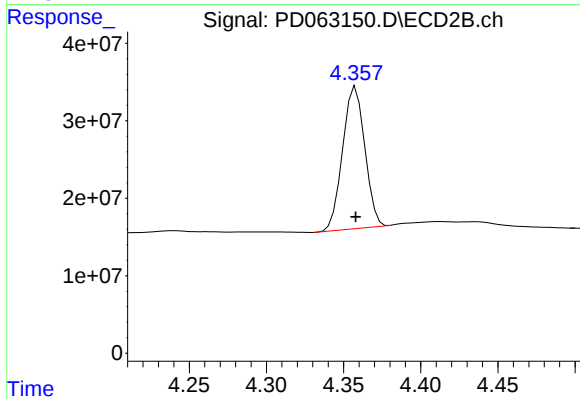

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 182863599
Conc: 10.01 ng/ml

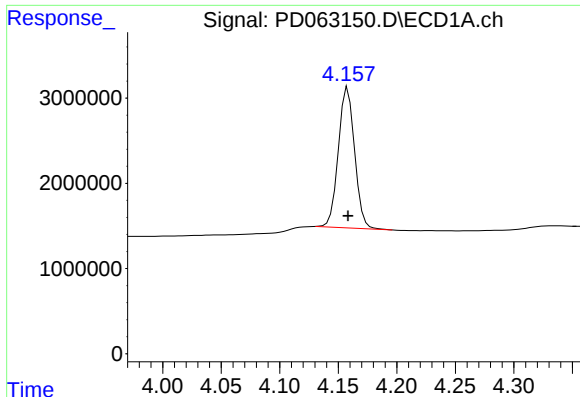

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 15902427
Conc: 9.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

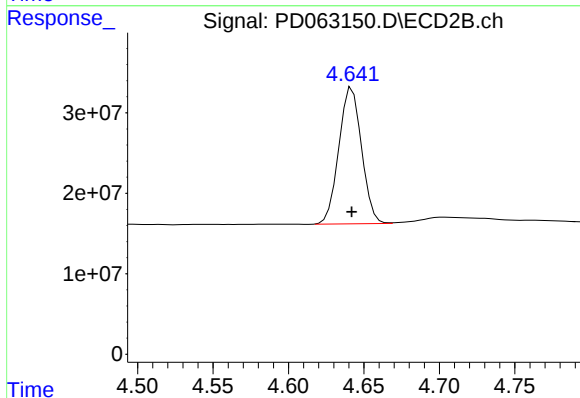


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 177473338
Conc: 10.25 ng/ml

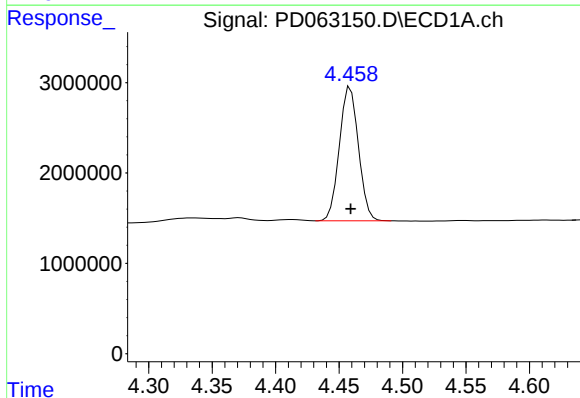


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 15514666
Conc: 9.86 ng/ml

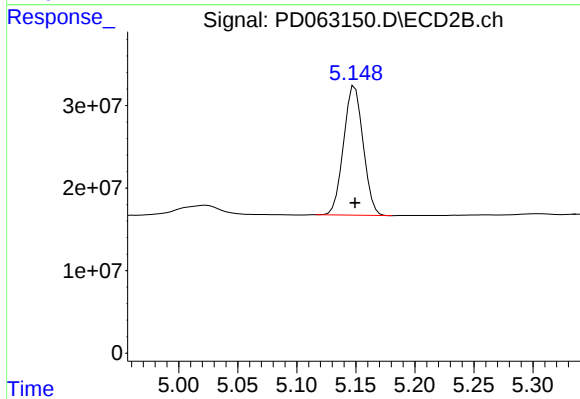

#4 Heptachlor


R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 180439575
Conc: 10.28 ng/ml

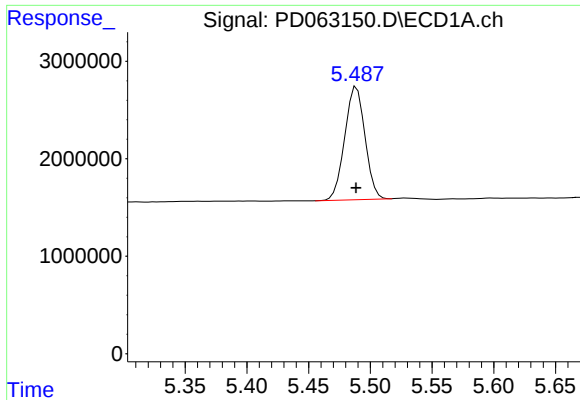

#9 Endosulfan I


R.T.: 5.489 min
Delta R.T.: 0.000 min
Response: 13231495
Conc: 9.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

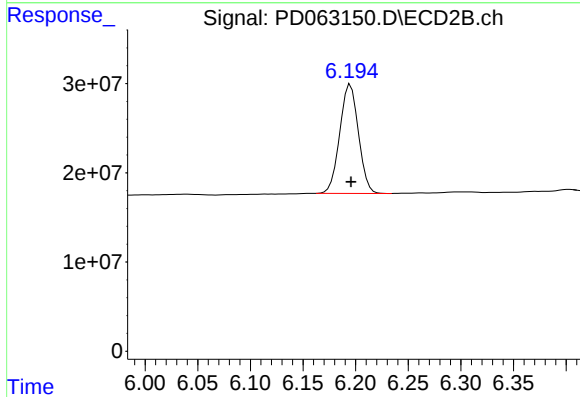


#9 Endosulfan I

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 151591667
Conc: 10.30 ng/ml

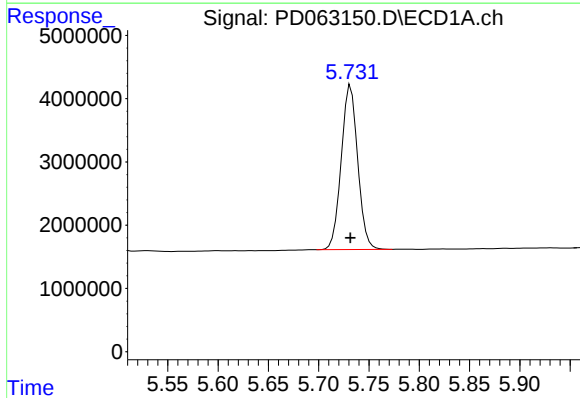


#13 Dieldrin

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 29510434
Conc: 19.28 ng/ml

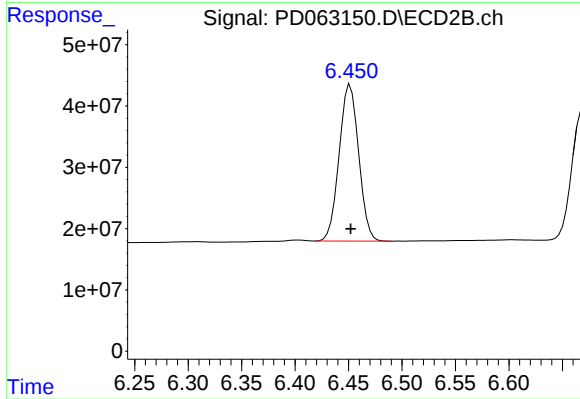

#13 Dieldrin


R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 324734930
Conc: 20.63 ng/ml

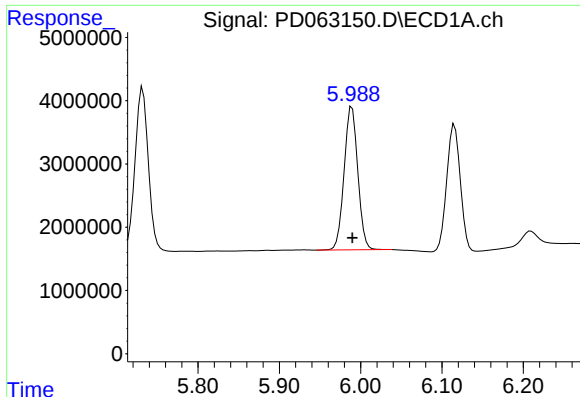

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 26458843
Conc: 19.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

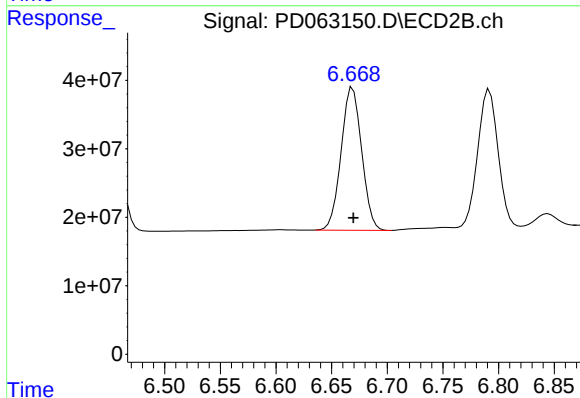


#14 Endrin

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 268223255
Conc: 20.59 ng/ml

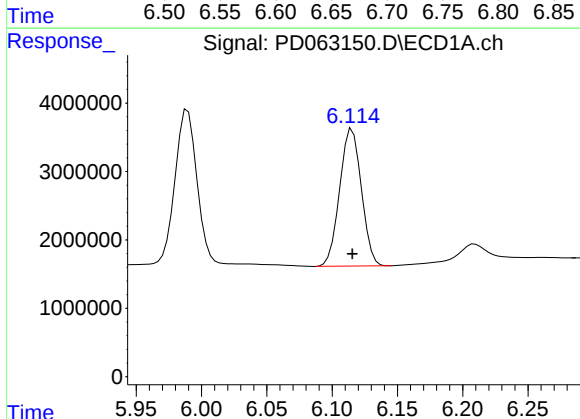


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 23249291
Conc: 19.12 ng/ml

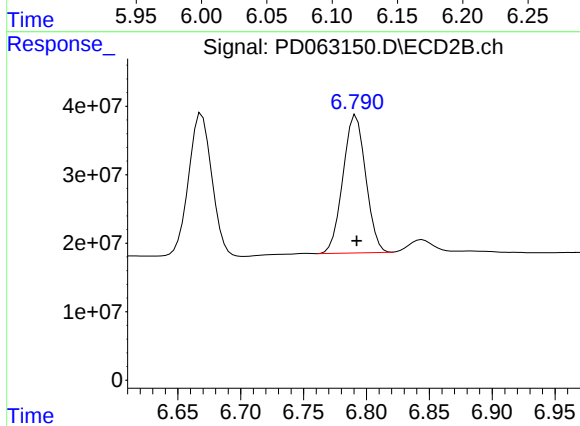

#16 4,4'-DDD


R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 253355576
Conc: 20.53 ng/ml

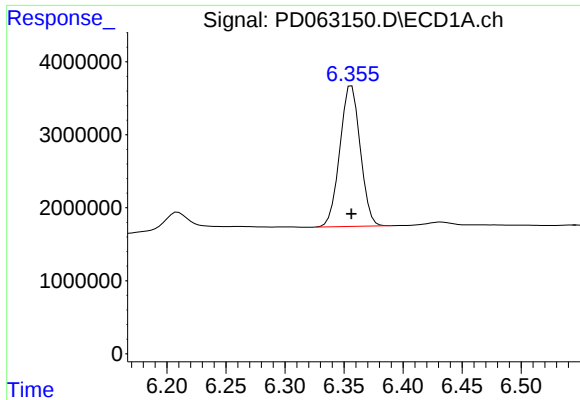

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 23138062
Conc: 18.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

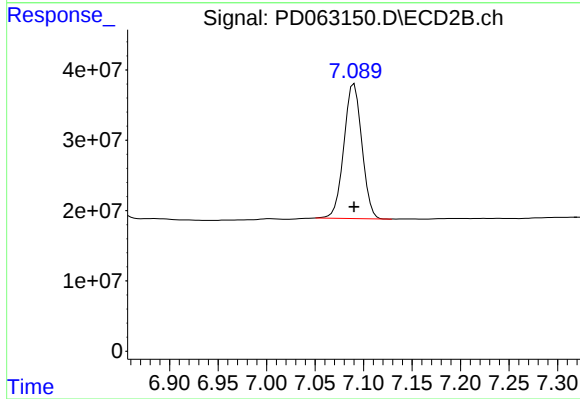


#17 4,4'-DDT

R.T.: 7.090 min
Delta R.T.: 0.000 min
Response: 247393129
Conc: 20.34 ng/ml

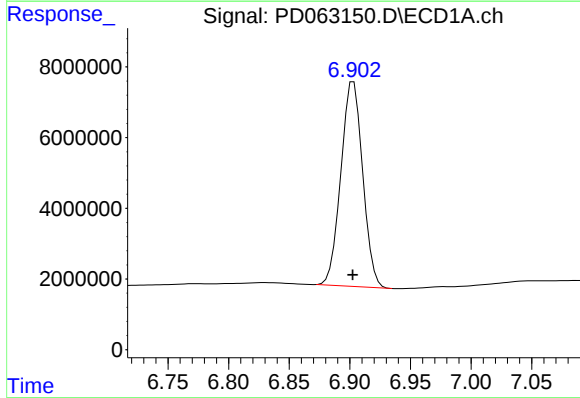


#20 Methoxychlor

R.T.: 6.903 min
Delta R.T.: 0.000 min
Response: 72401577
Conc: 99.74 ng/ml

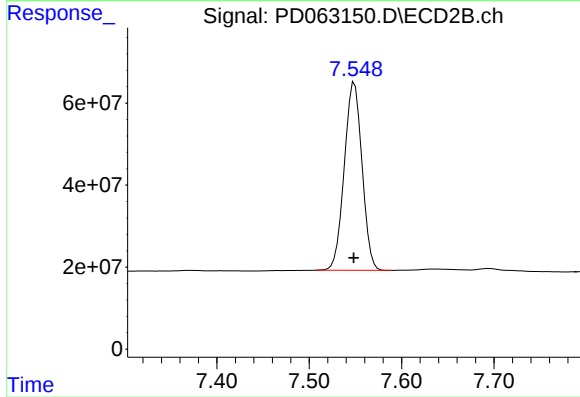

#20 Methoxychlor


R.T.: 7.549 min
Delta R.T.: 0.000 min
Response: 611610654
Conc: 105.48 ng/ml

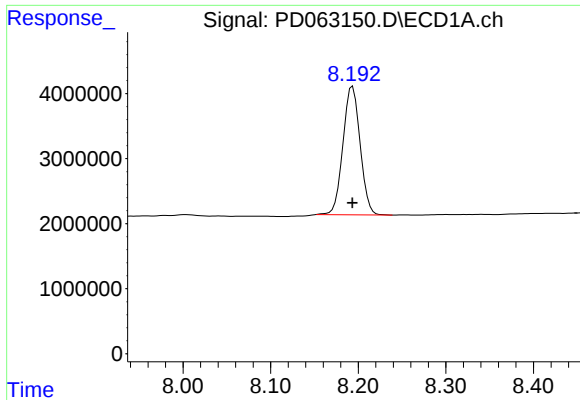

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 26935866
Conc: 20.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

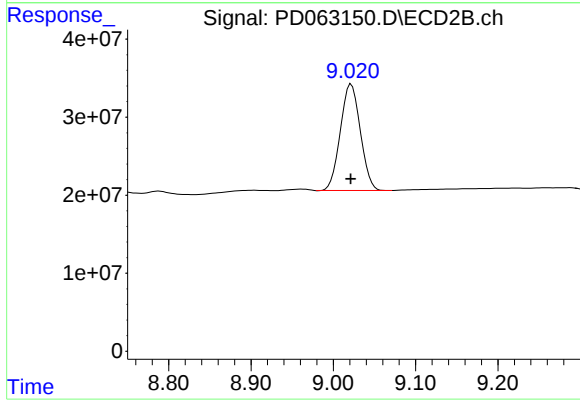

#27 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 230742123
Conc: 20.15 ng/ml