

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
 Data File : PD063152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 12:41
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 14:11:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 20 14:10:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	22815673	242.3E6	20.000	20.000
27)	SA Decachlor...	8.193	9.021	53360848	458.1E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.875	4.358	33589709	365.3E6	20.000	20.000
3)	MA gamma-BHC...	4.158	4.642	32006353	346.4E6	20.000	20.000
4)	MA Heptachlor	4.459	5.149	31476865	351.1E6	20.000	20.000
9)	A Endosulfan I	5.488	6.196	26729717	294.5E6	20.000	20.000
13)	MA Dieldrin	5.732	6.452	61225138	629.8E6	40.000	40.000
14)	MA Endrin	5.990	6.669	53955892	521.1E6	40.000	40.000
16)	A 4,4'-DDD	6.115	6.792	48638215	493.7E6	40.000	40.000
17)	MA 4,4'-DDT	6.356	7.090	49765229	486.5E6	40.000	40.000
20)	A Methoxychlor	6.902	7.548	145.2E6	1159.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
Data File : PD063152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 12:41
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 14:11:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 20 14:10:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

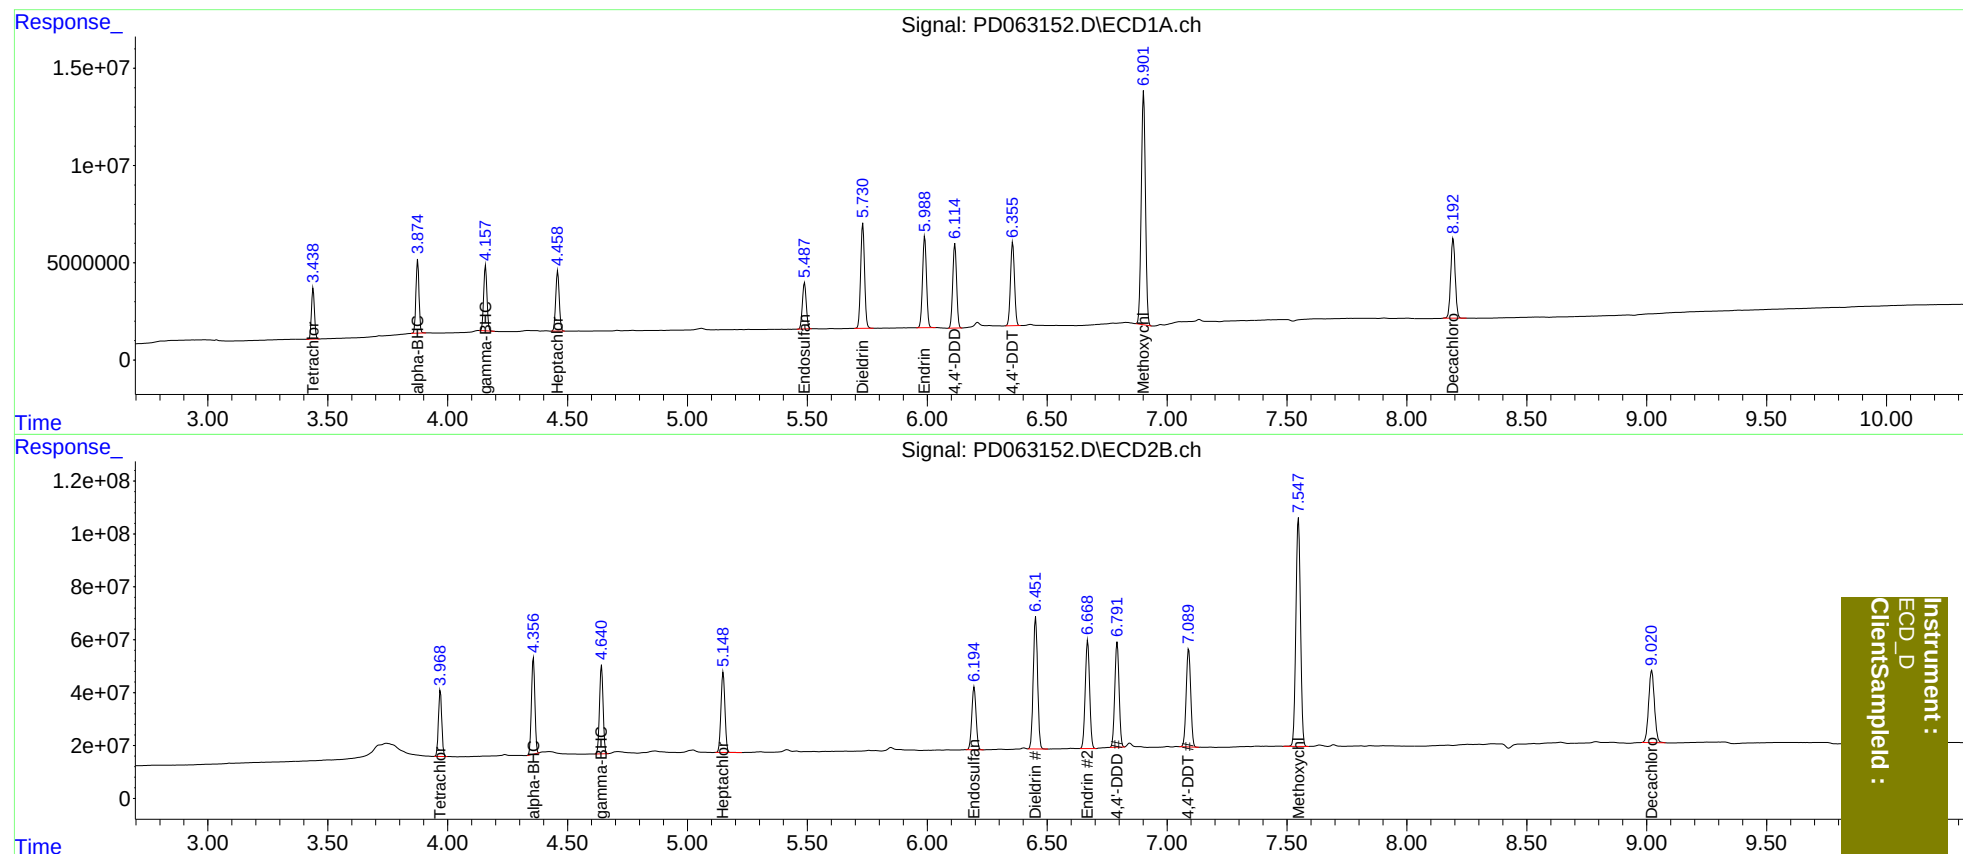


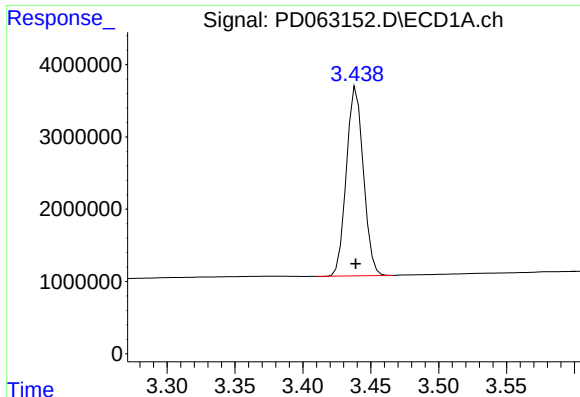

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 22815673
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

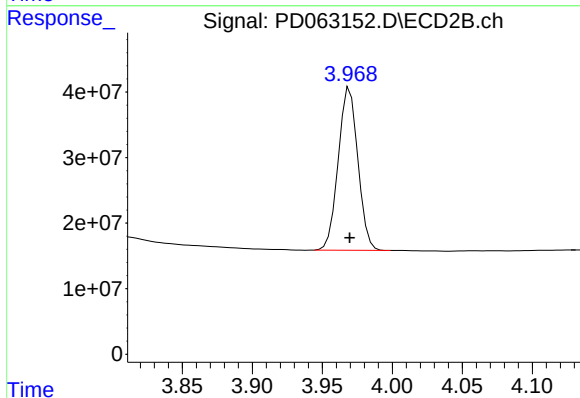


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 242284255
Conc: 20.00 ng/ml

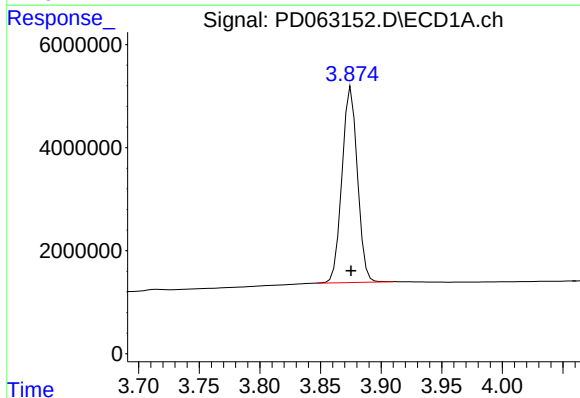


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 33589709
Conc: 20.00 ng/ml

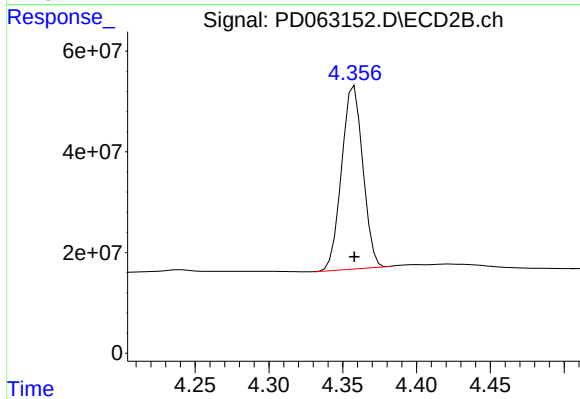

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 365282714
Conc: 20.00 ng/ml

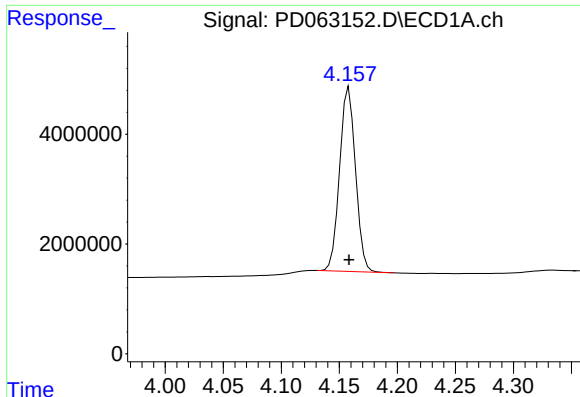

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 32006353
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

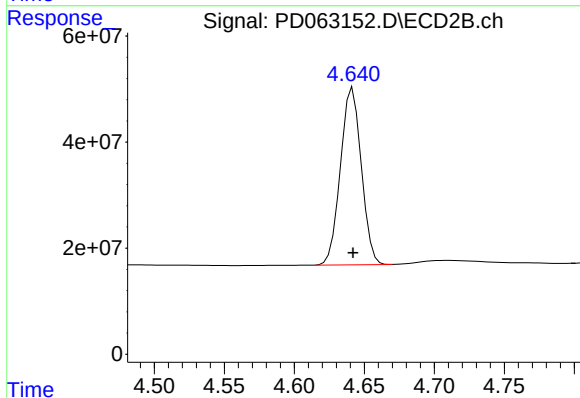


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 346400388
Conc: 20.00 ng/ml

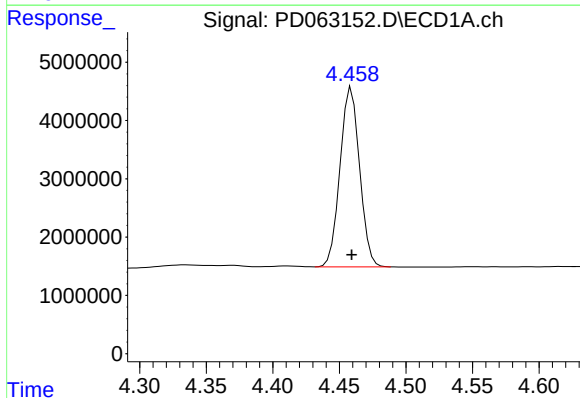


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 31476865
Conc: 20.00 ng/ml

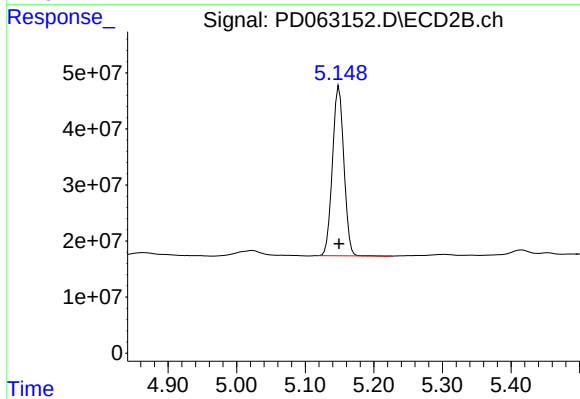

#4 Heptachlor


R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 351146274
Conc: 20.00 ng/ml

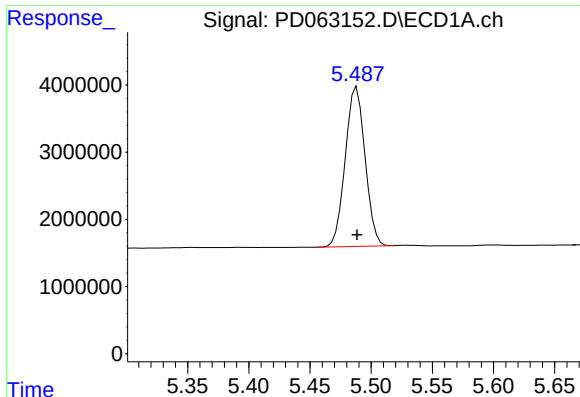

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 26729717
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

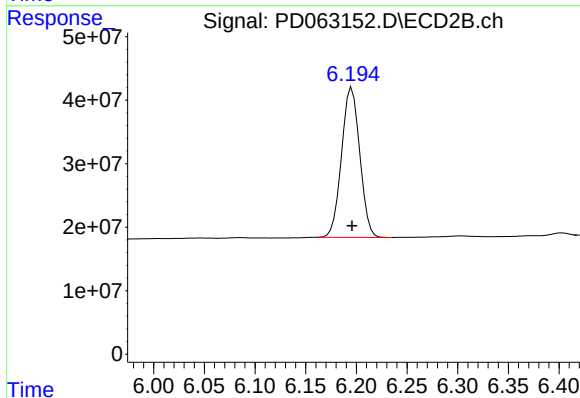


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 294477692
Conc: 20.00 ng/ml

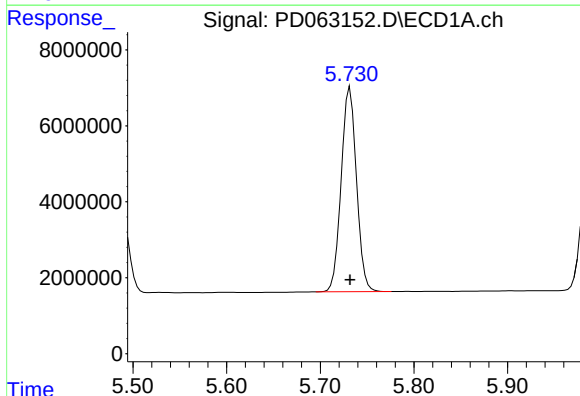


#13 Dieldrin

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 61225138
Conc: 40.00 ng/ml

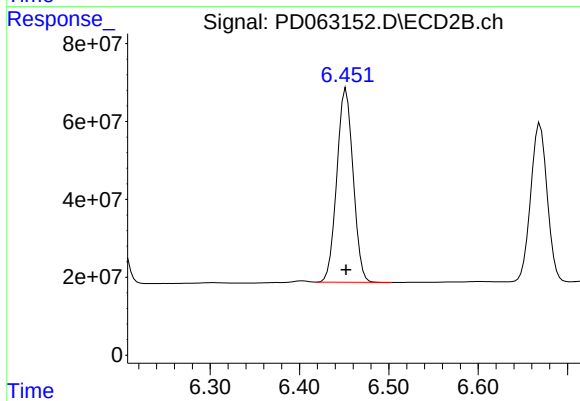

#13 Dieldrin


R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 629776999
Conc: 40.00 ng/ml

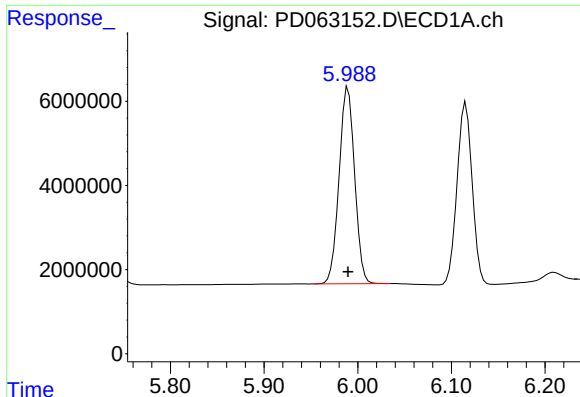

#14 Endrin


R.T.: 5.990 min
Delta R.T.: 0.000 min
Response: 53955892
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

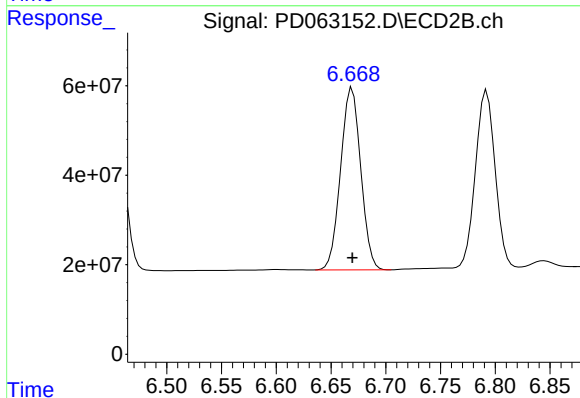


#14 Endrin

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 521131159
Conc: 40.00 ng/ml

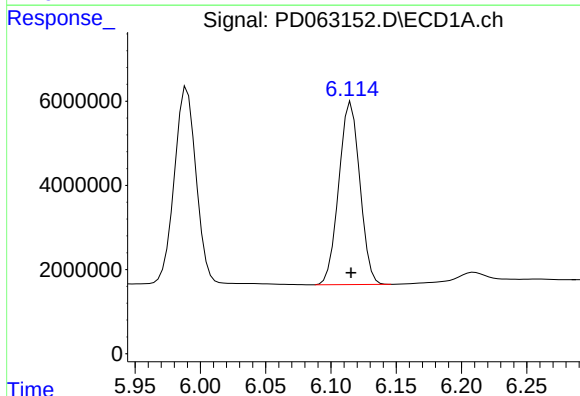


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 48638215
Conc: 40.00 ng/ml

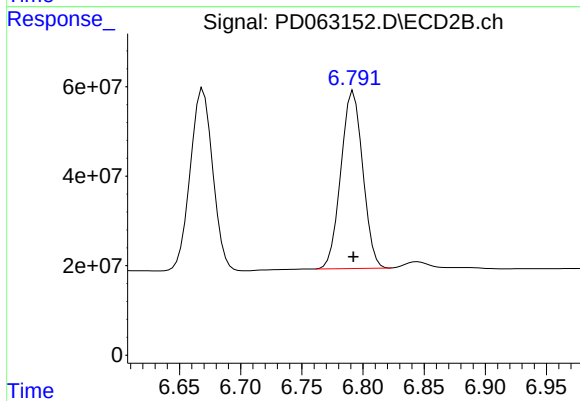

#16 4,4'-DDD


R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 493655556
Conc: 40.00 ng/ml

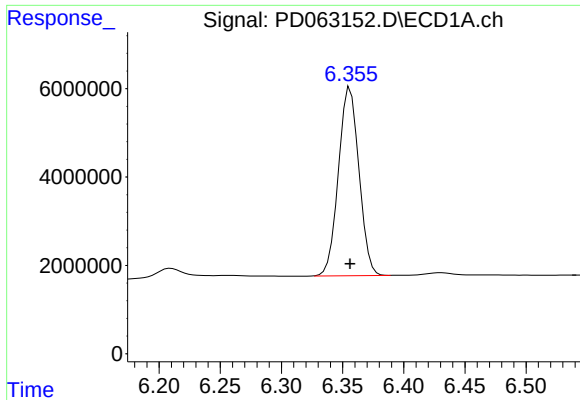

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 49765229
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

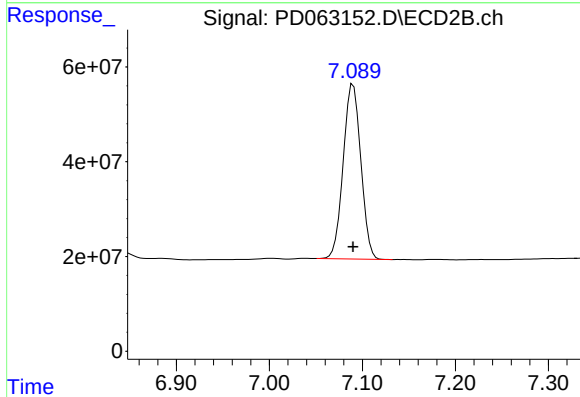


#17 4,4'-DDT

R.T.: 7.090 min
Delta R.T.: 0.000 min
Response: 486463997
Conc: 40.00 ng/ml

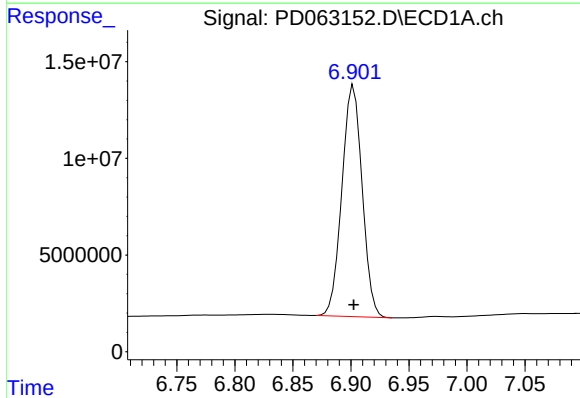


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 145183708
Conc: 200.00 ng/ml

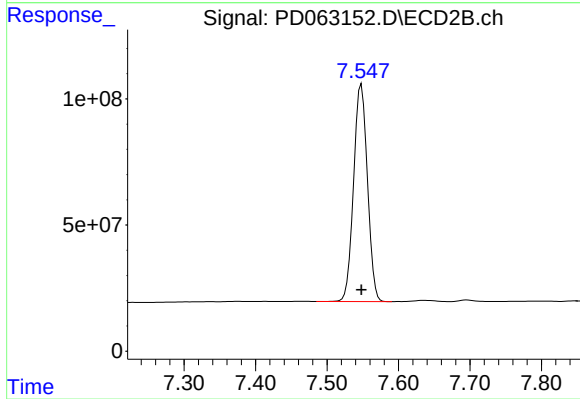

#20 Methoxychlor


R.T.: 7.548 min
Delta R.T.: 0.000 min
Response: 1159698546
Conc: 200.00 ng/ml

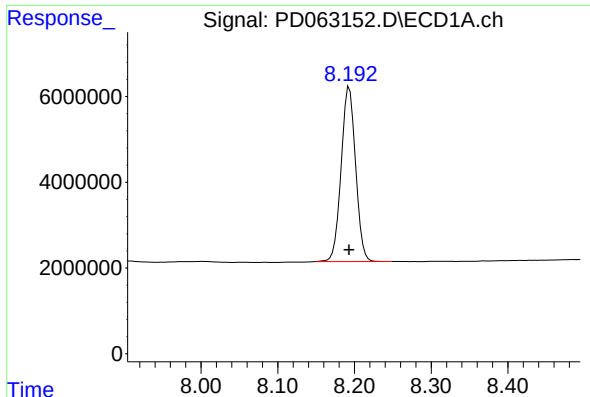

#27 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 53360848
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

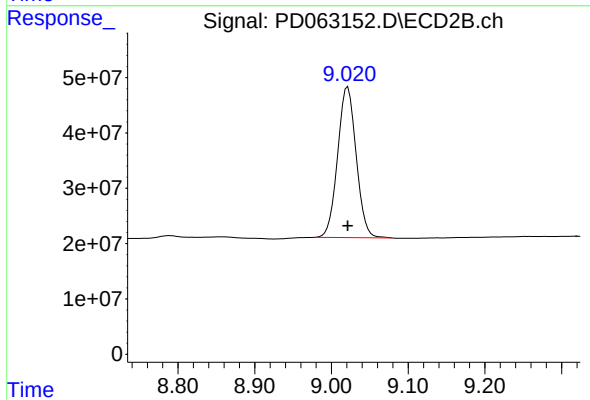

#27 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 458096104
Conc: 40.00 ng/ml