

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
 Data File : PD063154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 13:10
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 14:11:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 20 14:10:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	43161287	425.0E6	37.835	35.083
27)	SA Decachlor...	8.193	9.021	99508797	829.0E6	74.593	72.383
Target Compounds							
2)	A alpha-BHC	3.875	4.357	66139236	632.4E6	39.381	34.624
3)	MA gamma-BHC...	4.158	4.642	62274797	590.6E6	38.914	34.101
4)	MA Heptachlor	4.459	5.149	61187699	599.3E6	38.878	34.132
9)	A Endosulfan I	5.488	6.195	51259713	536.9E6	38.354	36.462
13)	MA Dieldrin	5.731	6.452	119.4E6	1162.1E6	78.010	73.808
14)	MA Endrin	5.989	6.669	104.7E6	964.1E6	77.621	74.001
16)	A 4,4'-DDD	6.115	6.792	94896410	929.1E6	78.043	75.282
17)	MA 4,4'-DDT	6.355	7.091	99466656	940.8E6	79.949	77.361
20)	A Methoxychlor	6.902	7.549	270.6E6	2165.2E6	372.811	373.400


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
Data File : PD063154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 13:10
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 14:11:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 20 14:10:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

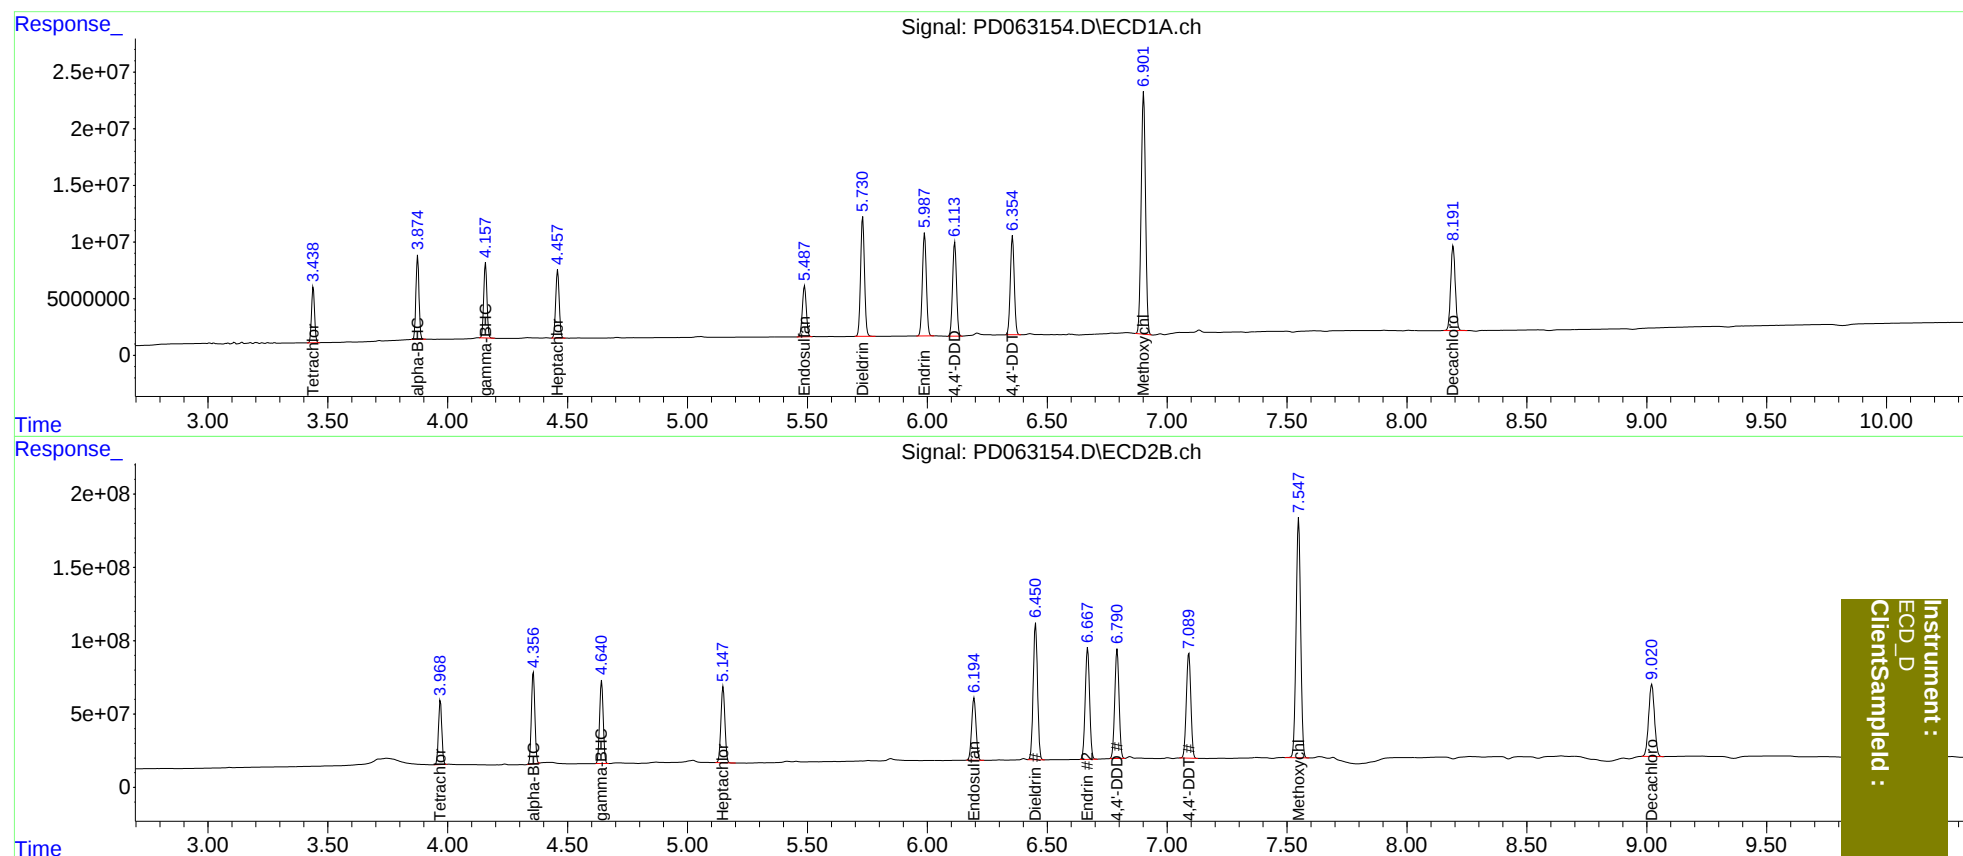


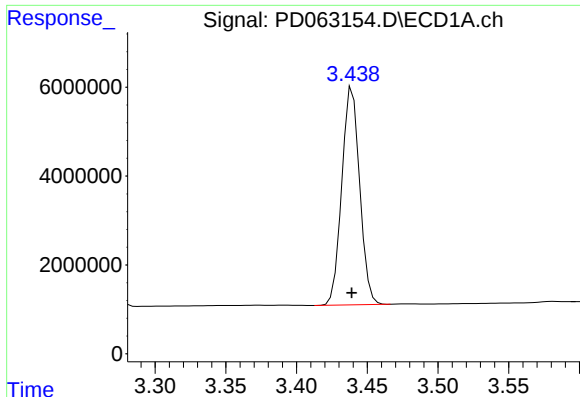

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 43161287
Conc: 37.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

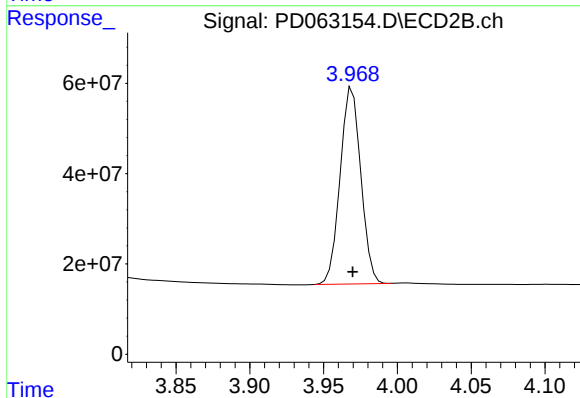


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 425006253
Conc: 35.08 ng/ml

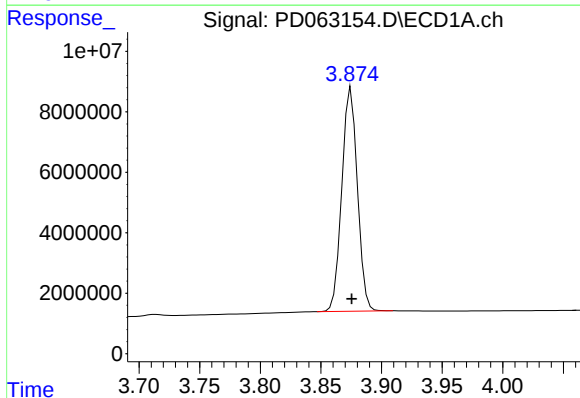


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 66139236
Conc: 39.38 ng/ml

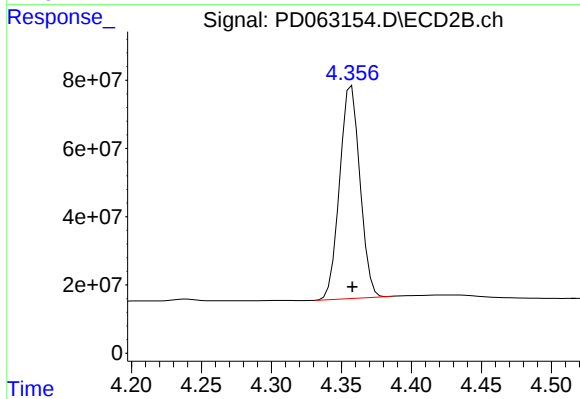

#2 alpha-BHC


R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 632383985
Conc: 34.62 ng/ml

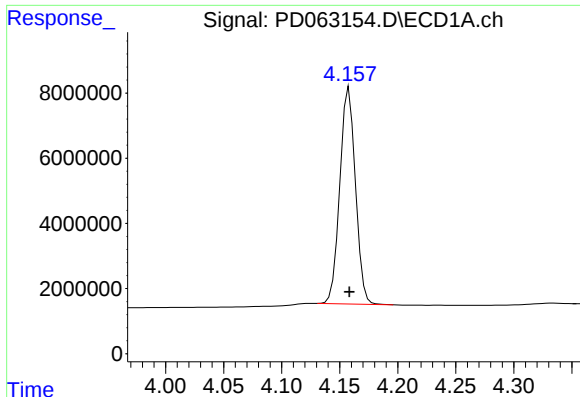

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 62274797
Conc: 38.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

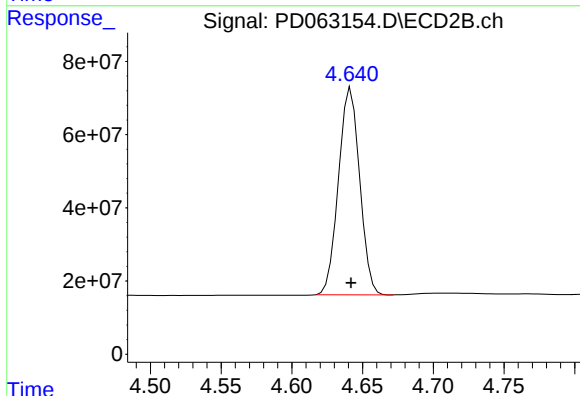


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 590637093
Conc: 34.10 ng/ml

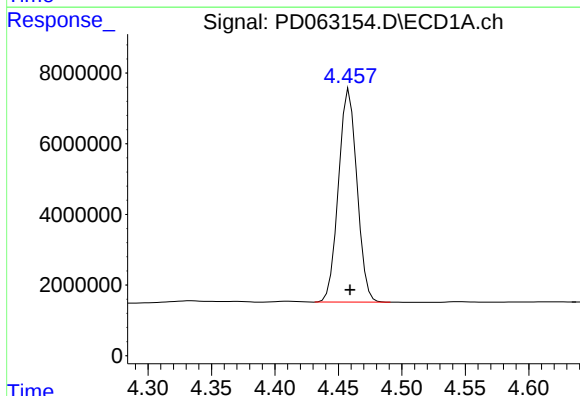


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 61187699
Conc: 38.88 ng/ml

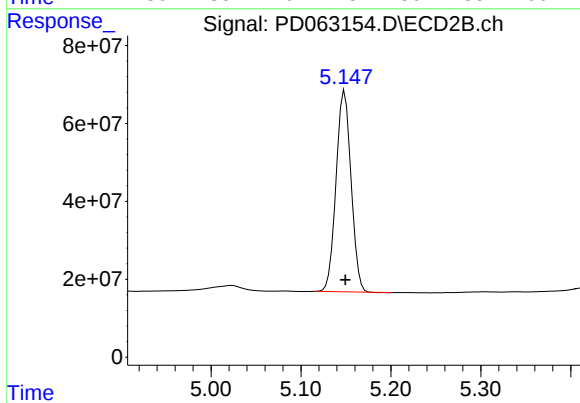

#4 Heptachlor


R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 599274035
Conc: 34.13 ng/ml

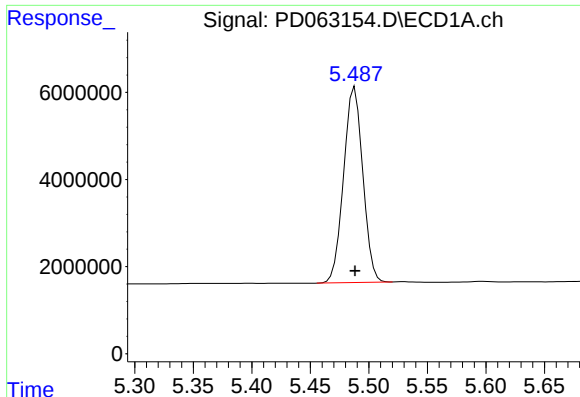

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 51259713
Conc: 38.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

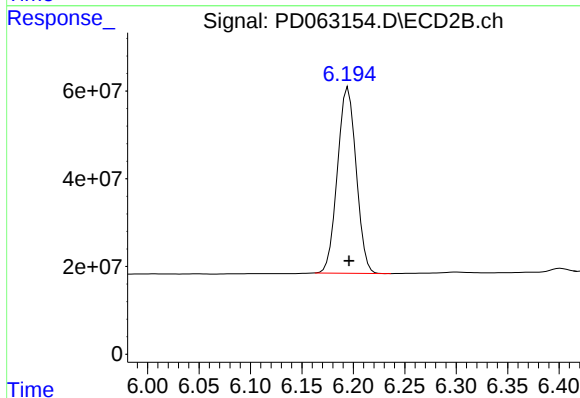


#9 Endosulfan I

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 536857309
Conc: 36.46 ng/ml

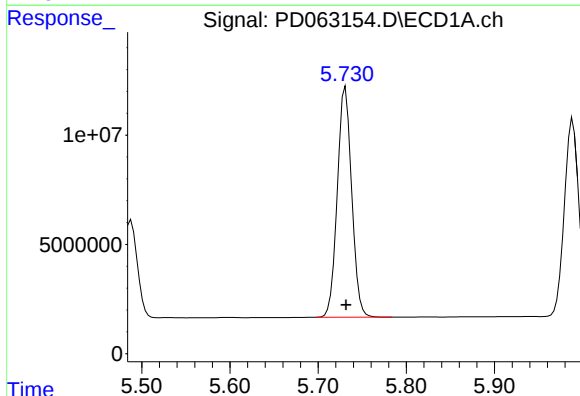


#13 Dieldrin

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 119403726
Conc: 78.01 ng/ml

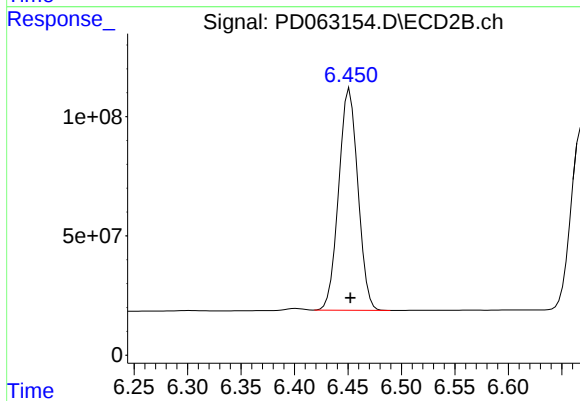

#13 Dieldrin


R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 1162060323
Conc: 73.81 ng/ml

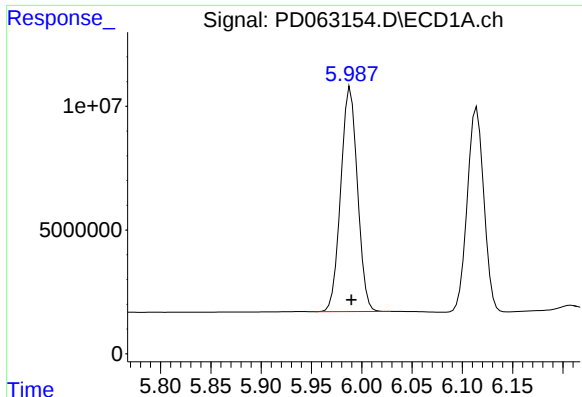

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 104703064
Conc: 77.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

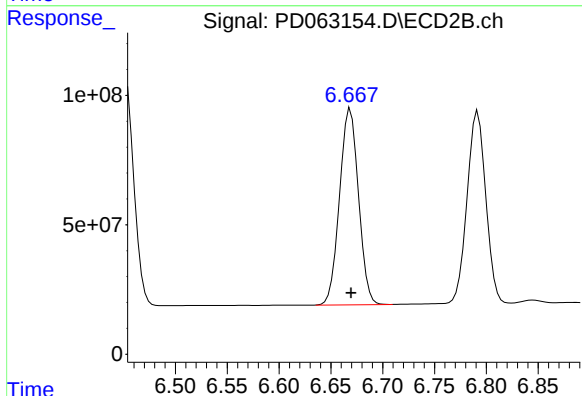


#14 Endrin

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 964099282
Conc: 74.00 ng/ml

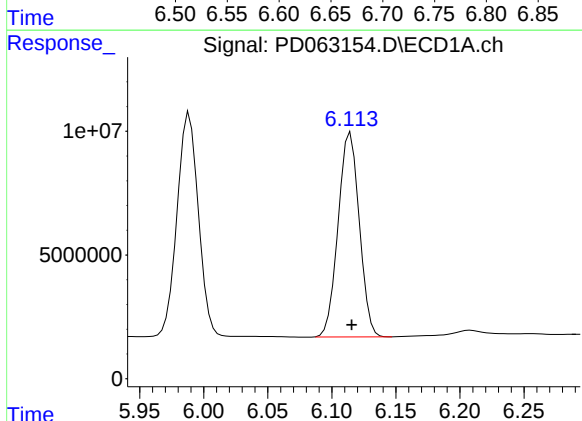


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 94896410
Conc: 78.04 ng/ml

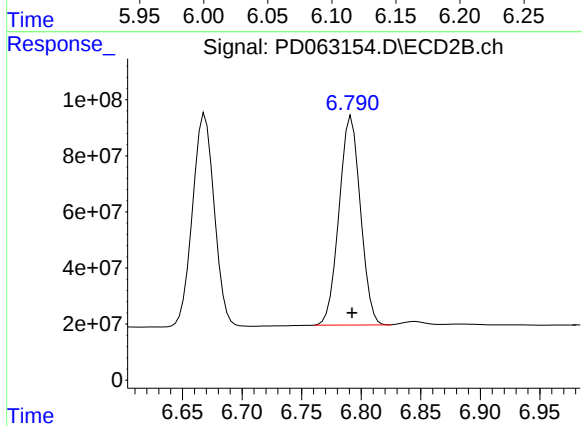

#16 4,4'-DDD


R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 929079690
Conc: 75.28 ng/ml

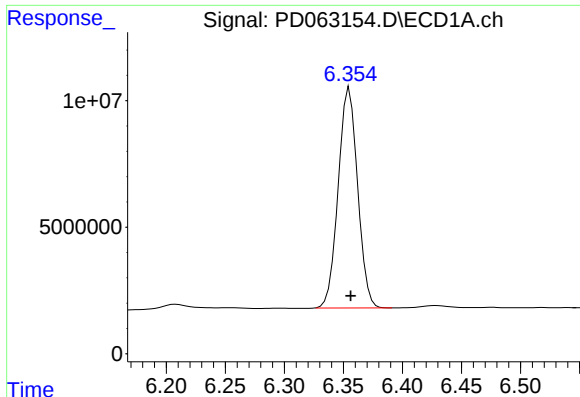

#17 4,4'-DDT


R.T.: 6.355 min
Delta R.T.: -0.001 min
Response: 99466656
Conc: 79.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

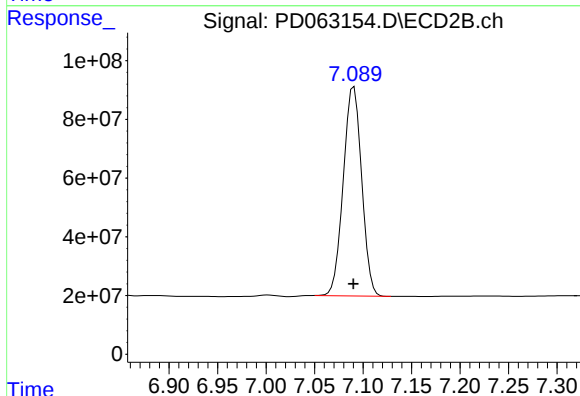


#17 4,4'-DDT

R.T.: 7.091 min
Delta R.T.: 0.000 min
Response: 940834864
Conc: 77.36 ng/ml

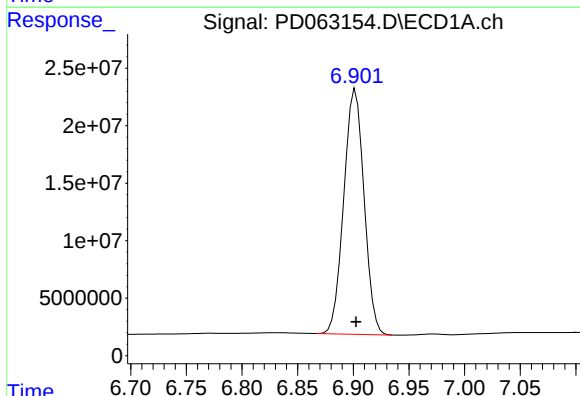


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 270630769
Conc: 372.81 ng/ml

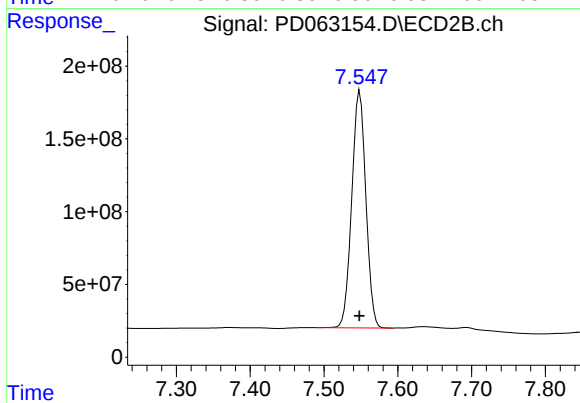

#20 Methoxychlor


R.T.: 7.549 min
Delta R.T.: 0.000 min
Response: 2165154901
Conc: 373.40 ng/ml

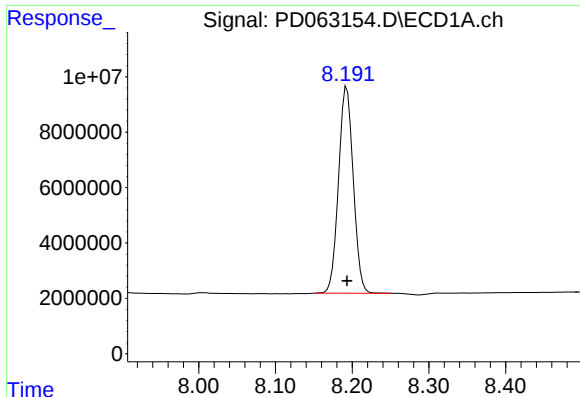

#27 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 99508797
Conc: 74.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

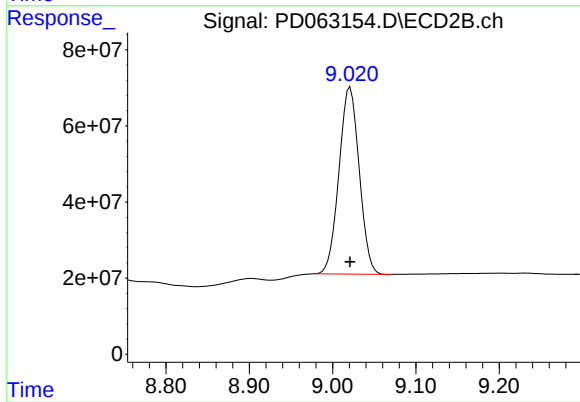

#27 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 828958821
Conc: 72.38 ng/ml