

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
 Data File : PD063156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 13:38
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 14:11:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 20 14:10:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	88583437	870.0E6	77.651	71.813
27)	SA Decachlor...	8.193	9.021	194.7E6	1623.8E6	145.922	141.787
Target Compounds							
2)	A alpha-BHC	3.876	4.358	142.2E6	1373.9E6	84.683	75.223
3)	MA gamma-BHC...	4.159	4.642	132.1E6	1281.7E6	82.567	74.000
4)	MA Heptachlor	4.459	5.149	128.0E6	1260.1E6	81.342	71.768
9)	A Endosulfan I	5.488	6.195	107.1E6	1062.6E6	80.143	72.169
13)	MA Dieldrin	5.732	6.452	252.5E6	2293.6E6	164.951	145.677
14)	MA Endrin	5.989	6.670	211.2E6	1832.0E6	156.602	140.618
16)	A 4,4'-DDD	6.114	6.792	202.4E6	1841.3E6	166.414	149.201
17)	MA 4,4'-DDT	6.356	7.090	212.9E6	1854.0E6	171.154	152.448
20)	A Methoxychlor	6.902	7.548	520.9E6	4040.9E6	717.544	696.892


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
Data File : PD063156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 13:38
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 14:11:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 20 14:10:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

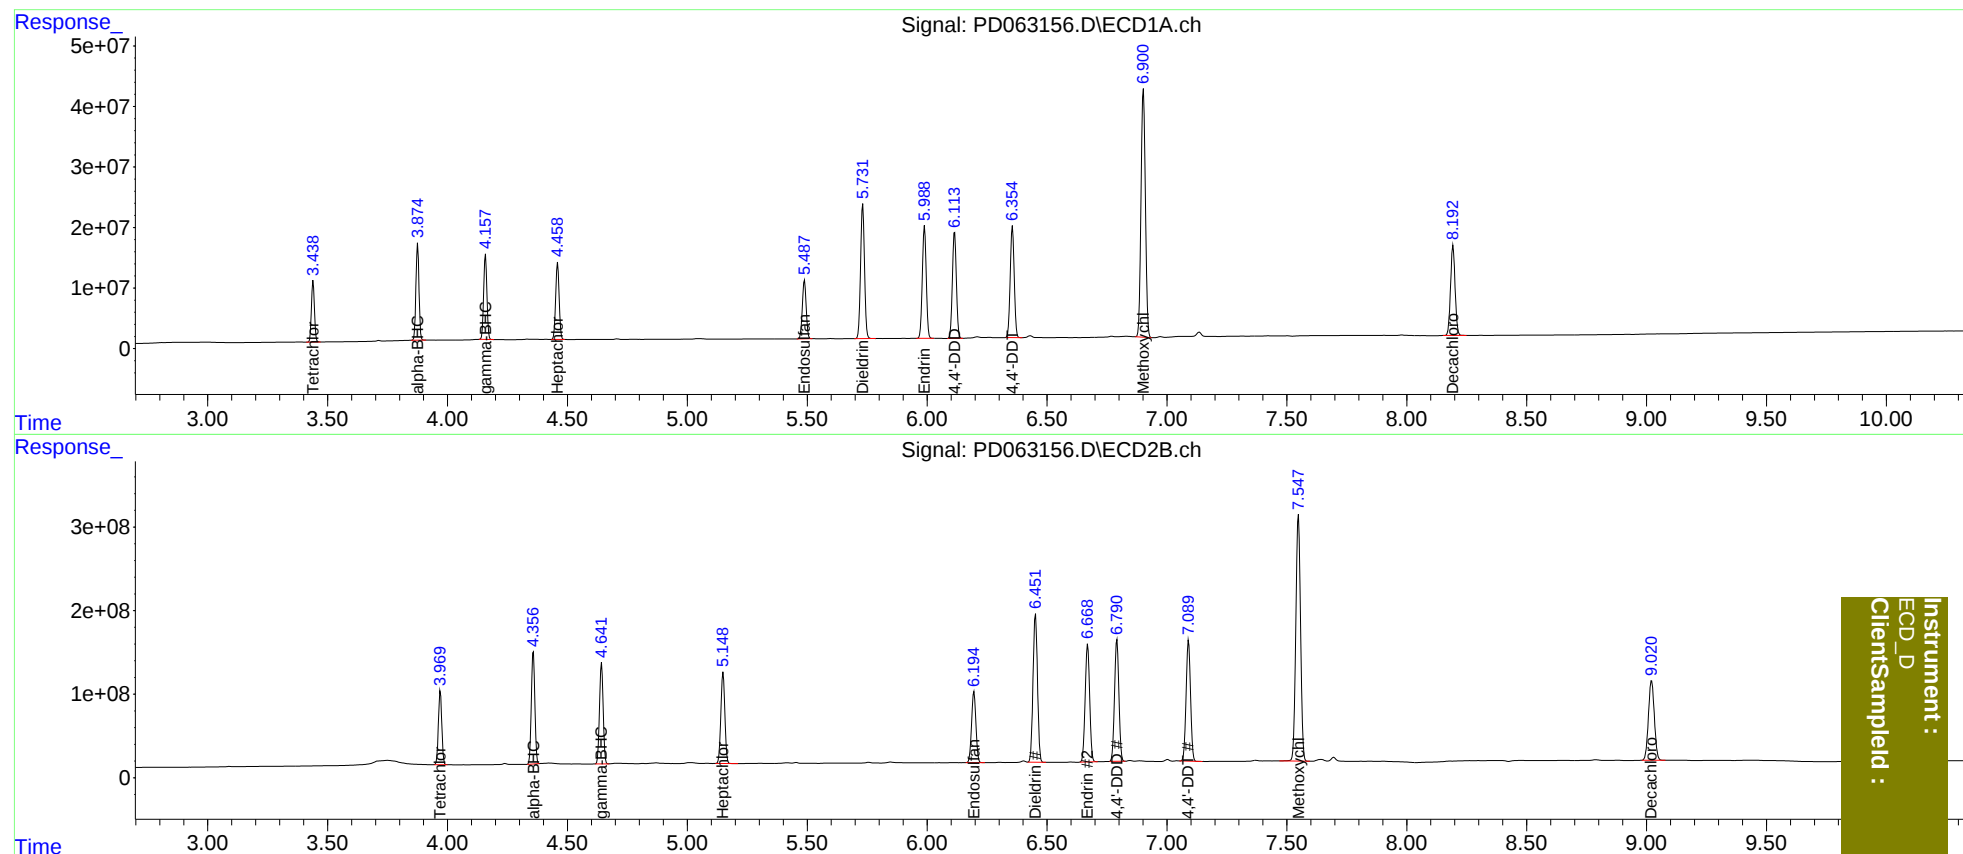


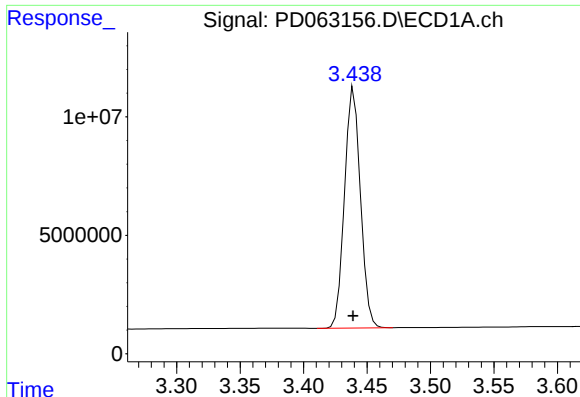

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 88583437
Conc: 77.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

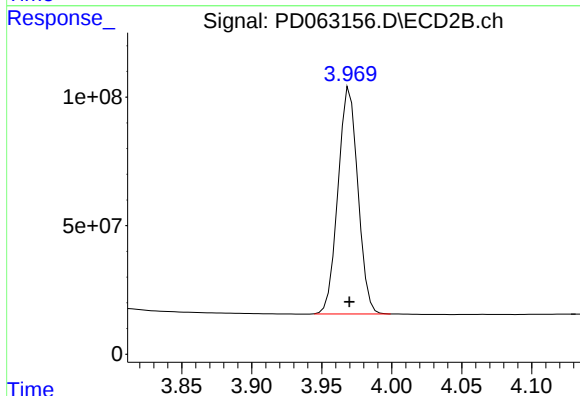


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 869959674
Conc: 71.81 ng/ml

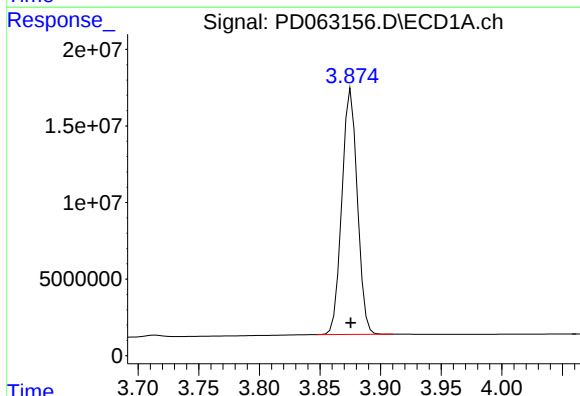


#2 alpha-BHC

R.T.: 3.876 min
Delta R.T.: 0.000 min
Response: 142224547
Conc: 84.68 ng/ml

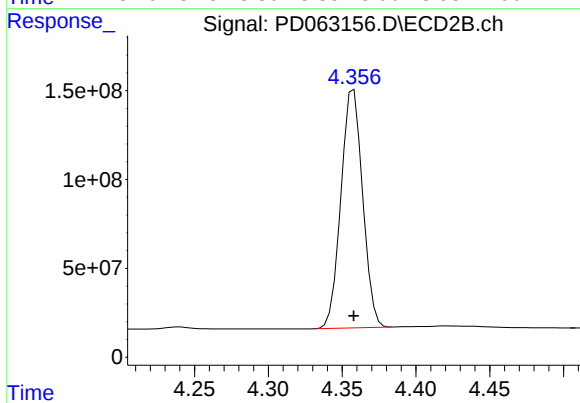

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 1373889514
Conc: 75.22 ng/ml

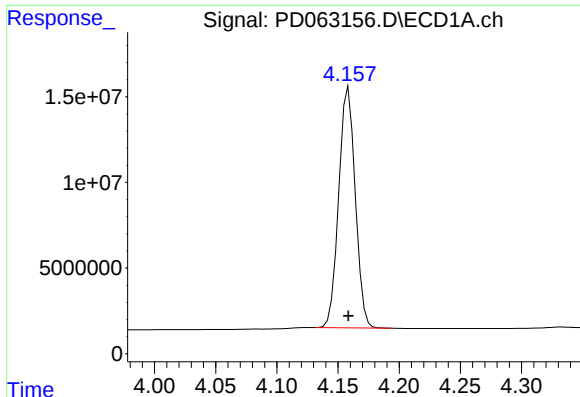

#3 gamma-BHC (Lindane)


R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 132133545
Conc: 82.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

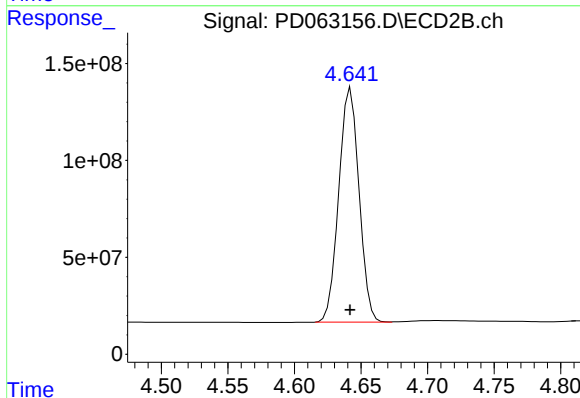


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 1281682332
Conc: 74.00 ng/ml

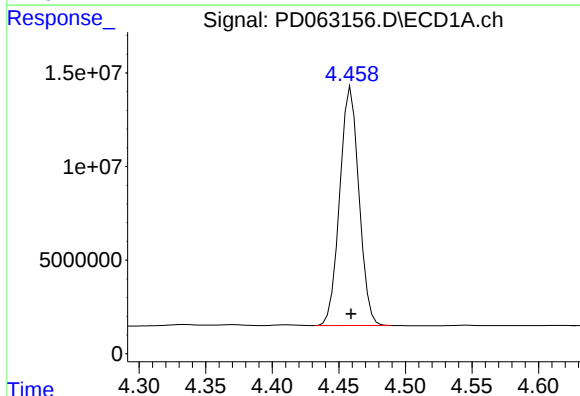


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 128019384
Conc: 81.34 ng/ml

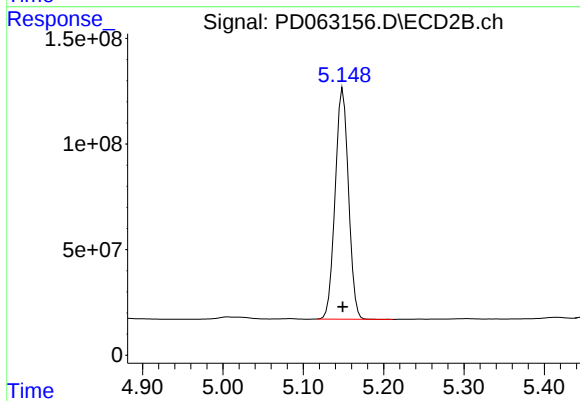

#4 Heptachlor


R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 1260060585
Conc: 71.77 ng/ml

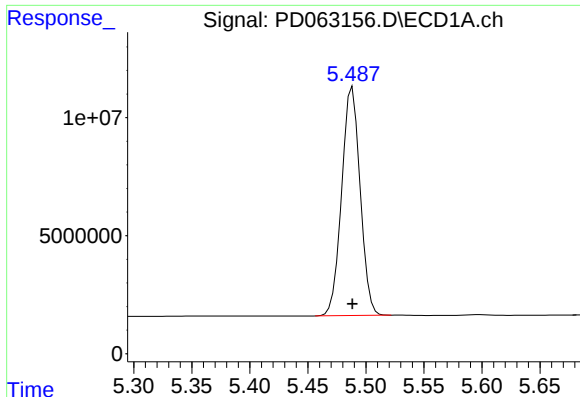

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 107110457
Conc: 80.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

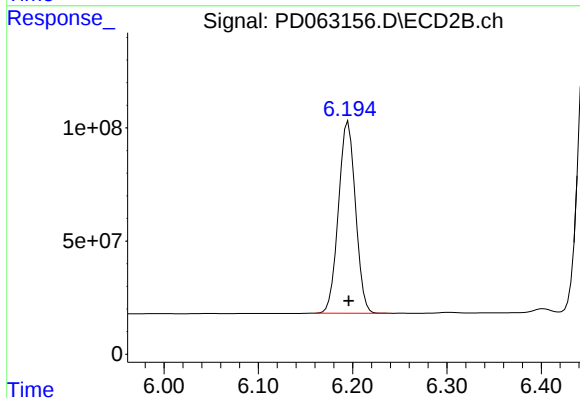


#9 Endosulfan I

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 1062601521
Conc: 72.17 ng/ml

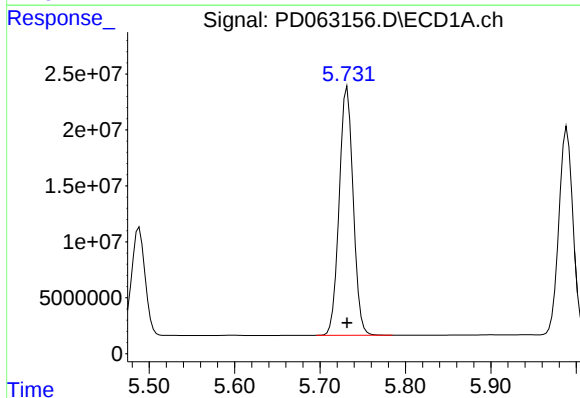


#13 Dieldrin

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 252479378
Conc: 164.95 ng/ml

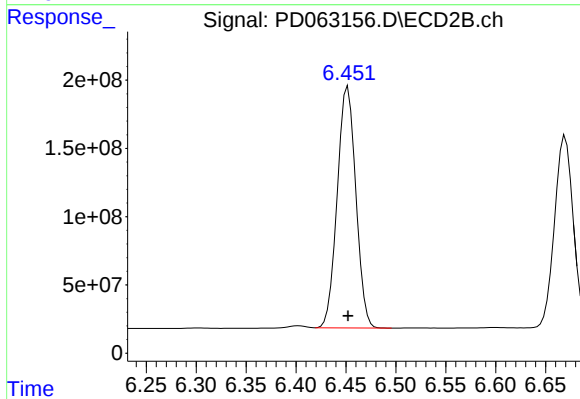

#13 Dieldrin


R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 2293594633
Conc: 145.68 ng/ml

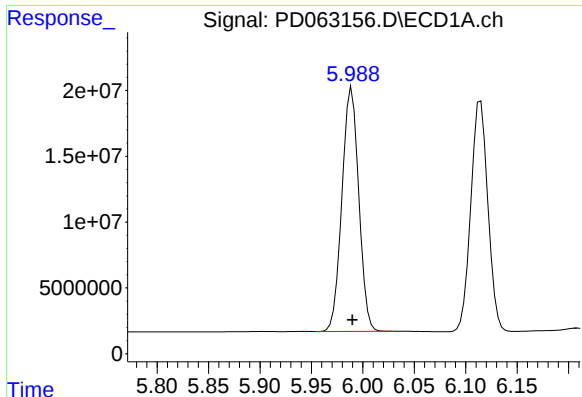

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 211239647
Conc: 156.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

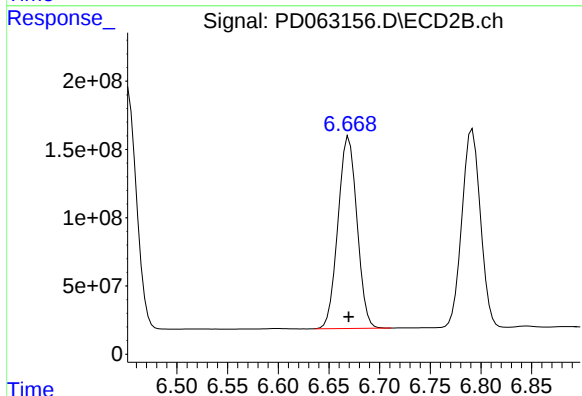


#14 Endrin

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 1832009550
Conc: 140.62 ng/ml

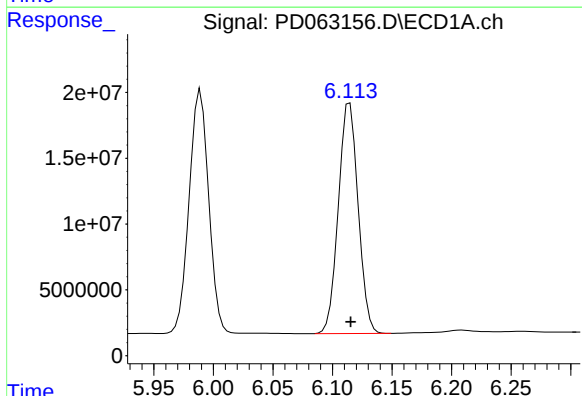


#16 4,4'-DDD

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 202352204
Conc: 166.41 ng/ml

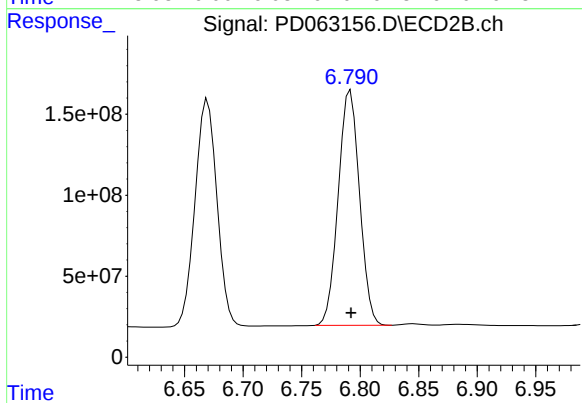

#16 4,4'-DDD


R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 1841343771
Conc: 149.20 ng/ml

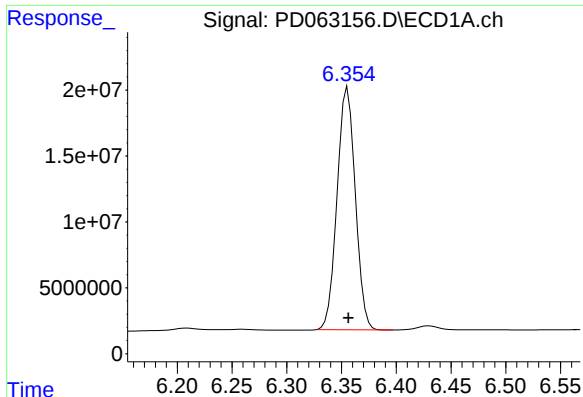

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 212938521
Conc: 171.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

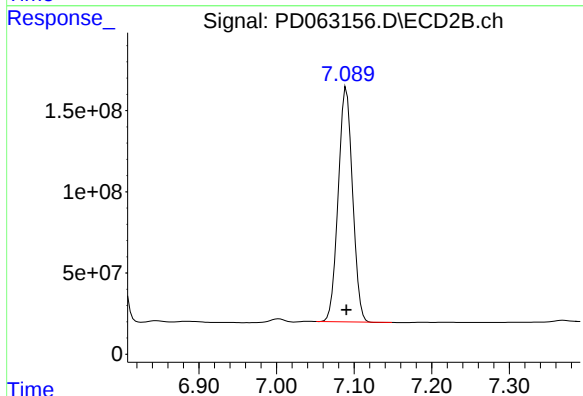


#17 4,4'-DDT

R.T.: 7.090 min
Delta R.T.: 0.000 min
Response: 1854011477
Conc: 152.45 ng/ml

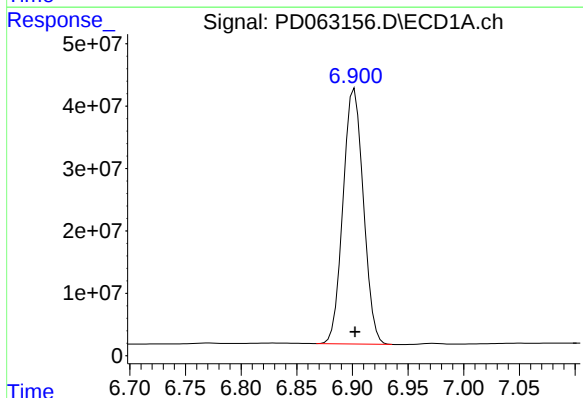


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 520878389
Conc: 717.54 ng/ml

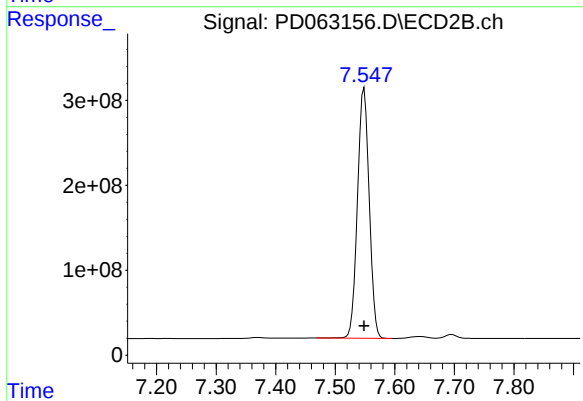

#20 Methoxychlor


R.T.: 7.548 min
Delta R.T.: 0.000 min
Response: 4040921810
Conc: 696.89 ng/ml

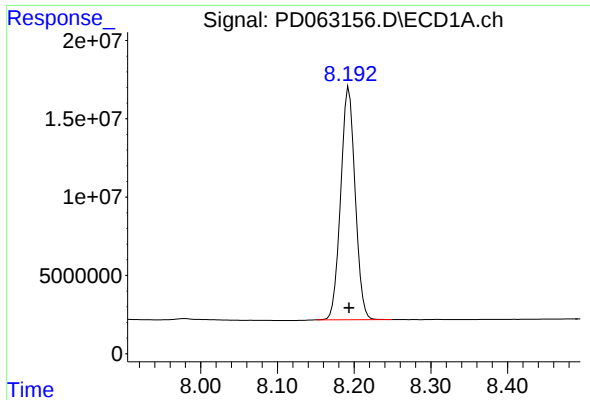

#27 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 194663094
Conc: 145.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

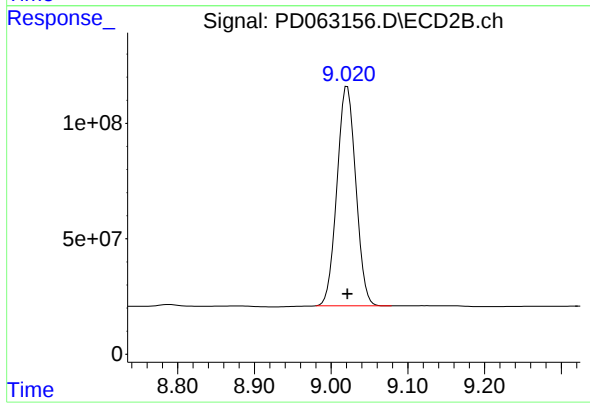

#27 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 1623804258
Conc: 141.79 ng/ml