

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
 Data File : PD063141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 10:07
 Operator : AR\AJ
 Sample : RESC06
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC006

Manual Integrations
 APPROVED

Ankita
 5/21/2021 11:22:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 18:40:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 20 14:55:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	23034951	246.3E6	20.367	21.012
27)	SA Decachlor...	8.193	9.023	51351140	454.8E6	39.484	41.008
Target Compounds							
2)	A alpha-BHC	3.875	4.358	16826920	189.6E6	10.068	10.886
3)	MA gamma-BHC...	4.158	4.642	16176097	182.8E6	10.098	10.955
4)	MA Heptachlor	4.459	5.150	15931380	182.5E6	10.254	10.846
5)	MB Aldrin	4.707	5.454	14900845	179.5E6	9.943	11.340
6)	B beta-BHC	4.409	4.813	7480993	75129496	10.356	10.634
7)	B delta-BHC	4.612	5.029	15554870	209.4E6	9.835m	11.652
8)	B Heptachlo...	5.150	5.840	14280417	177.4E6	10.149	11.400
9)	A Endosulfan I	5.488	6.195	13683133	156.0E6	10.379	10.868
10)	B trans-Chl...	5.377	6.073	14618891	162.2E6	10.161	10.463
11)	B cis-Chlor...	5.434	6.146	14319252	157.4E6	10.141	10.588
12)	B 4,4'-DDE	5.599	6.303	28701943	317.3E6	20.011	21.003
13)	MA Dieldrin	5.731	6.452	30792775	327.8E6	20.544	21.369
14)	MA Endrin	5.989	6.670	28300138	275.9E6	21.358	21.750
15)	B Endosulfa...	6.262	6.878	24159140	258.2E6	20.339	20.999
16)	A 4,4'-DDD	6.115	6.792	24274093	261.5E6	20.484	21.600
17)	MA 4,4'-DDT	6.356	7.091	24309184	255.7E6	20.160	21.148
18)	B Endrin al...	6.431	7.002	22837988	213.4E6	21.054	20.228
19)	B Endosulfa...	6.644	7.226	24076950	251.1E6	21.230	20.618
20)	A Methoxychlor	6.903	7.549	75016884	622.7E6	107.601	109.045
21)	B Endrin ke...	7.136	7.696	29754647	243.8E6	20.960	21.047

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
Data File : PD063141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 10:07
Operator : AR\AJ
Sample : RESC06
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 18:40:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 20 14:55:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

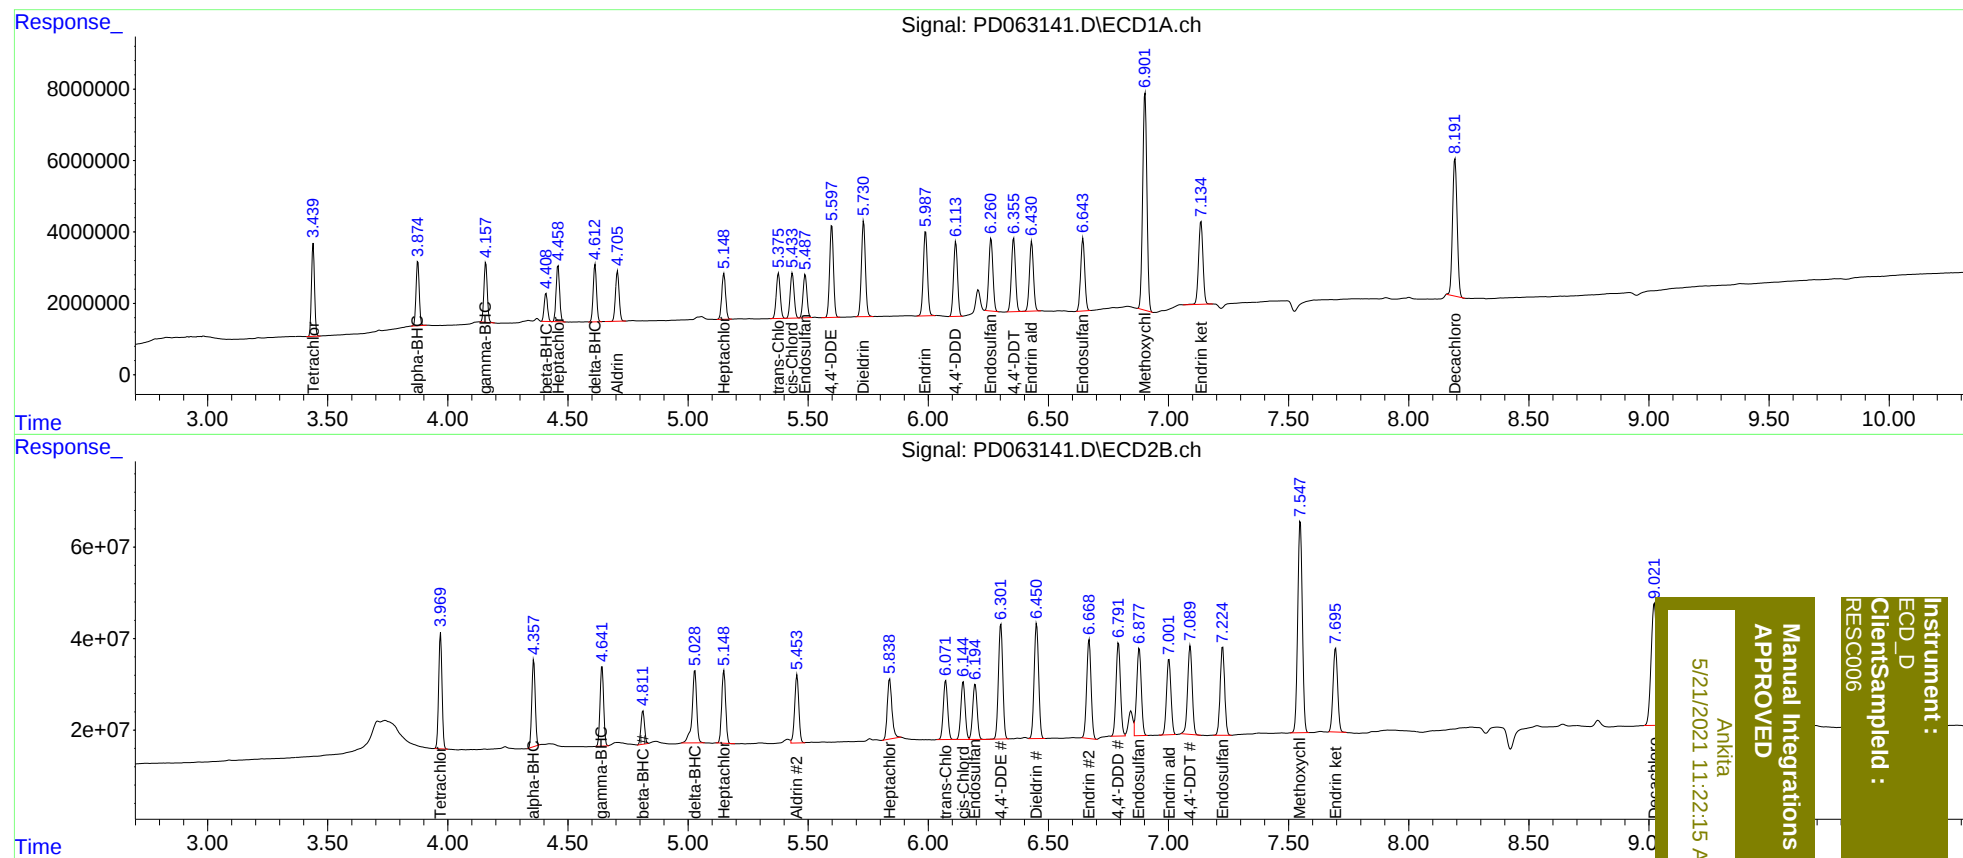

Manual Integrations
APPROVED

5/21/2021 11:22:15 AM

Ankita

Instrument :
ECD_D
ClientSample :
RESC006