

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
 Data File : PD063171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 17:08
 Operator : AR\AJ
 Sample : M2250-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

Ankita
 5/24/2021 3:23:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 01:47:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 21 01:37:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	20399869	216.6E6	18.037	18.474
2)	SA Decachlor...	8.192	9.022	50067910	430.8E6	38.497	38.841
Target Compounds							
2)	A alpha-BHC	3.875	4.358	1874924	13801587	1.122	0.792 #
3)	MA gamma-BHC...	4.159	4.642	2286777	15890013	1.428	0.953 #
4)	MA Heptachlor	4.459	5.149	1418113	17515202	0.913	1.041
5)	MB Aldrin	4.706	5.453	1382007	20047222	0.922m	1.248 #
6)	B beta-BHC	4.409	4.811	884015	6084262	1.204	0.861m#
7)	B delta-BHC	4.613	5.028	1360907	40279934	0.861	2.241 #
8)	B Heptachlo...	5.149	5.842	1327972	26802101	0.944	1.722 #
9)	A Endosulfan I	5.488	6.196	1185202	16930539	0.899	1.179 #
10)	B trans-Chl...	5.376	6.074	1337175	15371656	0.929	0.992
11)	B cis-Chlor...	5.434	6.146	1316926	15653695	0.933	1.053
12)	B 4,4'-DDE	5.598	6.303	1212896	15970541	0.846	1.057 #
13)	MA Dieldrin	5.731	6.452	1304953	16401735	0.871	1.069
14)	MA Endrin	5.989	6.669	1843819	13458706	1.392	1.061
15)	B Endosulfa...	6.263	6.878	1219714	14044390	1.027	1.142m
16)	A 4,4'-DDD	6.113	6.791	877332	11693206	0.740m	0.966m#
17)	MA 4,4'-DDT	6.355	7.091	730113	13650154	0.606	1.129 #
18)	B Endrin al...	6.431	7.002	1146006	11064493	1.057	1.049
19)	B Endosulfa...	6.644	7.226	1069117	13882157	0.943	1.140
20)	A Methoxychlor	6.901	7.549	646432	7697457	0.927m	1.348 #
21)	B Endrin ke...	7.134	7.694	1226015	11090569	0.864m	0.957m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
Data File : PD063171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 17:08
Operator : AR\AJ
Sample : M2250-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 01:47:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 21 01:37:02 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

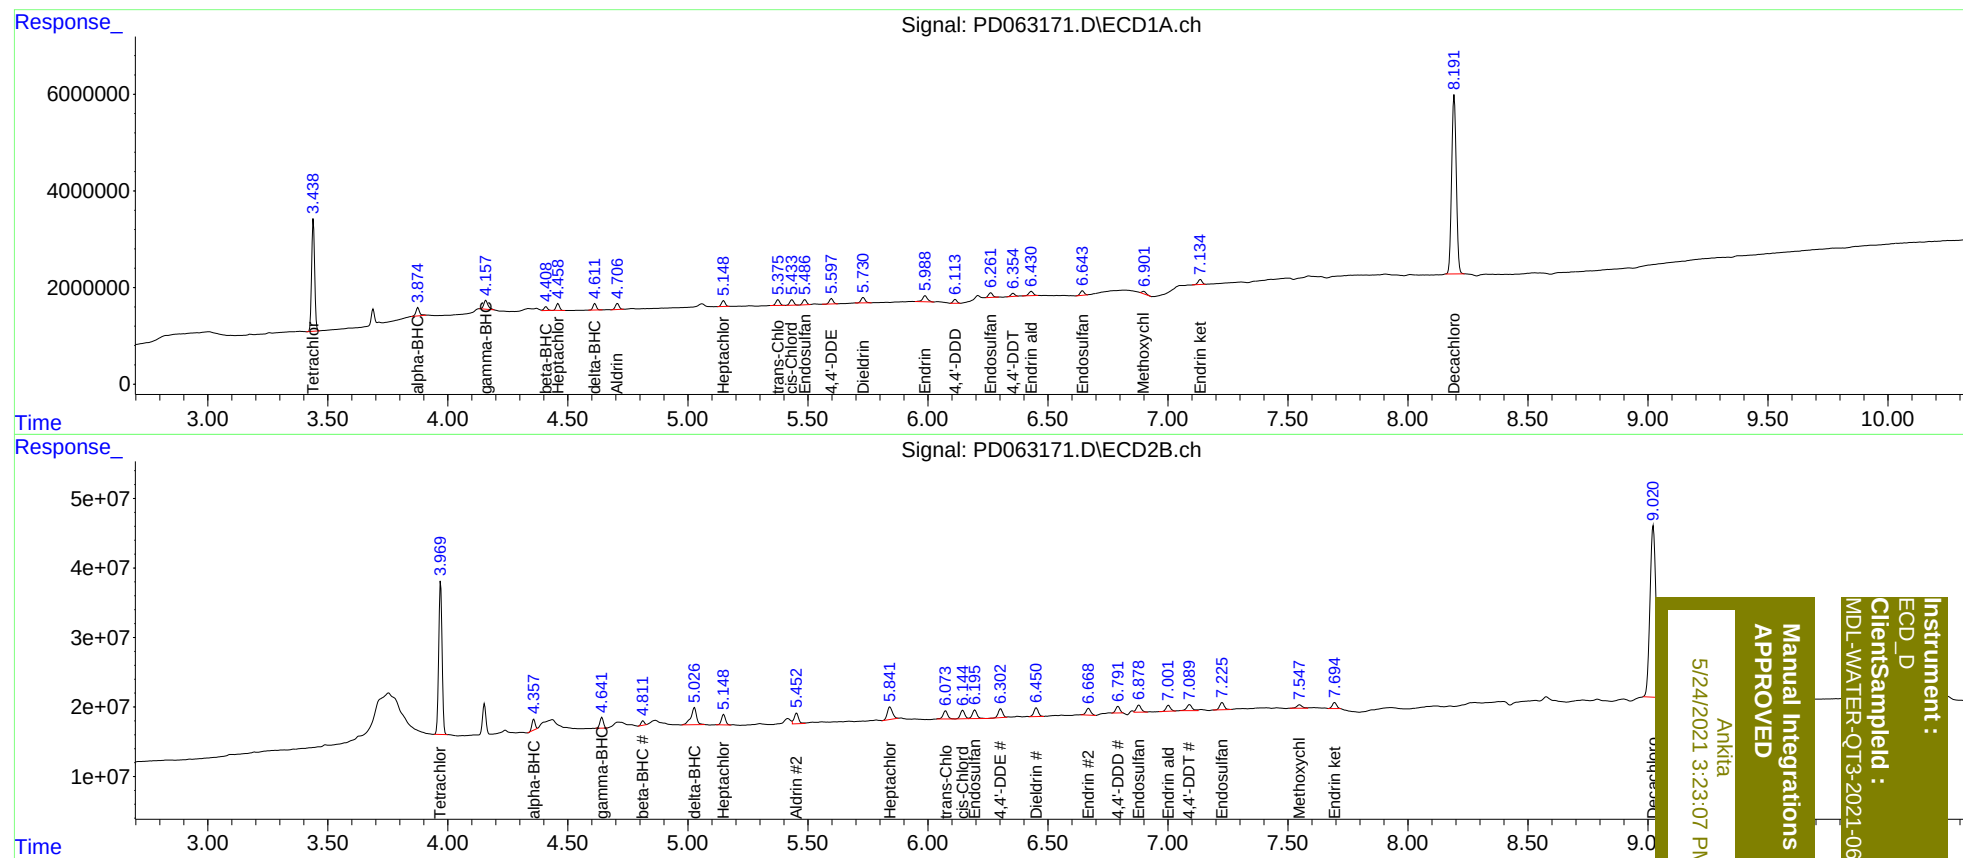

Manual Integrations
APPROVED

5/24/2021 3:23:07 PM
Ankitia

Instrument :
ECD_D
ClientSample :
MDL-WATER-QT3-2021-06