

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
 Data File : PD063172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 17:22
 Operator : AR\AJ
 Sample : M2250-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

Ankita
 5/21/2021 11:22:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 04:41:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 21 01:37:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	20891154	215.4E6	18.471	18.371
27)	SA Decachlor...	8.194	9.021	51863584	447.5E6	39.878	40.354
Target Compounds							
22)	Toxaphene-1	5.694	6.353	860654	6992490	97.223	109.796
23)	Toxaphene-2	5.855	6.642	839512	10601365	94.145	133.635 #
24)	Toxaphene-3	6.178	7.051	841650	12944430	88.080	115.804 #
25)	Toxaphene-4	6.297	7.125	2304308	32549076	98.918	108.012
26)	Toxaphene-5	7.032	7.623	3796914	14962809	144.198	114.109m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052121\
Data File : PD063172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 17:22
Operator : AR\AJ
Sample : M2250-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 04:41:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052121CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 21 01:37:02 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

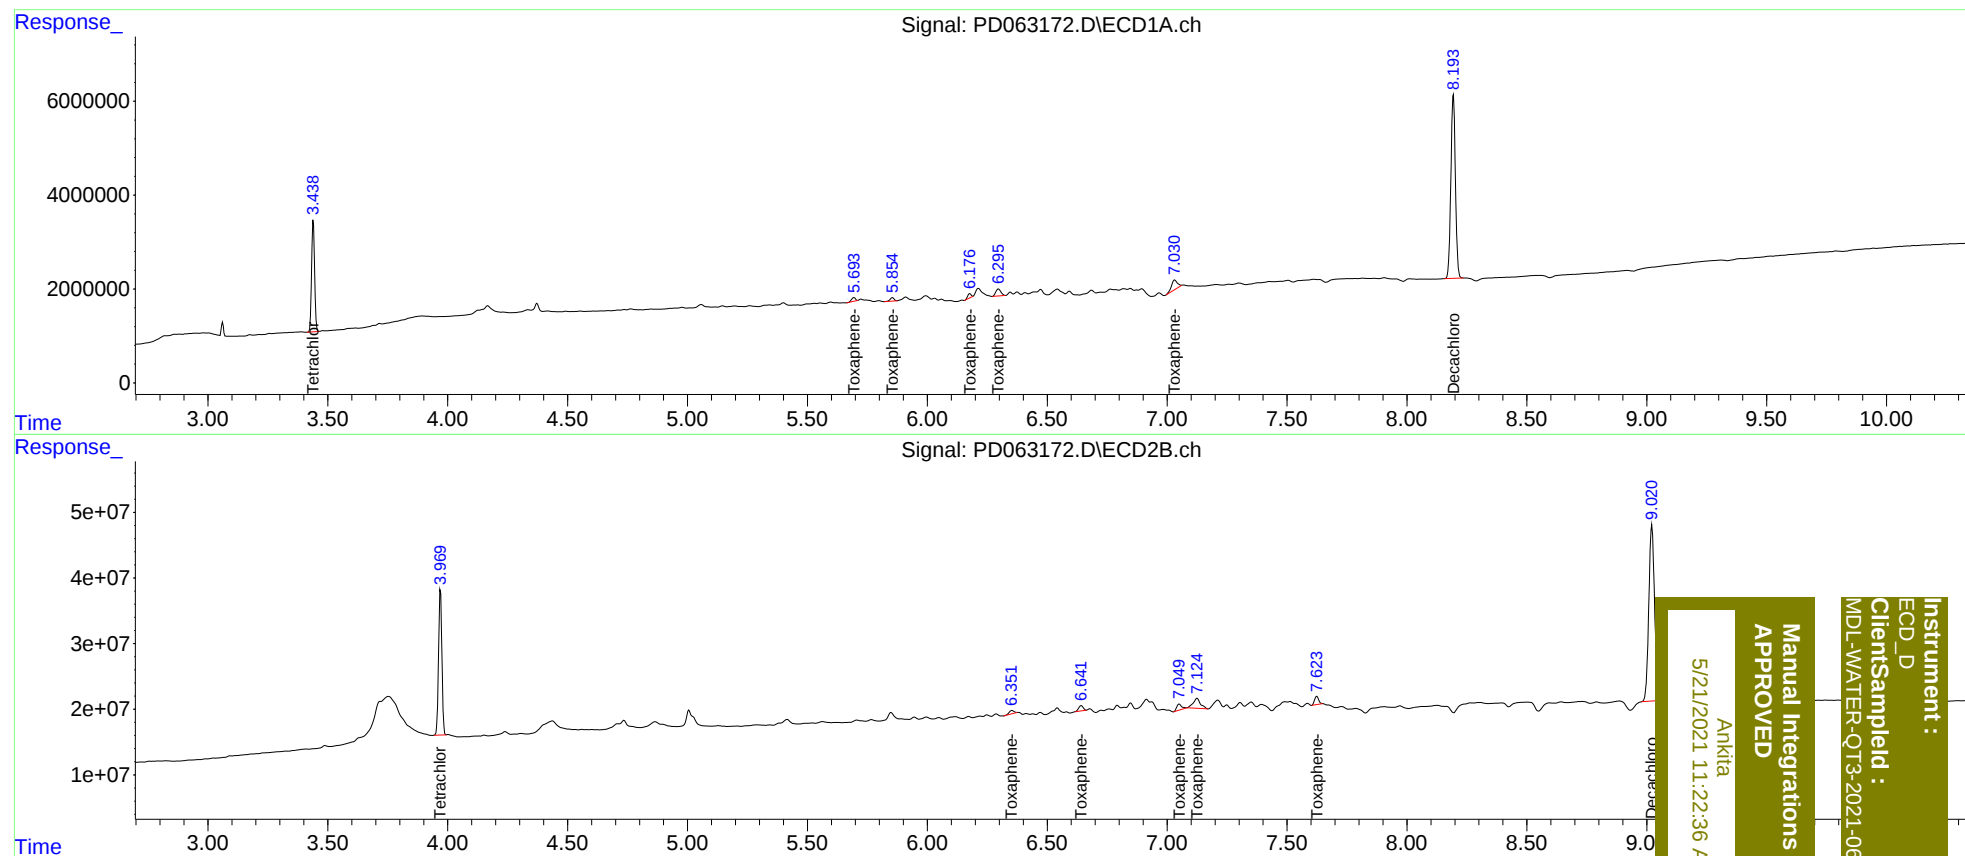

Manual Integrations
APPROVED

5/21/2021 11:22:36 AM
Ankita

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT3-2021-06