

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052122\
 Data File : PD069727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 08:37
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 00:05:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Fri May 20 02:34:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	4.201f	0	8447132	N.D.	0.884 #
Target Compounds						
4) MA Heptachlor	0.000	5.384	0	2803602	N.D.	0.226 #
8) B Heptachlo...	5.188f	6.073	9944251	428.6E6	7.854	48.027 #
12) B 4,4'-DDE	0.000	6.571f	0	5317078	N.D.	0.536 #
13) MA Dieldrin	5.717f	0.000	6974669	0	5.642	N.D. #
14) MA Endrin	6.017f	0.000	8438576	0	7.595	N.D. #
17) MA 4,4'-DDT	0.000	7.343	0	9257723	N.D.	1.126 #
19) B Endosulfa...	0.000	7.477	0	3013966	N.D.	0.377 #
21) B Endrin ke...	7.118f	0.000	48934287	0	39.061	N.D. #
24) Chlordane-2	4.843f	0.000	13622477	0	289.713	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052122\
Data File : PD069727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 08:37
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 00:05:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Fri May 20 02:34:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

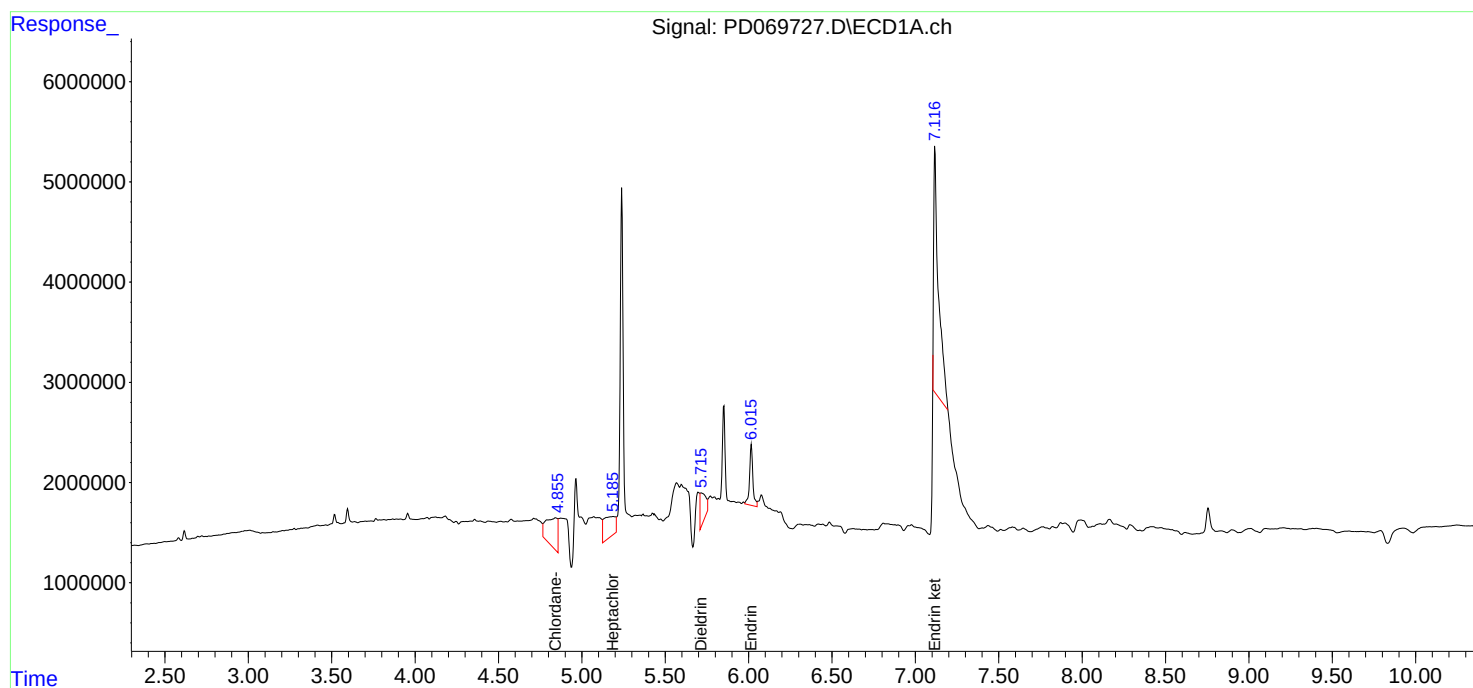


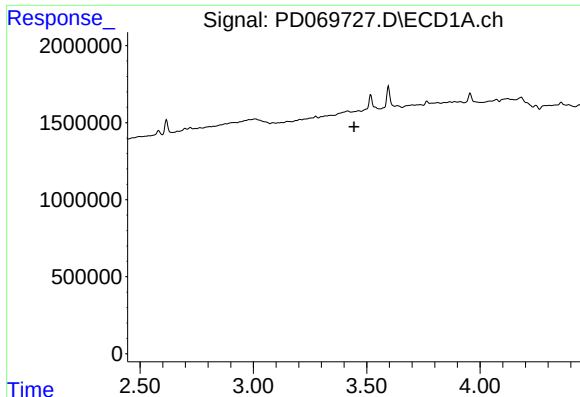

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

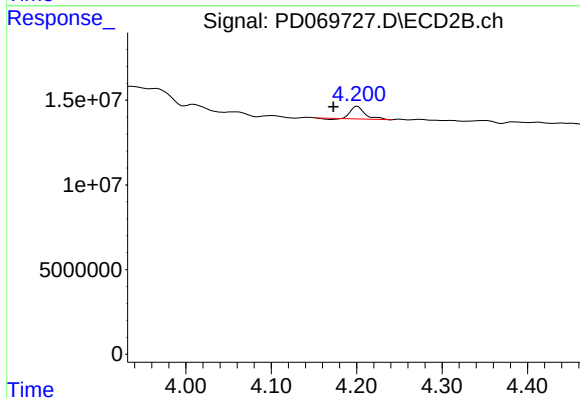


#1 Tetrachloro-m-xylene

R.T.: 4.201 min
Delta R.T.: 0.028 min
Response: 8447132
Conc: 0.88 ng/ml

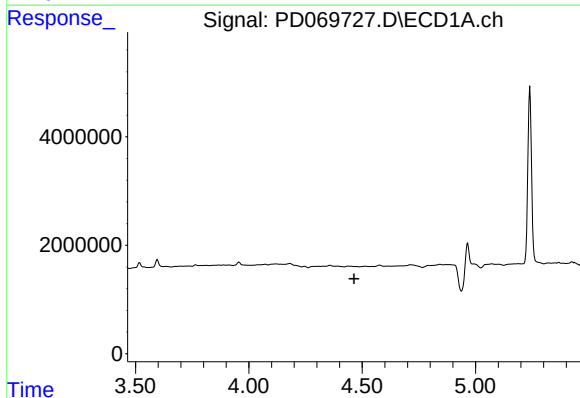


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.464 min
Response: 0
Conc: N.D.

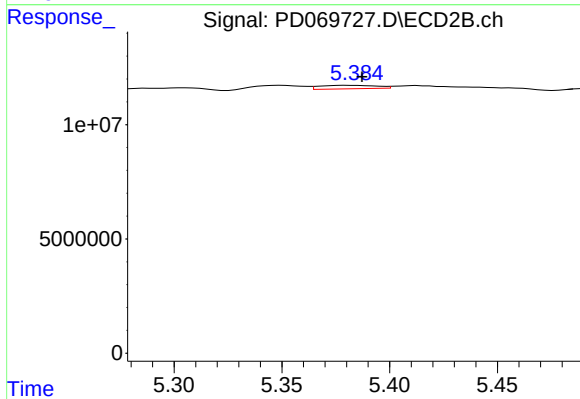

#4 Heptachlor


R.T.: 5.384 min
Delta R.T.: -0.003 min
Response: 2803602
Conc: 0.23 ng/ml

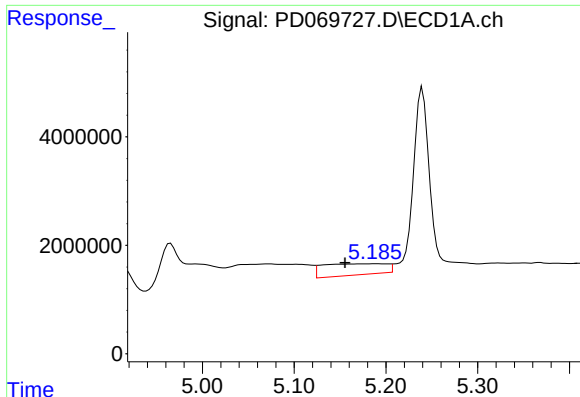

#8 Heptachlor epoxide


R.T.: 5.188 min
Delta R.T.: 0.033 min
Response: 9944251
Conc: 7.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

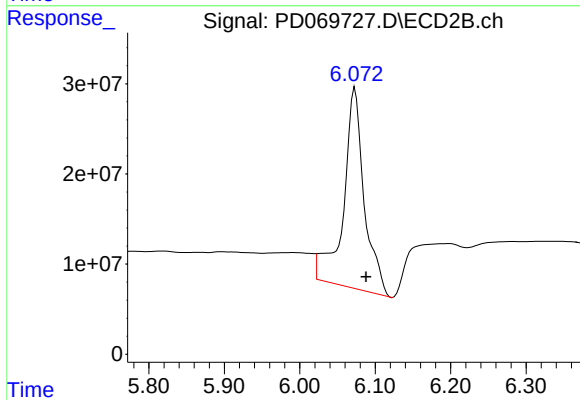


#8 Heptachlor epoxide

R.T.: 6.073 min
Delta R.T.: -0.015 min
Response: 428554711
Conc: 48.03 ng/ml

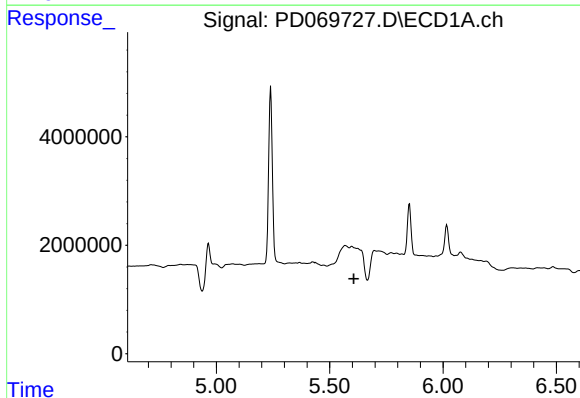


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.606 min
Response: 0
Conc: N.D.

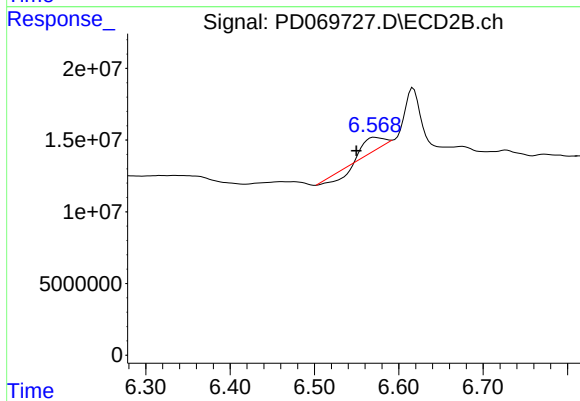

#12 4,4'-DDE


R.T.: 6.571 min
Delta R.T.: 0.022 min
Response: 5317078
Conc: 0.54 ng/ml

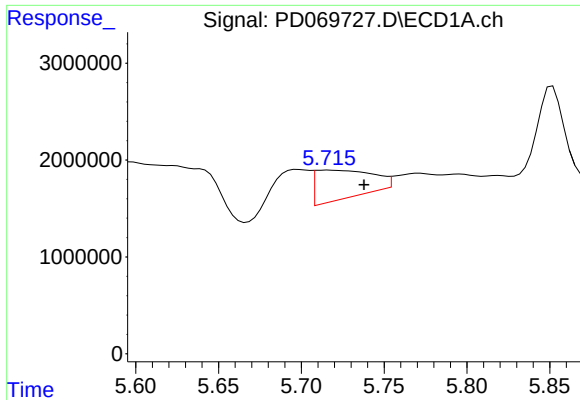

#13 Dieldrin


R.T.: 5.717 min
Delta R.T.: -0.021 min
Response: 6974669
Conc: 5.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

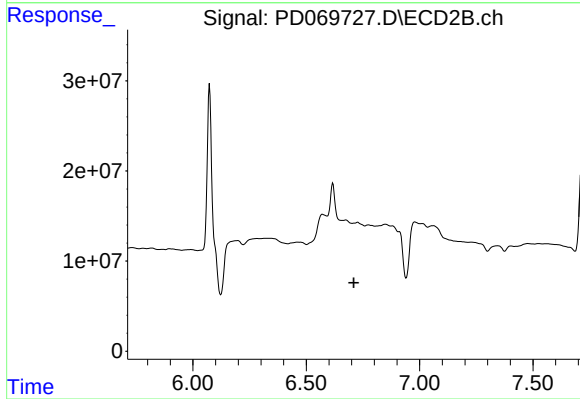


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

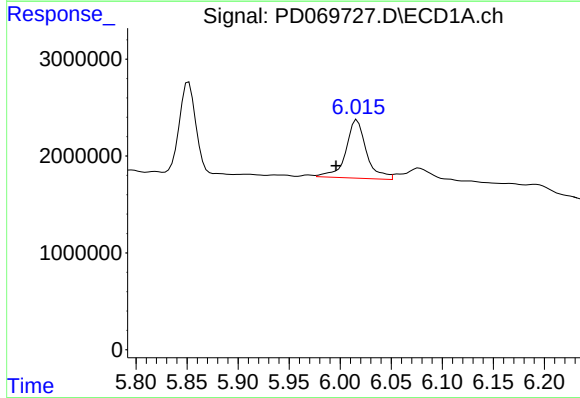


#14 Endrin

R.T.: 6.017 min
Delta R.T.: 0.021 min
Response: 8438576
Conc: 7.59 ng/ml

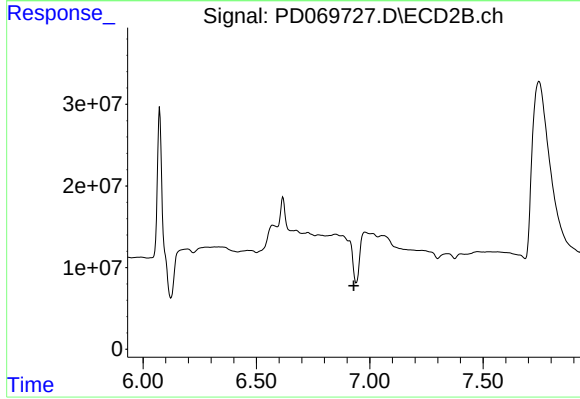

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.930 min
Response: 0
Conc: N.D.

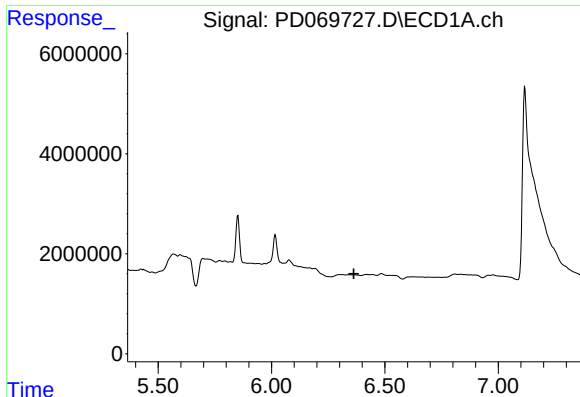

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

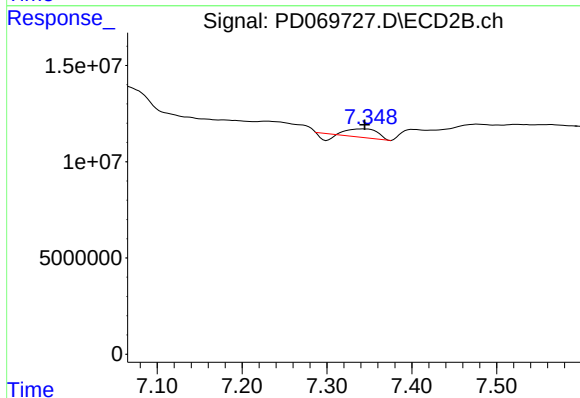


#17 4,4'-DDT

R.T.: 7.343 min
Delta R.T.: -0.001 min
Response: 9257723
Conc: 1.13 ng/ml

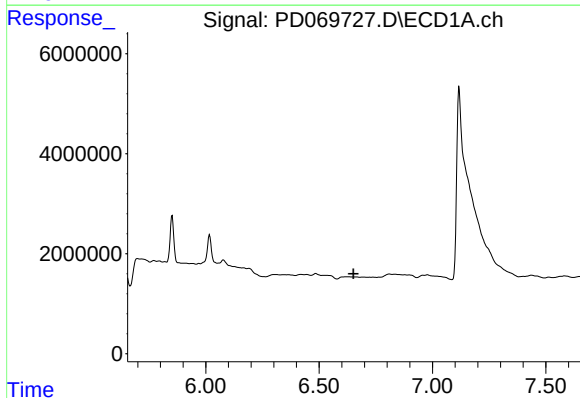


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.652 min
Response: 0
Conc: N.D.

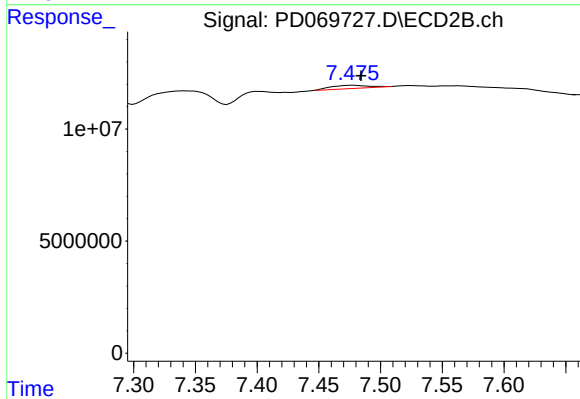

#19 Endosulfan Sulfate


R.T.: 7.477 min
Delta R.T.: -0.007 min
Response: 3013966
Conc: 0.38 ng/ml

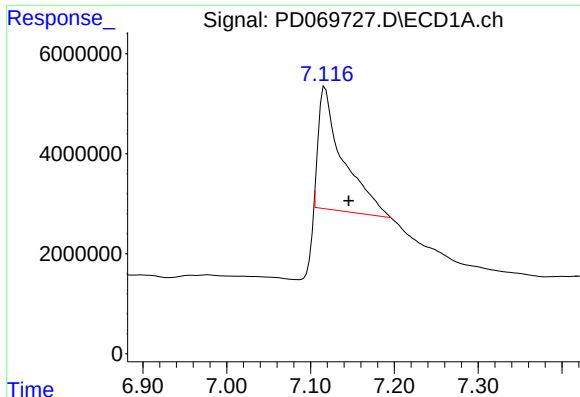

#21 Endrin ketone


R.T.: 7.118 min
Delta R.T.: -0.028 min
Response: 48934287
Conc: 39.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

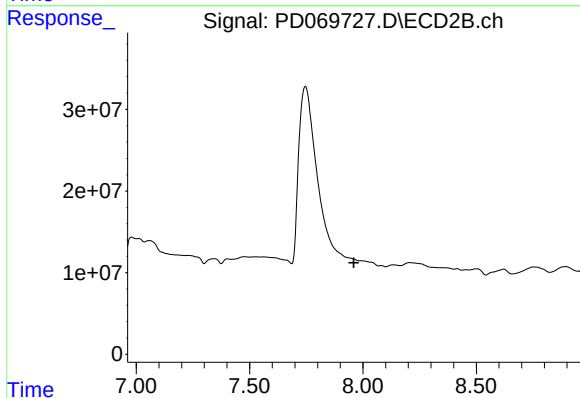


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.960 min
Response: 0
Conc: N.D.

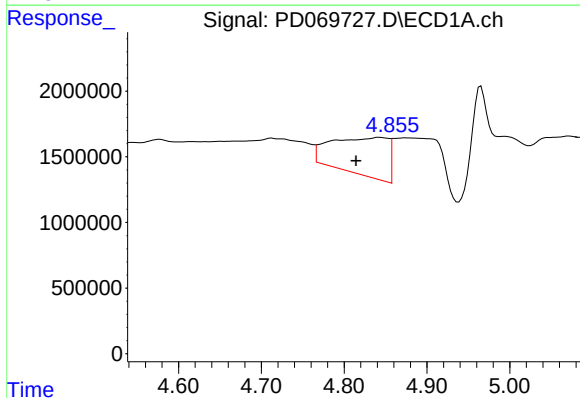


#24 Chlordane-2

R.T.: 4.843 min
Delta R.T.: 0.029 min
Response: 13622477
Conc: 289.71 ng/ml

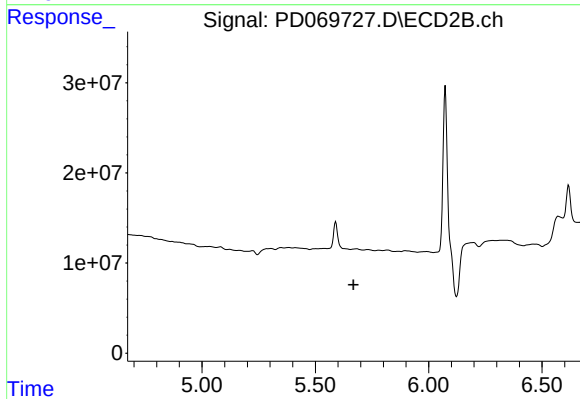

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.669 min
Response: 0
Conc: N.D.

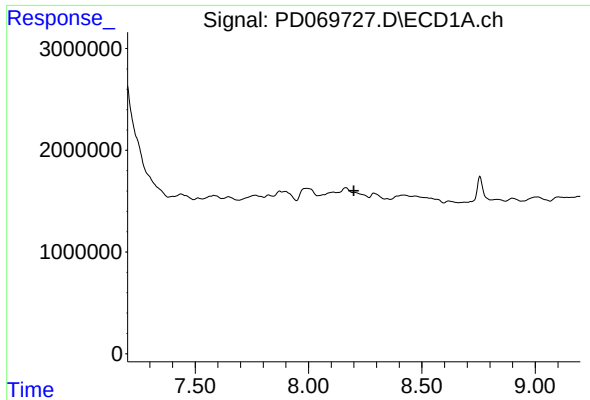

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

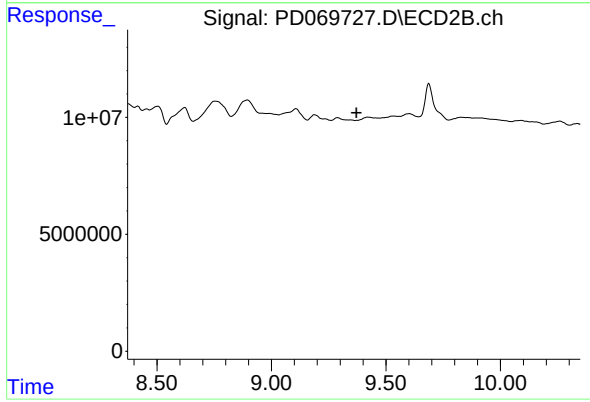

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.371 min
Response: 0
Conc: N.D.