

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052124\
 Data File : PD082920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2024 07:38
 Operator : AR\AJ
 Sample : P2518-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-MH-LL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/20/2024
 Supervised By : Ankita Jodhani 05/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 00:54:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
 Quant Title : GC Extractables
 QLast Update : Mon May 13 15:39:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.566	2.778	33362980	93313082	21.550	23.545
2) SA Decachlor...	9.121	7.902	35821999	74050384	17.939	19.157m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052124\
Data File : PD082920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2024 07:38
Operator : AR\AJ
Sample : P2518-05
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WC-MH-LL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/20/2024
Supervised By : Ankita Jodhani 05/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 00:54:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
Quant Title : GC Extractables
QLast Update : Mon May 13 15:39:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

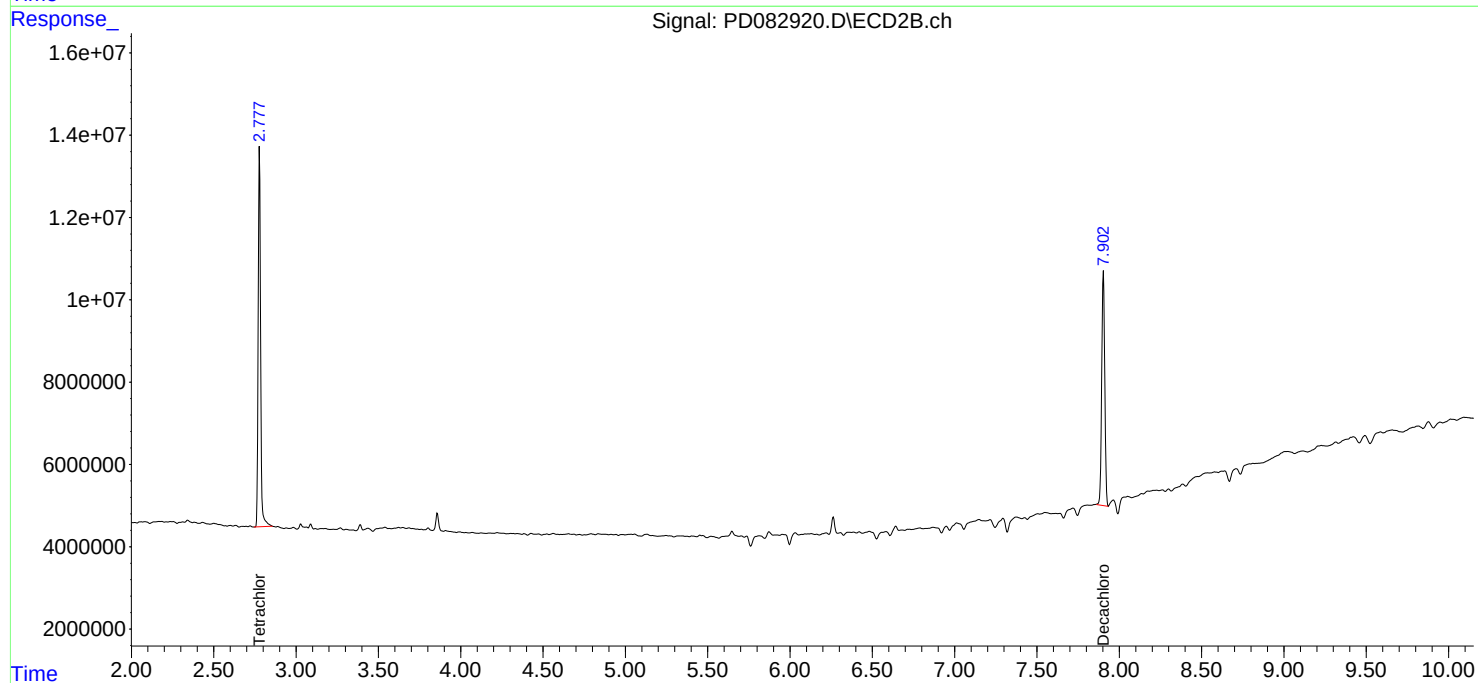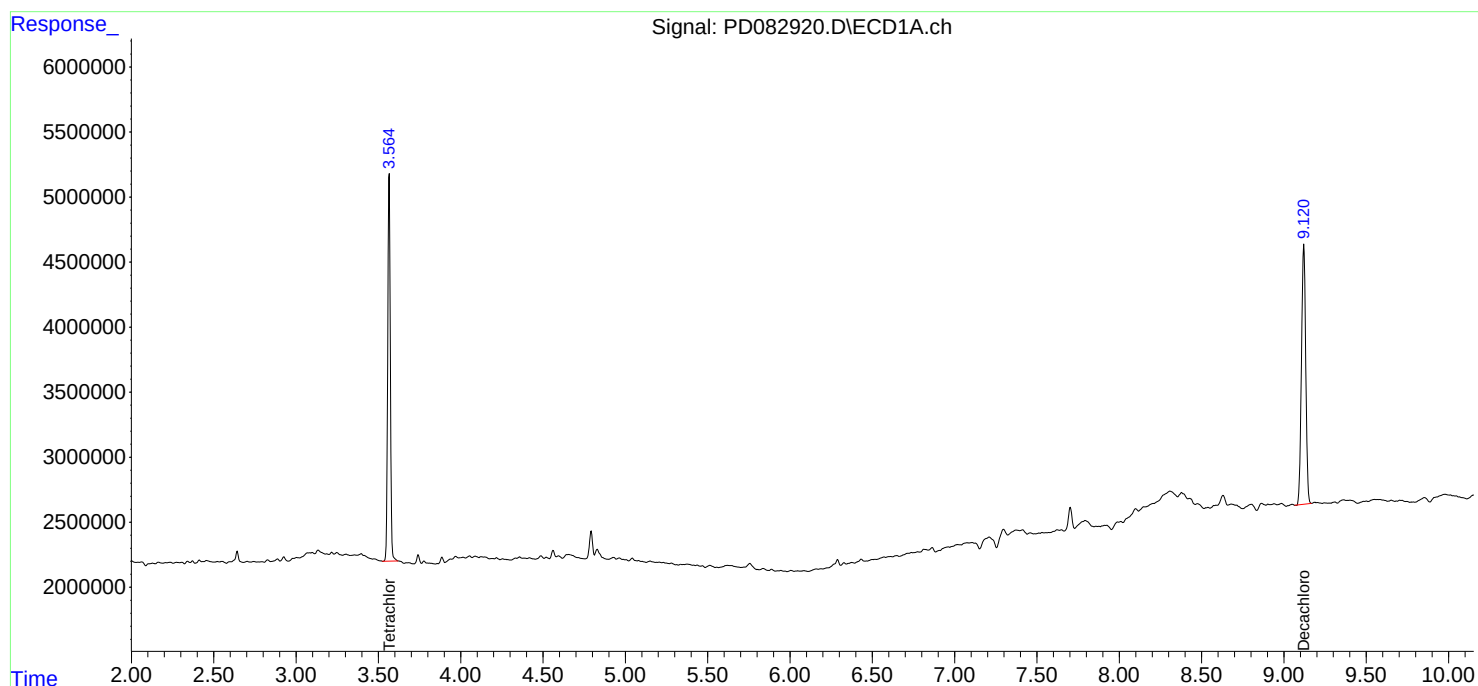

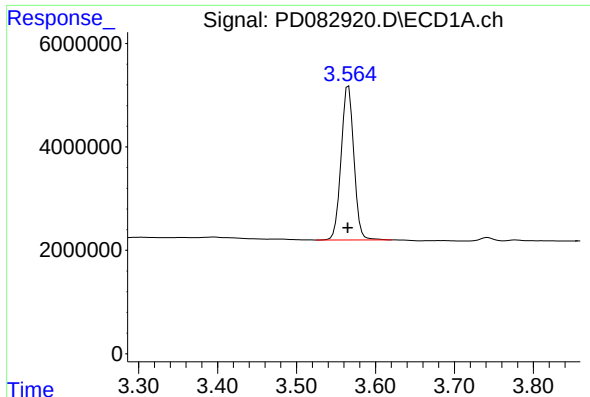


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 33362980
Conc: 21.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-MH-LL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/20/2024
Supervised By :Ankita Jodhani 05/20/2024

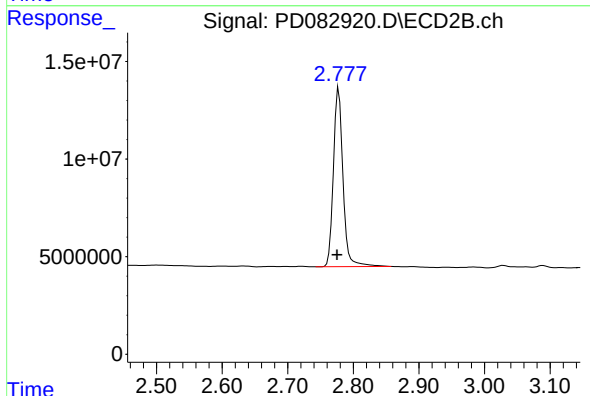


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.002 min
Response: 93313082
Conc: 23.54 ng/ml

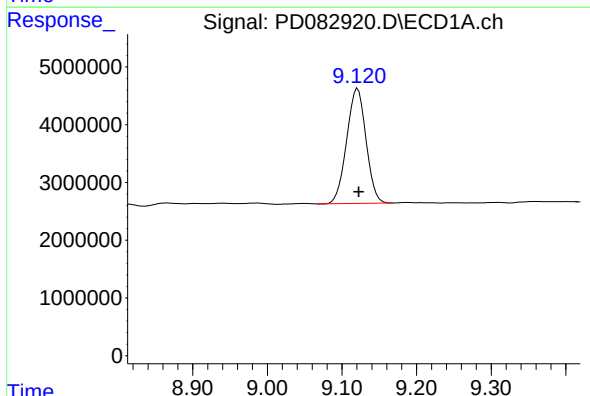

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.001 min
Response: 35821999
Conc: 17.94 ng/ml

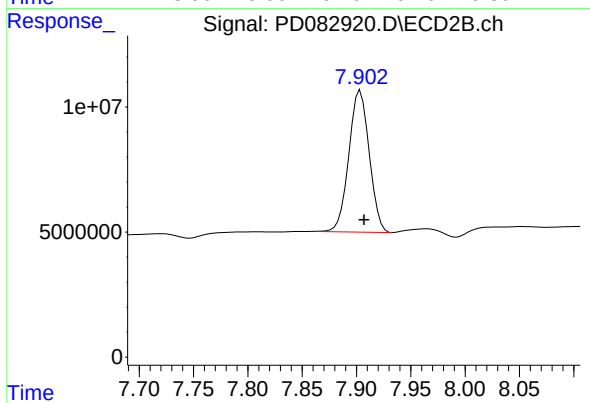

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 74050384
Conc: 19.16 ng/ml m