

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052219\
 Data File : PD053340.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 May 2019 11:54
 Operator : SM\AJ
 Sample : K2862-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFHK8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:10:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 22 06:53:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	3.985	14687912	20442850	20.046	20.764
27)	SA Decachlor...	8.014	9.028	21202164	32152791	32.051	31.127
Target Compounds							
3)	MA gamma-BHC...	0.000	4.683f	0	407862	N.D.	0.349
4)	MA Heptachlor	4.356f	5.141	2043894	2757017	2.812	2.371
5)	MB Aldrin	4.567	0.000	10674607	0	11.930	N.D. #
6)	B beta-BHC	4.238f	0.000	196886	0	0.474	N.D. #
7)	B delta-BHC	0.000	5.016	0	17199340	N.D.	14.136
8)	B Heptachlo...	0.000	5.862	0	232024	N.D.	0.198
10)	B trans-Chl...	0.000	6.065	0	1493203	N.D.	1.168
15)	B Endosulfa...	0.000	6.849f	0	725055	N.D.	0.690
16)	A 4,4'-DDD	0.000	6.849f	0	725055	N.D.	0.785

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052219\
Data File : PD053340.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 May 2019 11:54
Operator : SM\AJ
Sample : K2862-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:10:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 22 06:53:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

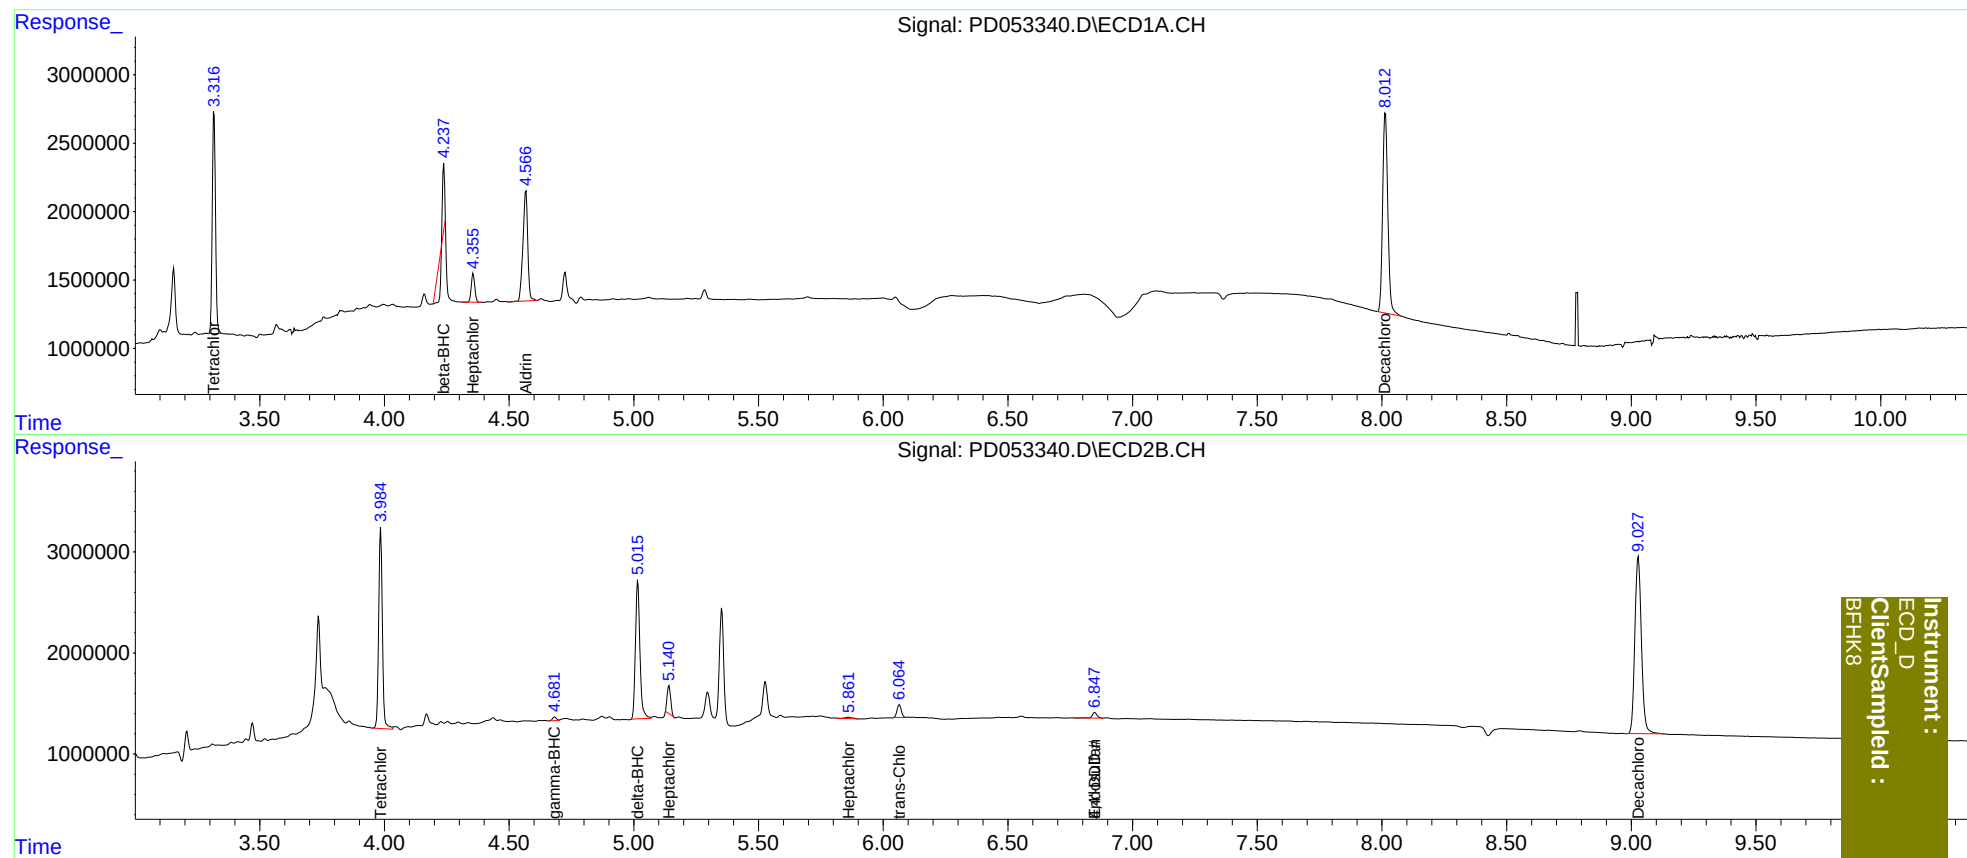


Instrument :
ECD_D
ClientSampled :
BFHK8

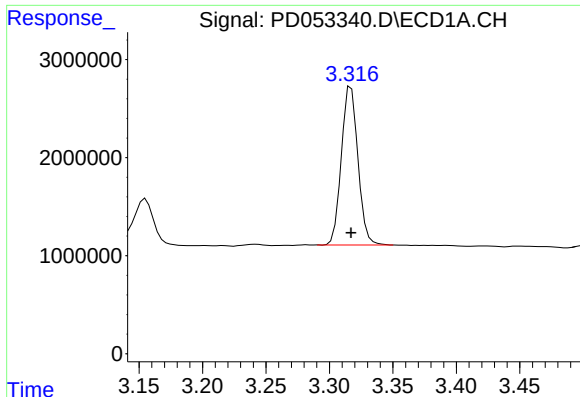

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 14687912
Conc: 20.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFHK8

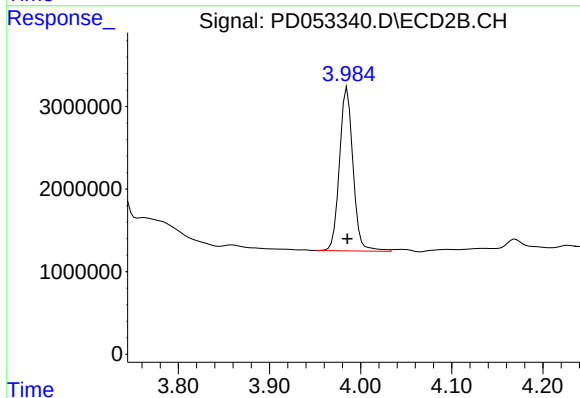


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 20442850
Conc: 20.76 ng/ml

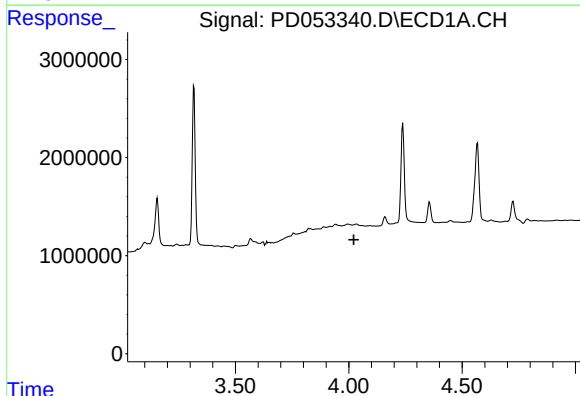


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.023 min
Response: 0
Conc: N.D.

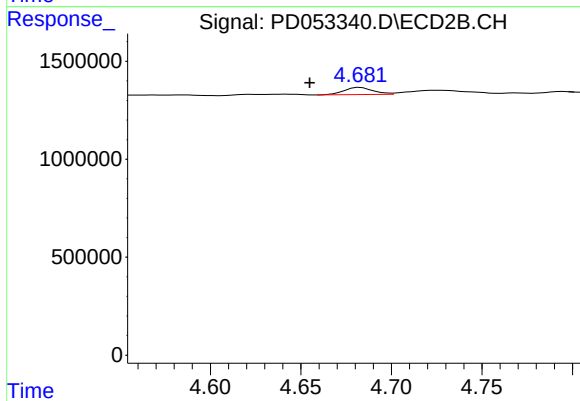

#3 gamma-BHC (Lindane)


R.T.: 4.683 min
Delta R.T.: 0.028 min
Response: 407862
Conc: 0.35 ng/ml

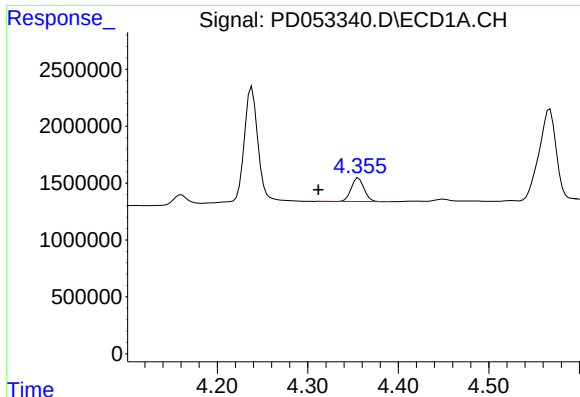

#4 Heptachlor


R.T.: 4.356 min
Delta R.T.: 0.044 min
Response: 2043894
Conc: 2.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFHK8

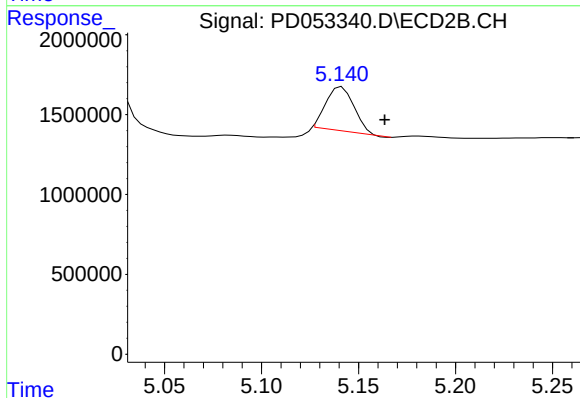


#4 Heptachlor

R.T.: 5.141 min
Delta R.T.: -0.022 min
Response: 2757017
Conc: 2.37 ng/ml

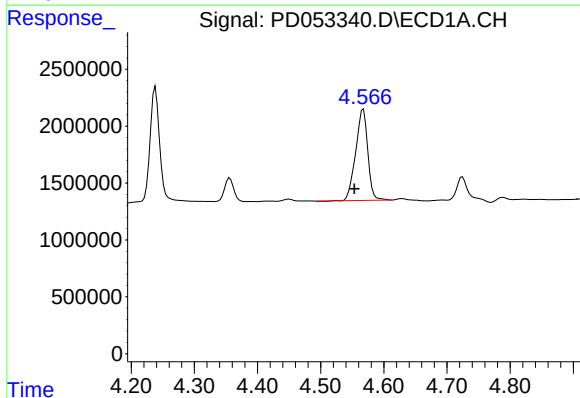


#5 Aldrin

R.T.: 4.567 min
Delta R.T.: 0.014 min
Response: 10674607
Conc: 11.93 ng/ml

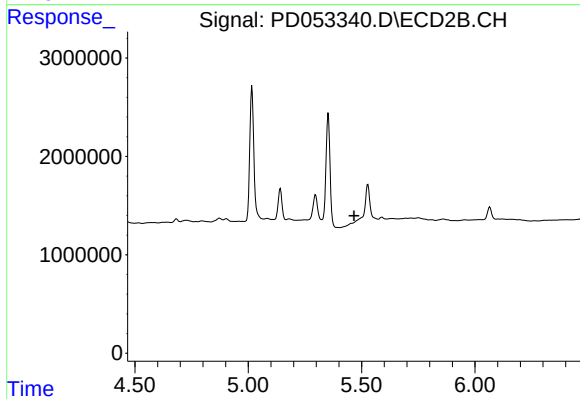

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.467 min
Response: 0
Conc: N.D.

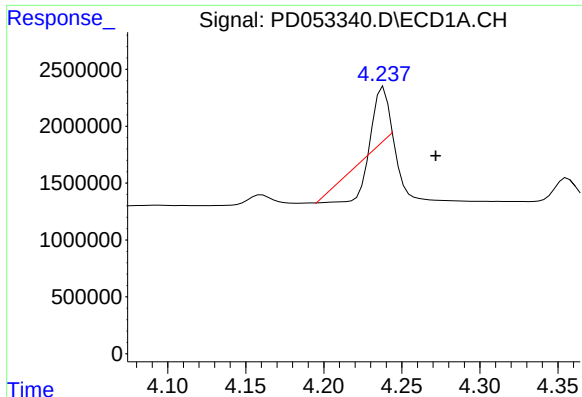

#6 beta-BHC


R.T.: 4.238 min
Delta R.T.: -0.033 min
Response: 196886
Conc: 0.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFHK8

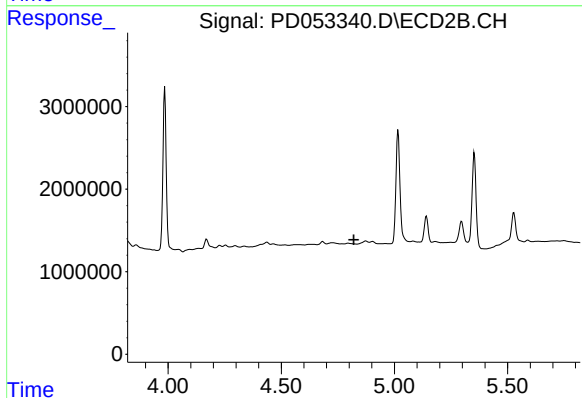


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.821 min
Response: 0
Conc: N.D.

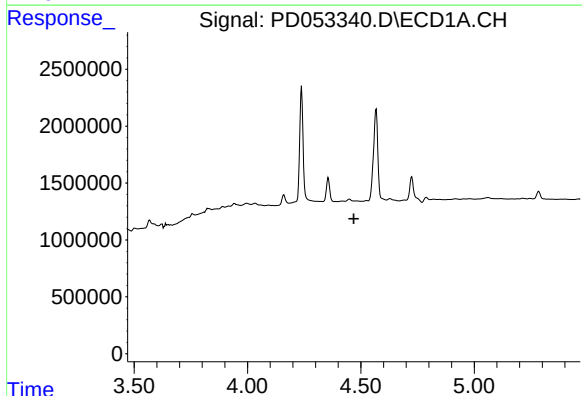


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.470 min
Response: 0
Conc: N.D.

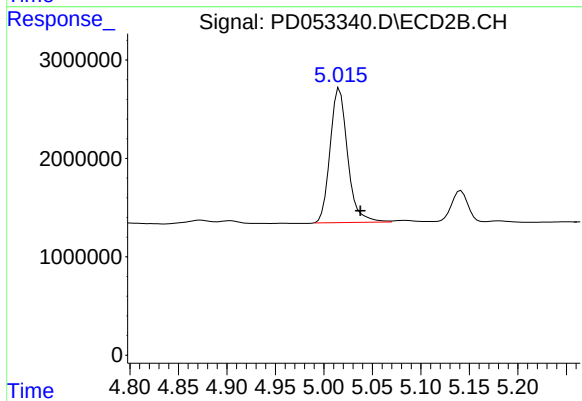

#7 delta-BHC


R.T.: 5.016 min
Delta R.T.: -0.021 min
Response: 17199340
Conc: 14.14 ng/ml

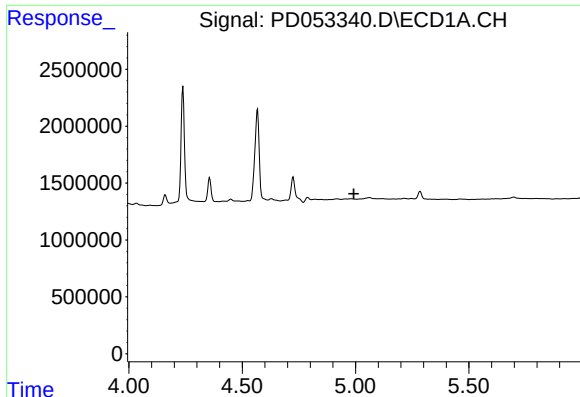

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFHK8

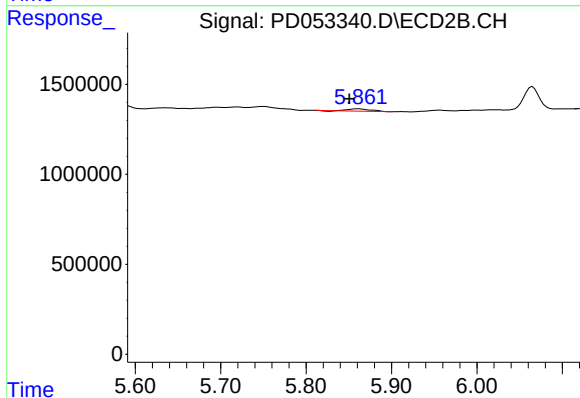


#8 Heptachlor epoxide

R.T.: 5.862 min
Delta R.T.: 0.011 min
Response: 232024
Conc: 0.20 ng/ml

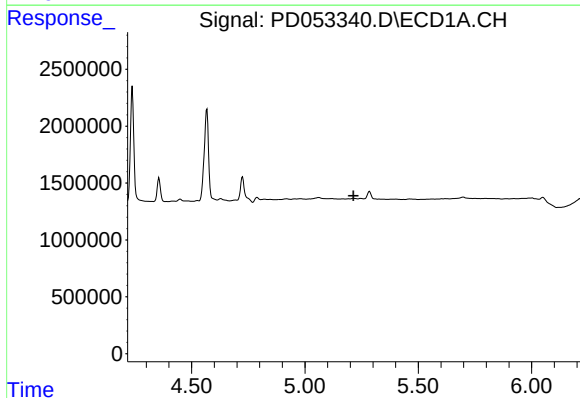


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.215 min
Response: 0
Conc: N.D.

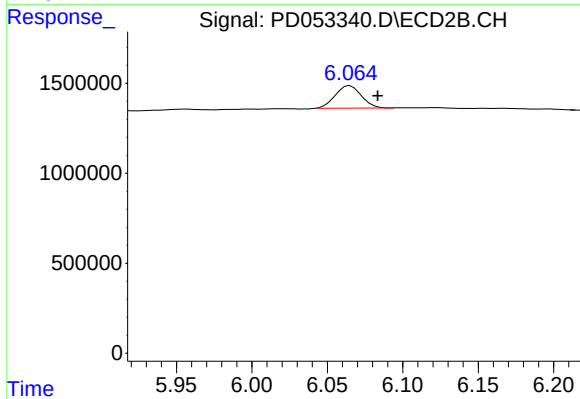

#10 trans-Chlordane


R.T.: 6.065 min
Delta R.T.: -0.018 min
Response: 1493203
Conc: 1.17 ng/ml

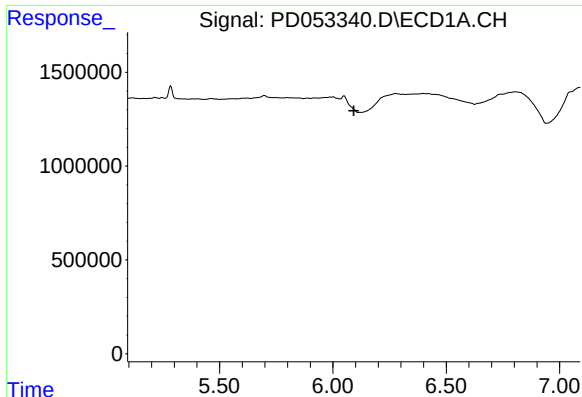

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.093 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFHK8

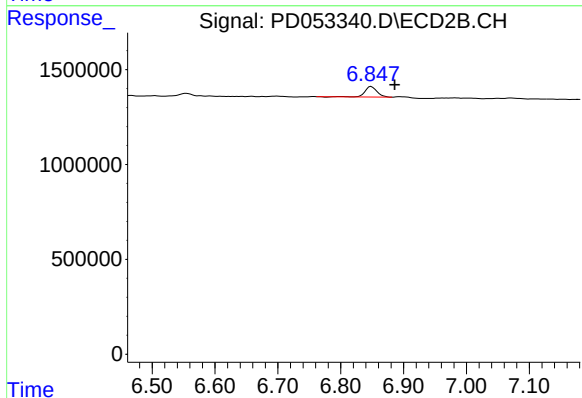


#15 Endosulfan II

R.T.: 6.849 min
Delta R.T.: -0.038 min
Response: 725055
Conc: 0.69 ng/ml

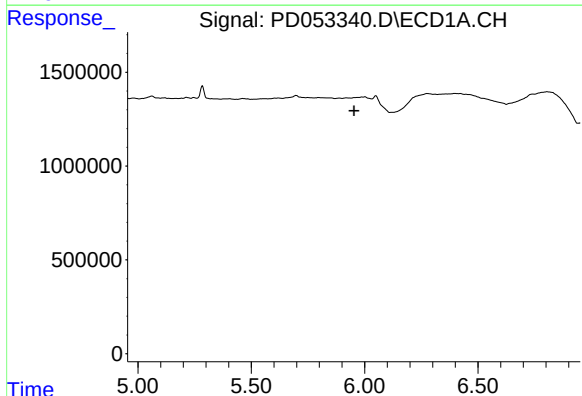


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.953 min
Response: 0
Conc: N.D.

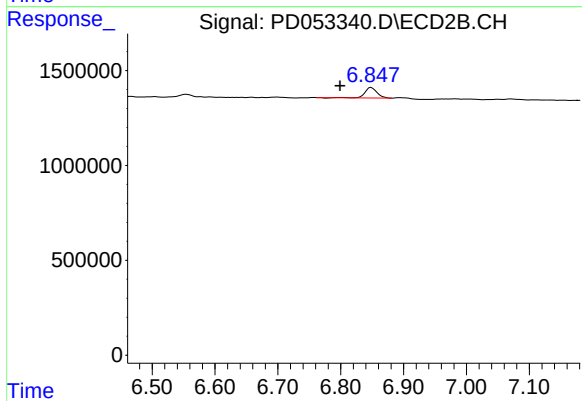

#16 4,4'-DDD


R.T.: 6.849 min
Delta R.T.: 0.050 min
Response: 725055
Conc: 0.78 ng/ml

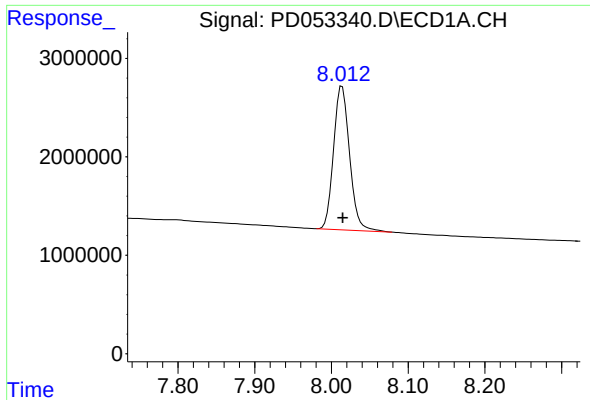

#27 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.001 min
Response: 21202164
Conc: 32.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFHK8

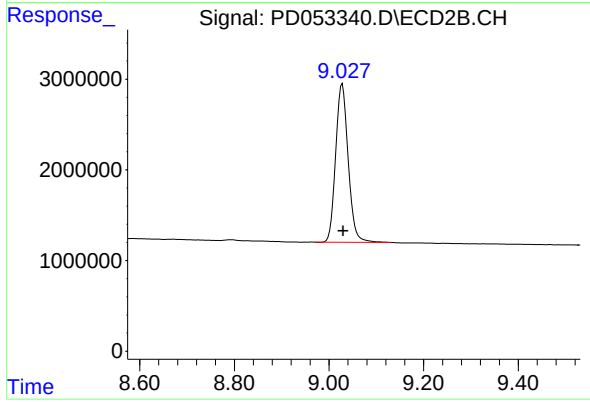

#27 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.001 min
Response: 32152791
Conc: 31.13 ng/ml