

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052220\
 Data File : PD058081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2020 08:36
 Operator : AJ\MA
 Sample : L2733-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5CB5

Manual Integrations
 APPROVED

mohammad
 5/26/2020 1:49:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 13:14:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051820CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue May 19 05:31:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.865	29034458	22280973	37.035m	18.976m#
27)	SA Decachlor...	7.848	8.850	15482979	24186302	17.897m	21.523m
Target Compounds							
10)	B trans-Chl...	5.069	5.940	6045737	12923872	6.470m	9.400m#
11)	B cis-Chlor...	5.127	6.014	7186673	16435959	7.645	11.860 #
13)	MA Dieldrin	5.416	6.316	11046903	16161647	11.233	11.554
14)	MA Endrin	5.675	6.528	2426117	834230	2.844	0.719m#
17)	MA 4,4'-DDT	6.058	6.918f	28268185	45353691	39.837m	41.577

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052220\
Data File : PD058081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2020 08:36
Operator : AJ\MA
Sample : L2733-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:14:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051820CLP.M
Quant Title : GC Extractables
QLast Update : Tue May 19 05:31:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

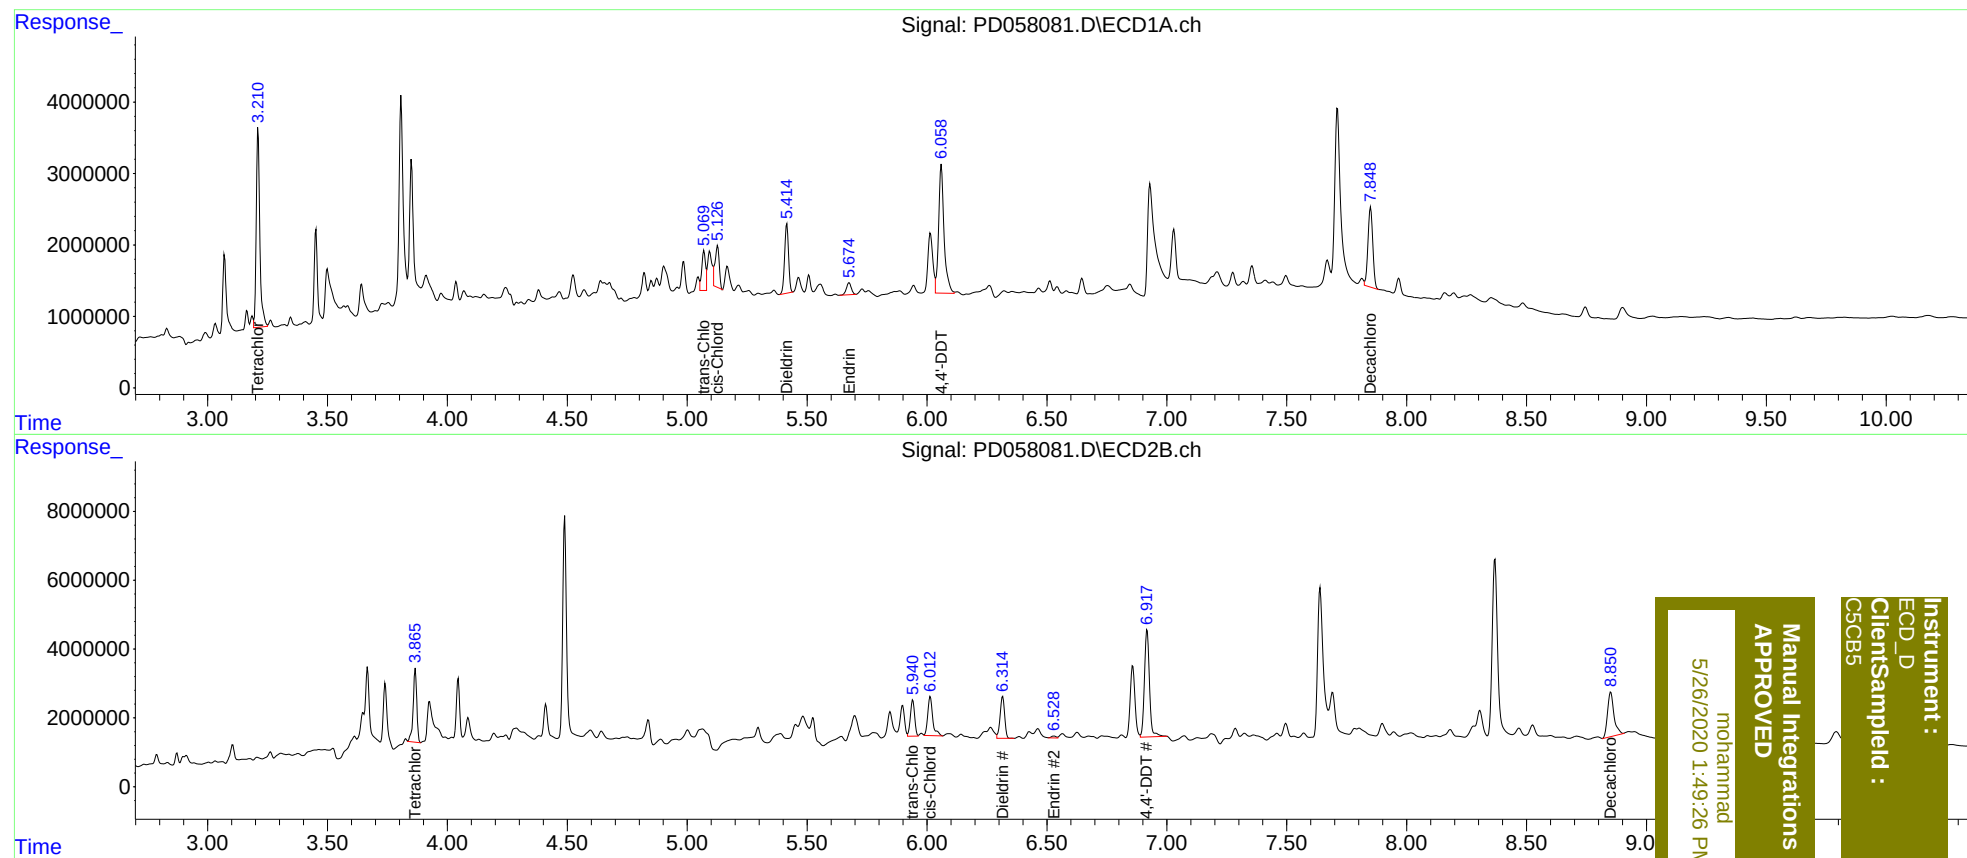

Manual Integrations
APPROVED

mohammad
5/26/2020 1:49:26 PM

Instrument :
ECD_D
ClientSampled :
C5CB5