

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052221\
 Data File : PD063200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2021 11:44
 Operator : AR\AJ
 Sample : PB136573TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB136573TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 11:57:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	23708271	246.5E6	21.523	21.269
28)	SA Decachlor...	8.194	9.021	26361032	224.0E6	20.946	21.955
Target Compounds							
7)	B delta-BHC	0.000	5.024	0	19254314	N.D.	1.378 #
8)	B Heptachlo...	0.000	5.850	0	6651195	N.D.	0.435 #
15)	B Endosulfa...	0.000	6.898f	0	3787975	N.D.	0.316 #
16)	A 4,4'-DDD	0.000	6.809f	0	4847165	N.D.	0.400 #
18)	B Endrin al...	0.000	7.001	0	703715	N.D.	0.069 #
21)	B Endrin ke...	0.000	7.721f	0	2296591	N.D.	0.191 #
23)	Chlordane-1	4.335f	4.944f	122465	2391358	3.351	3.573
24)	Chlordane-2	0.000	5.415	0	6458726	N.D.	13.251 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052221\
Data File : PD063200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2021 11:44
Operator : AR\AJ
Sample : PB136573TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB136573TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 11:57:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

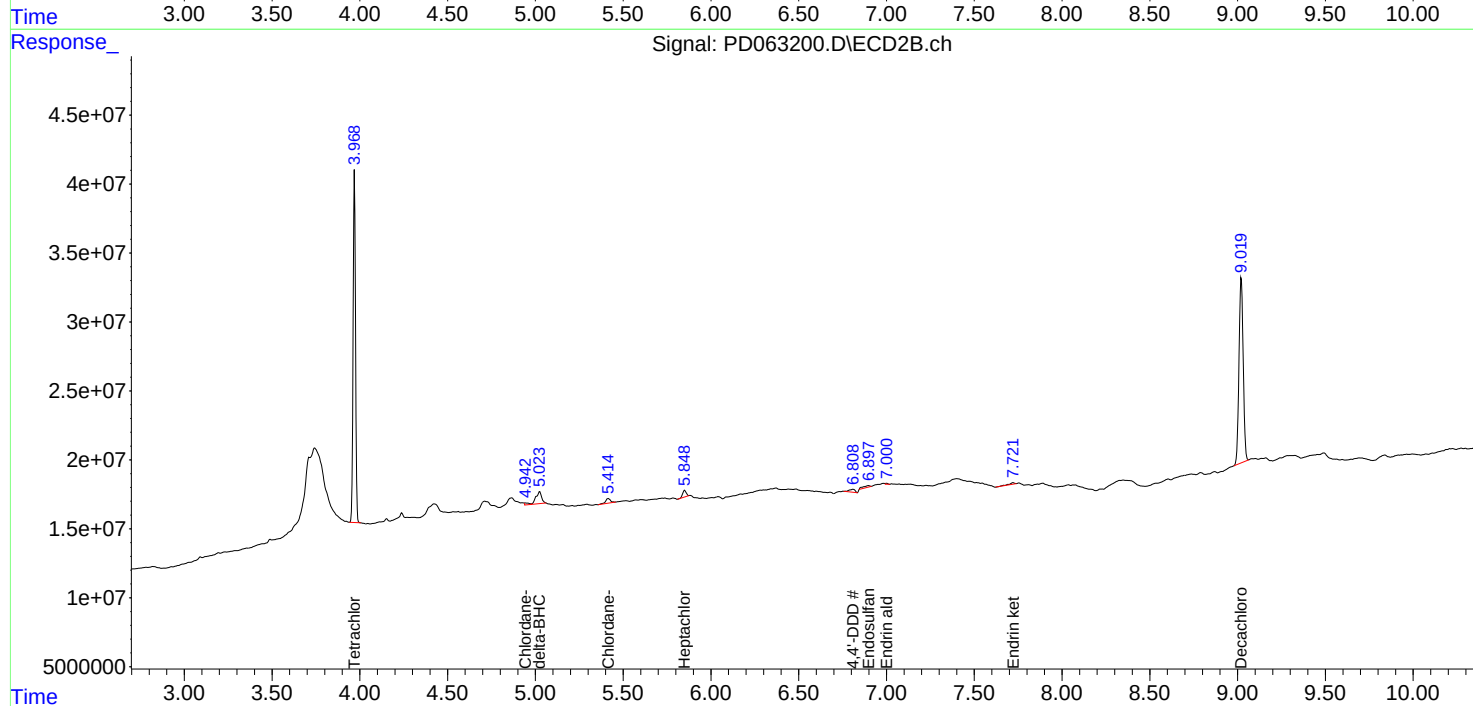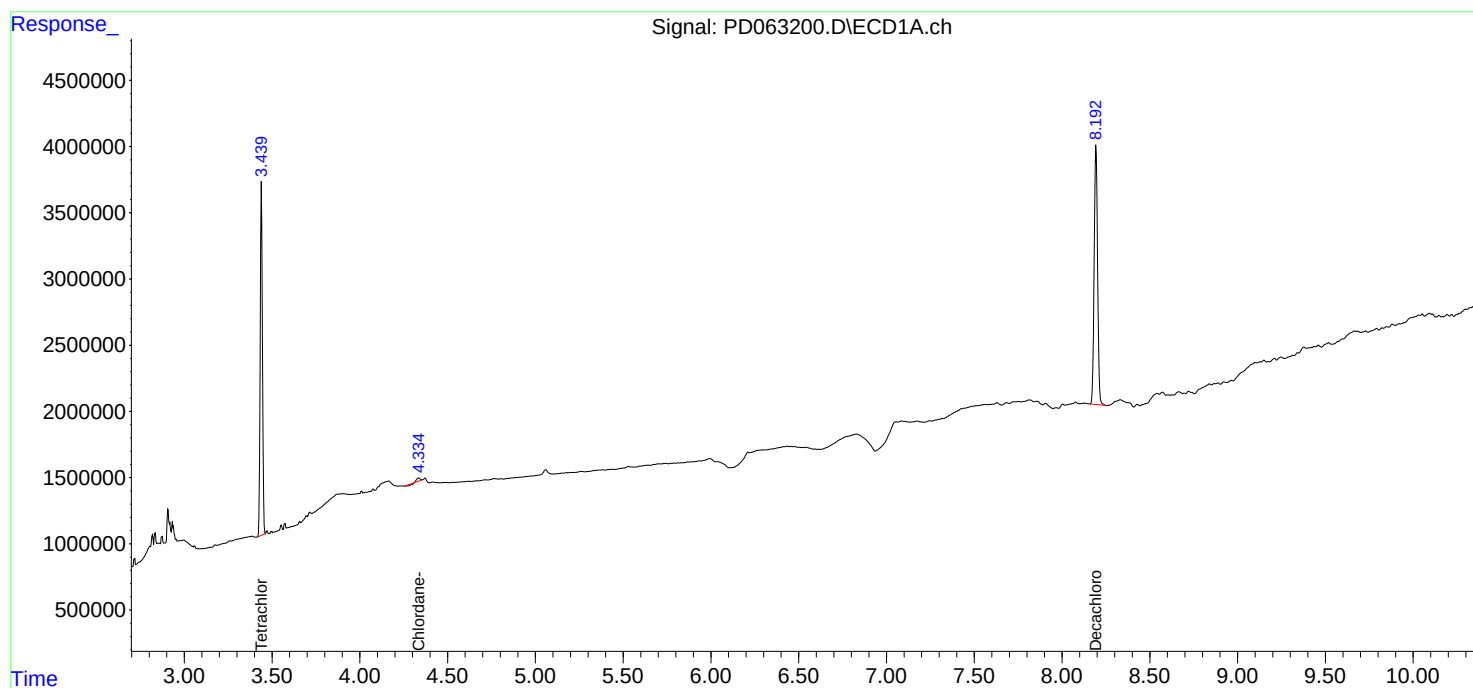


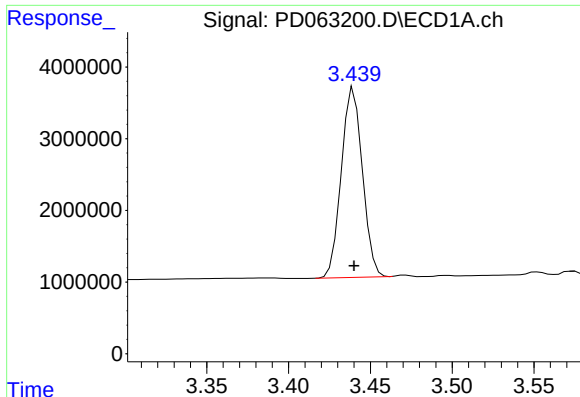

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 23708271
Conc: 21.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB136573TB

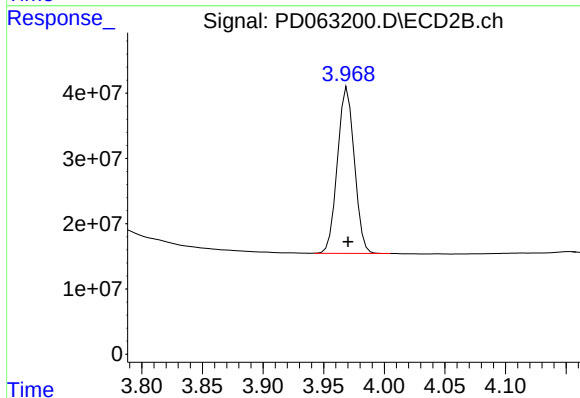


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 246472992
Conc: 21.27 ng/ml

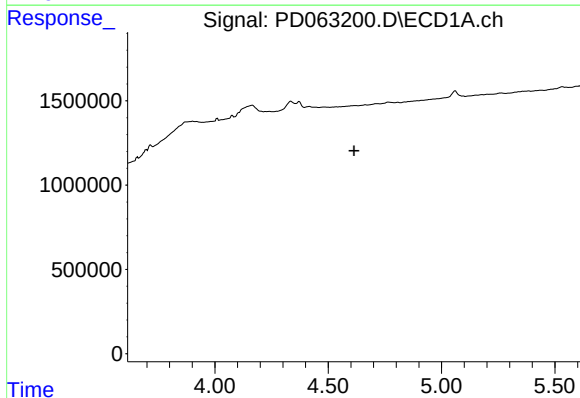


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.614 min
Response: 0
Conc: N.D.

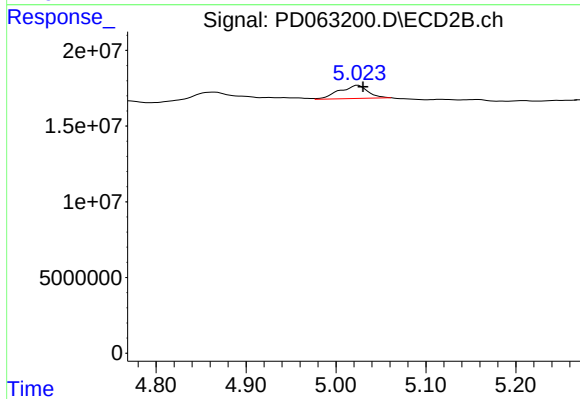

#7 delta-BHC


R.T.: 5.024 min
Delta R.T.: -0.006 min
Response: 19254314
Conc: 1.38 ng/ml

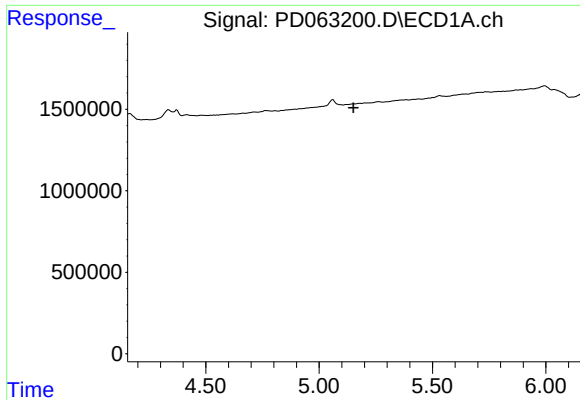

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136573TB

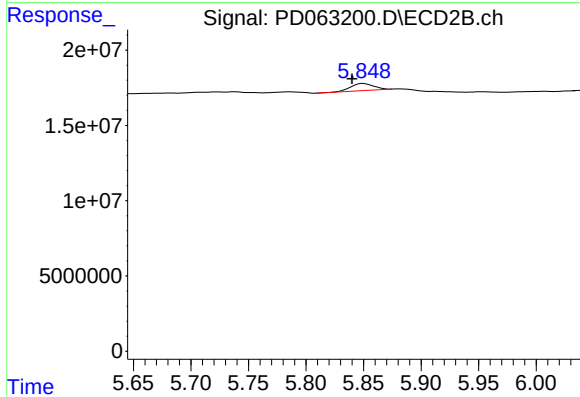


#8 Heptachlor epoxide

R.T.: 5.850 min
Delta R.T.: 0.010 min
Response: 6651195
Conc: 0.43 ng/ml

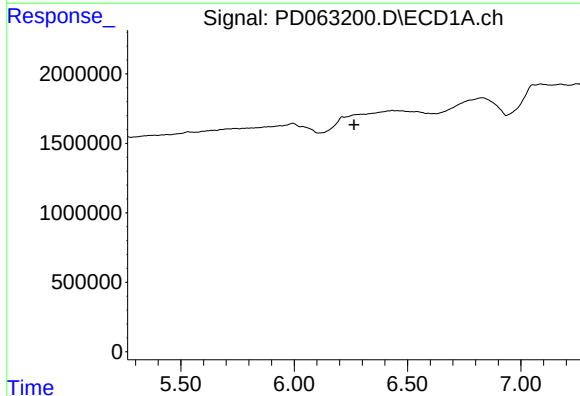


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.264 min
Response: 0
Conc: N.D.

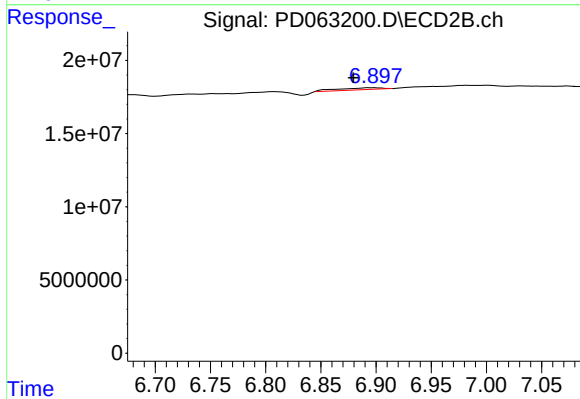

#15 Endosulfan II


R.T.: 6.898 min
Delta R.T.: 0.018 min
Response: 3787975
Conc: 0.32 ng/ml

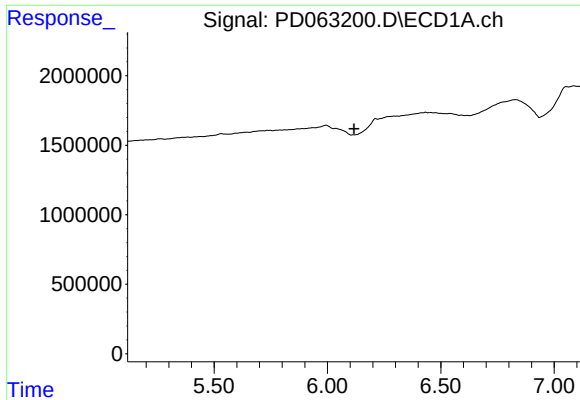

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136573TB

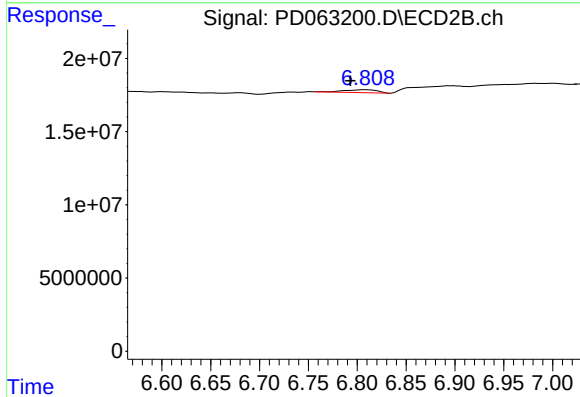


#16 4,4'-DDD

R.T.: 6.809 min
Delta R.T.: 0.016 min
Response: 4847165
Conc: 0.40 ng/ml

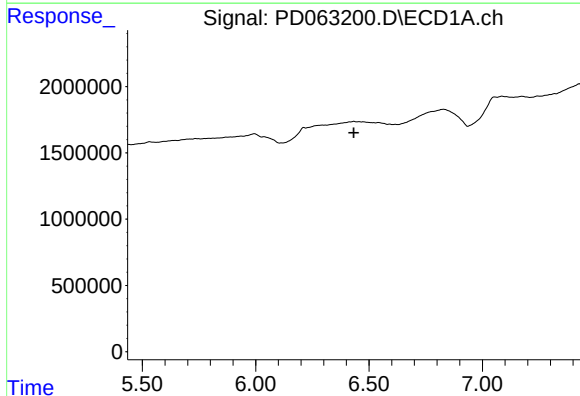


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.433 min
Response: 0
Conc: N.D.

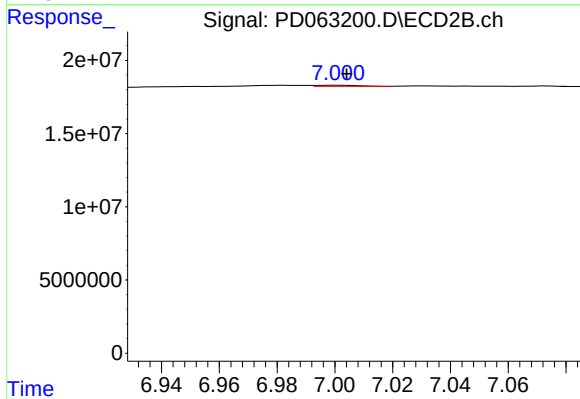

#18 Endrin aldehyde


R.T.: 7.001 min
Delta R.T.: -0.003 min
Response: 703715
Conc: 0.07 ng/ml

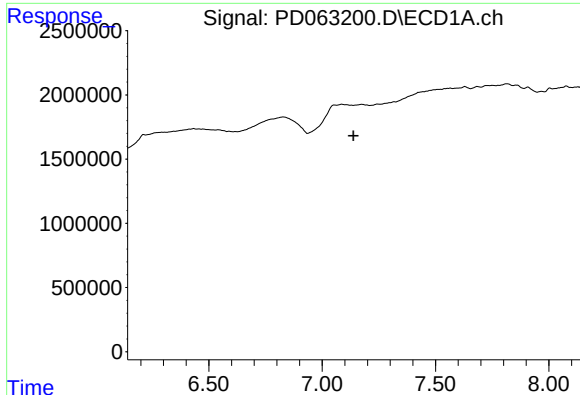

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136573TB

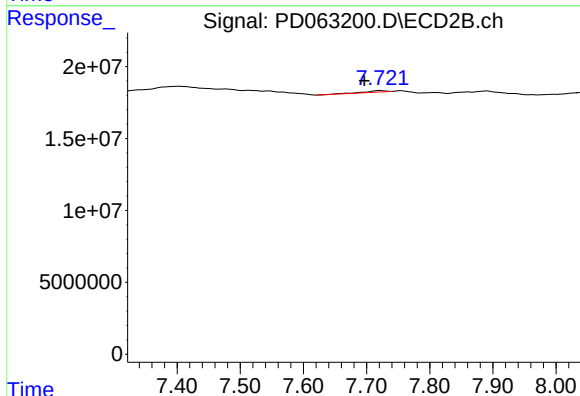


#21 Endrin ketone

R.T.: 7.721 min
Delta R.T.: 0.025 min
Response: 2296591
Conc: 0.19 ng/ml

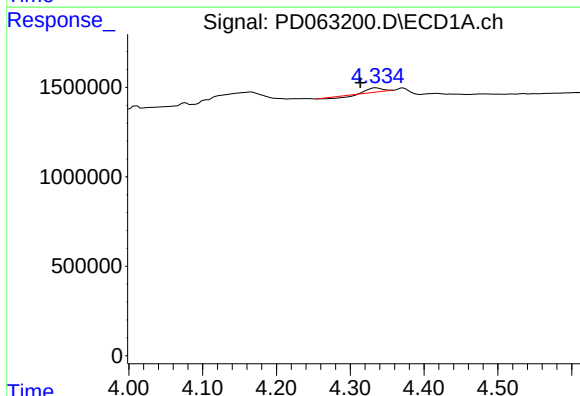


#23 Chlordane-1

R.T.: 4.335 min
Delta R.T.: 0.021 min
Response: 122465
Conc: 3.35 ng/ml

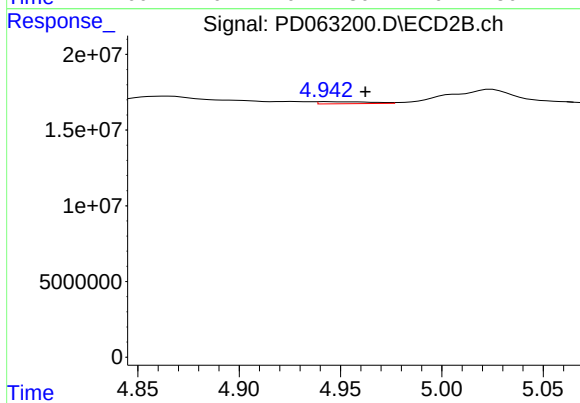

#23 Chlordane-1


R.T.: 4.944 min
Delta R.T.: -0.019 min
Response: 2391358
Conc: 3.57 ng/ml

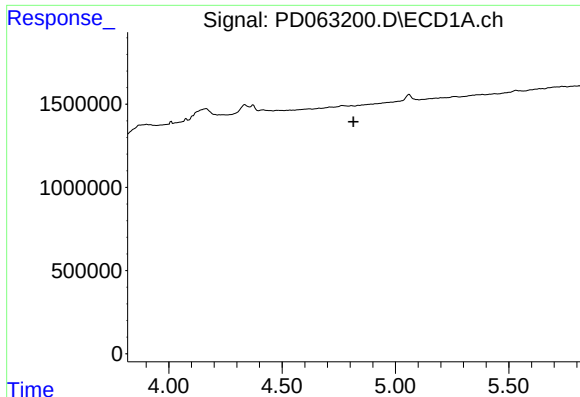

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136573TB

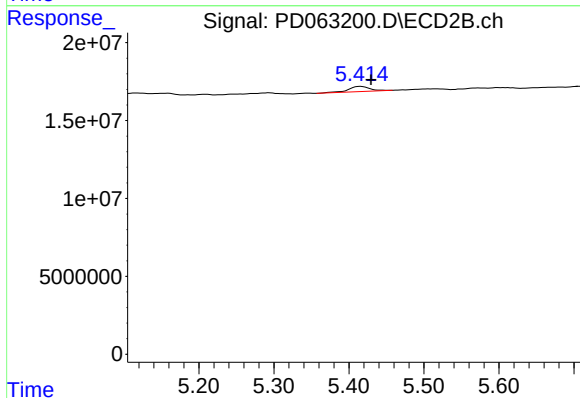


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: -0.015 min
Response: 6458726
Conc: 13.25 ng/ml

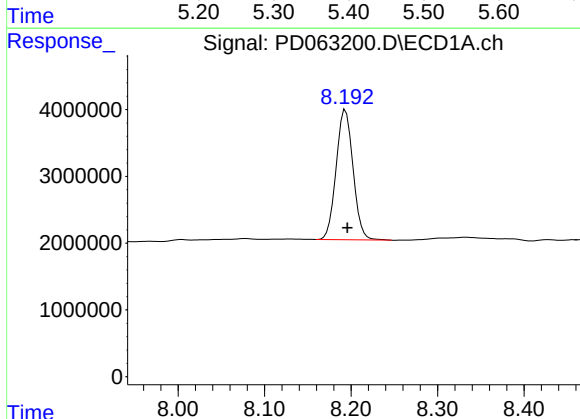

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 26361032
Conc: 20.95 ng/ml

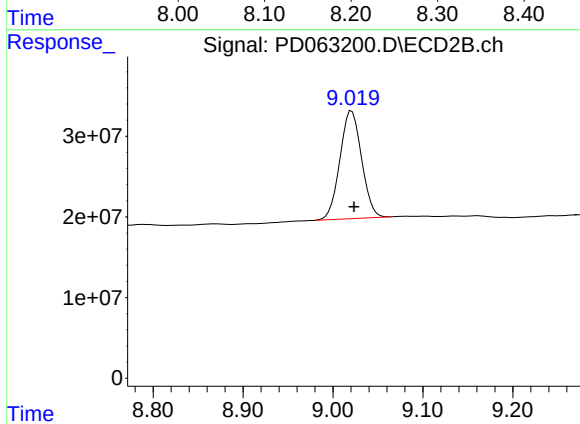

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: -0.003 min
Response: 223981836
Conc: 21.95 ng/ml