

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052221\
 Data File : PD063195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2021 10:27
 Operator : AR\AJ
 Sample : M2437-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-3RE

Manual Integrations
 APPROVED

Ankita
 5/24/2021 2:58:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 11:54:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.969	15027350	120.5E6	13.642m	10.401m
28)	SA Decachlor...	8.199	9.024	92694030	839.8E6	73.651	82.314

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052221\
Data File : PD063195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2021 10:27
Operator : AR\AJ
Sample : M2437-08RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-3RE


Manual Integrations
APPROVED

Ankita
5/24/2021 2:58:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 11:54:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

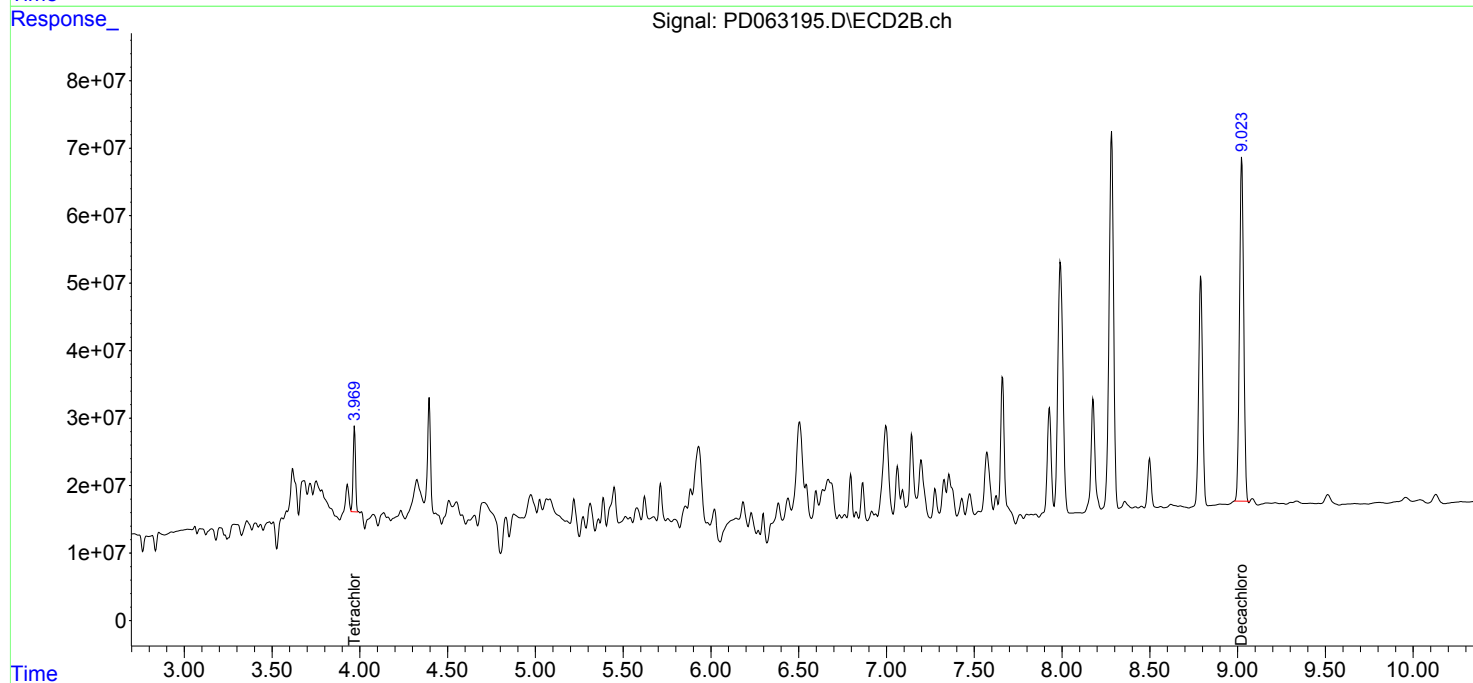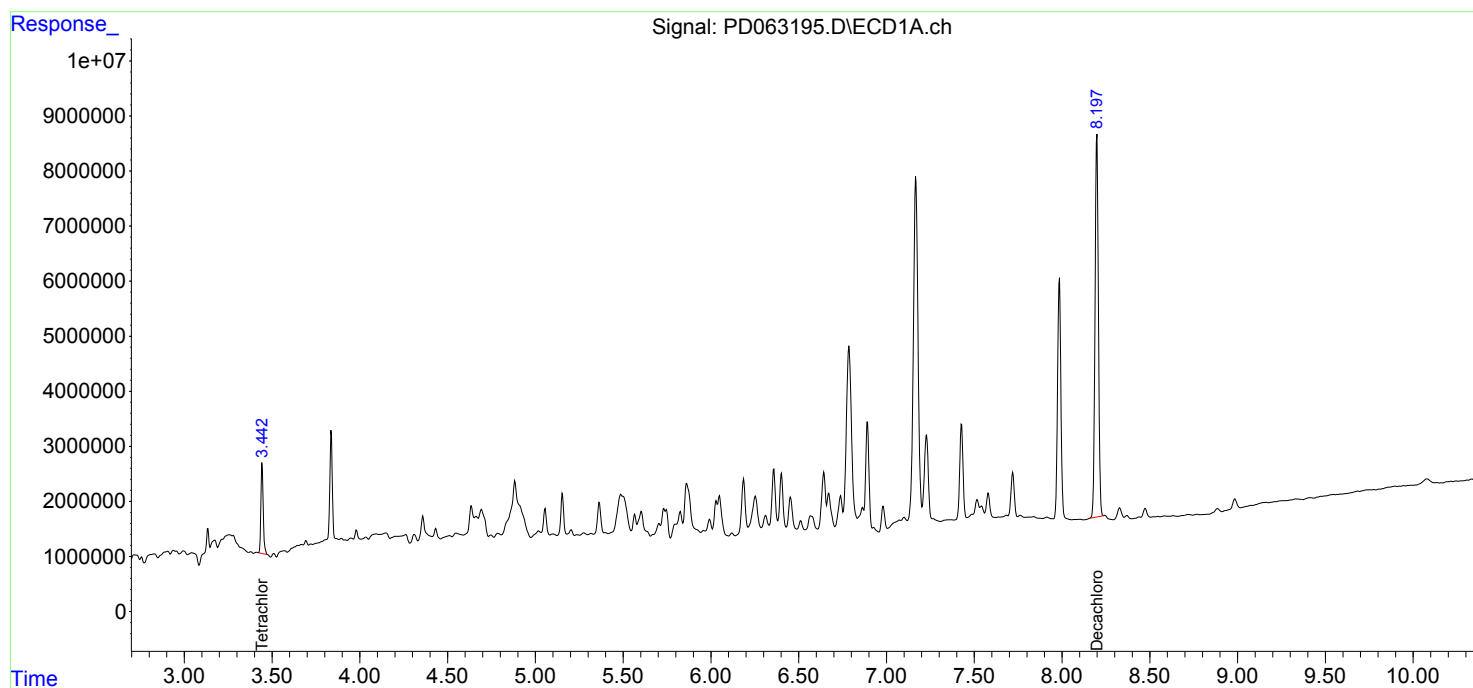

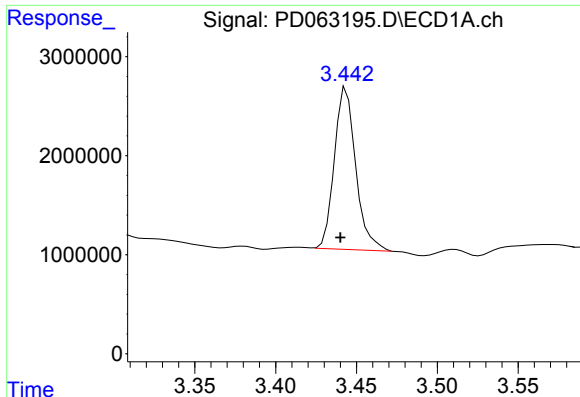


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.002 min
Response: 15027350
Conc: 13.64 ng/ml m

Instrument :
ECD_D
ClientSampleId :
TP-3RE


Manual Integrations
APPROVED

Ankita
5/24/2021 2:58:40 PM

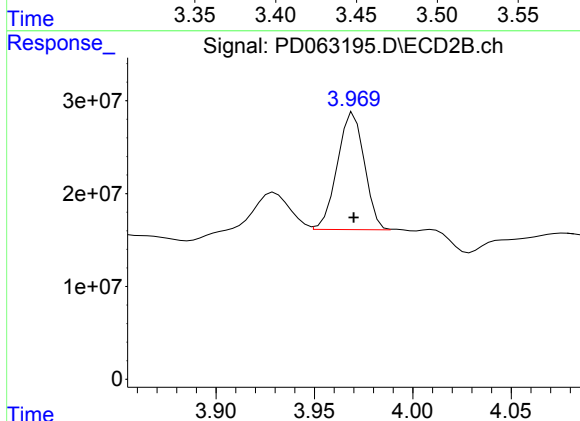


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 120529276
Conc: 10.40 ng/ml m

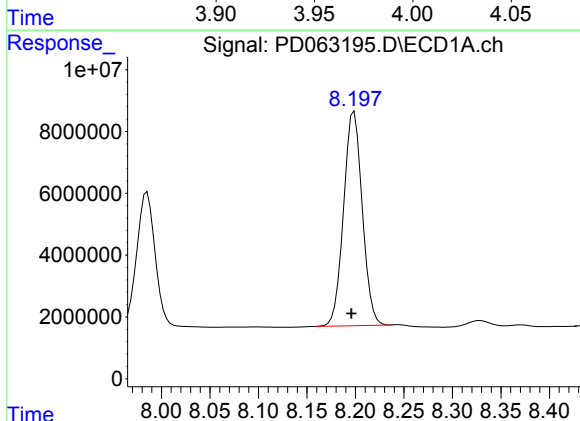

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.003 min
Response: 92694030
Conc: 73.65 ng/ml

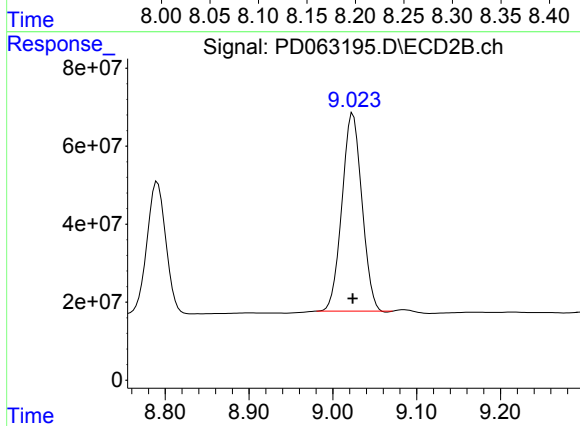

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 839766699
Conc: 82.31 ng/ml