

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052225\
 Data File : PD088689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2025 13:36
 Operator : AR\AJ
 Sample : Q2068-03RE 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LAW-25-0074RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/22/2025
 Supervised By : mohammad ahmed 05/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 14:40:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051925.M
 Quant Title : GC Extractables
 QLast Update : Mon May 19 15:27:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.894	2711029	152.3E6	1.253m	10.066m#
28) SA Decachlor...	9.067	8.073	1297012	6492270	0.379m	0.356m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052225\
Data File : PD088689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2025 13:36
Operator : AR\AJ
Sample : Q2068-03RE 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
LAW-25-0074RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/22/2025
Supervised By : mohammad ahmed 05/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 14:40:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051925.M
Quant Title : GC Extractables
QLast Update : Mon May 19 15:27:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

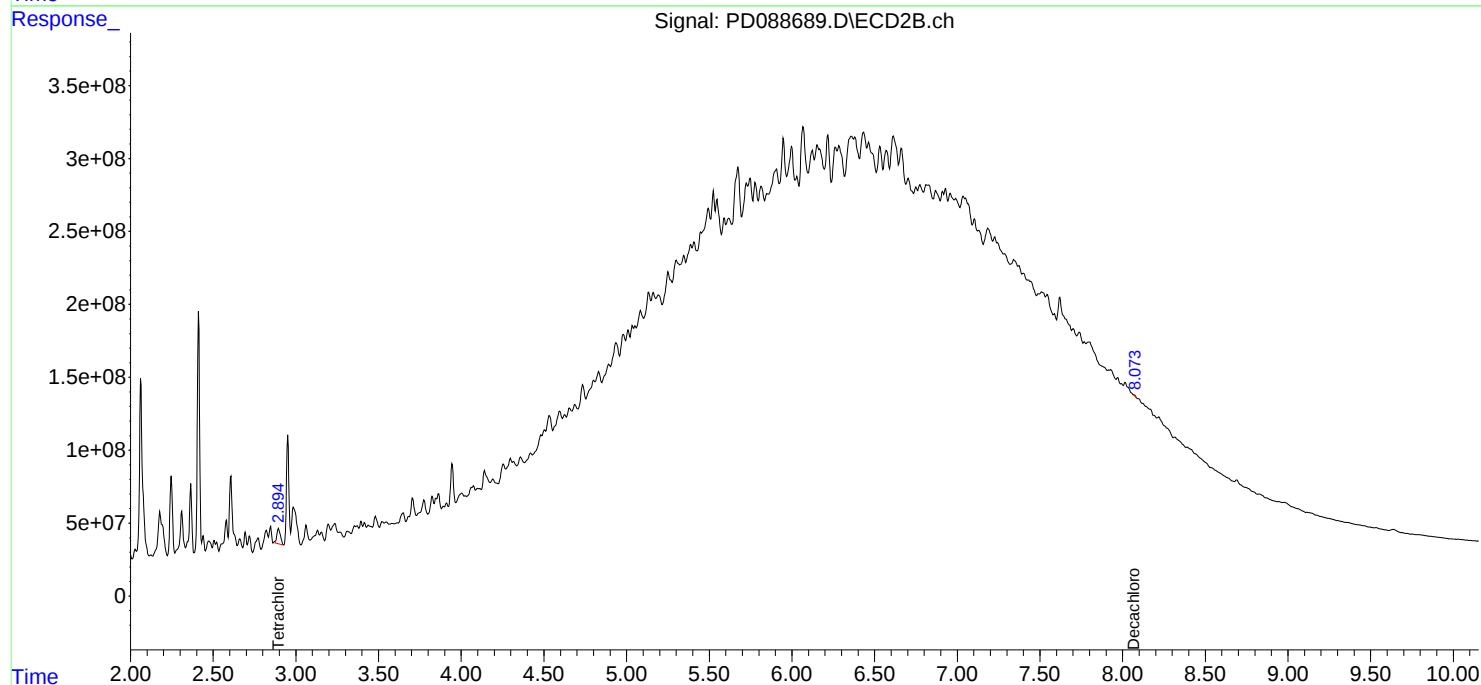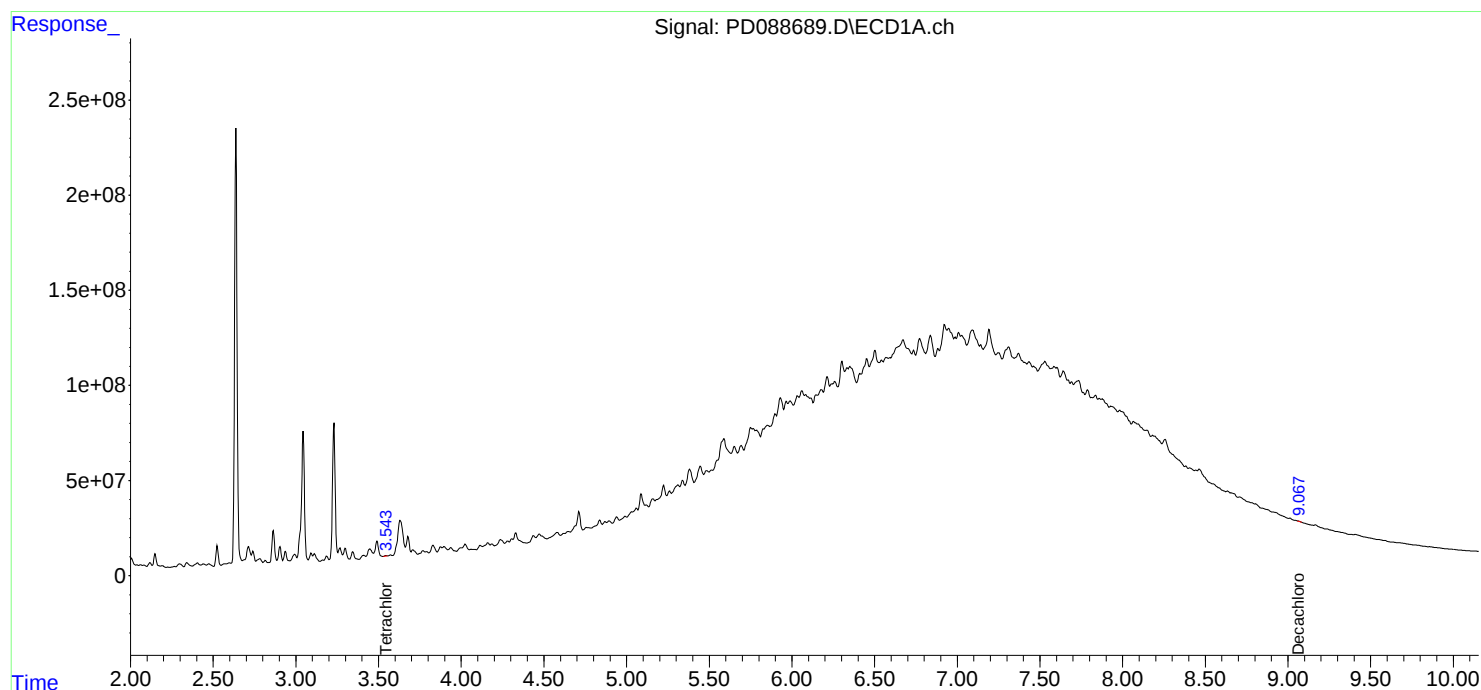

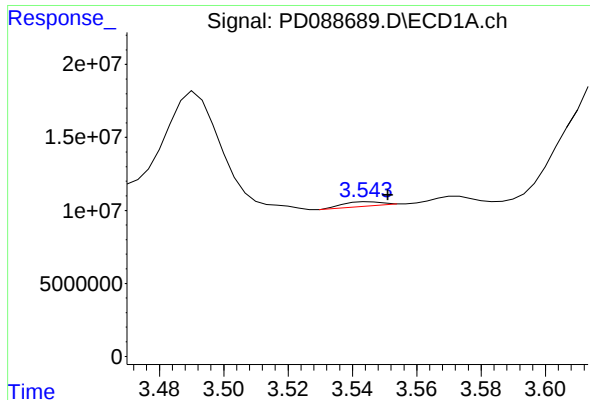


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.008 min
Response: 2711029
Conc: 1.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
LAW-25-0074RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/22/2025
Supervised By :mohammad ahmed 05/23/2025

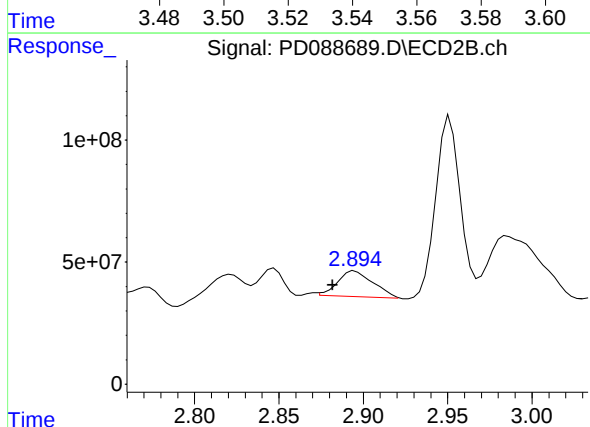


#1 Tetrachloro-m-xylene

R.T.: 2.894 min
Delta R.T.: 0.012 min
Response: 152260809
Conc: 10.07 ng/ml m

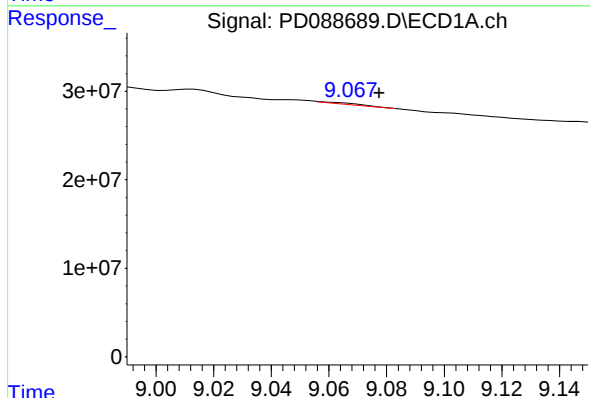

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: -0.011 min
Response: 1297012
Conc: 0.38 ng/ml m

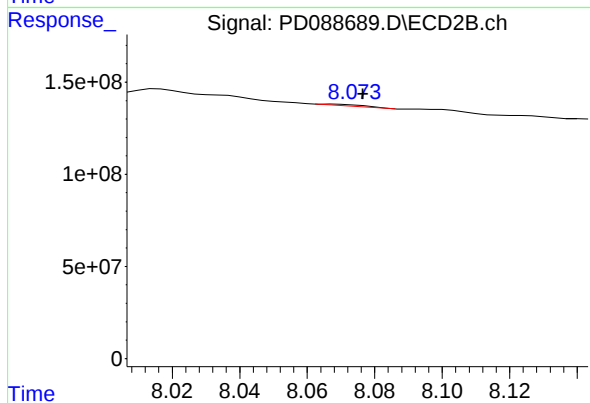

#28 Decachlorobiphenyl

R.T.: 8.073 min
Delta R.T.: -0.003 min
Response: 6492270
Conc: 0.36 ng/ml m