

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
 Data File : PD069768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 00:35
 Operator : AR\AJ
 Sample : N2873-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 03:22:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.172	11988934	151.9E6	11.964	15.898 #
28)	SA Decachlor...	8.196	9.366	8507670	53123603	7.887	8.864
Target Compounds							
3)	MA gamma-BHC...	4.173	0.000	7181290	0	4.864	N.D. #
10)	B gamma-Chl...	0.000	6.325	0	6171861	N.D.	0.577 #
13)	MA Dieldrin	0.000	6.707	0	12401130	N.D.	1.211 #
25)	Chlordane-3	0.000	6.325	0	6171861	N.D.	4.214 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
Data File : PD069768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 00:35
Operator : AR\AJ
Sample : N2873-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 03:22:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

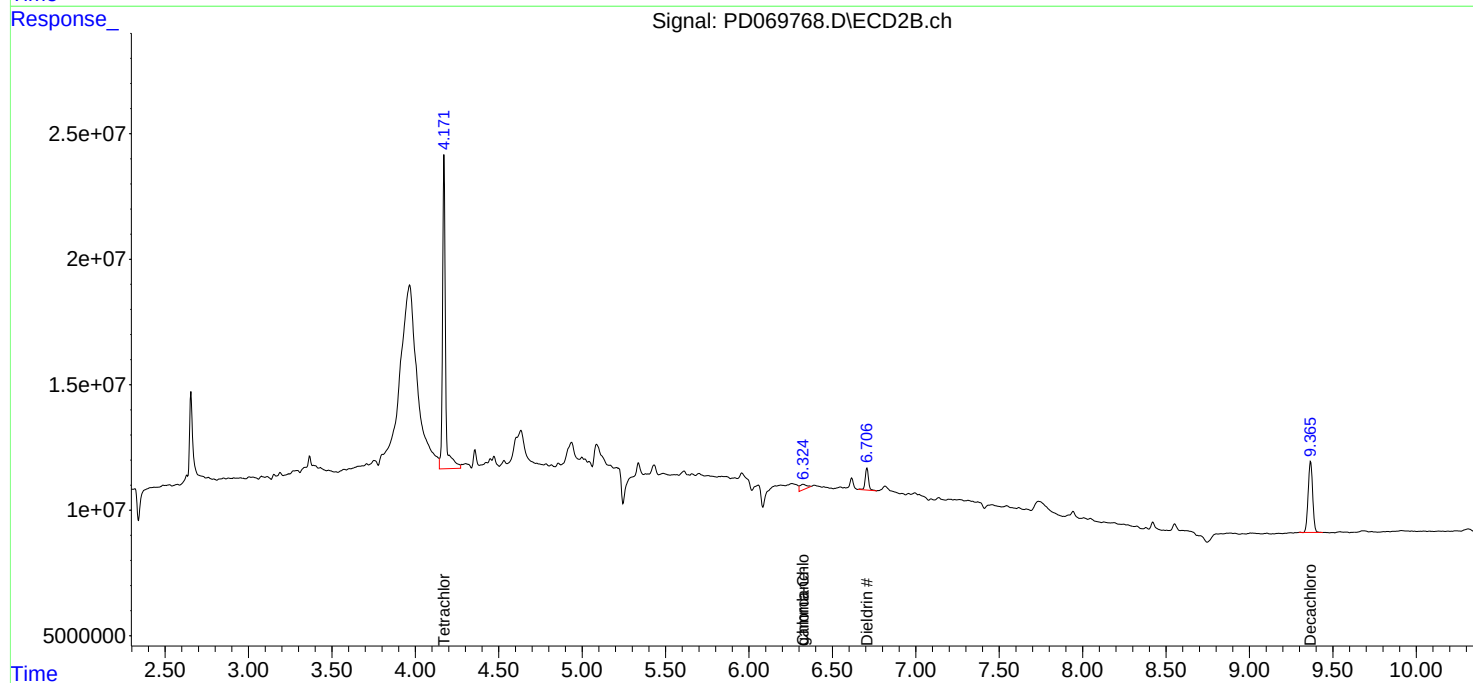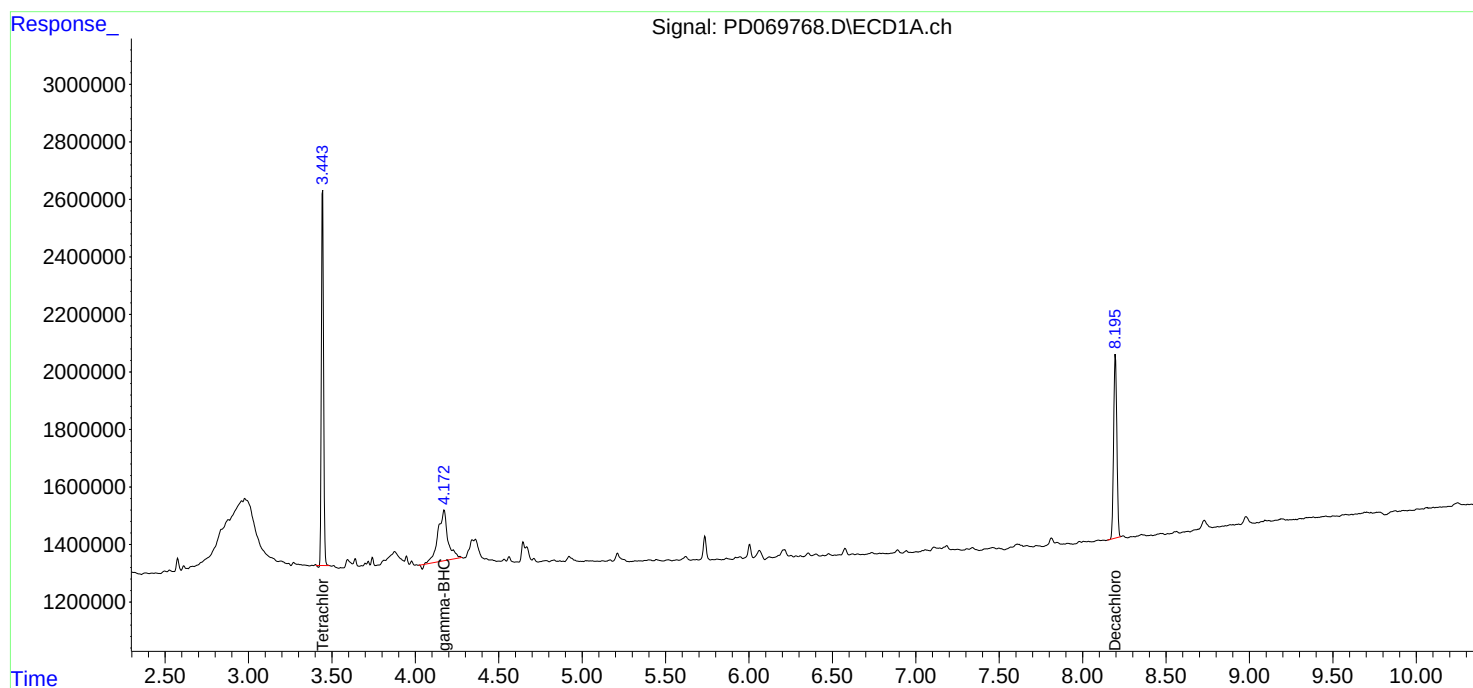


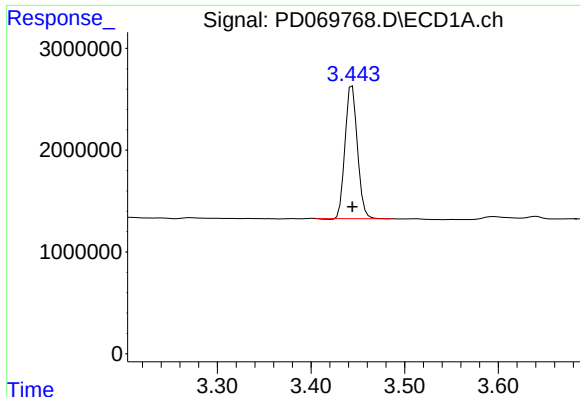

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 11988934
Conc: 11.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

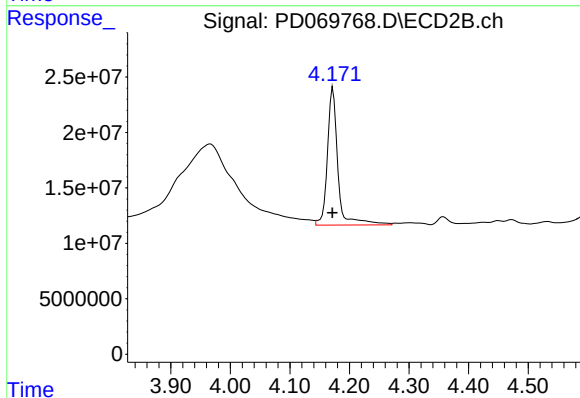


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.001 min
Response: 151891588
Conc: 15.90 ng/ml

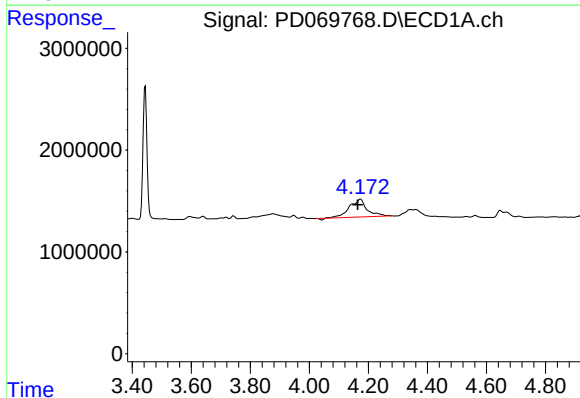


#3 gamma-BHC (Lindane)

R.T.: 4.173 min
Delta R.T.: 0.009 min
Response: 7181290
Conc: 4.86 ng/ml

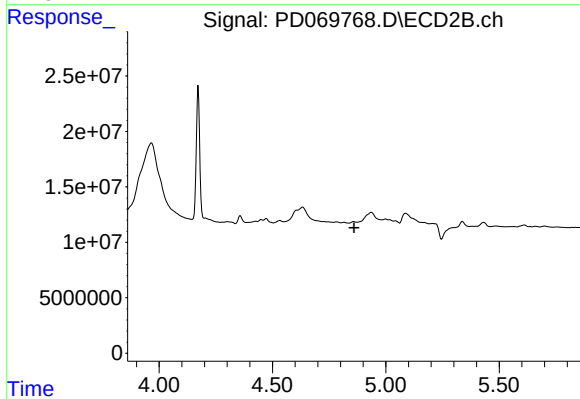

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.860 min
Response: 0
Conc: N.D.

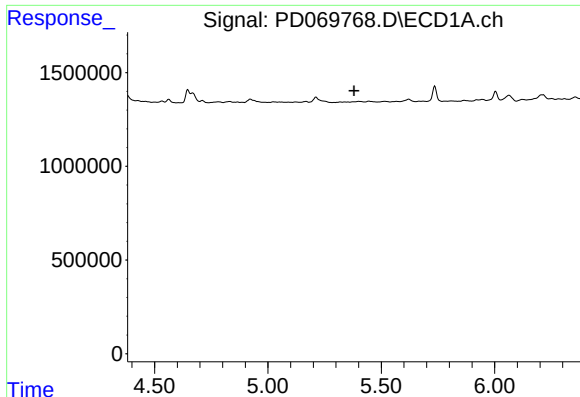

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.380 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

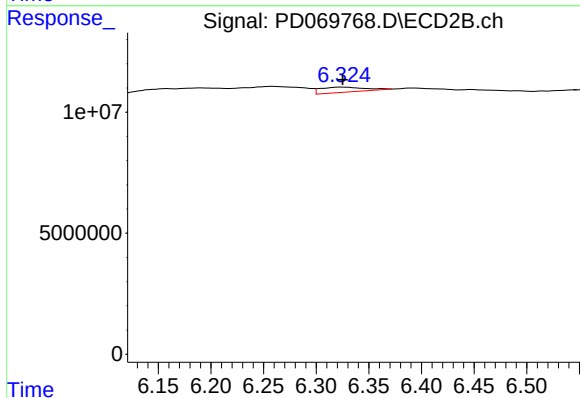


#10 gamma-Chlordane

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 6171861
Conc: 0.58 ng/ml

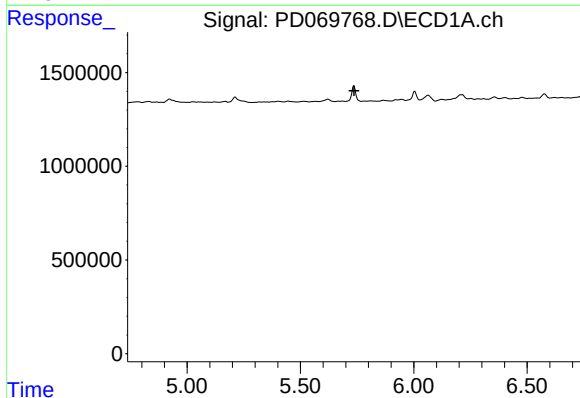


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

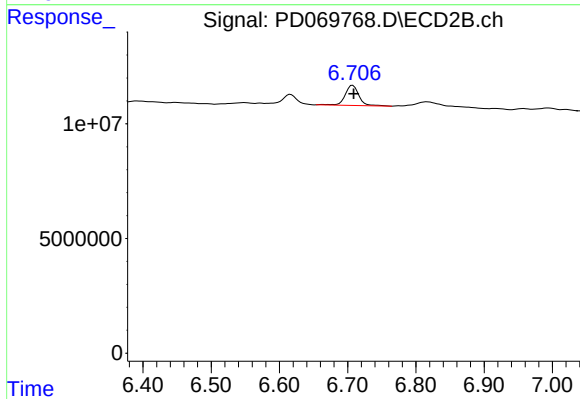

#13 Dieldrin


R.T.: 6.707 min
Delta R.T.: -0.002 min
Response: 12401130
Conc: 1.21 ng/ml

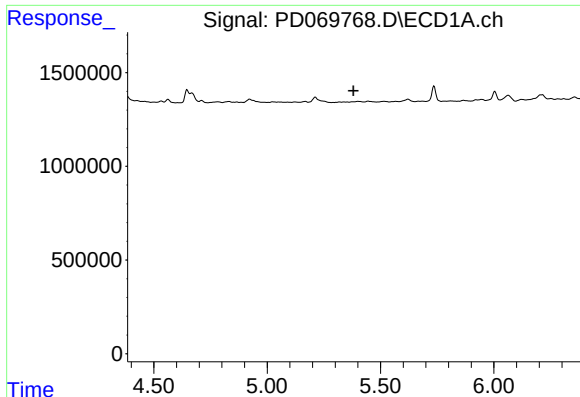

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.381 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

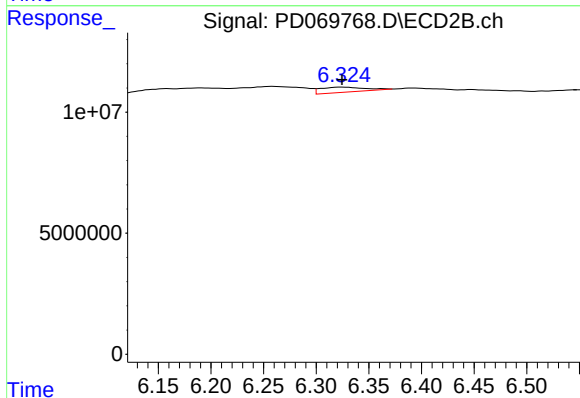


#25 Chlordane-3

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 6171861
Conc: 4.21 ng/ml

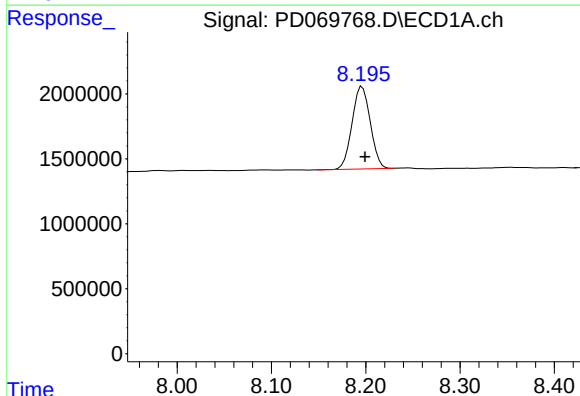

#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: -0.003 min
Response: 8507670
Conc: 7.89 ng/ml

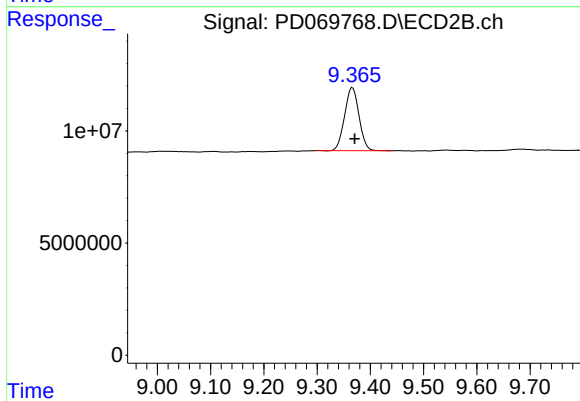

#28 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.004 min
Response: 53123603
Conc: 8.86 ng/ml