

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
 Data File : PD069782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 06:12
 Operator : AR\AJ
 Sample : N2876-04 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 03:24:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.172	1715076	32566614	1.712	3.409 #
28)	SA Decachlor...	0.000	9.365	0	13608574	N.D.	2.271 #
Target Compounds							
4)	MA Heptachlor	0.000	5.385	0	20419542	N.D.	1.644 #
13)	MA Dieldrin	0.000	6.693f	0	27293891	N.D.	2.666 #
15)	B Endosulfa...	0.000	7.120	0	15654490	N.D.	1.903 #
16)	A 4,4'-DDD	0.000	7.049	0	62766799	N.D.	7.747 #
17)	MA 4,4'-DDT	6.356	7.317f	7466353	80612893	7.777	9.802 #
19)	B Endosulfa...	6.644	0.000	4103003	0	3.730	N.D. #
20)	A Methoxychlor	6.889f	0.000	10998460	0	19.082	N.D. #
21)	B Endrin ke...	7.165f	0.000	2698035	0	2.154	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
Data File : PD069782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 06:12
Operator : AR\AJ
Sample : N2876-04 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 03:24:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

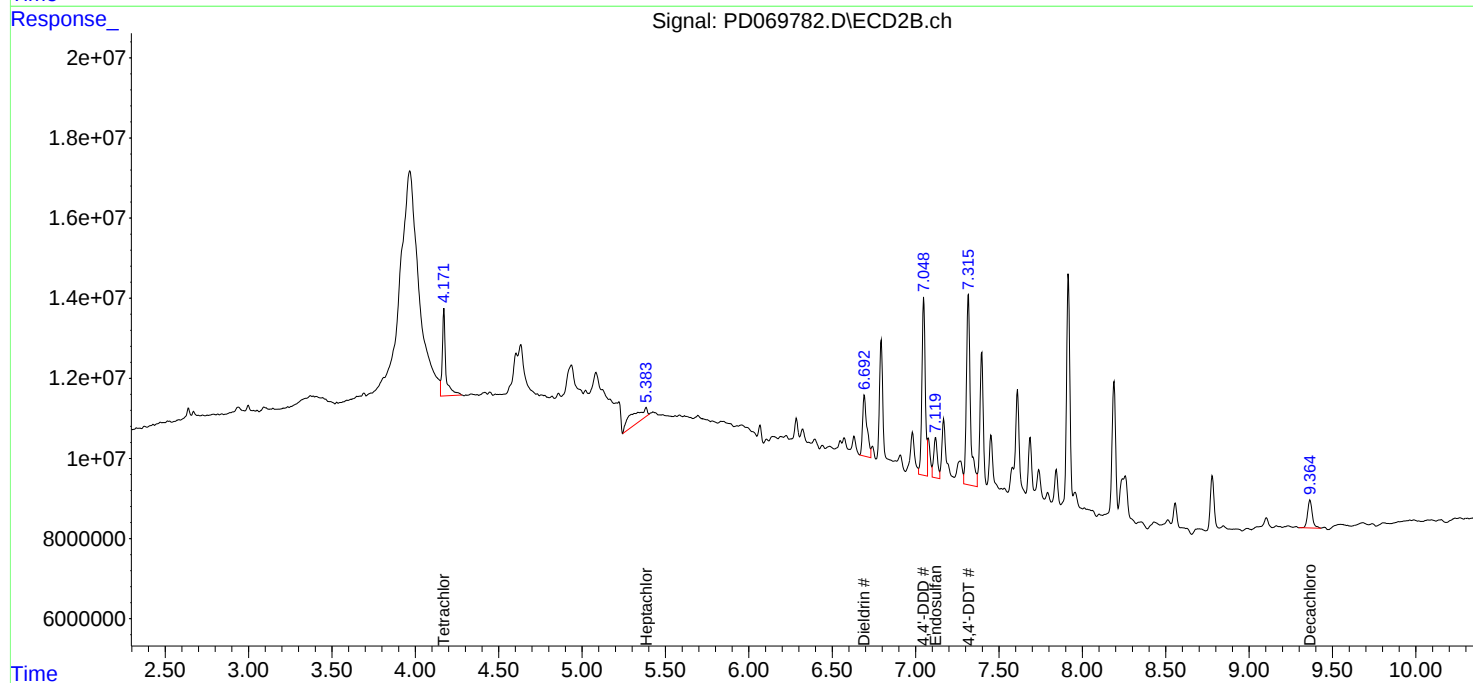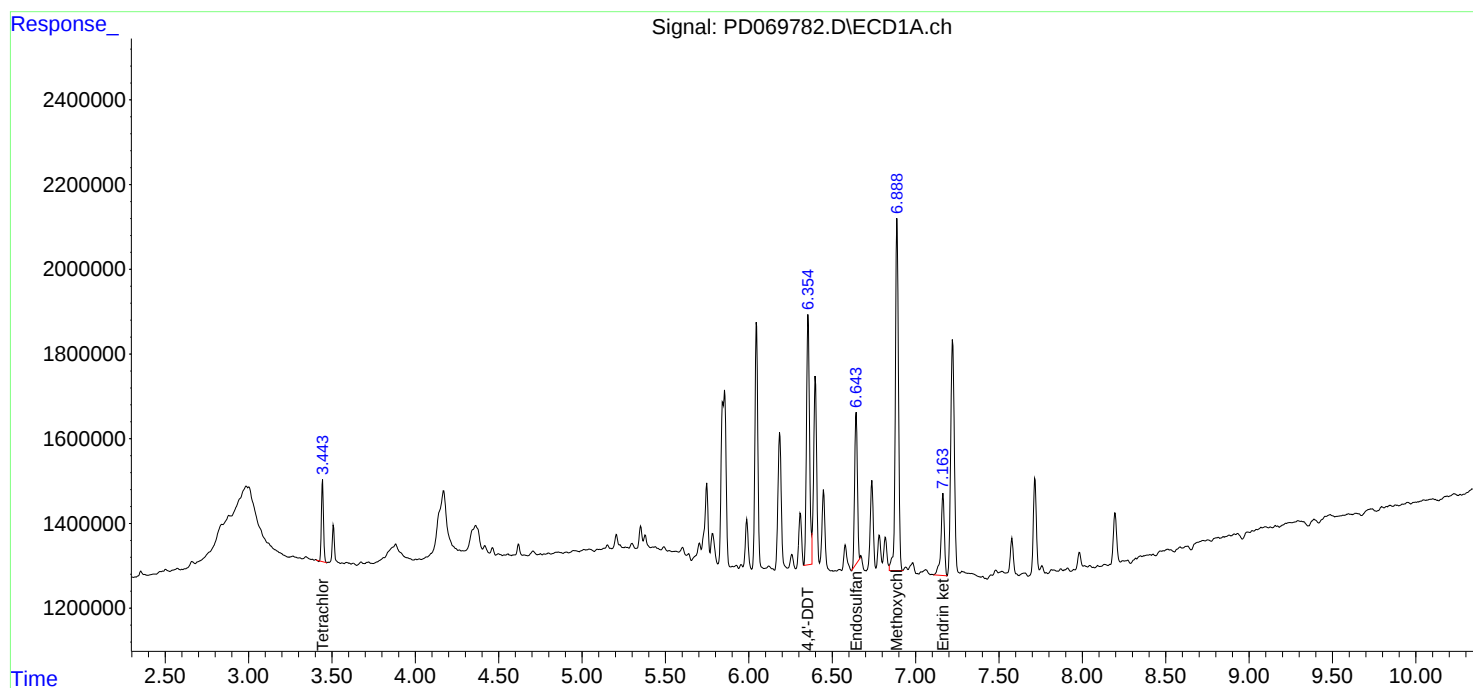


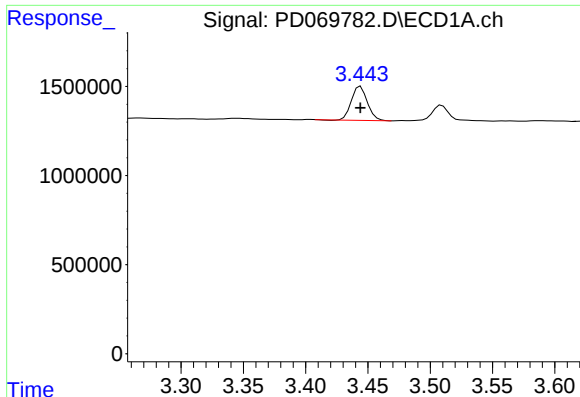

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 1715076
Conc: 1.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

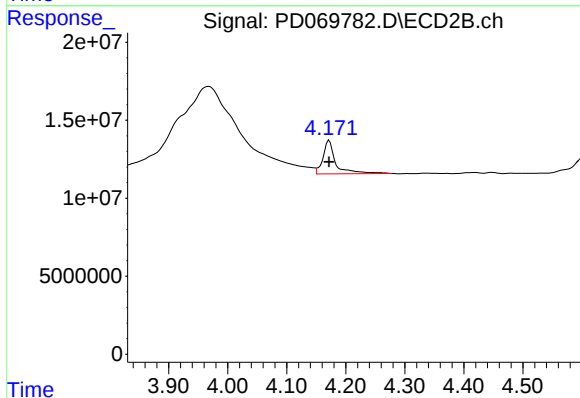


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 32566614
Conc: 3.41 ng/ml

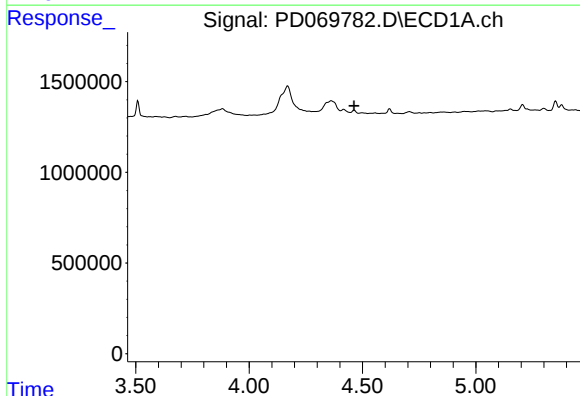


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.463 min
Response: 0
Conc: N.D.

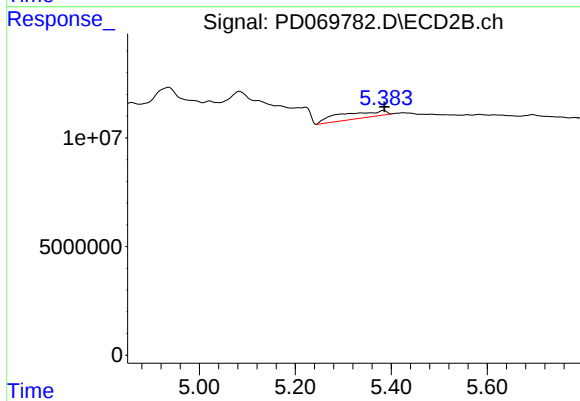

#4 Heptachlor


R.T.: 5.385 min
Delta R.T.: -0.001 min
Response: 20419542
Conc: 1.64 ng/ml

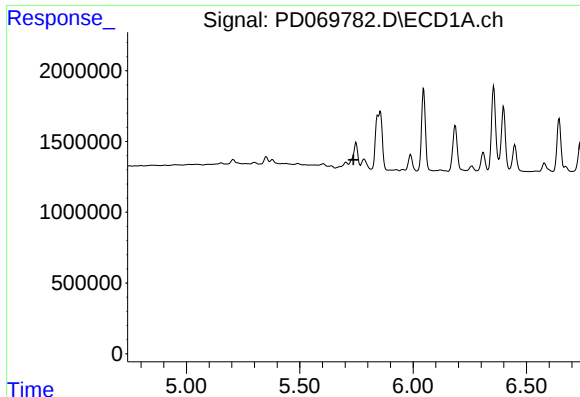

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

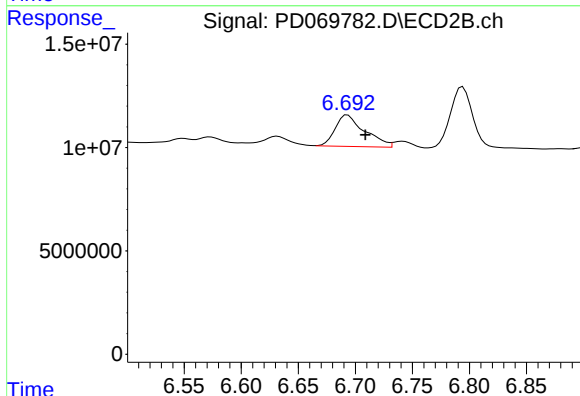


#13 Dieldrin

R.T.: 6.693 min
Delta R.T.: -0.016 min
Response: 27293891
Conc: 2.67 ng/ml

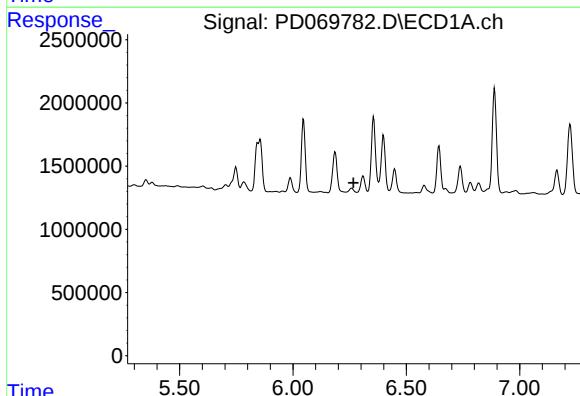


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.267 min
Response: 0
Conc: N.D.

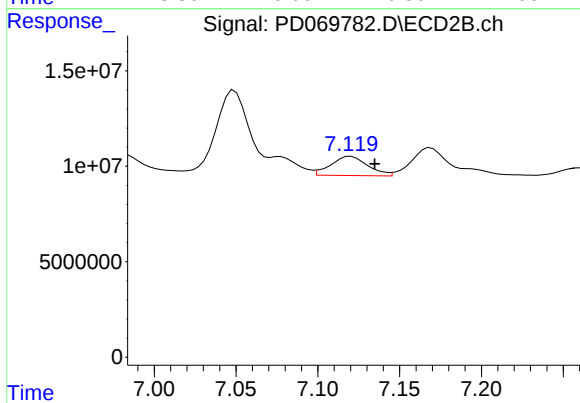

#15 Endosulfan II


R.T.: 7.120 min
Delta R.T.: -0.015 min
Response: 15654490
Conc: 1.90 ng/ml

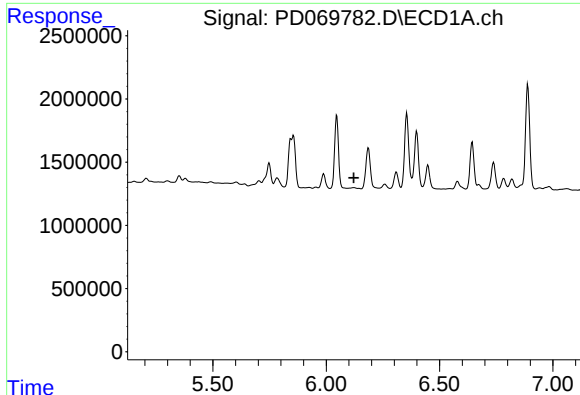

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.122 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

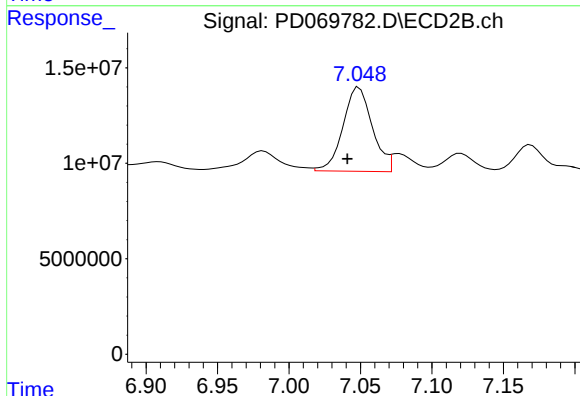


#16 4,4'-DDD

R.T.: 7.049 min
Delta R.T.: 0.008 min
Response: 62766799
Conc: 7.75 ng/ml

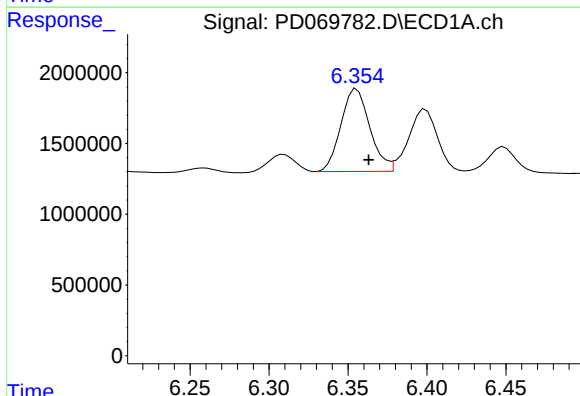


#17 4,4'-DDT

R.T.: 6.356 min
Delta R.T.: -0.007 min
Response: 7466353
Conc: 7.78 ng/ml

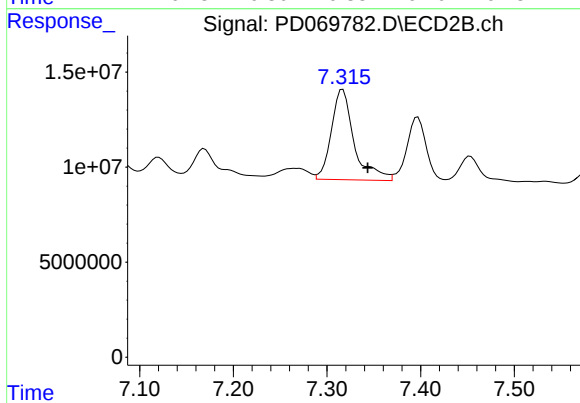

#17 4,4'-DDT


R.T.: 7.317 min
Delta R.T.: -0.027 min
Response: 80612893
Conc: 9.80 ng/ml

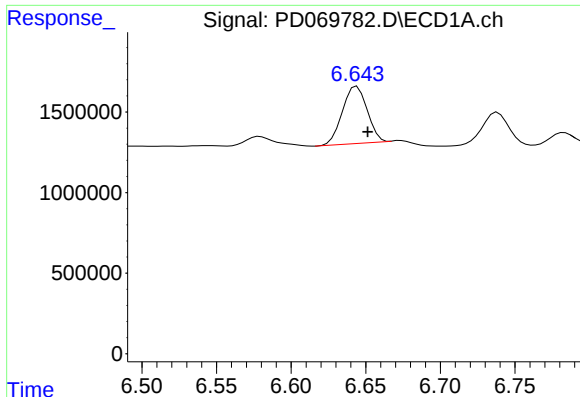

#19 Endosulfan Sulfate


R.T.: 6.644 min
Delta R.T.: -0.007 min
Response: 4103003
Conc: 3.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

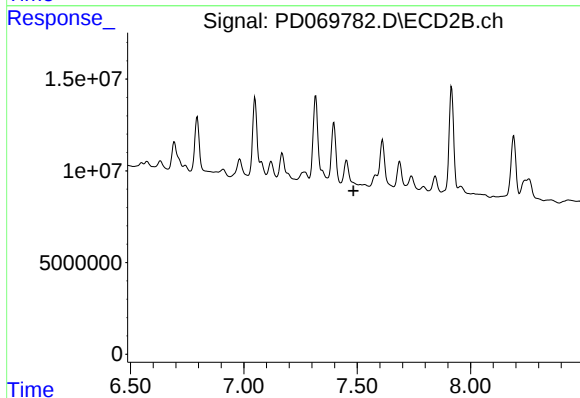


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.484 min
Response: 0
Conc: N.D.

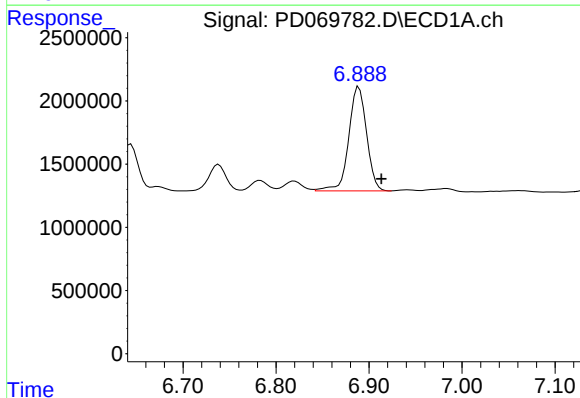


#20 Methoxychlor

R.T.: 6.889 min
Delta R.T.: -0.024 min
Response: 10998460
Conc: 19.08 ng/ml

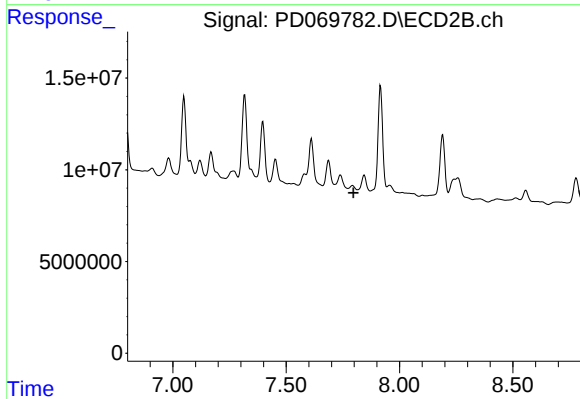

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.798 min
Response: 0
Conc: N.D.

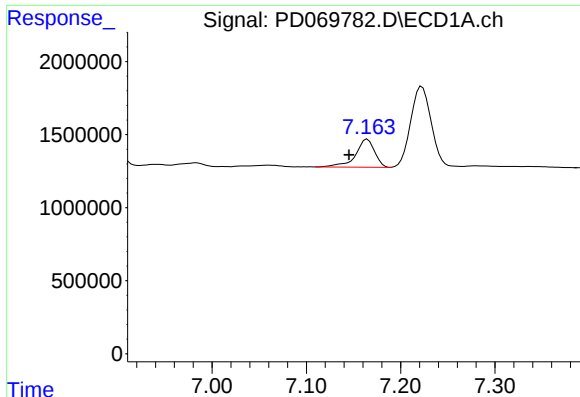

#21 Endrin ketone


R.T.: 7.165 min
Delta R.T.: 0.020 min
Response: 2698035
Conc: 2.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

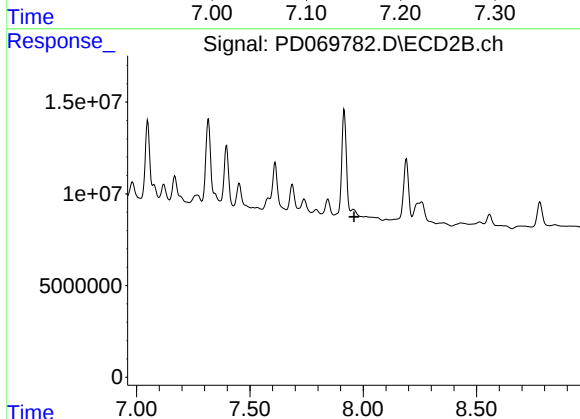


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.959 min
Response: 0
Conc: N.D.

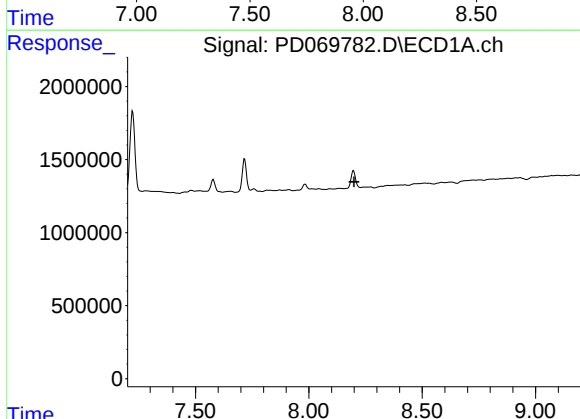

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.199 min
Response: 0
Conc: N.D.

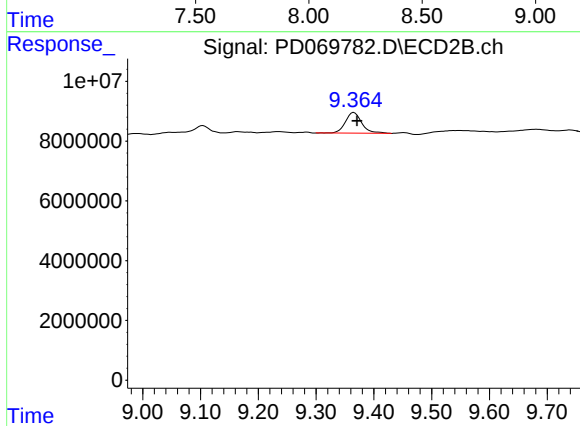

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: -0.006 min
Response: 13608574
Conc: 2.27 ng/ml