

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
 Data File : PD069783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 06:26
 Operator : AR\AJ
 Sample : N2876-04910X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 03:24:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	4.172	0	25096000	N.D.	2.627 #
28)	SA Decachlor...	0.000	9.366	0	10739871	N.D.	1.792 #
Target Compounds							
13)	MA Dieldrin	0.000	6.692f	0	11719099	N.D.	1.145 #
16)	A 4,4'-DDD	0.000	7.049	0	23668815	N.D.	2.921 #
17)	MA 4,4'-DDT	6.356	7.317f	2195045	26969998	2.286	3.279 #
20)	A Methoxychlor	6.890f	0.000	3519786	0	6.107	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
Data File : PD069783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 06:26
Operator : AR\AJ
Sample : N2876-04910X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 03:24:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

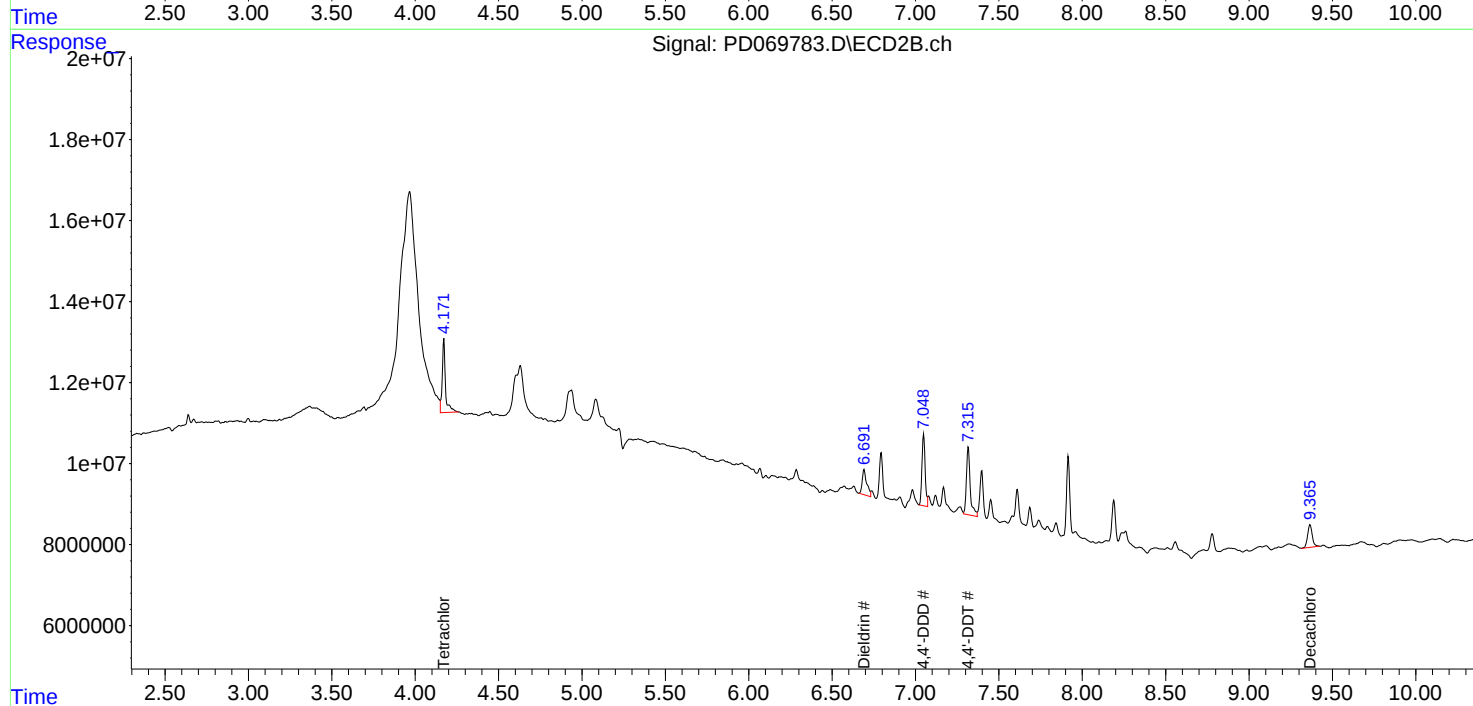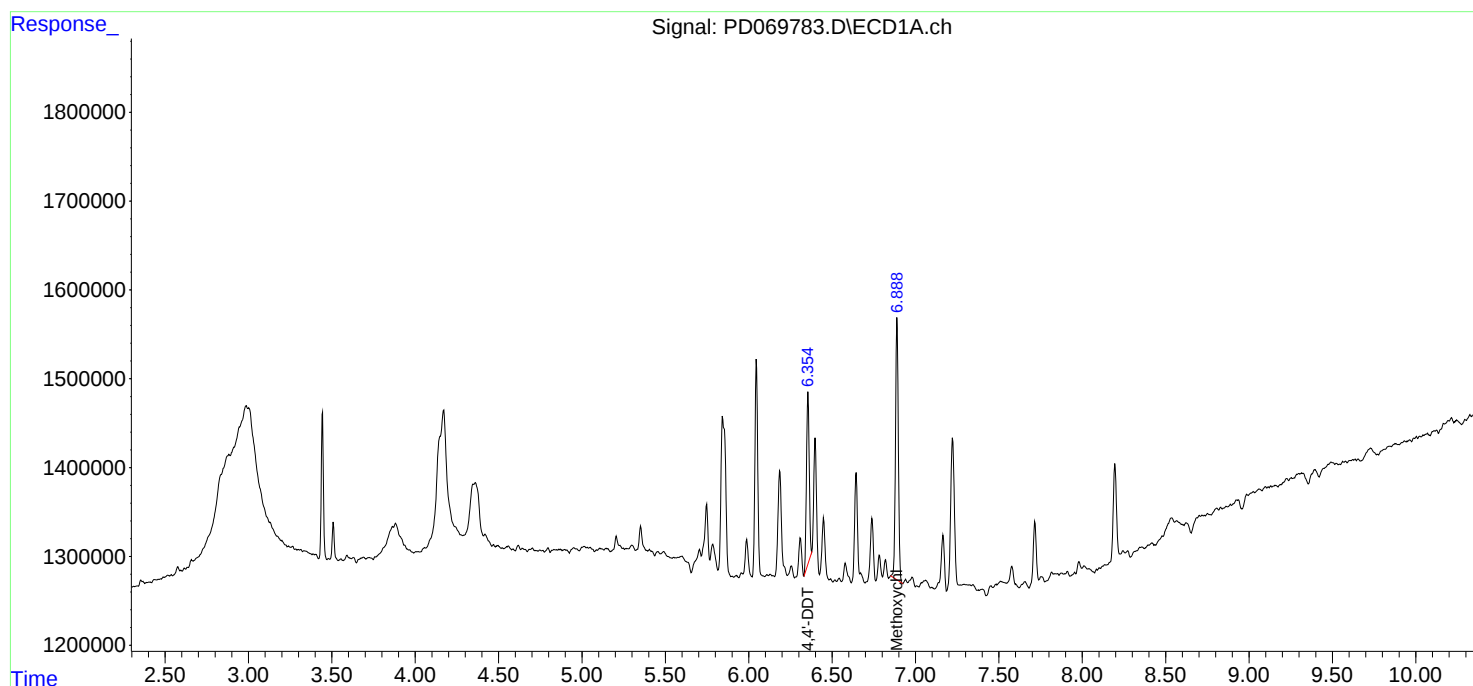


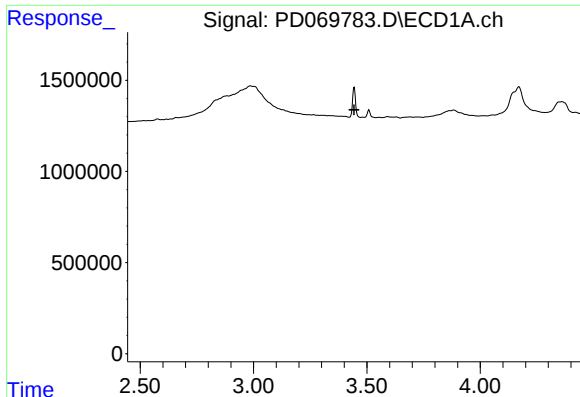

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

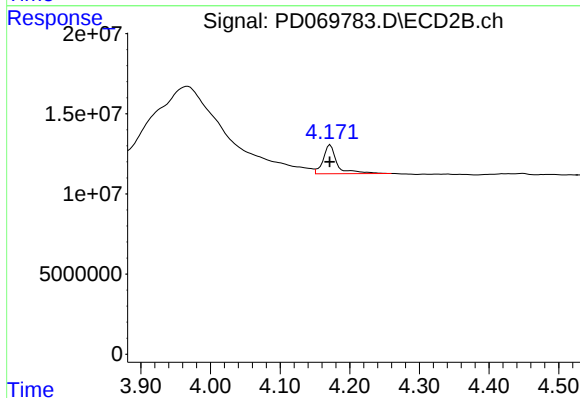


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 25096000
Conc: 2.63 ng/ml

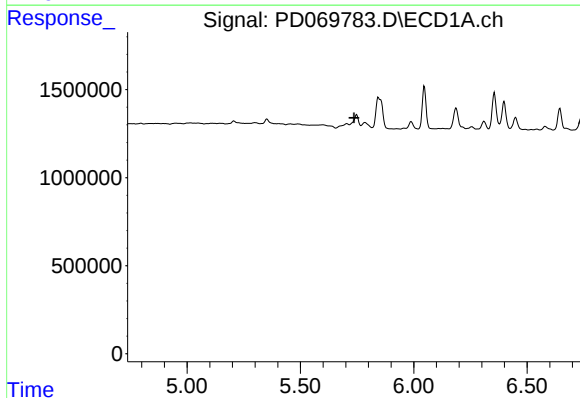


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

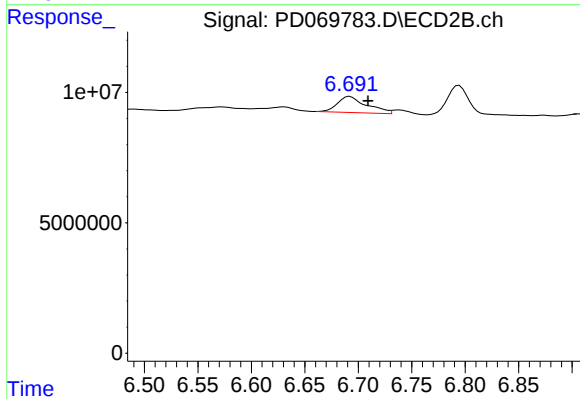

#13 Dieldrin


R.T.: 6.692 min
Delta R.T.: -0.017 min
Response: 11719099
Conc: 1.14 ng/ml

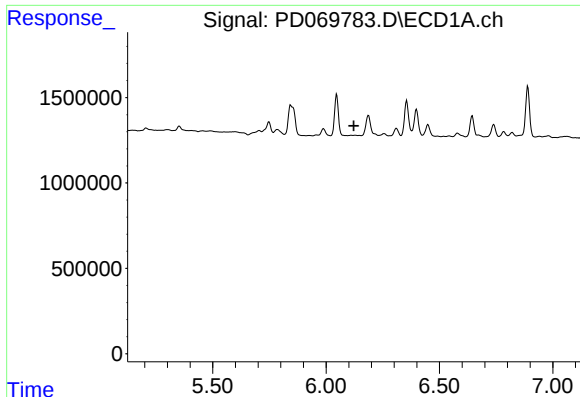

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.122 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

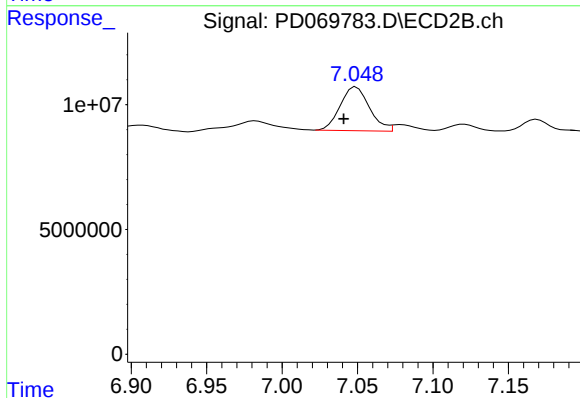


#16 4,4'-DDD

R.T.: 7.049 min
Delta R.T.: 0.008 min
Response: 23668815
Conc: 2.92 ng/ml

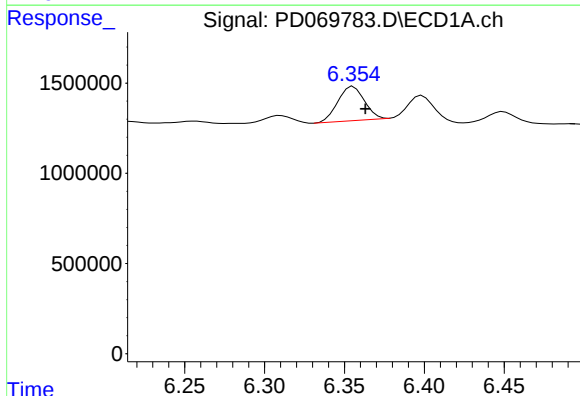


#17 4,4'-DDT

R.T.: 6.356 min
Delta R.T.: -0.007 min
Response: 2195045
Conc: 2.29 ng/ml

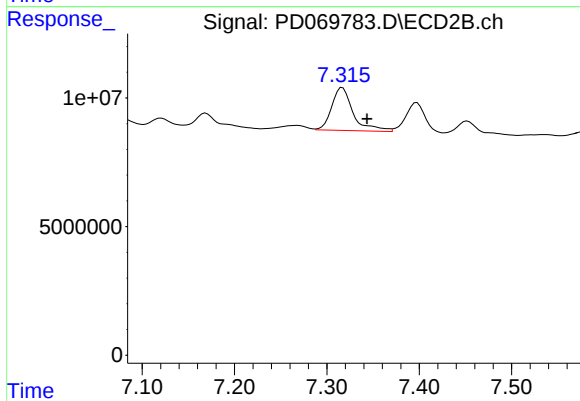

#17 4,4'-DDT


R.T.: 7.317 min
Delta R.T.: -0.027 min
Response: 26969998
Conc: 3.28 ng/ml

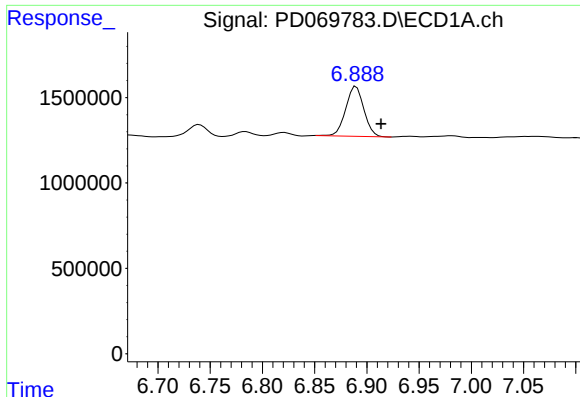

#20 Methoxychlor


R.T.: 6.890 min
Delta R.T.: -0.024 min
Response: 3519786
Conc: 6.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

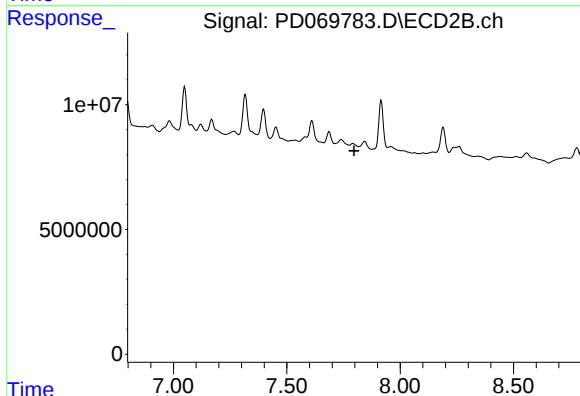


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.798 min
Response: 0
Conc: N.D.

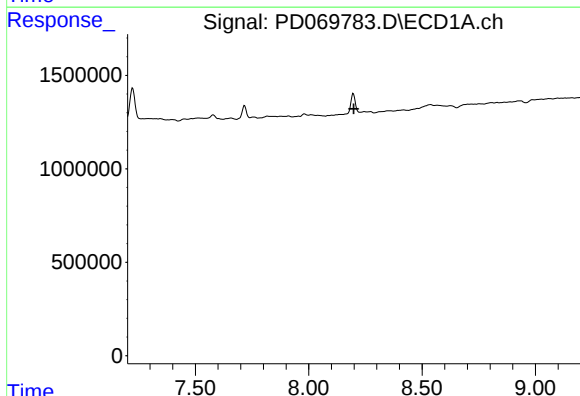

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.199 min
Response: 0
Conc: N.D.

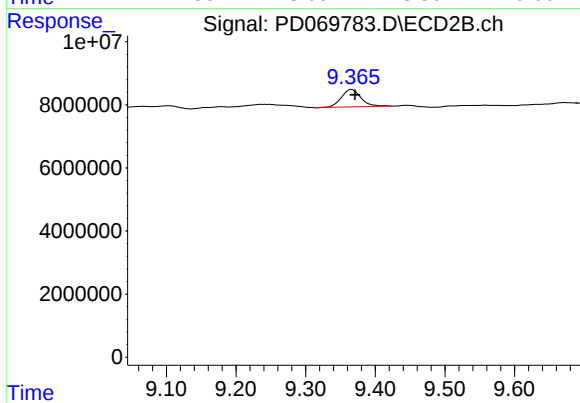

#28 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.005 min
Response: 10739871
Conc: 1.79 ng/ml