

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
 Data File : PD069768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 00:35
 Operator : AR\AJ
 Sample : N2873-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P032-SS001-1824-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/23/2022
 Supervised By :Ankita Jodhani 05/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 03:22:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.444	4.171	11988934	123.6E6	11.964	12.938m
2) SA Decachlor...	8.196	9.366	8507670	53123603	7.887	8.864
Target Compounds						
13) MA Dieldrin	5.735	6.707	999569	12401130	0.809m	1.211 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
Data File : PD069768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 00:35
Operator : AR\AJ
Sample : N2873-13
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P032-SS001-1824-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/23/2022
Supervised By : Ankita Jodhani 05/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 03:22:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

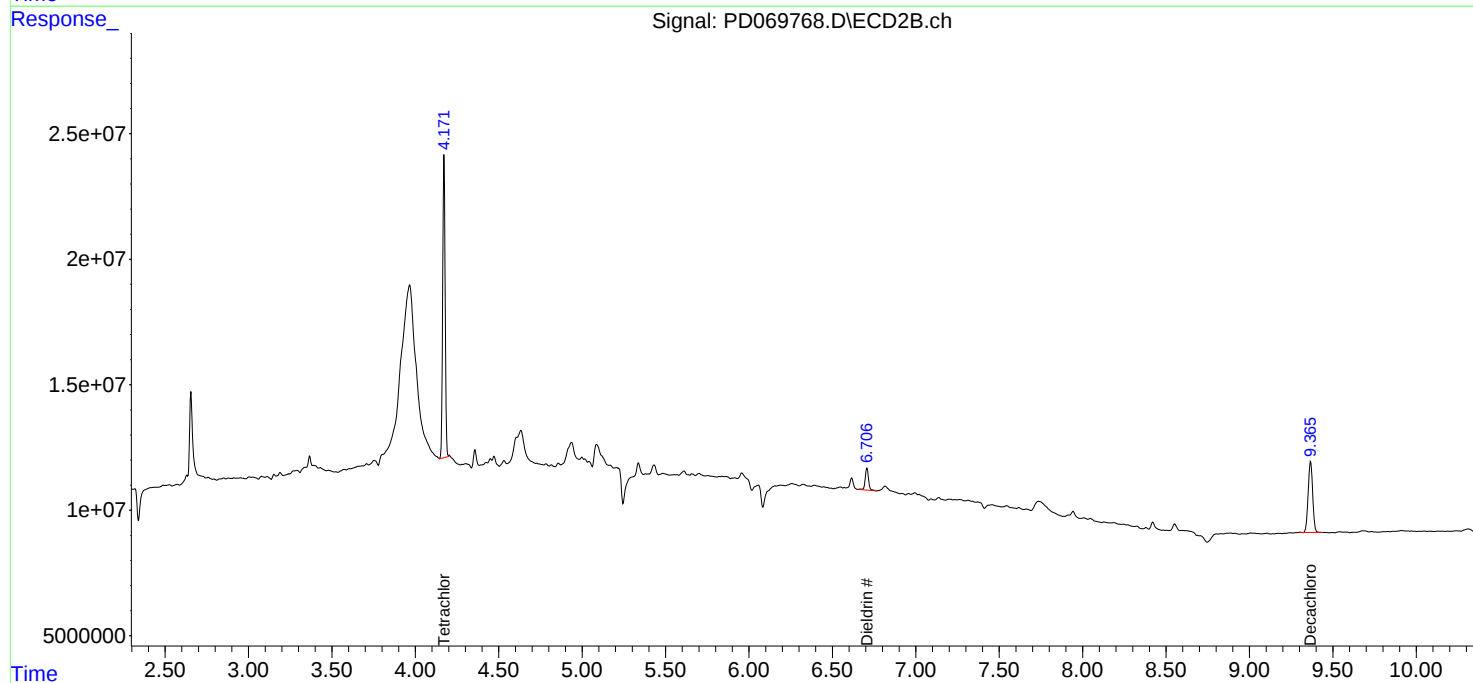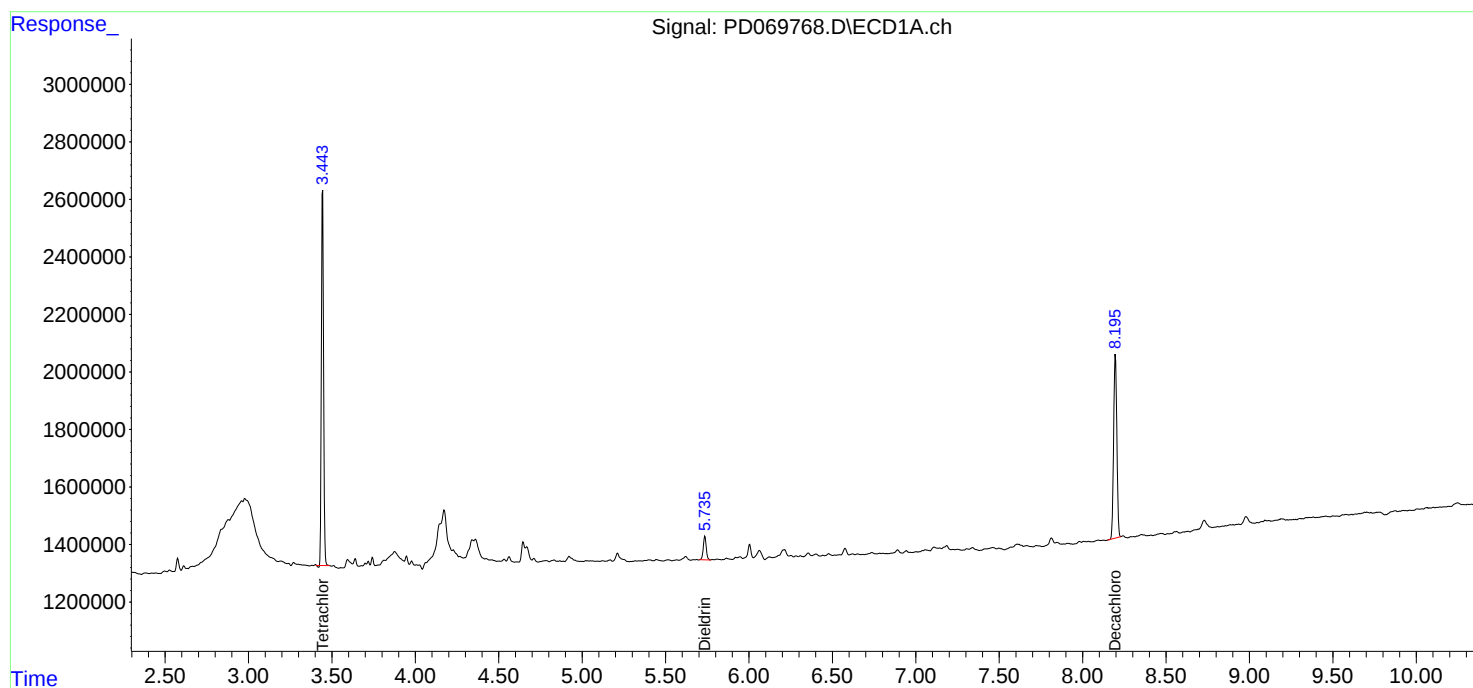

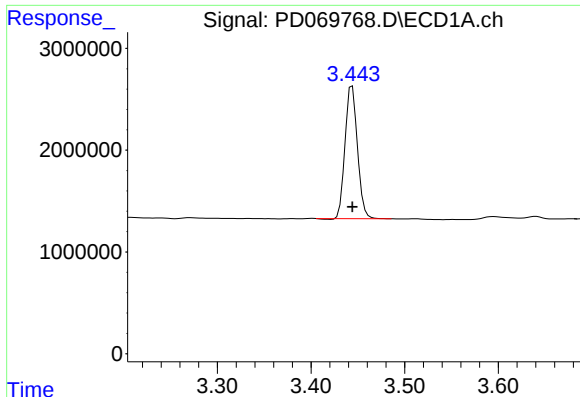


#1 Tetrachloro-m-xylene

R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 11988934
Conc: 11.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
P032-SS001-1824-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

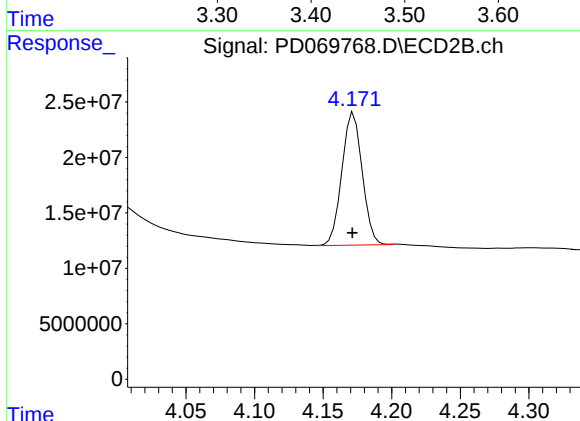


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 123614810
Conc: 12.94 ng/ml m

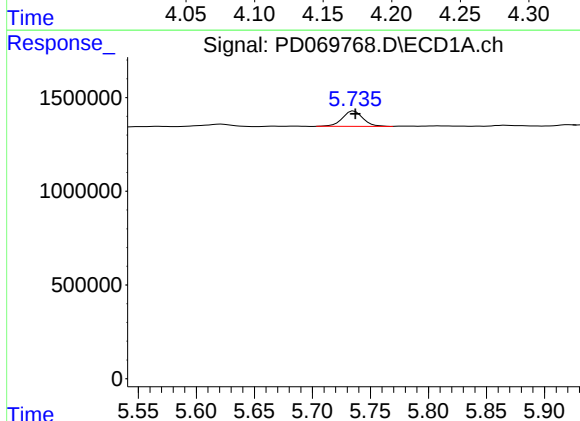


#13 Dieldrin

R.T.: 5.735 min
Delta R.T.: -0.003 min
Response: 999569
Conc: 0.81 ng/ml m

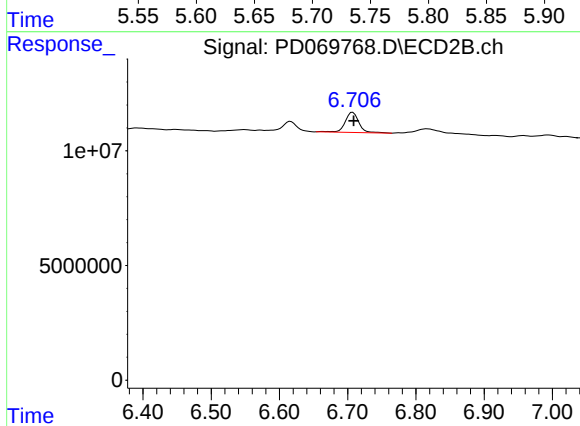

#13 Dieldrin

R.T.: 6.707 min
Delta R.T.: -0.002 min
Response: 12401130
Conc: 1.21 ng/ml

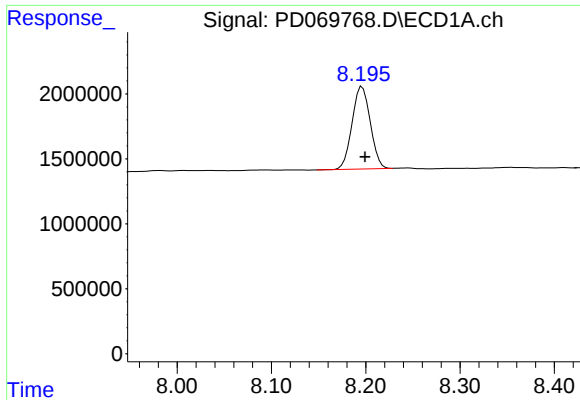


#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: -0.003 min
Response: 8507670
Conc: 7.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
P032-SS001-1824-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

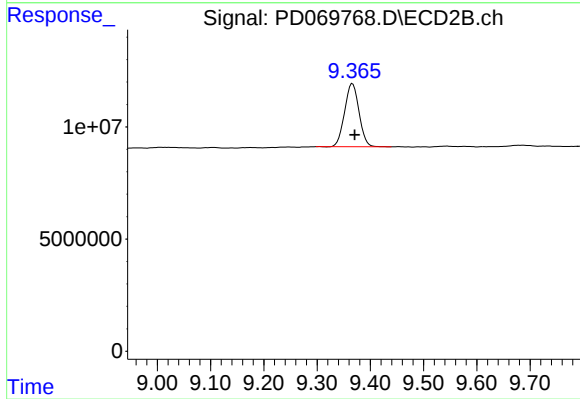

#28 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.004 min
Response: 53123603
Conc: 8.86 ng/ml