

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
 Data File : PD069771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 01:17
 Operator : AR\AJ
 Sample : N2979-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NB-7-052022

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/23/2022
 Supervised By : Ankita Jodhani 05/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 03:22:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.444	4.172	13258912	152.6E6	13.231	15.975
2) SA Decachlor...	8.195	9.364	15847469	96979149	14.692	16.182
Target Compounds						
12) B 4,4'-DDE	5.602	6.548	589191	6252813	0.509m	0.630

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
Data File : PD069771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 01:17
Operator : AR\AJ
Sample : N2979-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NB-7-052022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 03:22:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

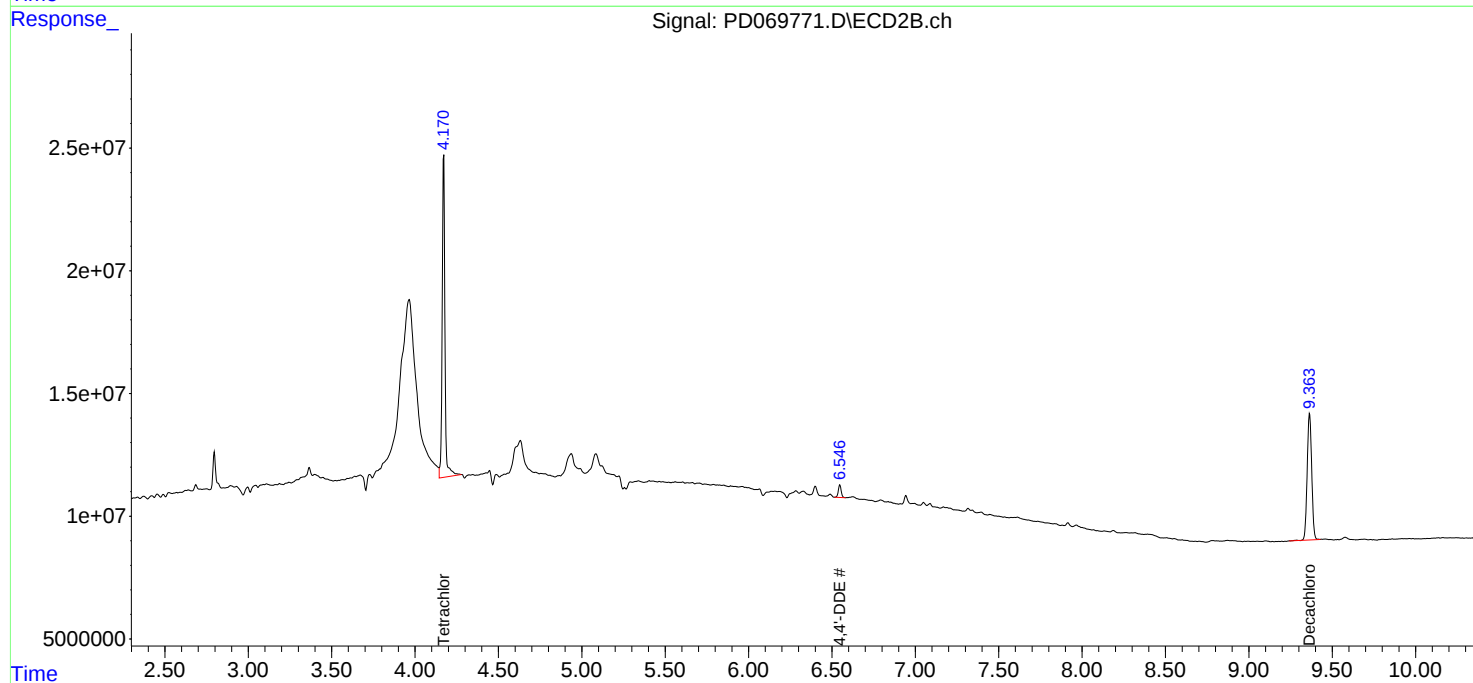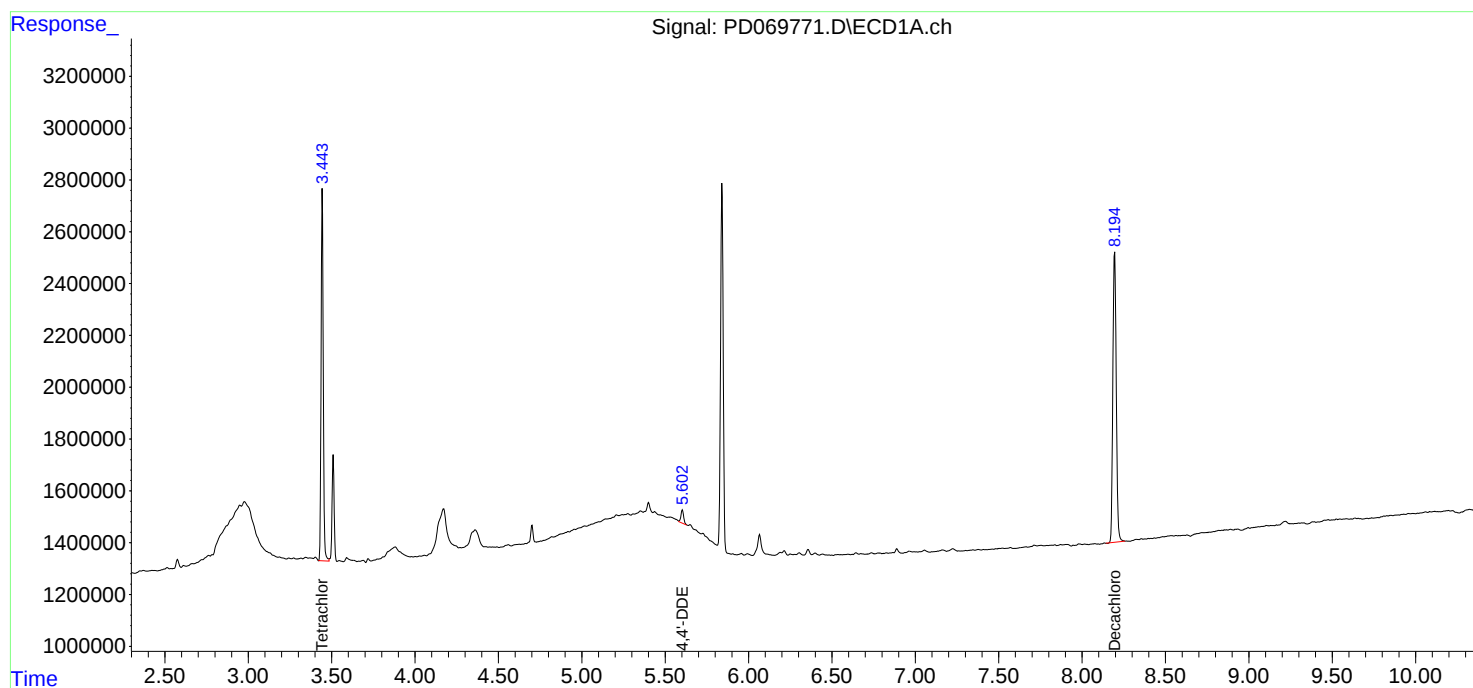

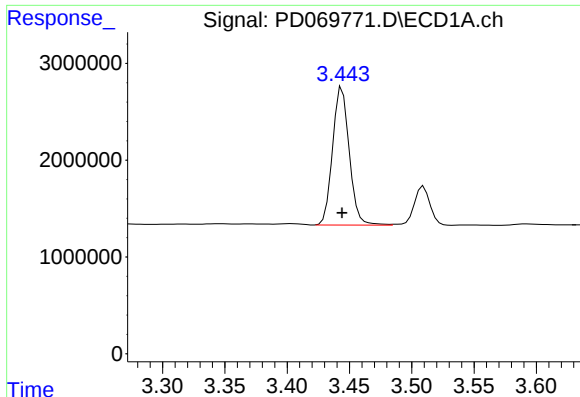


#1 Tetrachloro-m-xylene

R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 13258912
Conc: 13.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
NB-7-052022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

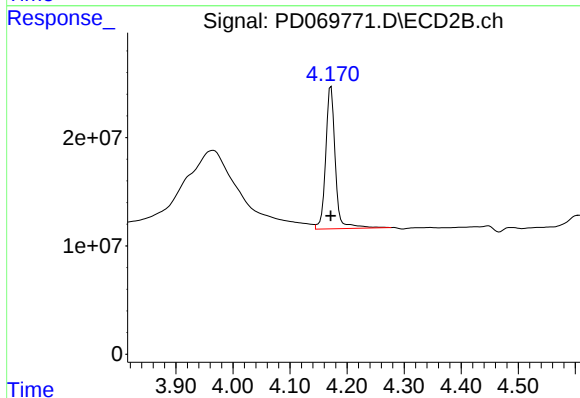


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 152624608
Conc: 15.97 ng/ml

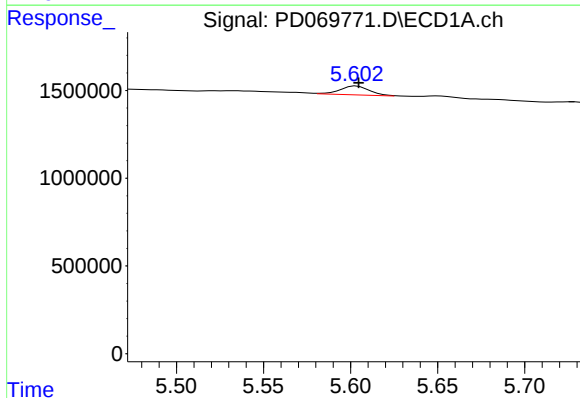


#12 4,4'-DDE

R.T.: 5.602 min
Delta R.T.: -0.003 min
Response: 589191
Conc: 0.51 ng/ml m

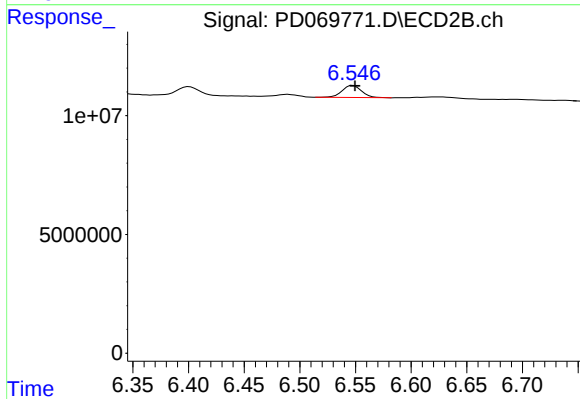

#12 4,4'-DDE

R.T.: 6.548 min
Delta R.T.: -0.002 min
Response: 6252813
Conc: 0.63 ng/ml

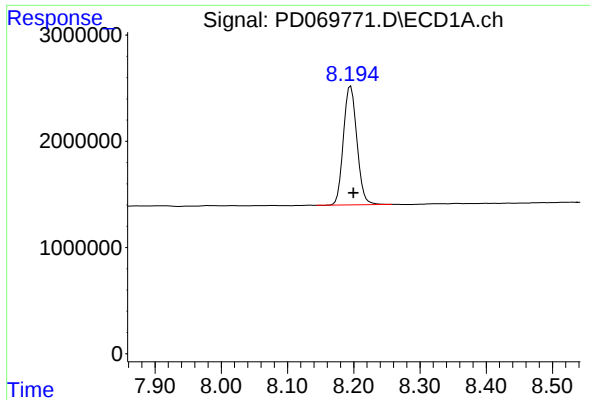

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: -0.004 min
Response: 15847469
Conc: 14.69 ng/ml

Instrument :

ECD_D

ClientSampleId :


NB-7-052022

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 05/23/2022

Supervised By :Ankita Jodhani 05/23/2022

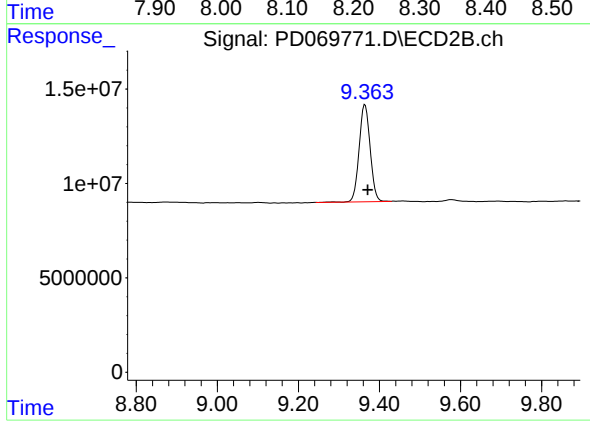

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: -0.006 min
Response: 96979149
Conc: 16.18 ng/ml