

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
 Data File : PD069778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 02:56
 Operator : AR\AJ
 Sample : N2936-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/23/2022
 Supervised By : Ankita Jodhani 05/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 03:23:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.430	4.167	30367995	61561247	30.305m	6.443m#
2) SA Decachlor...	8.191	9.369	7986095	86311896	7.404m	14.402 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052322\
Data File : PD069778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 02:56
Operator : AR\AJ
Sample : N2936-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 03:23:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

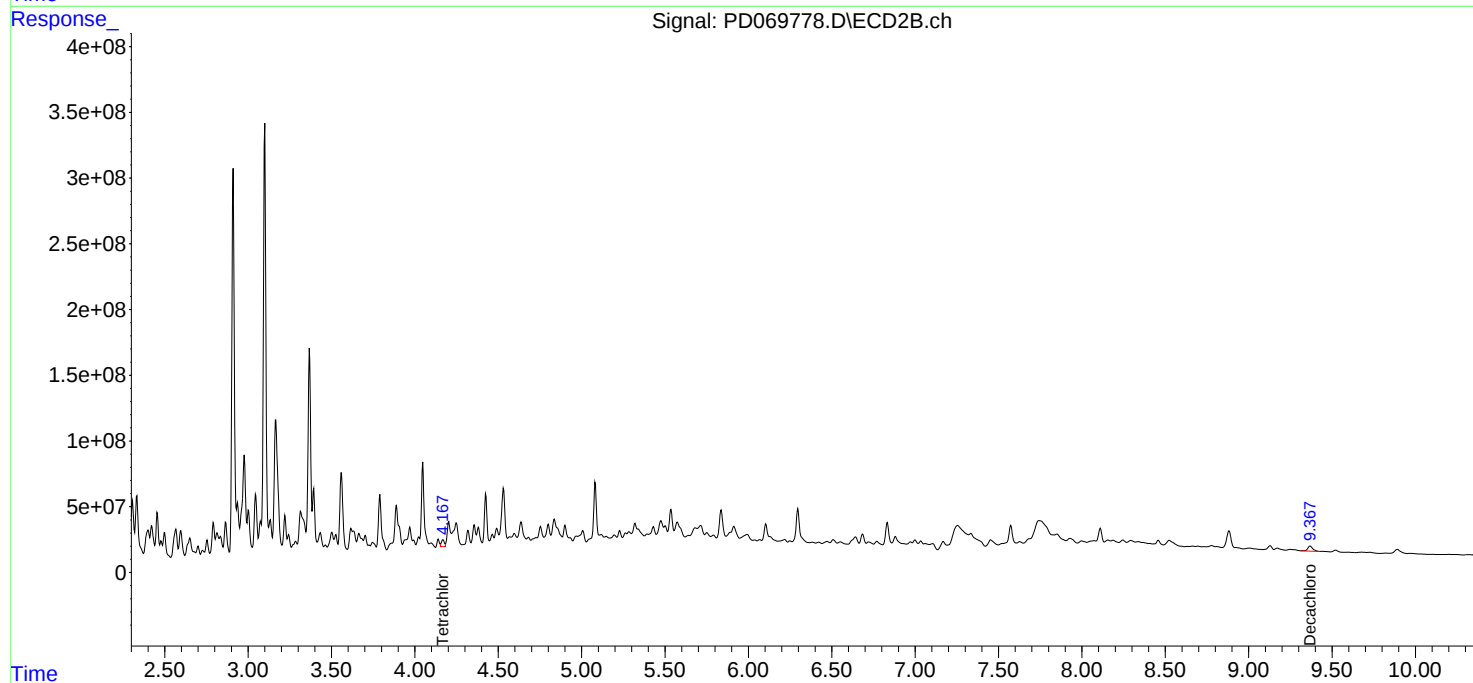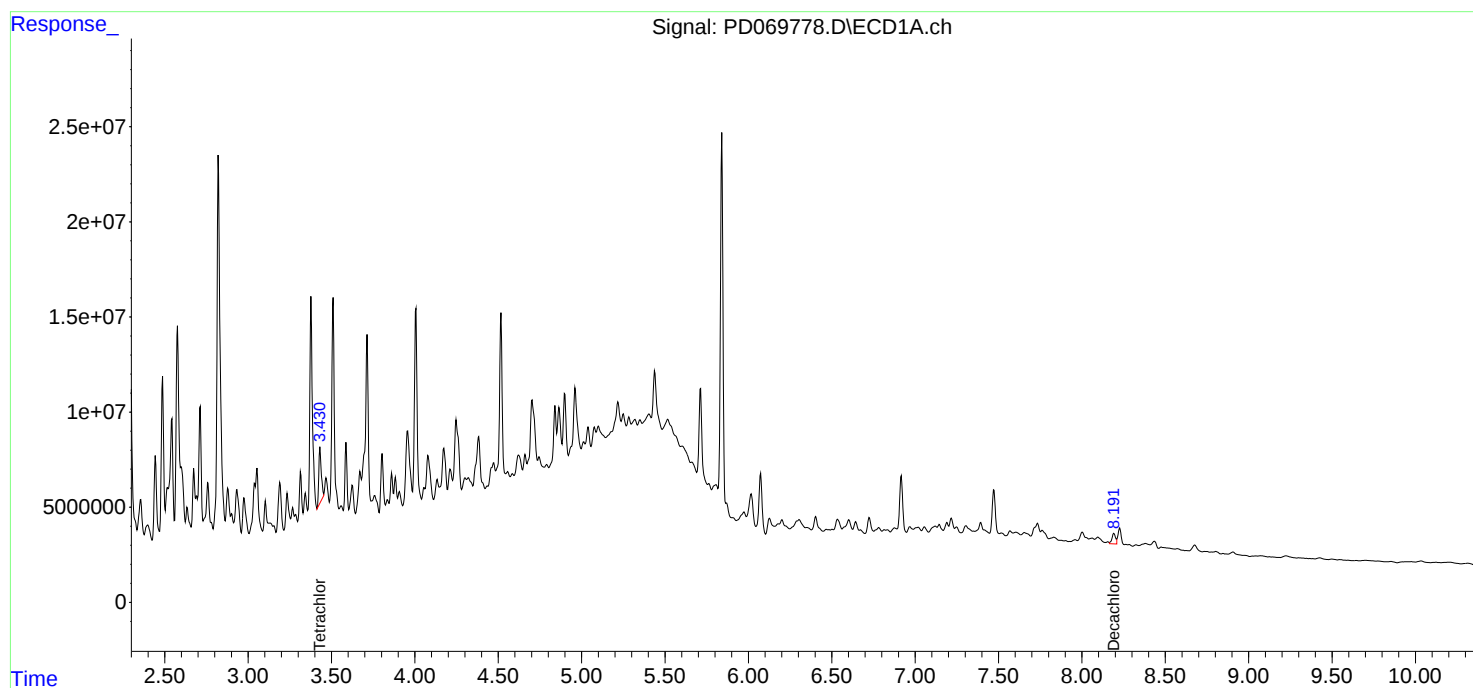

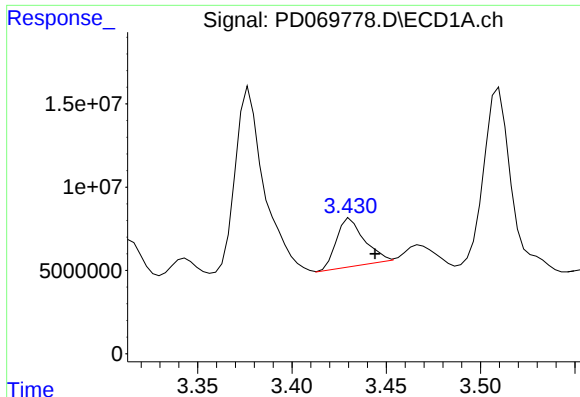


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.014 min
Response: 30367995
Conc: 30.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

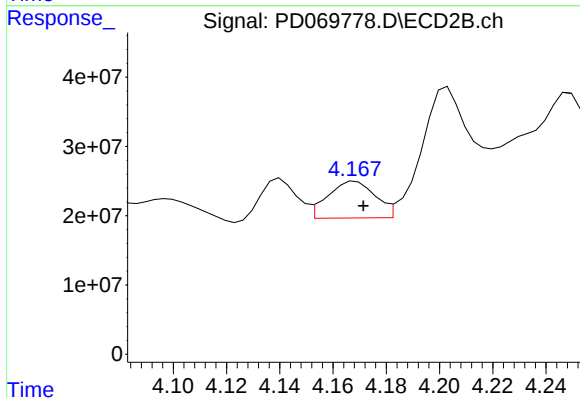


#1 Tetrachloro-m-xylene

R.T.: 4.167 min
Delta R.T.: -0.004 min
Response: 61561247
Conc: 6.44 ng/ml m

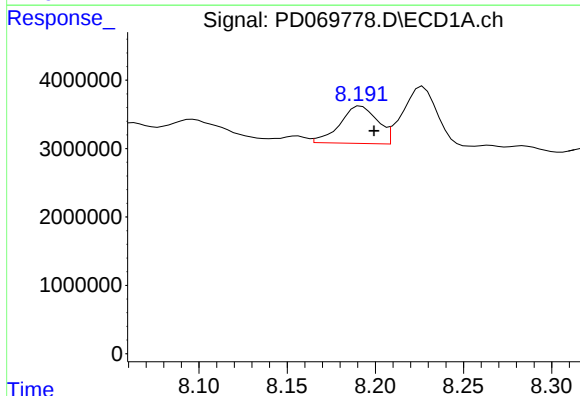

#28 Decachlorobiphenyl

R.T.: 8.191 min
Delta R.T.: -0.009 min
Response: 7986095
Conc: 7.40 ng/ml m

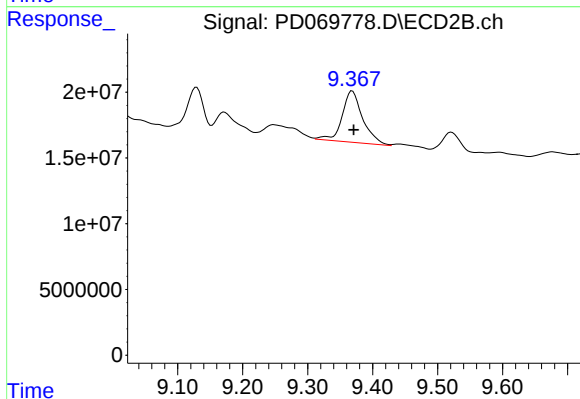

#28 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: -0.002 min
Response: 86311896
Conc: 14.40 ng/ml