

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052324\
Data File : PD082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2024 12:14
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-04

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 22:49:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

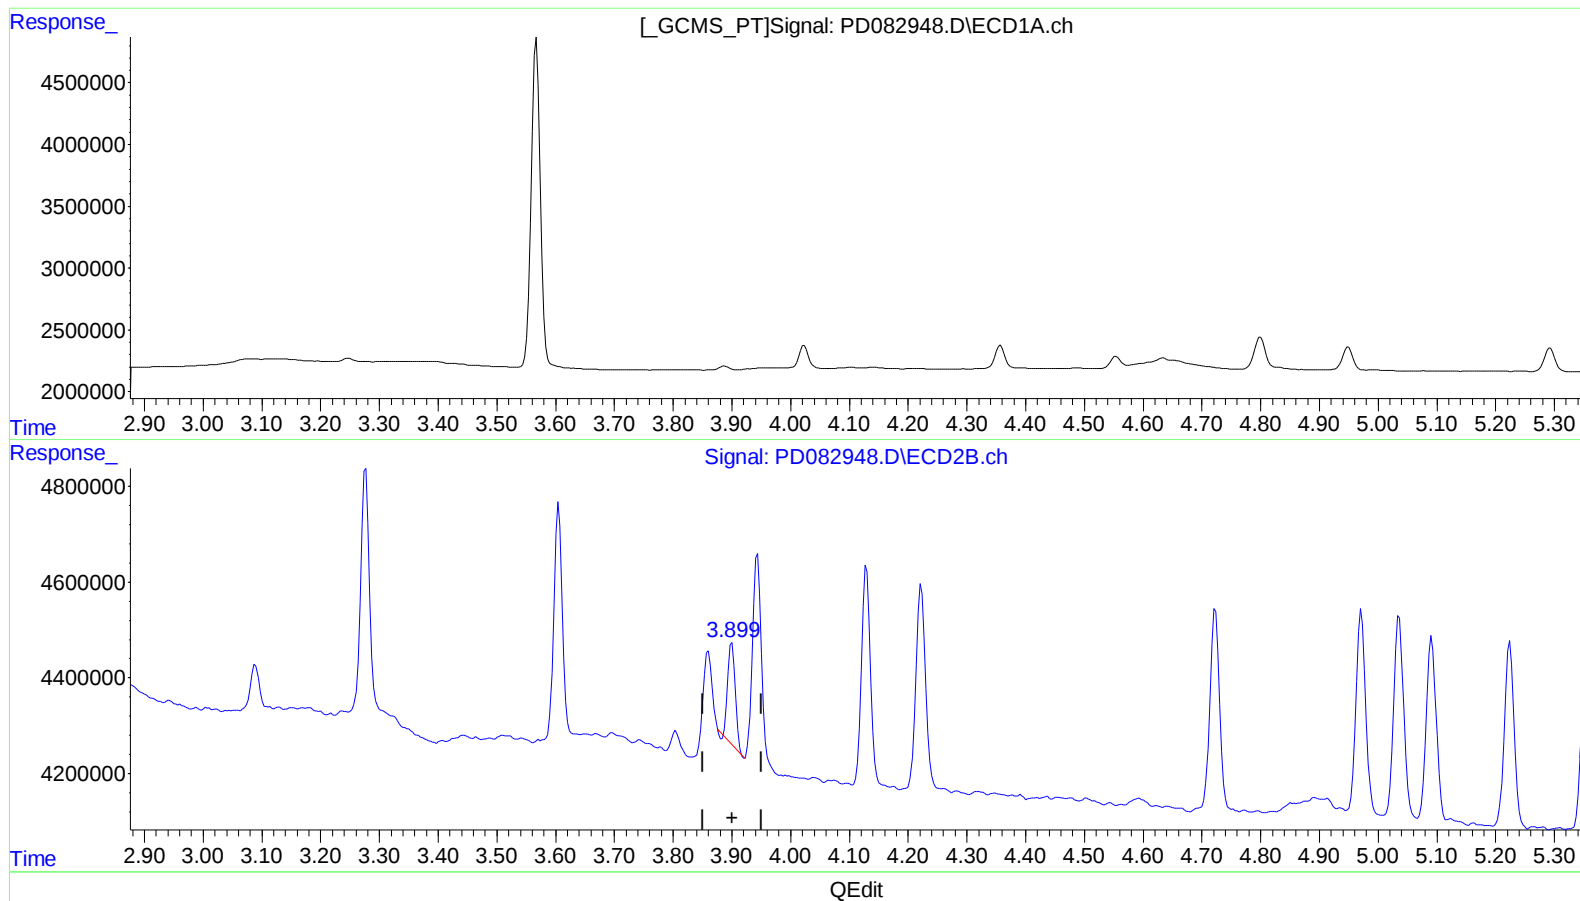

(6) beta-BHC (B)

0.000min 0.000 ng/ml

response 0

(6) beta-BHC #2 (B)

3.900min 0.777 ng/ml

response 1949334

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052324\
Data File : PD082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2024 12:14
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-04

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 22:49:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

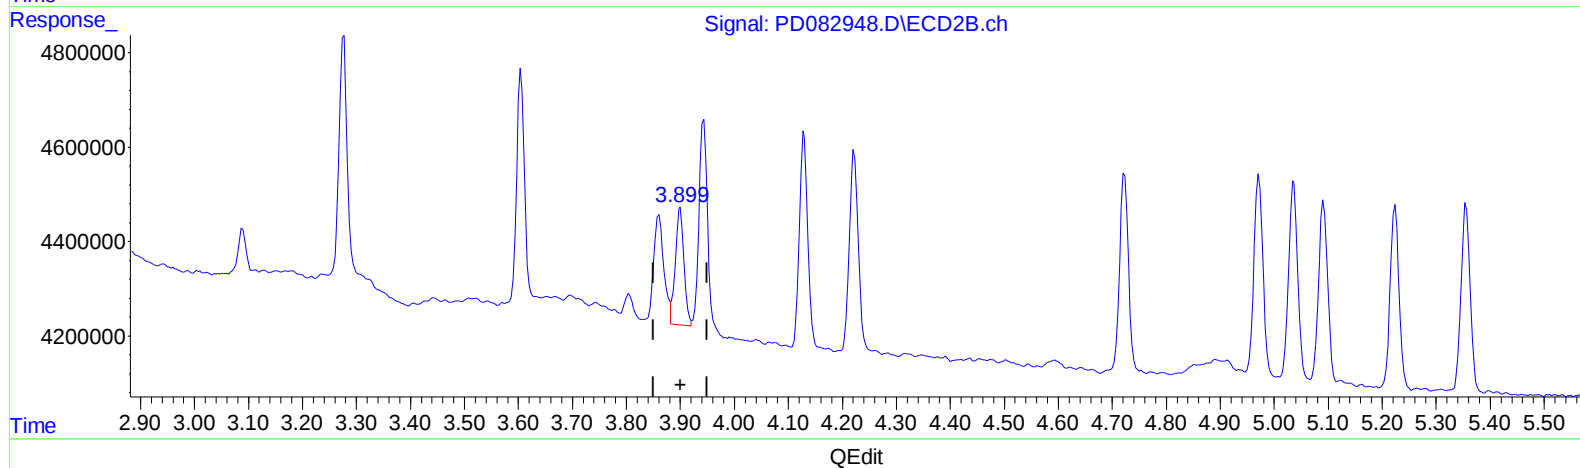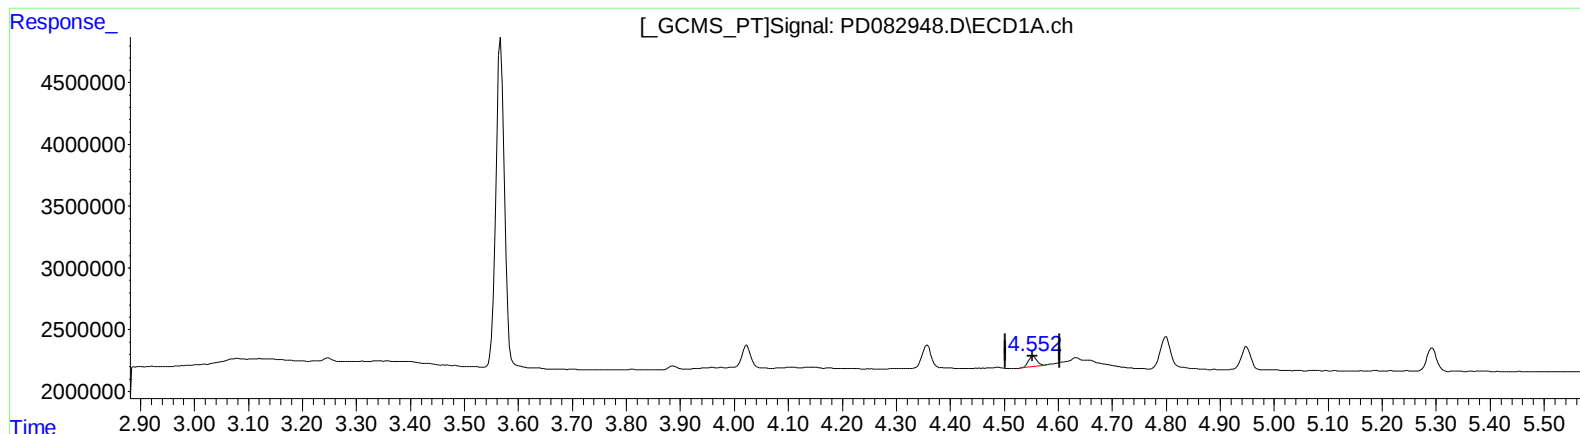

(6) beta-BHC (B)

4.552min 0.864 ng/ml m

response 937157

(6) beta-BHC #2 (B)

3.899min 1.097 ng/ml m

response 2751300

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052324\
Data File : PD082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2024 12:14
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-04

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 22:49:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

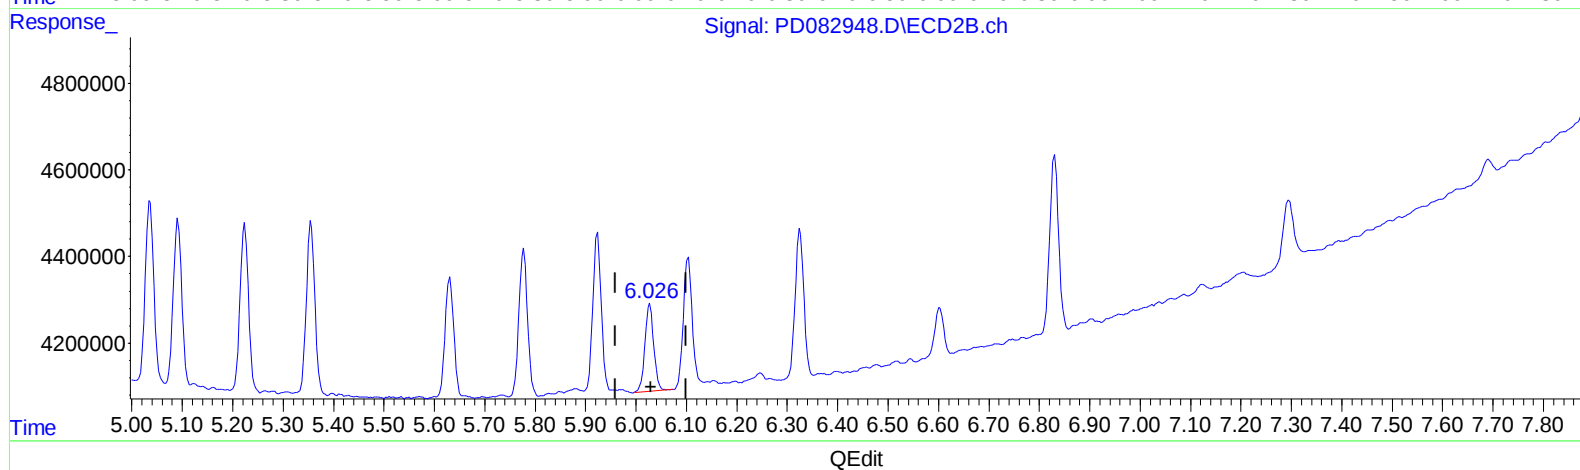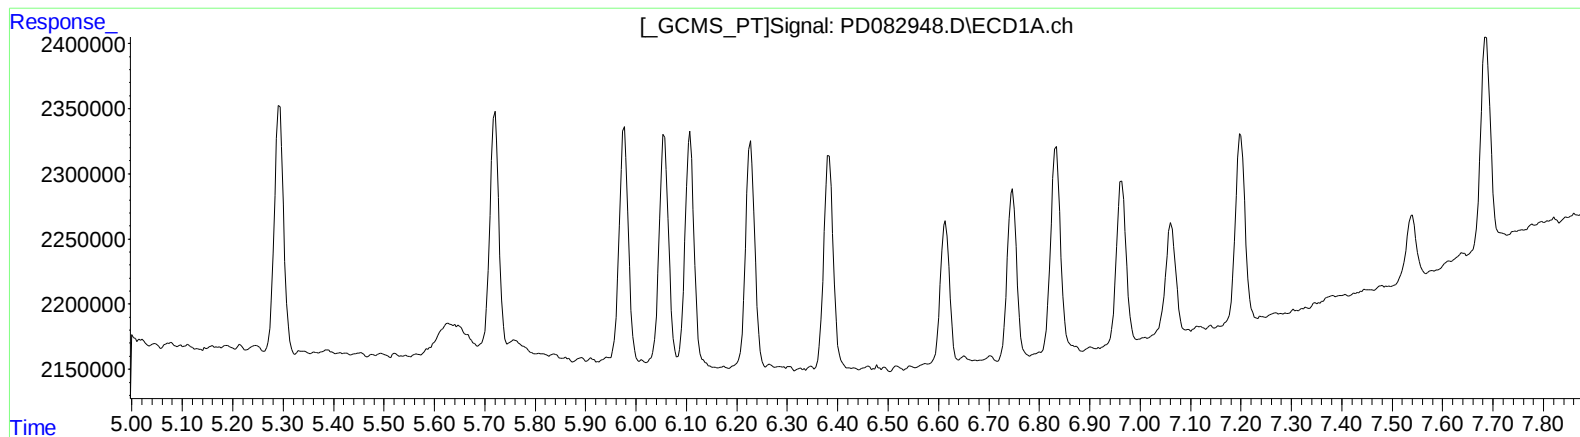

(17) 4,4'-DDT (MA)
0.000min 0.000 ng/ml
response 0

(17) 4,4'-DDT #2 (MA)
6.027min 0.633 ng/ml
response 2430086

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052324\
Data File : PD082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2024 12:14
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-04

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 22:49:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

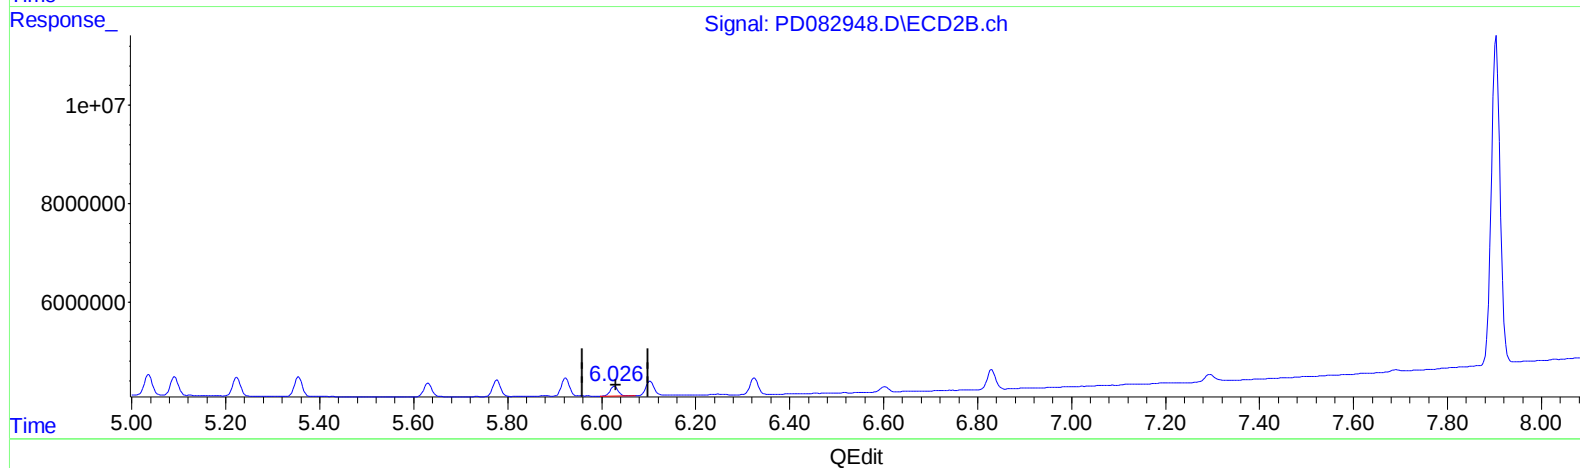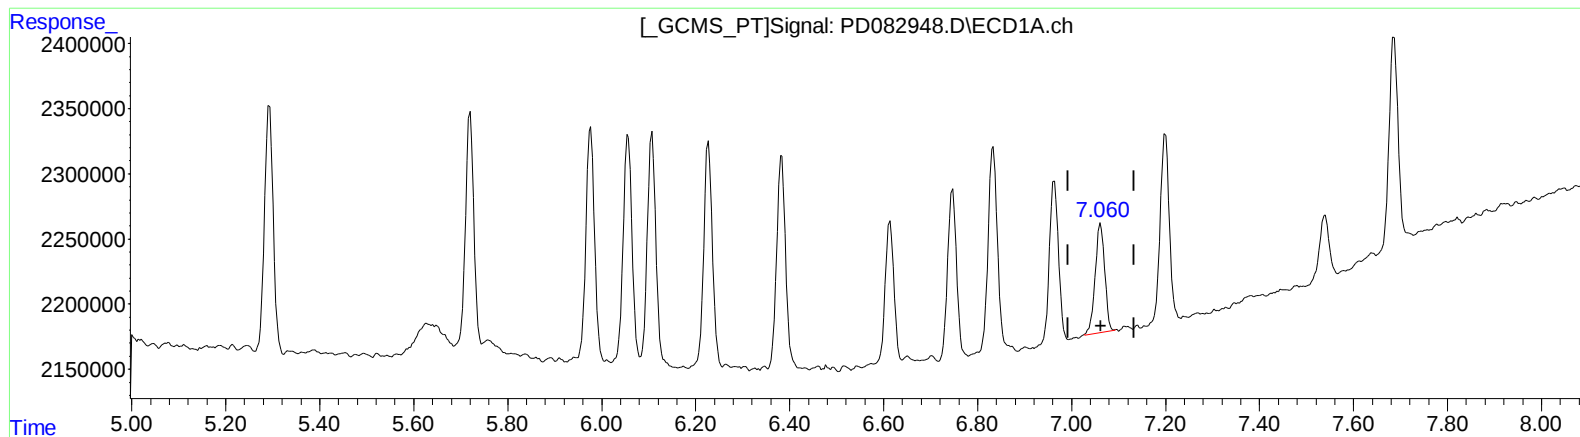

(17) 4,4'-DDT (MA)
7.060min 0.725 ng/ml m
response 1166125

(17) 4,4'-DDT #2 (MA)
6.027min 0.633 ng/ml
response 2430086

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052324\
Data File : PD082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2024 12:14
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-04

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 22:49:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

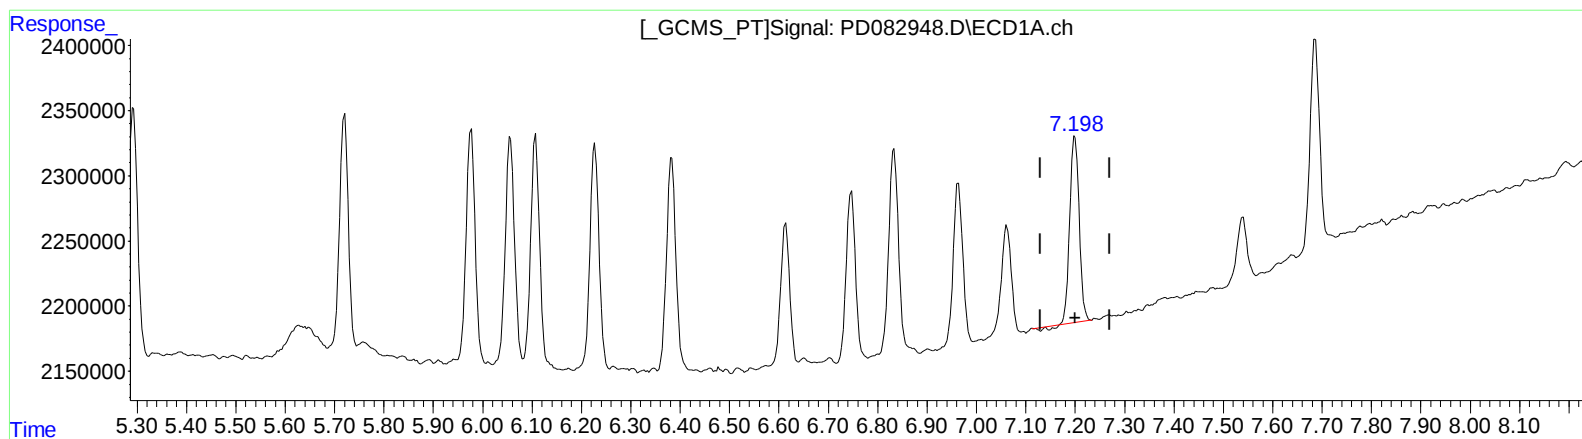

(19) Endosulfan Sulfate (B)

7.200min 1.061 ng/ml

response 1872964

(19) Endosulfan Sulfate #2 (B)

6.326min 1.019 ng/ml

response 4096248

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052324\
Data File : PD082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2024 12:14
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-04

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 22:49:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

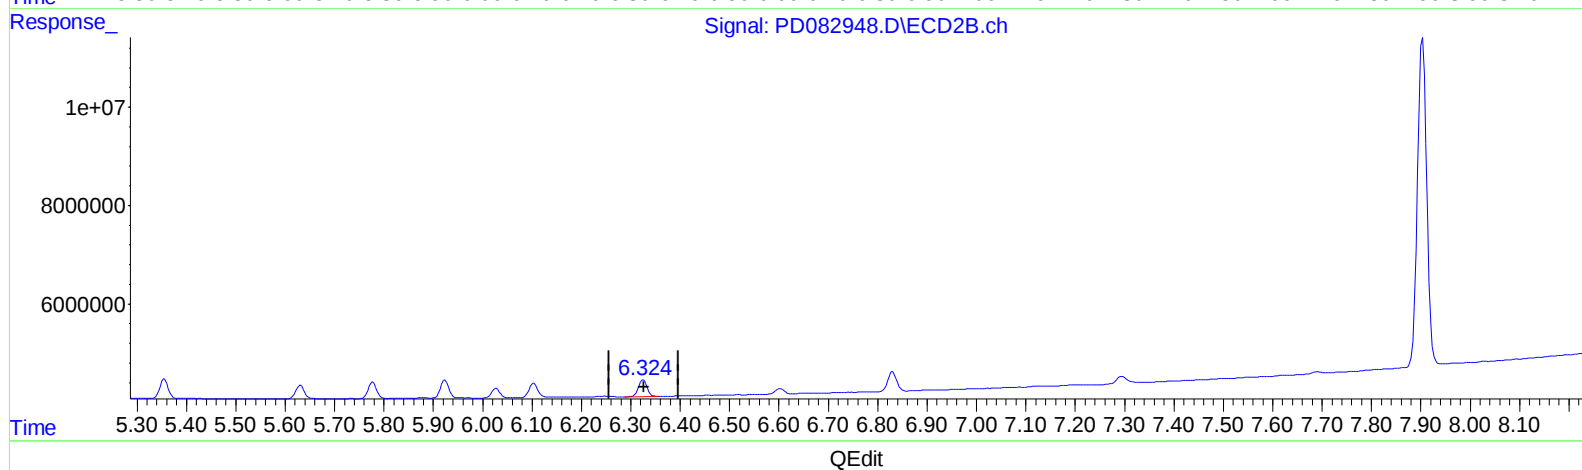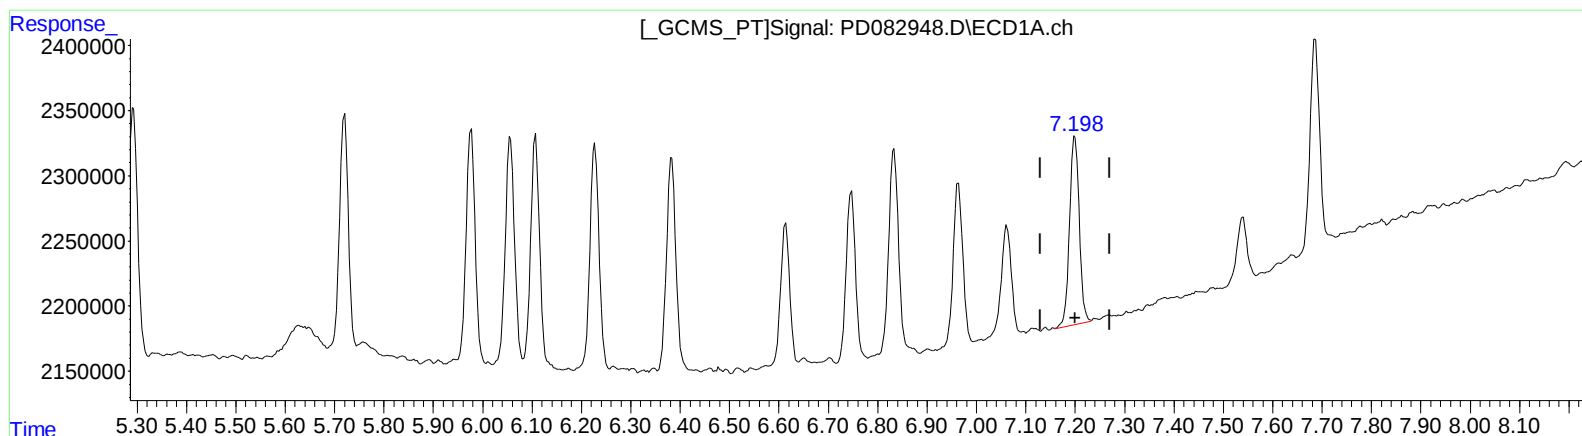

(19) Endosulfan Sulfate (B)

7.198min 1.126 ng/ml m

response 1987136

(19) Endosulfan Sulfate #2 (B)

6.326min 1.019 ng/ml

response 4096248

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052324\
Data File : PD082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2024 12:14
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-04

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 22:49:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

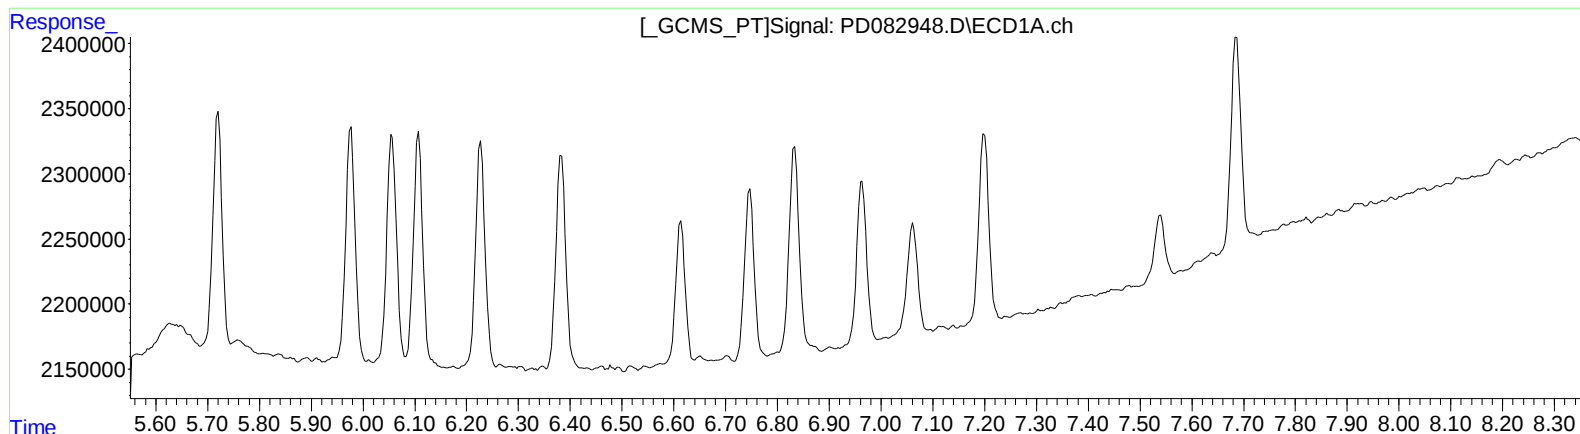

Signal: PD082948.D\ECD2B.ch

6.601

QEdit

(20) Methoxychlor (A)

0.000min 0.000 ng/ml

response 0

(20) Methoxychlor #2 (A)

6.603min 0.694 ng/ml

response 1362242

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052324\
Data File : PD082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2024 12:14
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT2-2024-04

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 05/22/2024
Supervised By :Ankita Jodhani 05/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 22:49:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

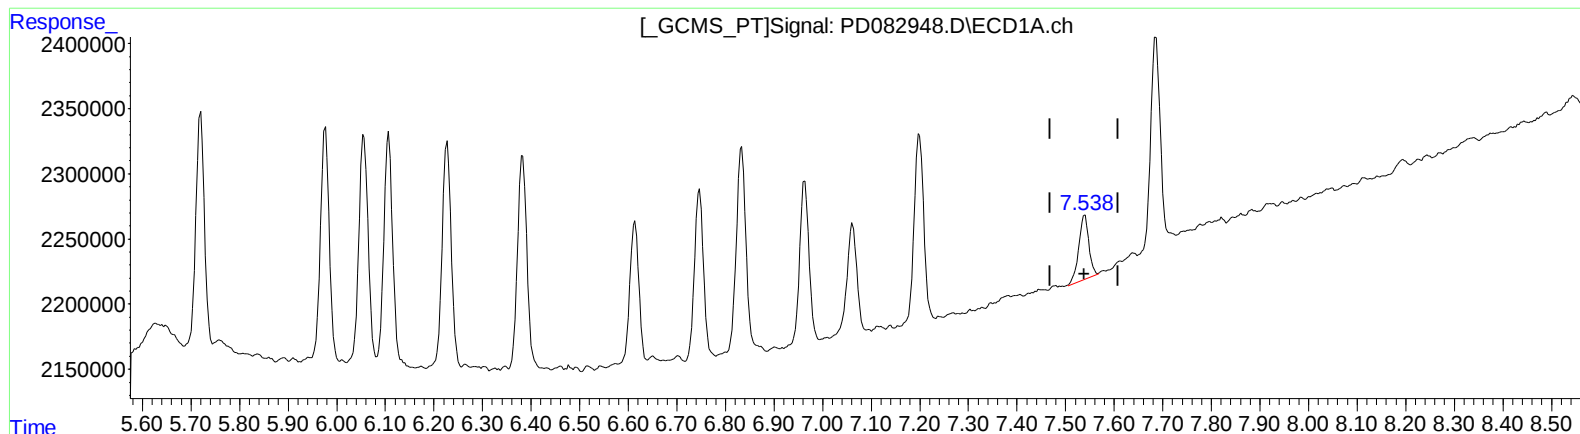

(20) Methoxychlor (A)

7.538min 0.813 ng/ml m

response 703713

(20) Methoxychlor #2 (A)

6.601min 0.710 ng/ml m

response 1394150