

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 05:27
 Operator : SM\AJ
 Sample : K2993-11
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-11 2.0-2.5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 05:44:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	3.937	192.4E6	49803260	19.862	19.994
28) SA Decachlor...	7.991	8.972	168.0E6	47085715	16.713	17.739
Target Compounds						
15) B Endosulfa...	0.000	6.861f	0	7591657	N.D.	2.815 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 05:27
Operator : SM\AJ
Sample : K2993-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-11 2.0-2.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 05:44:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

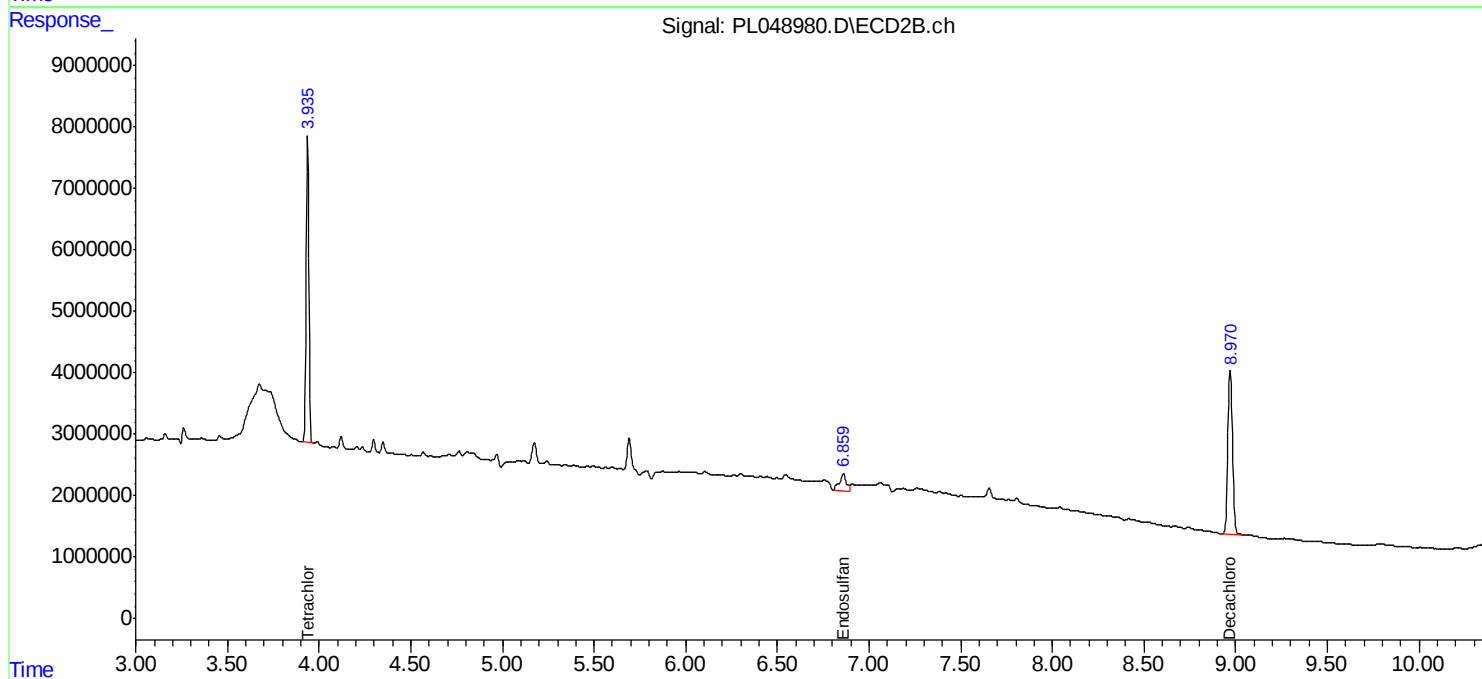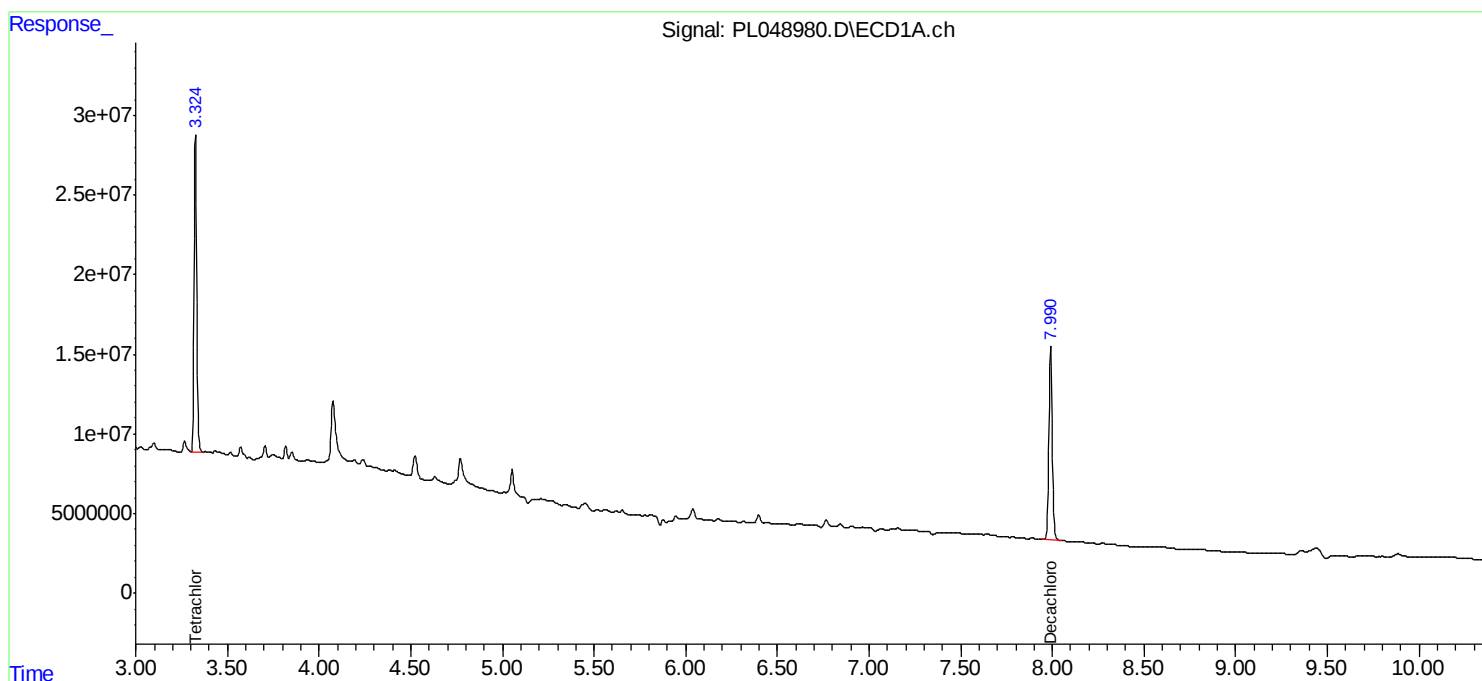


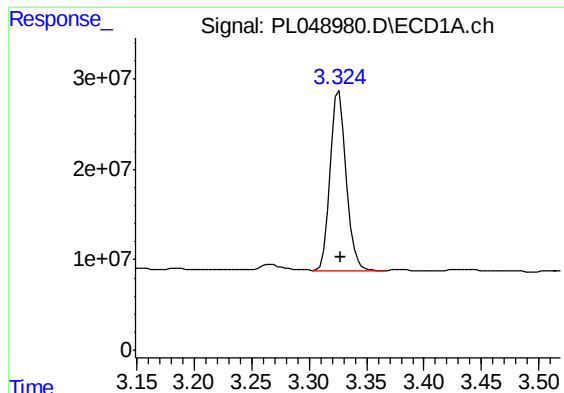

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 192396299
Conc: 19.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-11 2.0-2.5

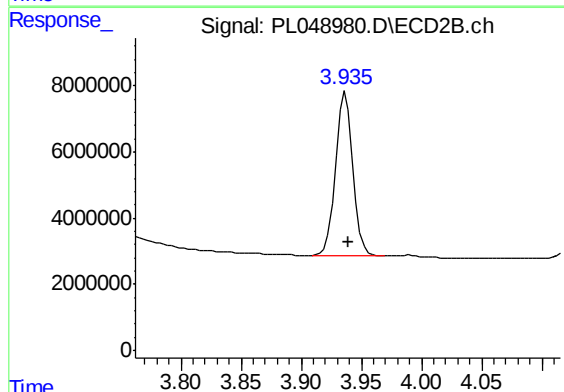


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 49803260
Conc: 19.99 ng/ml

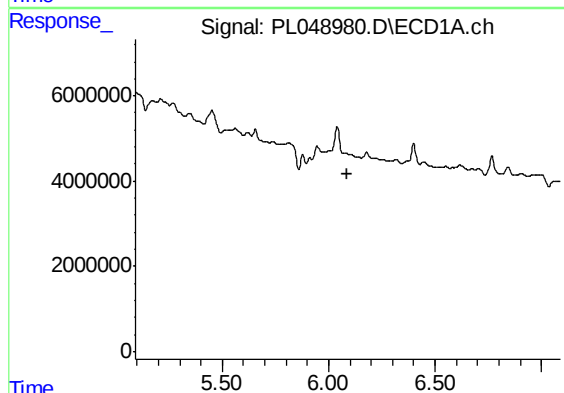


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

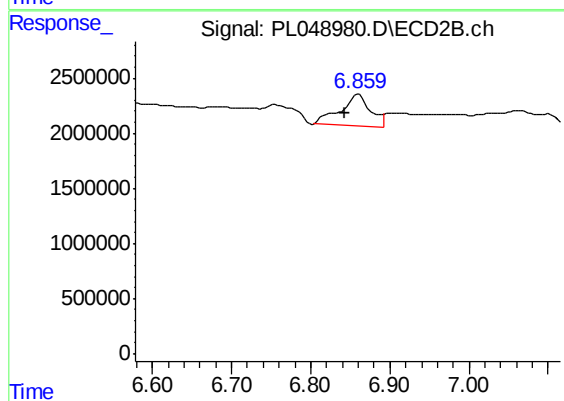

#15 Endosulfan II


R.T.: 6.861 min
Delta R.T.: 0.018 min
Response: 7591657
Conc: 2.82 ng/ml

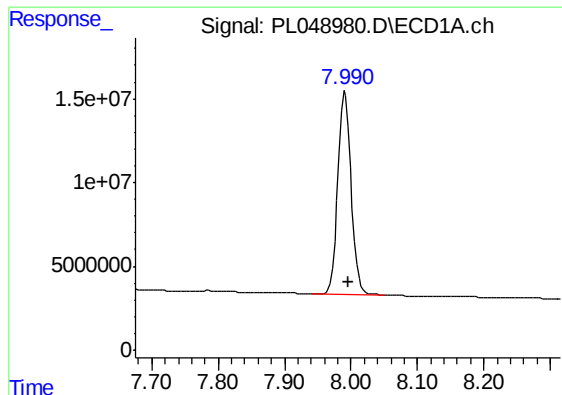

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.005 min
Response: 168038872
Conc: 16.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-11 2.0-2.5

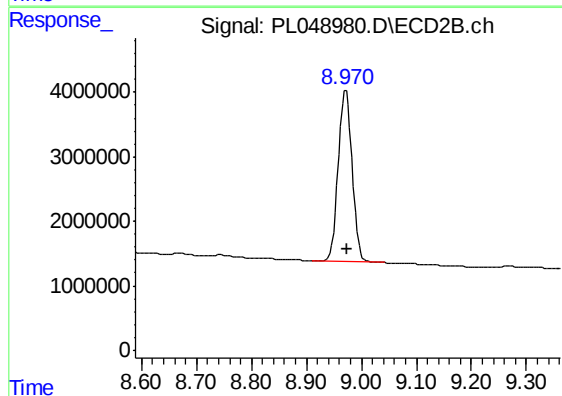

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: -0.003 min
Response: 47085715
Conc: 17.74 ng/ml