

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 11:15
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 13:36:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 13:35:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	143.5E6	1127.7E6	105.163	98.527
28)	SA Decachlor...	8.197	9.023	121.2E6	1022.4E6	101.216	98.963
Target Compounds							
23)	Chlordane-1	4.309	4.962	45609411	537.3E6	1019.917	982.446
24)	Chlordane-2	4.811	5.429	53105582	509.7E6	988.950	985.510
25)	Chlordane-3	5.379	6.074	167.7E6	2195.0E6	1047.792	1004.394
26)	Chlordane-4	5.437	6.148	137.2E6	2497.7E6	1052.725	1001.499
27)	Chlordane-5	6.274	6.952	50645589	440.9E6	1032.538	1136.686



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 11:15
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 13:36:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 13:35:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

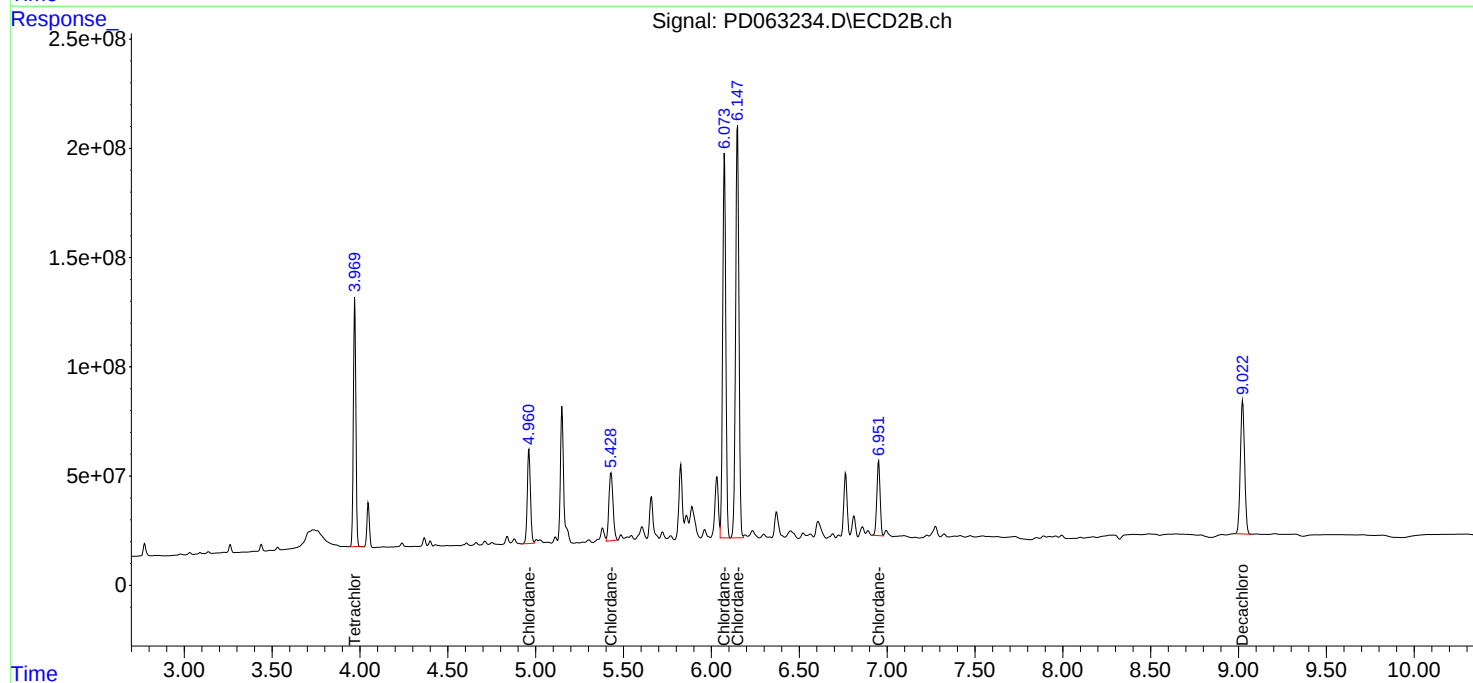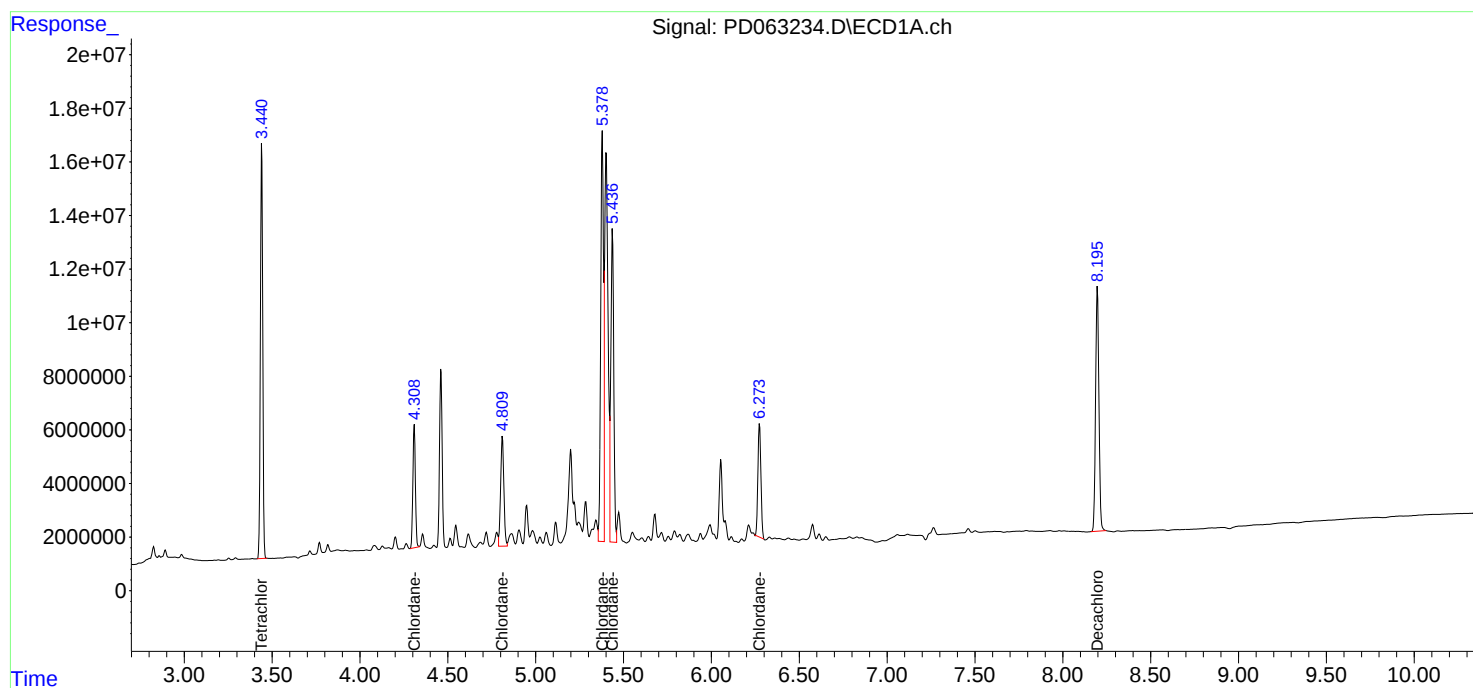


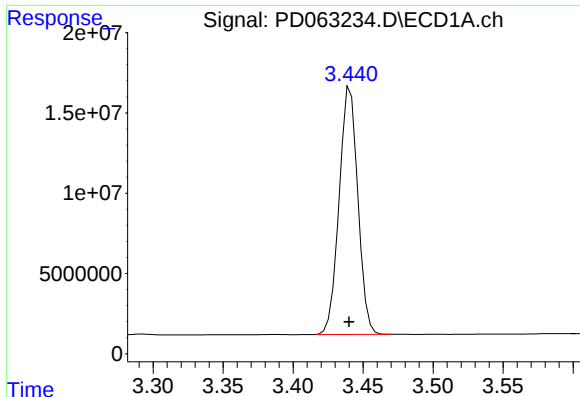

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 143498112
Conc: 105.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

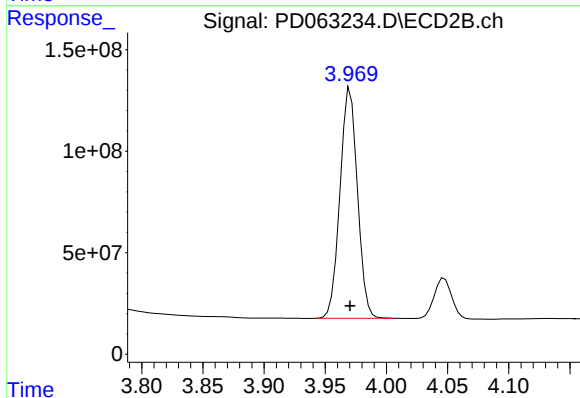


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 1127663972
Conc: 98.53 ng/ml

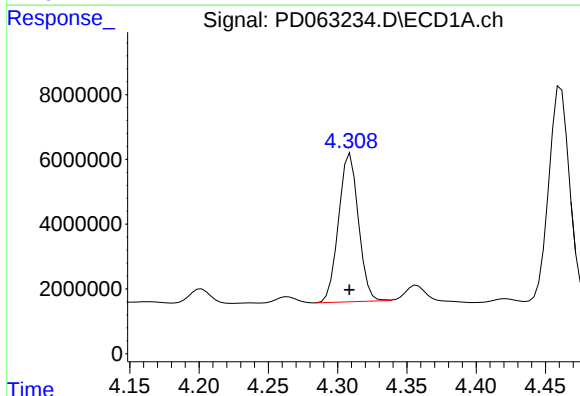


#23 Chlordane-1

R.T.: 4.309 min
Delta R.T.: 0.000 min
Response: 45609411
Conc: 1019.92 ng/ml

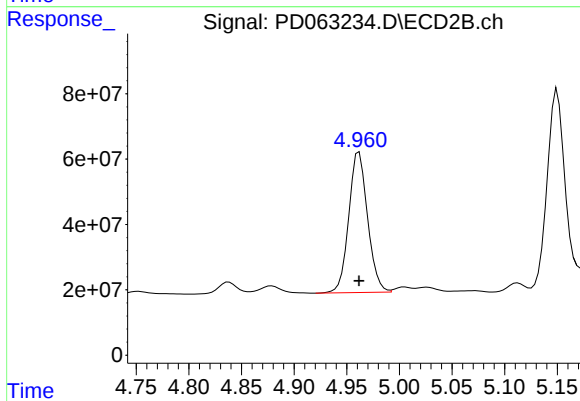

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 537258500
Conc: 982.45 ng/ml

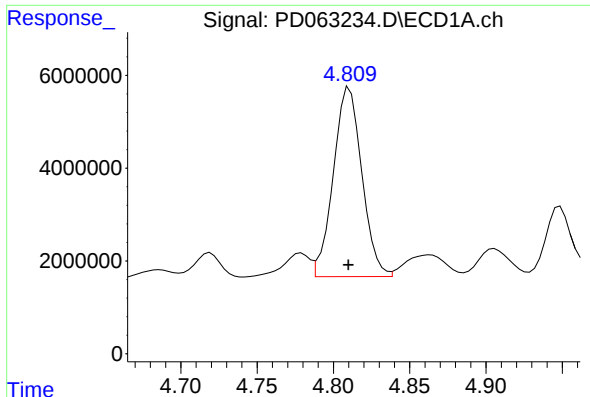

#24 Chlordane-2


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 53105582
Conc: 988.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

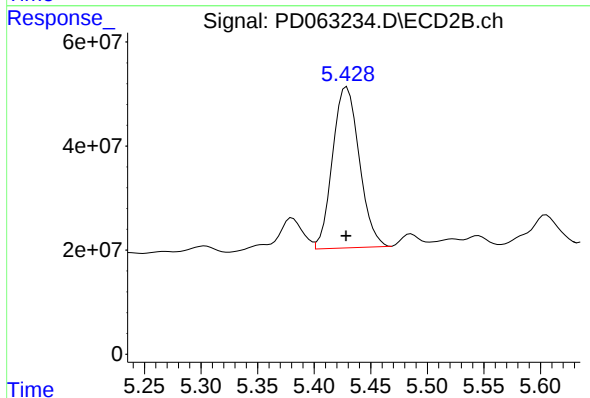


#24 Chlordane-2

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 509724048
Conc: 985.51 ng/ml

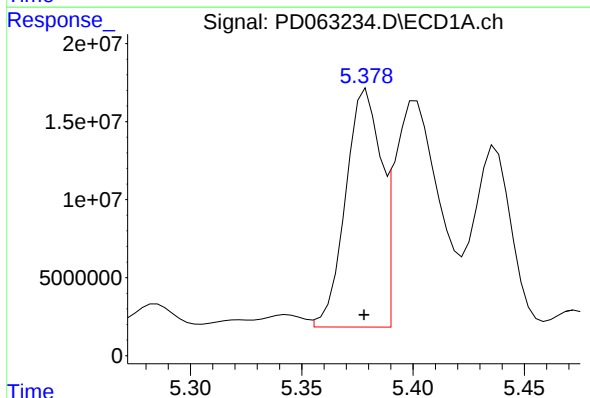


#25 Chlordane-3

R.T.: 5.379 min
Delta R.T.: 0.001 min
Response: 167708737
Conc: 1047.79 ng/ml

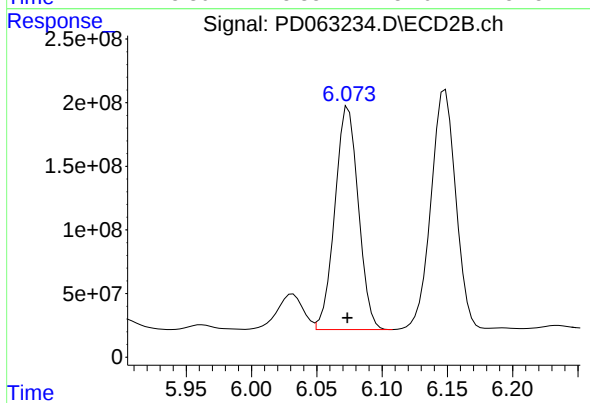

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 2195033426
Conc: 1004.39 ng/ml

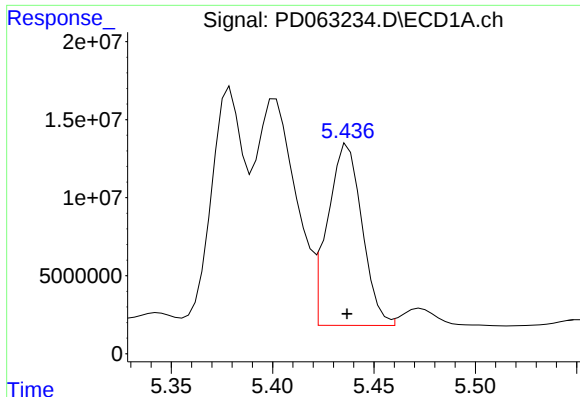

#26 Chlordane-4


R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 137233443
Conc: 1052.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

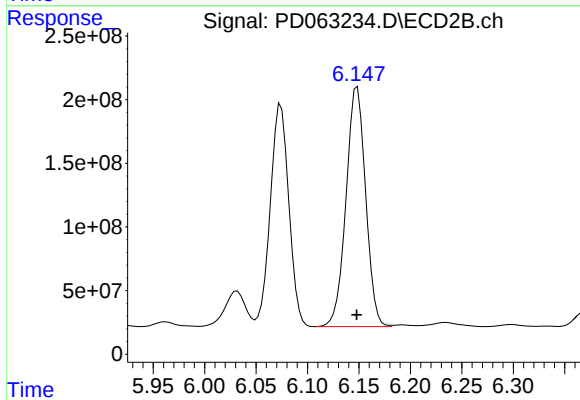


#26 Chlordane-4

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 2497724390
Conc: 1001.50 ng/ml

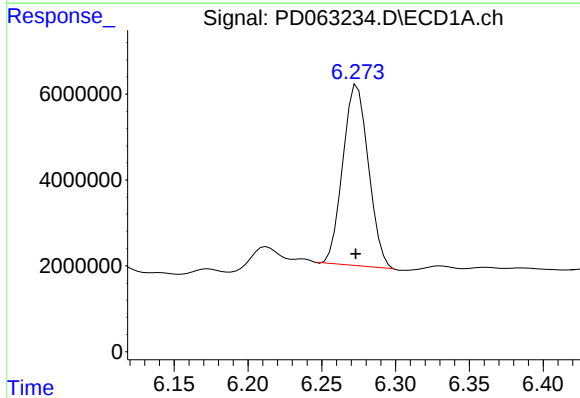


#27 Chlordane-5

R.T.: 6.274 min
Delta R.T.: 0.001 min
Response: 50645589
Conc: 1032.54 ng/ml

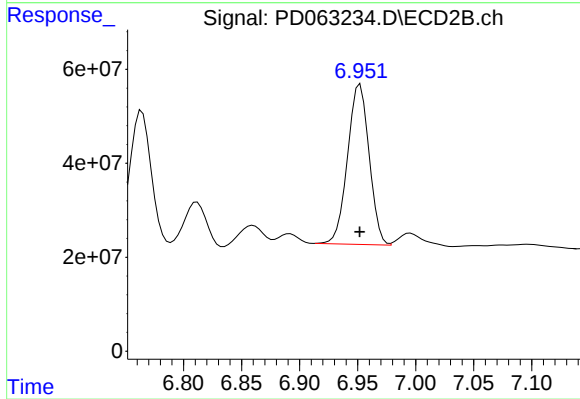

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 440931483
Conc: 1136.69 ng/ml

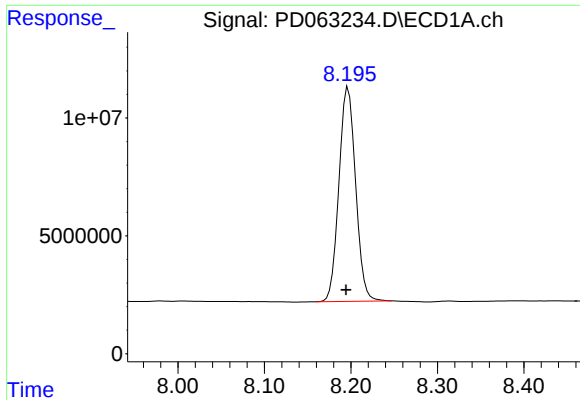

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: 0.002 min
Response: 121175839
Conc: 101.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

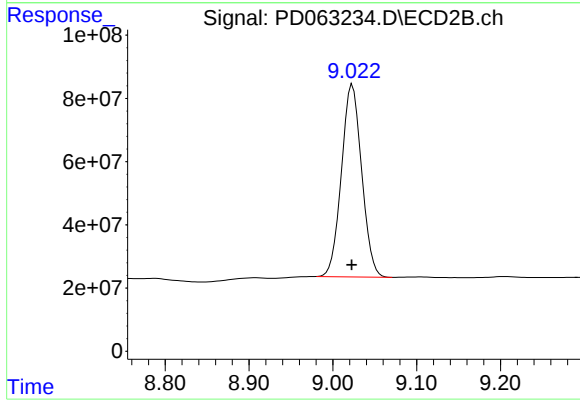

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 1022381955
Conc: 98.96 ng/ml