

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 12:26
 Operator : AR\AJ
 Sample : PTOXICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 13:59:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 13:58:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.440	3.970	126.2E6	1145.2E6	101.522	95.895
7) SA Decachlor...	8.194	9.022	128.5E6	1045.3E6	98.706	94.901
Target Compounds						
2) Toxaphene-1	5.996	6.543	9314444	143.3E6	954.396	961.670
3) Toxaphene-2	6.177	7.049	10999120	111.5E6	1005.773	943.675
4) Toxaphene-3	6.298	7.125	25202089	312.7E6	1022.061	963.537
5) Toxaphene-4	6.542	7.211	25826843	195.3E6	1054.137	970.099
6) Toxaphene-5	7.030	7.624	25843401	135.6E6	1022.535	1001.145

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 12:26
Operator : AR\AJ
Sample : PTOXICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 13:59:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 13:58:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

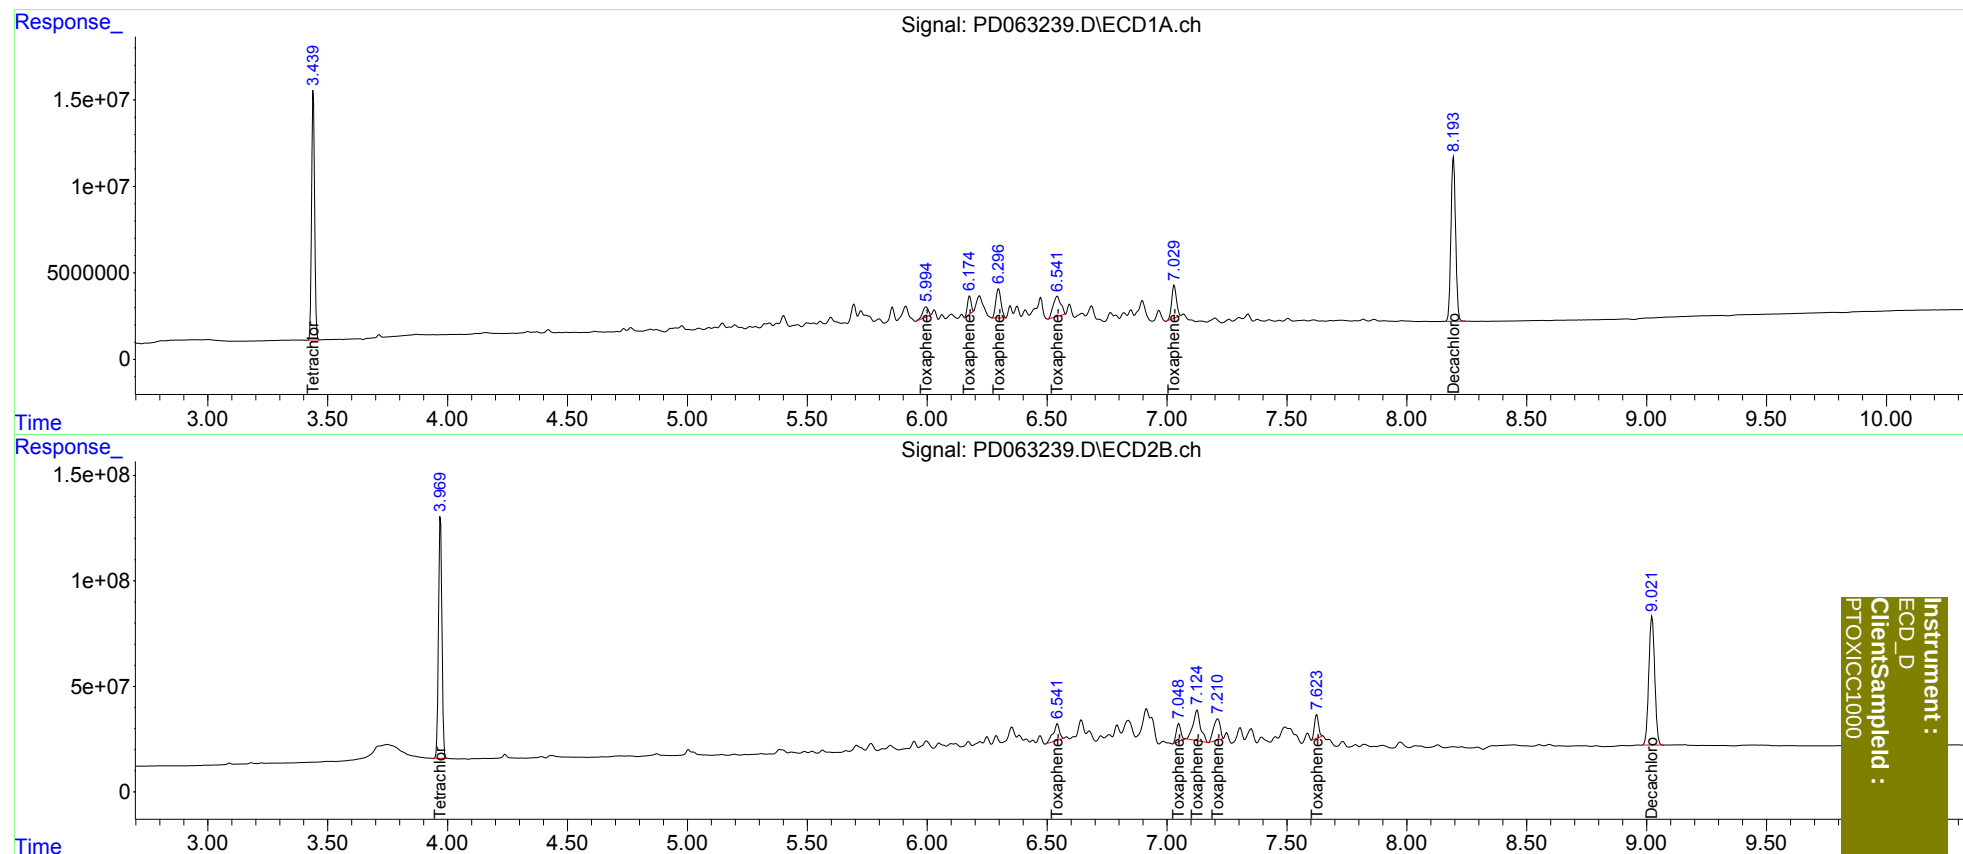

Instrument :
ECD_D
ClientSampled :
PTOXICC1000