

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 14:10
 Operator : AR\AJ
 Sample : PTOXICC100
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC100

Manual Integrations
 APPROVED

Ankita
 5/25/2021 4:05:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 14:25:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 14:25:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.445	3.971	11641429	117.4E6	9.367	9.830
7) SA Decachlor...	8.201	9.026	12276684	100.5E6	9.433	9.125
Target Compounds						
2) Toxaphene-1	6.001	6.545	1230596	15933727	126.092	106.957
3) Toxaphene-2	6.184	7.051	982116	11192425	89.806	94.722m
4) Toxaphene-3	6.303	7.127	2354358	28263529	95.480	87.092
5) Toxaphene-4	6.548	7.214	2143789	14826351	87.500	73.653
6) Toxaphene-5	7.038	7.628	3570232	10620689	141.262	78.417 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 14:10
Operator : AR\AJ
Sample : PTOXICC100
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 14:25:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 14:25:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

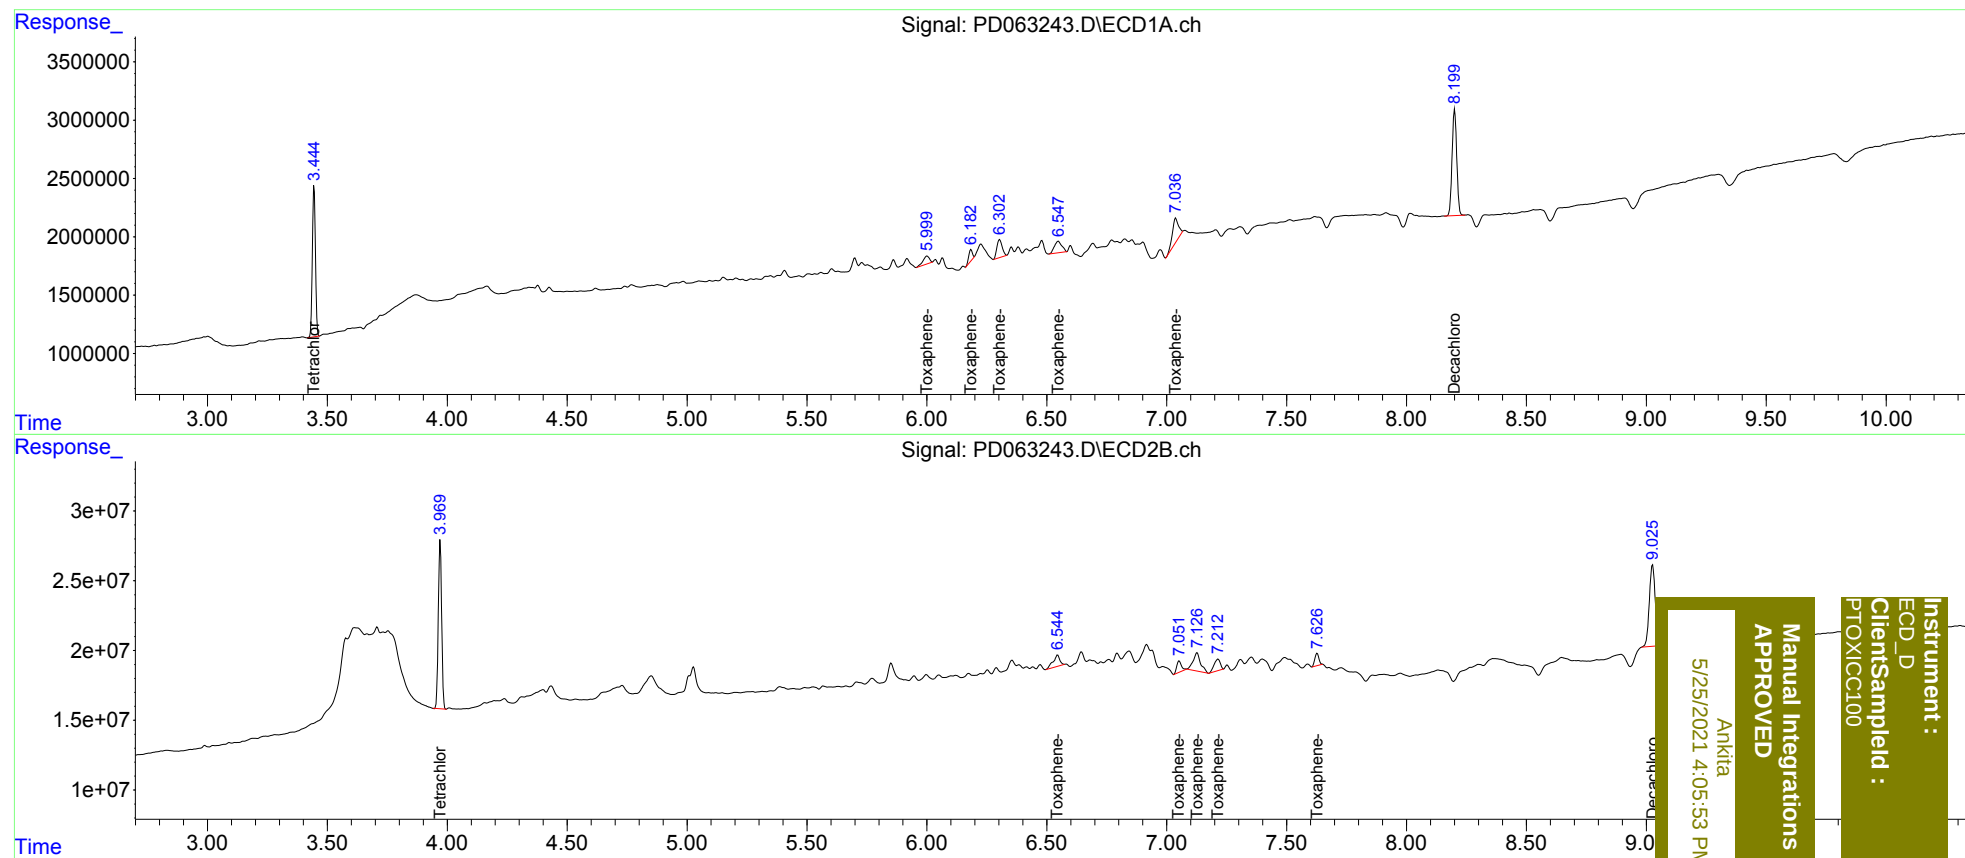

Manual Integrations
APPROVED

Ankita
5/25/2021 4:05:53 PM

Instrument :
ECD_D
ClientSampled :
PTOXICC100