

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 14:38
 Operator : AR\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD052421

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 14:49:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 14:27:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.440	3.970	62755164	597.1E6	50.354	50.006
7) SA Decachlor...	8.195	9.022	65032326	561.9E6	50.259	52.051
Target Compounds						
2) Toxaphene-1	5.996	6.543	4853094	74827114	470.468	496.444
3) Toxaphene-2	6.178	7.048	5443029	59625984	504.887	556.695
4) Toxaphene-3	6.298	7.125	12446291	166.1E6	505.448	536.038
5) Toxaphene-4	6.543	7.212	12369010	100.2E6	506.810	535.432
6) Toxaphene-5	7.031	7.624	12604238	70041667	457.787	551.776

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 14:38
Operator : AR\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 14:49:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 14:27:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

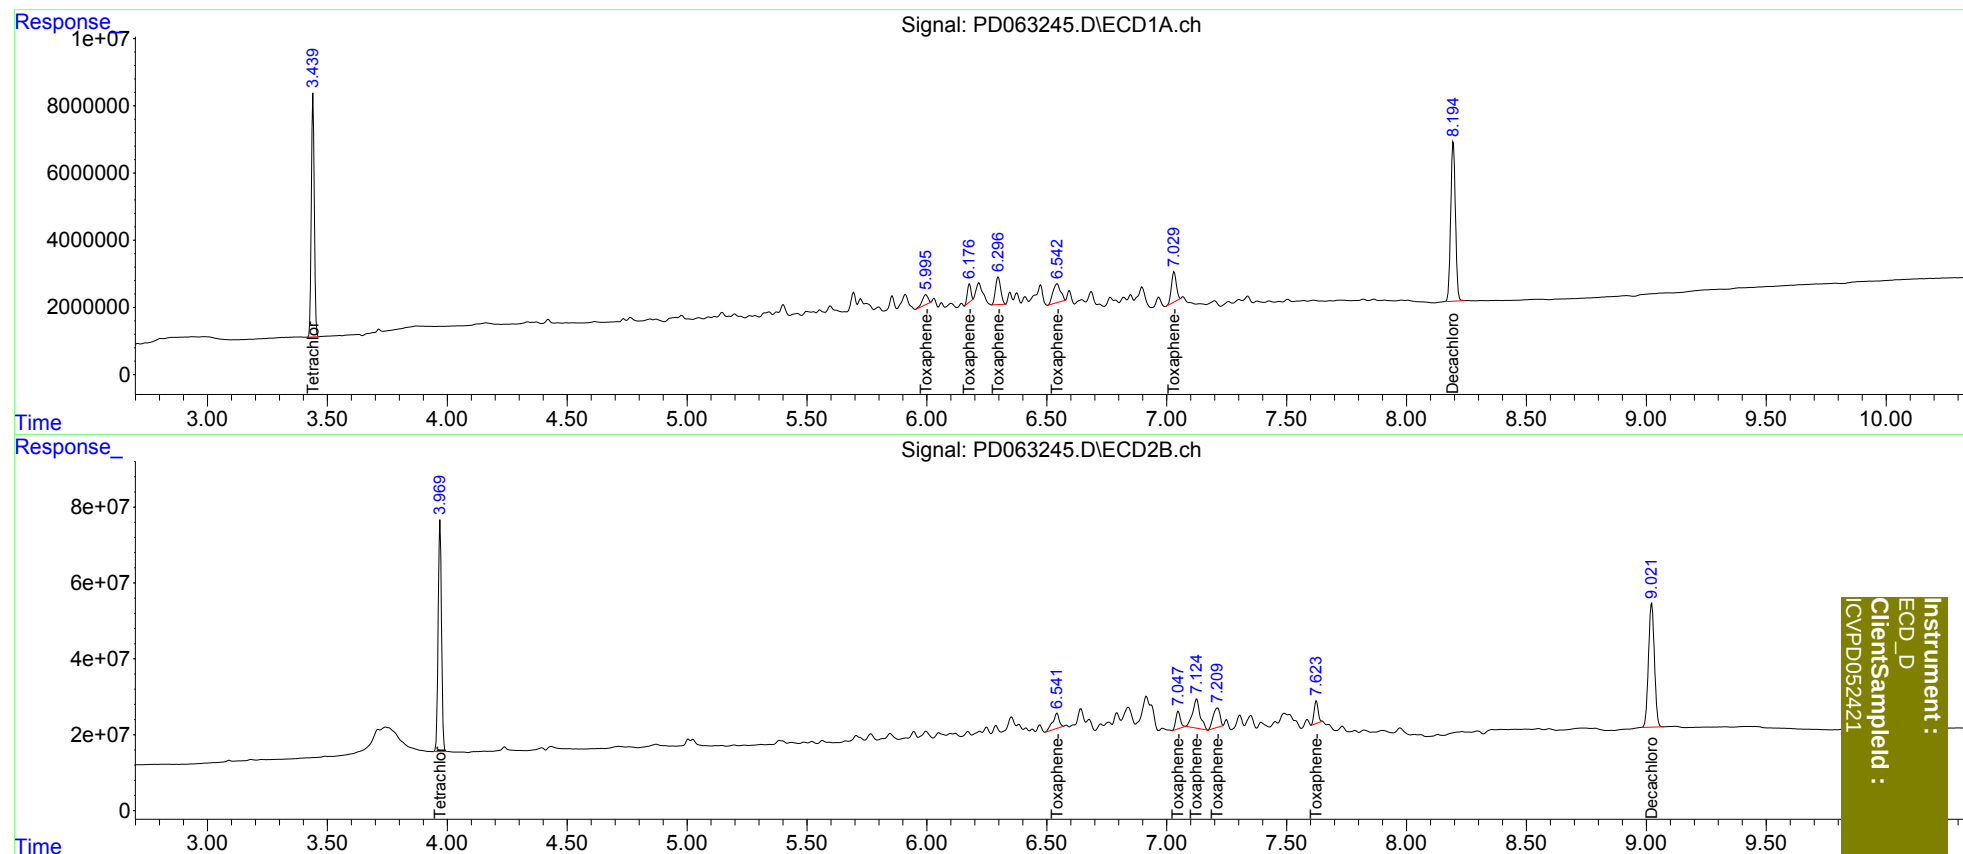

Instrument :
ECD_D
ClientSampled :
ICV/PD052421