

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 11:01
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 15:53:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 14:48:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	3.971	24725716	242.3E6	22.447	20.910
28)	SA Decachlor...	8.206	9.029	24552651	206.0E6	19.509	20.190
Target Compounds							
9)	A Endosulfan I	5.500	6.199	13345575	150.2E6	9.835	10.576
10)	B gamma-Chl...	5.389	6.077	15127505	164.5E6	10.313	10.553
12)	B 4,4'-DDE	5.611	6.307	30714072	307.9E6	21.409	20.399
13)	MA Dieldrin	5.744	6.456	31614502	309.7E6	21.366	20.425
19)	B Endosulfa...	6.657	7.230	21784288	232.8E6	18.074	18.973
20)	A Methoxychlor	6.915	7.553	53437089	450.9E6	79.630	78.605
21)	B Endrin ke...	7.149	7.700	27324666	223.0E6	18.491	18.593



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 11:01
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 15:53:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 14:48:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

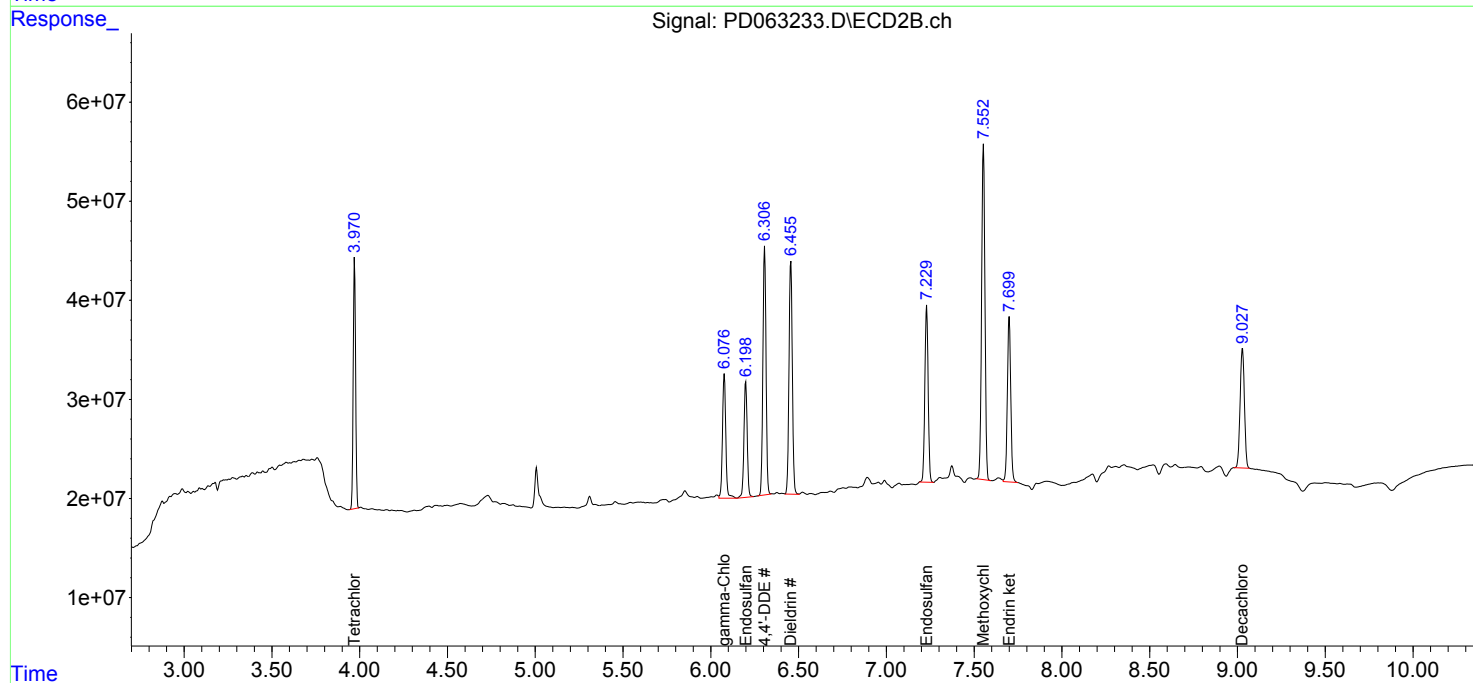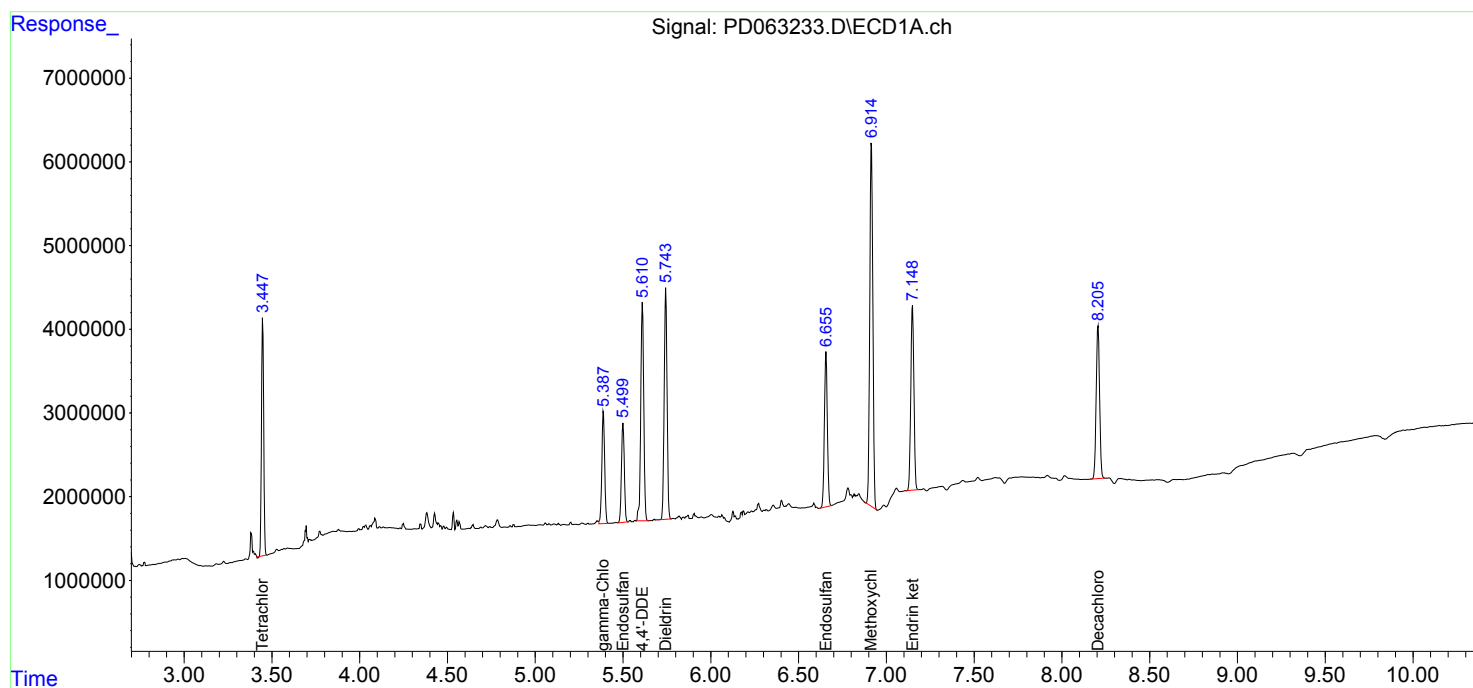


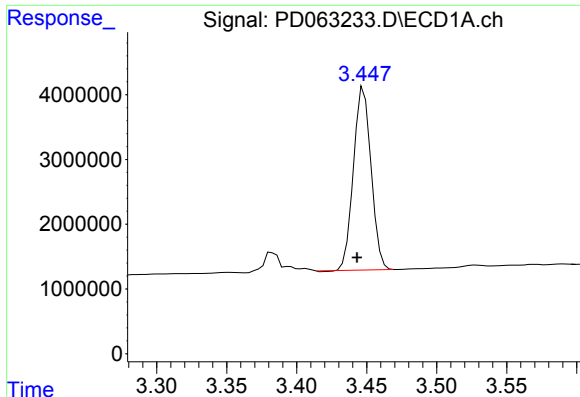

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.005 min
Response: 24725716
Conc: 22.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

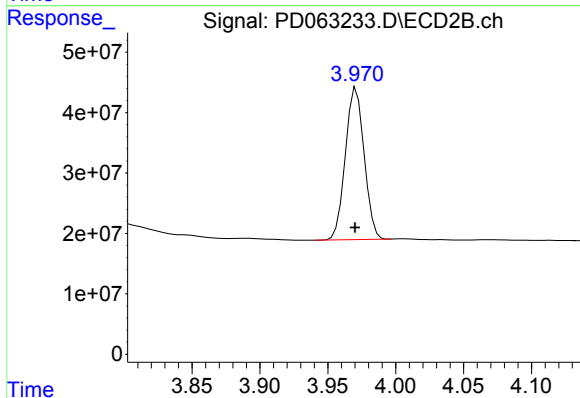


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.001 min
Response: 242307152
Conc: 20.91 ng/ml

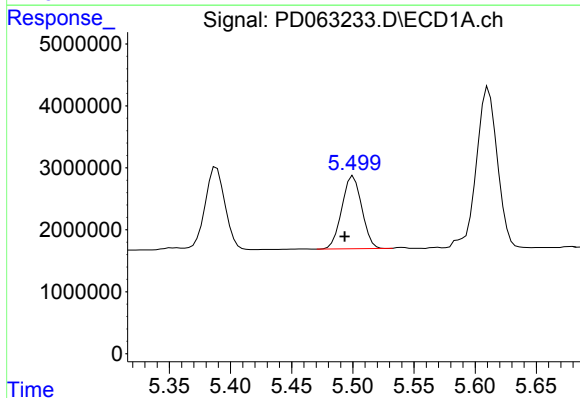


#9 Endosulfan I

R.T.: 5.500 min
Delta R.T.: 0.007 min
Response: 13345575
Conc: 9.83 ng/ml

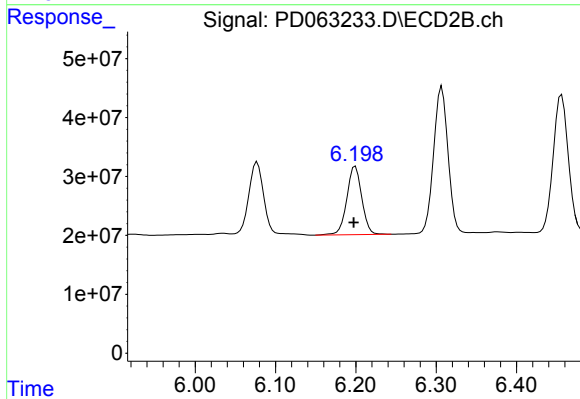

#9 Endosulfan I


R.T.: 6.199 min
Delta R.T.: 0.002 min
Response: 150234823
Conc: 10.58 ng/ml

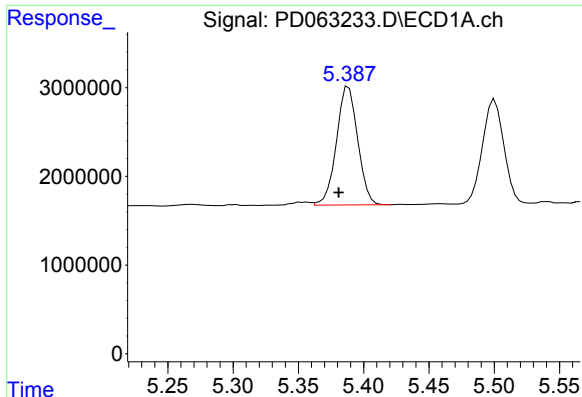

#10 gamma-Chlordane


R.T.: 5.389 min
Delta R.T.: 0.008 min
Response: 15127505
Conc: 10.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

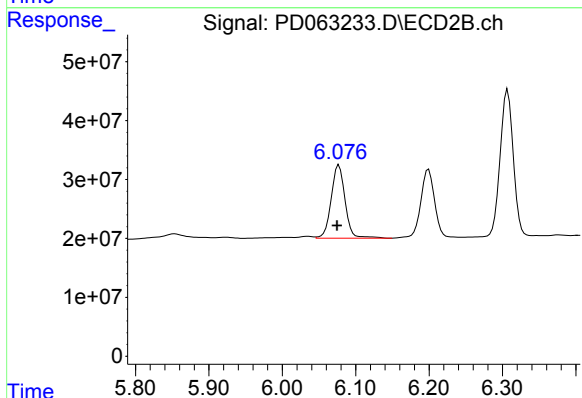


#10 gamma-Chlordane

R.T.: 6.077 min
Delta R.T.: 0.003 min
Response: 164504346
Conc: 10.55 ng/ml

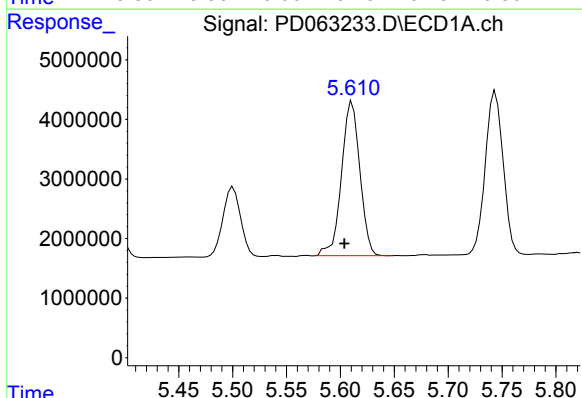


#12 4,4'-DDE

R.T.: 5.611 min
Delta R.T.: 0.007 min
Response: 30714072
Conc: 21.41 ng/ml

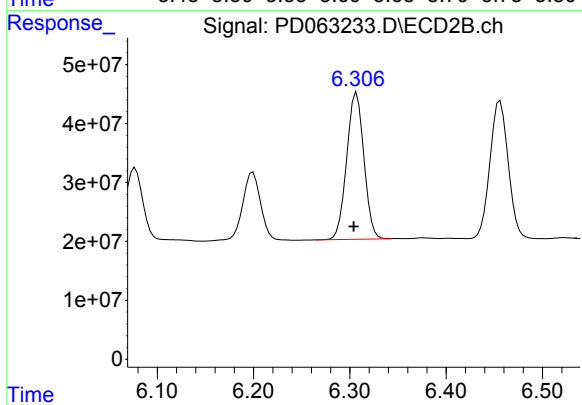

#12 4,4'-DDE


R.T.: 6.307 min
Delta R.T.: 0.003 min
Response: 307899854
Conc: 20.40 ng/ml

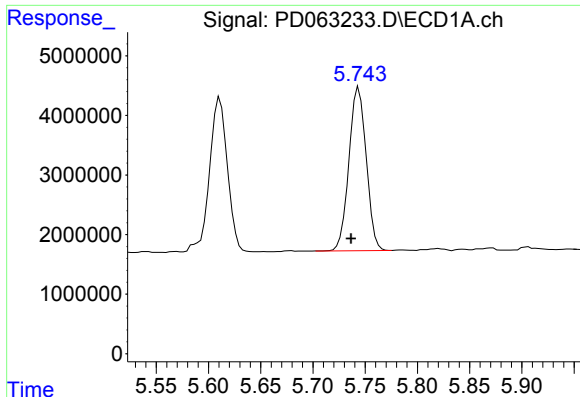

#13 Dieldrin


R.T.: 5.744 min
Delta R.T.: 0.007 min
Response: 31614502
Conc: 21.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

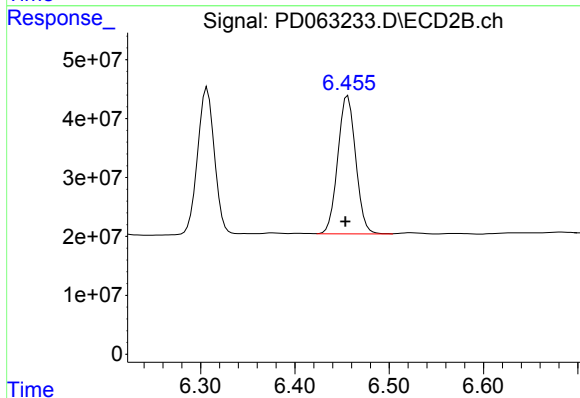


#13 Dieldrin

R.T.: 6.456 min
Delta R.T.: 0.002 min
Response: 309707582
Conc: 20.42 ng/ml

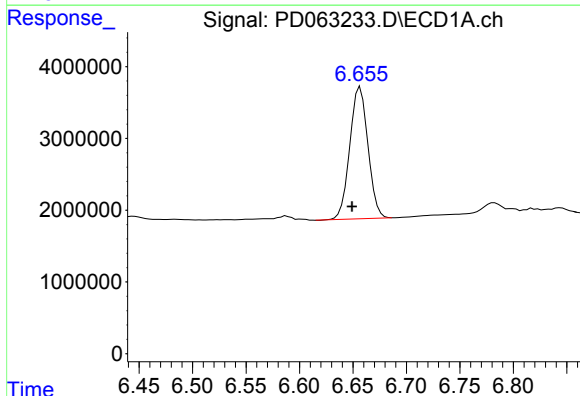


#19 Endosulfan Sulfate

R.T.: 6.657 min
Delta R.T.: 0.008 min
Response: 21784288
Conc: 18.07 ng/ml

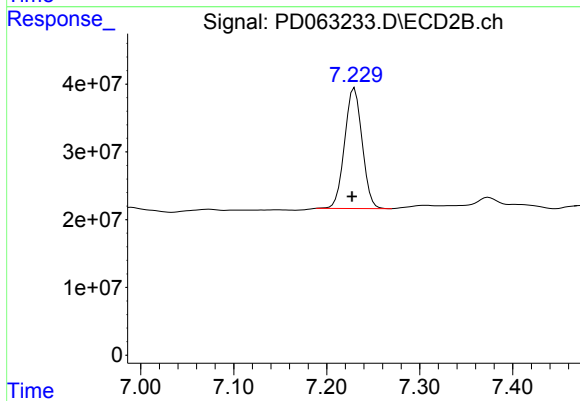

#19 Endosulfan Sulfate


R.T.: 7.230 min
Delta R.T.: 0.003 min
Response: 232799989
Conc: 18.97 ng/ml

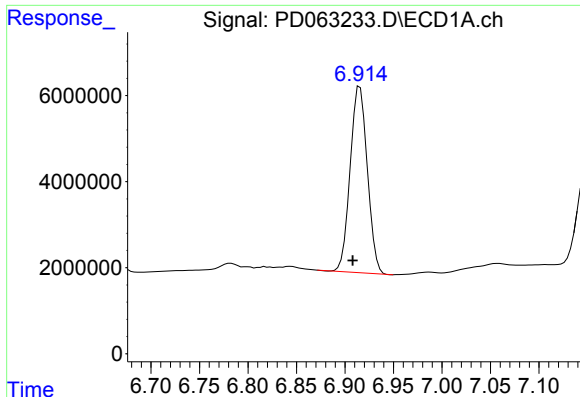

#20 Methoxychlor


R.T.: 6.915 min
Delta R.T.: 0.008 min
Response: 53437089
Conc: 79.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

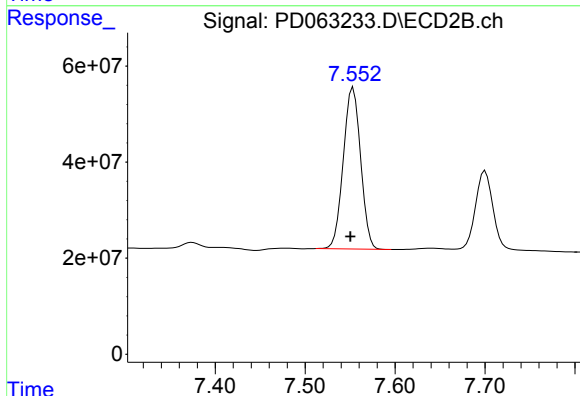


#20 Methoxychlor

R.T.: 7.553 min
Delta R.T.: 0.003 min
Response: 450931906
Conc: 78.61 ng/ml

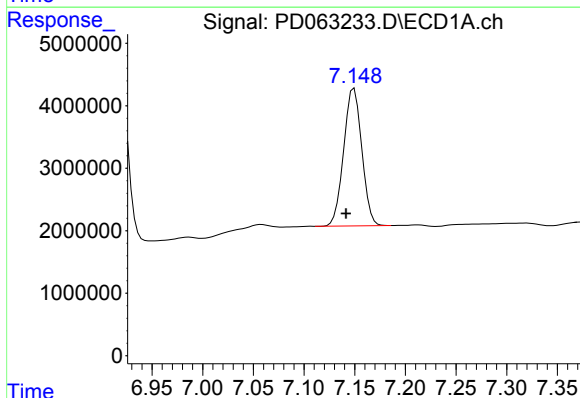


#21 Endrin ketone

R.T.: 7.149 min
Delta R.T.: 0.008 min
Response: 27324666
Conc: 18.49 ng/ml

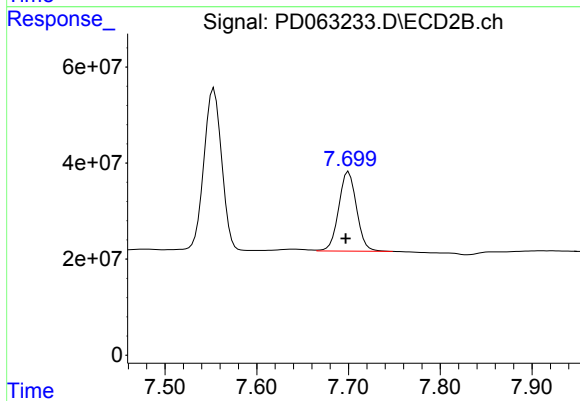

#21 Endrin ketone

R.T.: 7.700 min
Delta R.T.: 0.003 min
Response: 223031095
Conc: 18.59 ng/ml

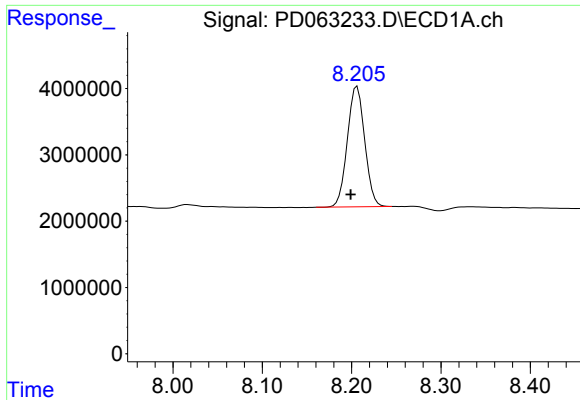

#28 Decachlorobiphenyl


R.T.: 8.206 min

Delta R.T.: 0.007 min

Response: 24552651

Conc: 19.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

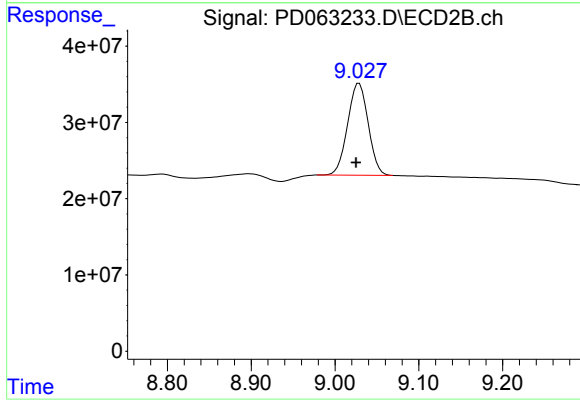

#28 Decachlorobiphenyl

R.T.: 9.029 min

Delta R.T.: 0.004 min

Response: 205978901

Conc: 20.19 ng/ml